


A Extraction and quality control workflow

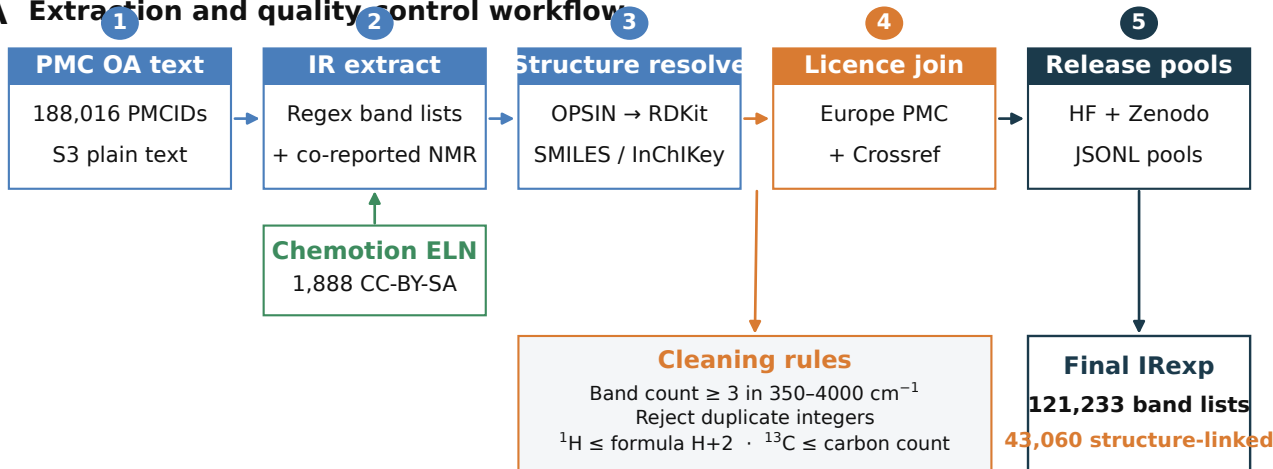

B Automated QC rejections

⊗ Band count too low

IR (KBr): **3421, 2923, 2854** cm^{-1} — <3 unique peaks after de-duplication.

⊗ IR band outside window

IR (neat): 3200, 2958, **4180**, 1520 cm^{-1} — 4180 outside 350-4000 cm^{-1} .

⊗ ^1H integral vs formula

^1H : **(5H)+(5H)+(10H)=20H**; $\text{C}_6\text{H}_5\text{NO}_2$ (7H) — integral > H+2.