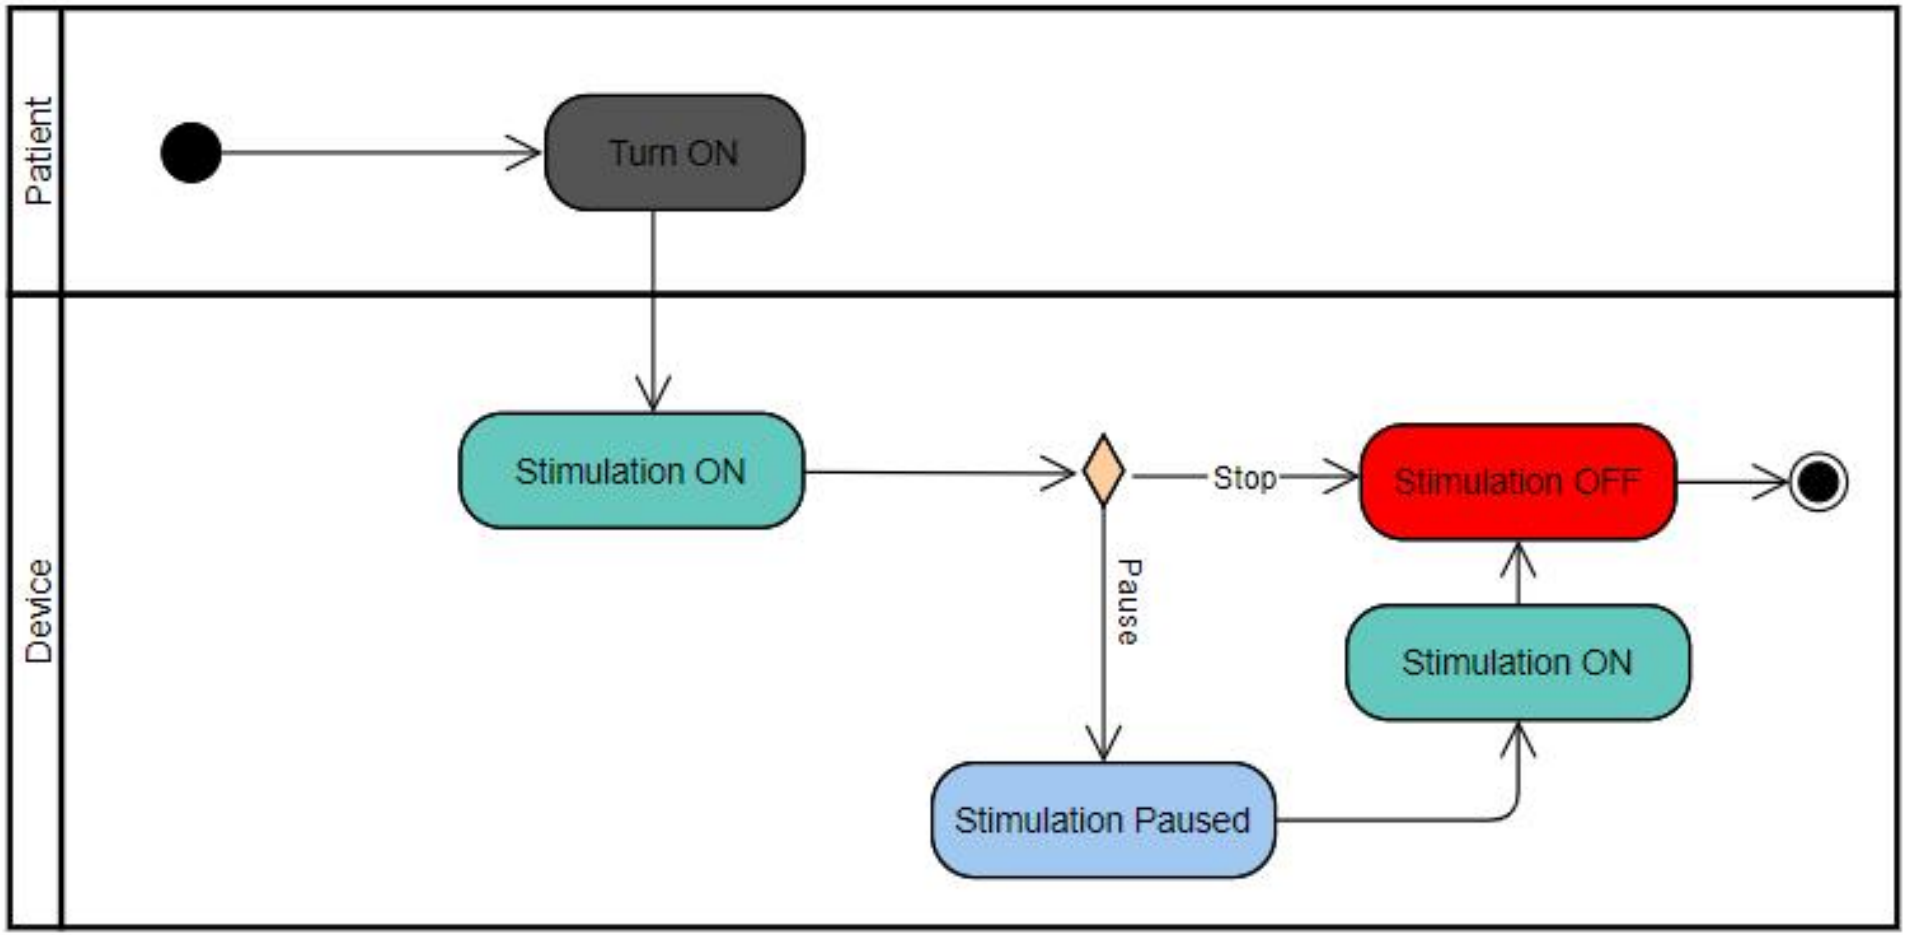
Patient
Turn ON
Device
Stimulation ON
Stop
Stimulation OFF
Pause
Stimulation ON
Stimulation Paused