




TENS Device Waveform Simulation - Mode 1 (15 Hz)

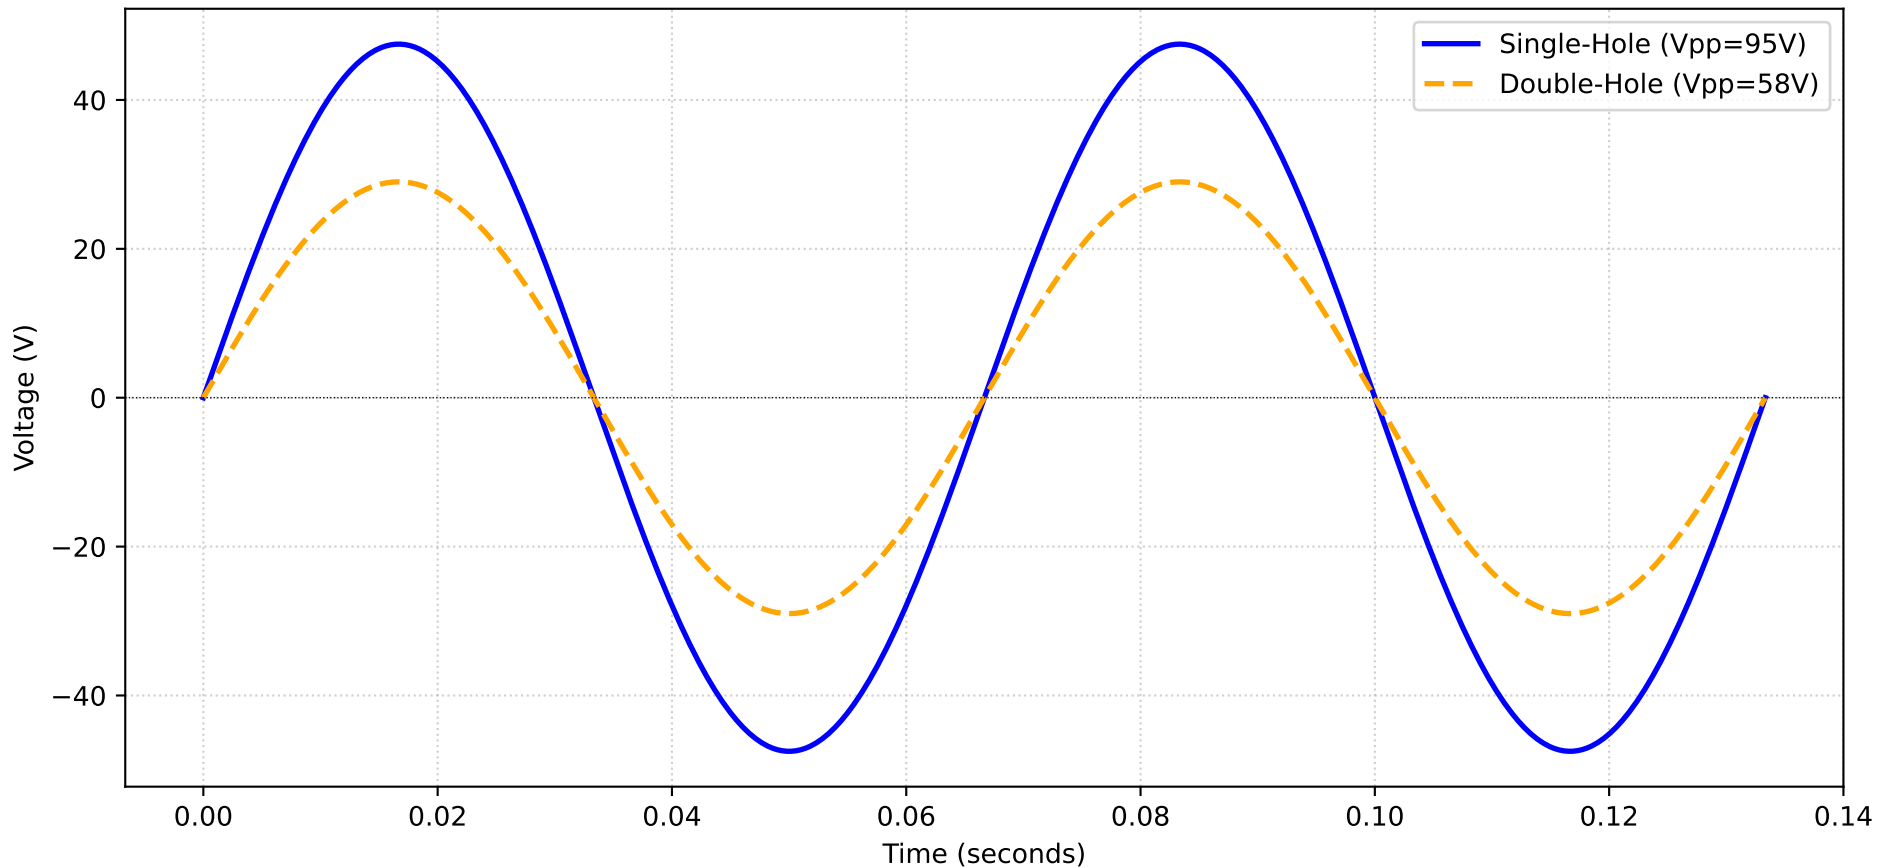


TENS Device Waveform Simulation - Mode 2 (38 Hz)

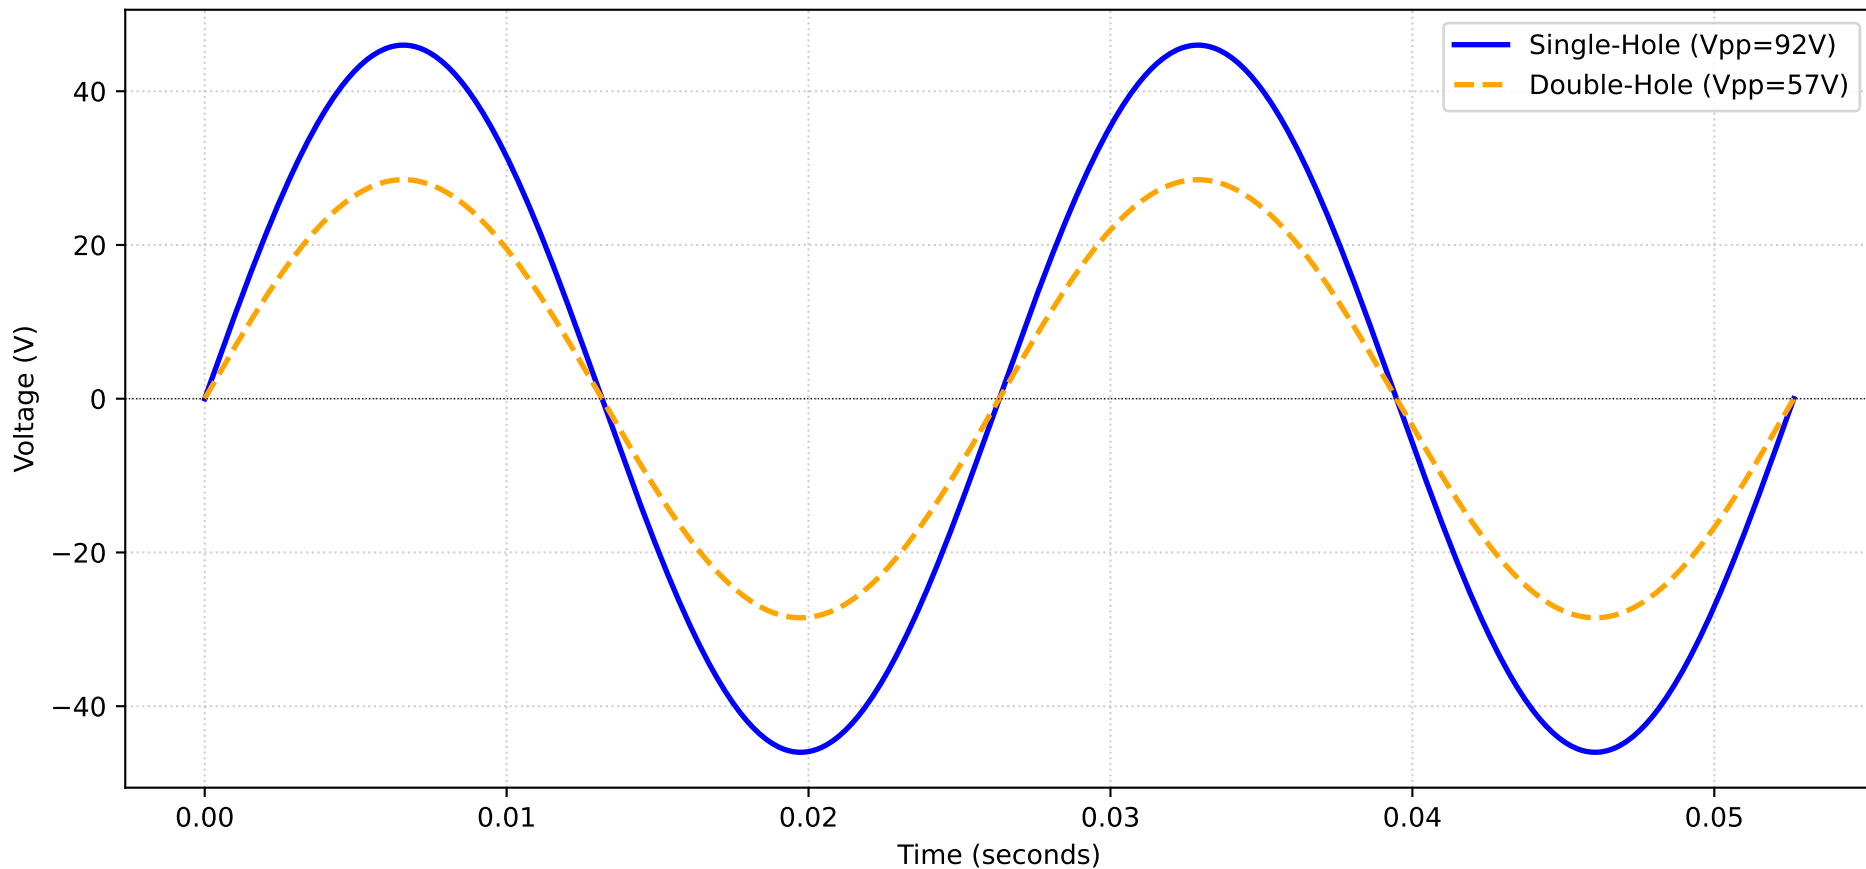


TENS Device Waveform Simulation - Mode 3 (38-22-38 Hz)

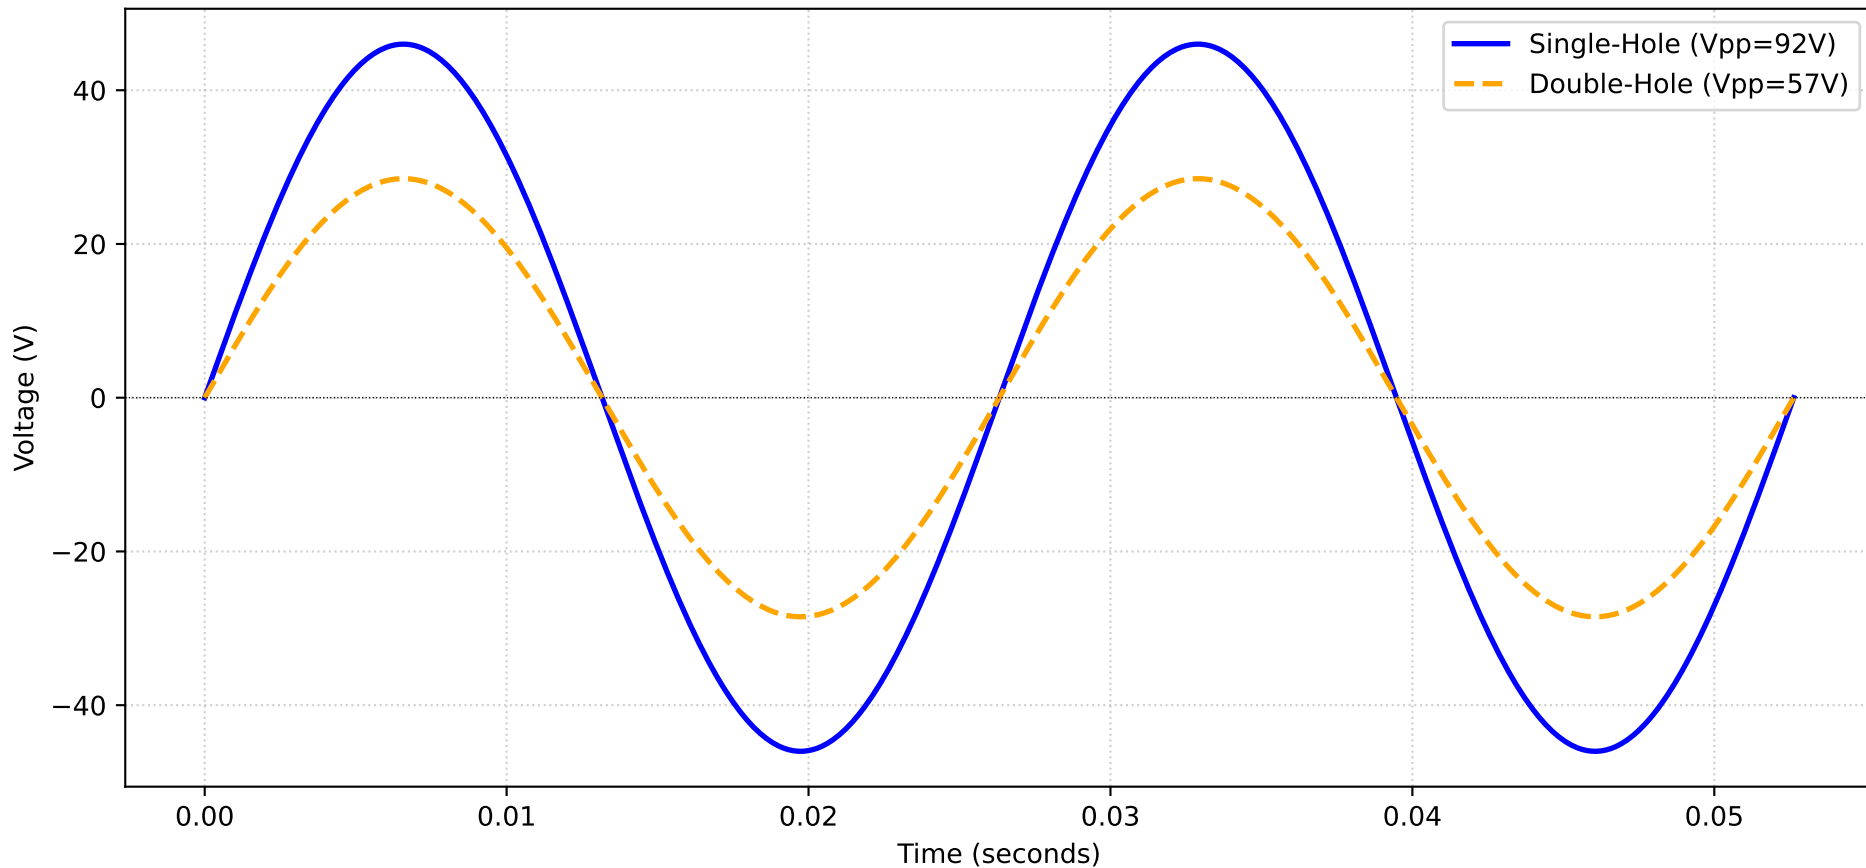


TENS Device Waveform Simulation - Mode 4 (35-22-35 Hz)

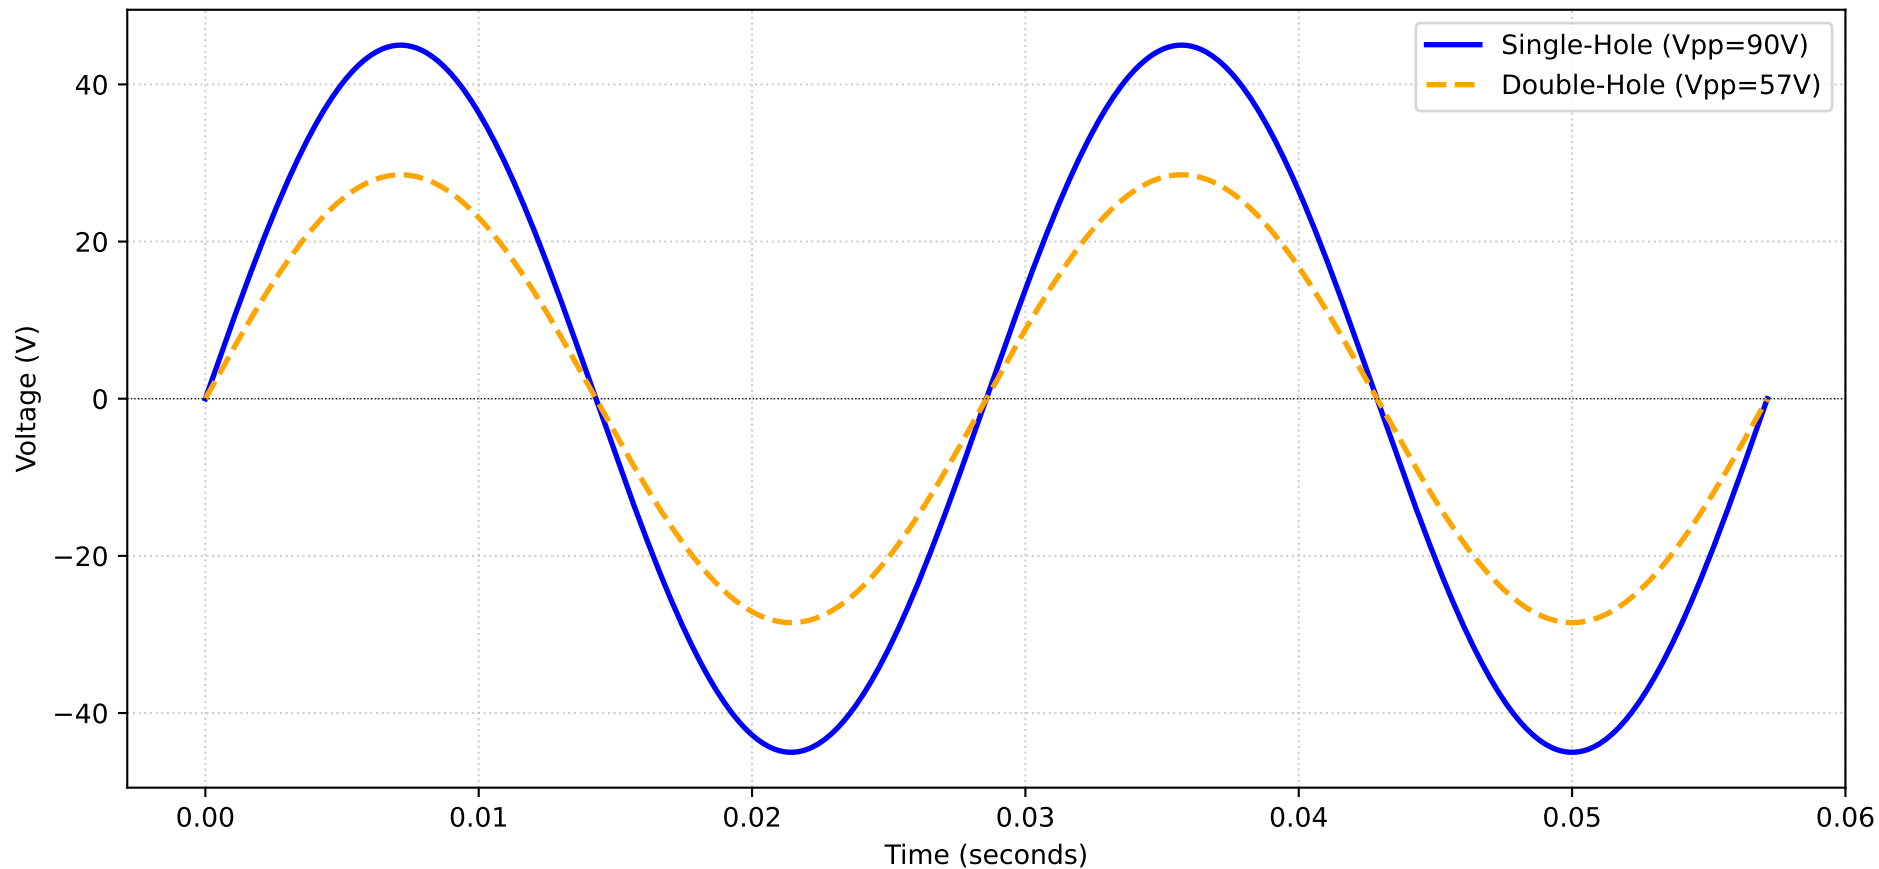


TENS Device Waveform Simulation - Mode 5 (2 Hz)

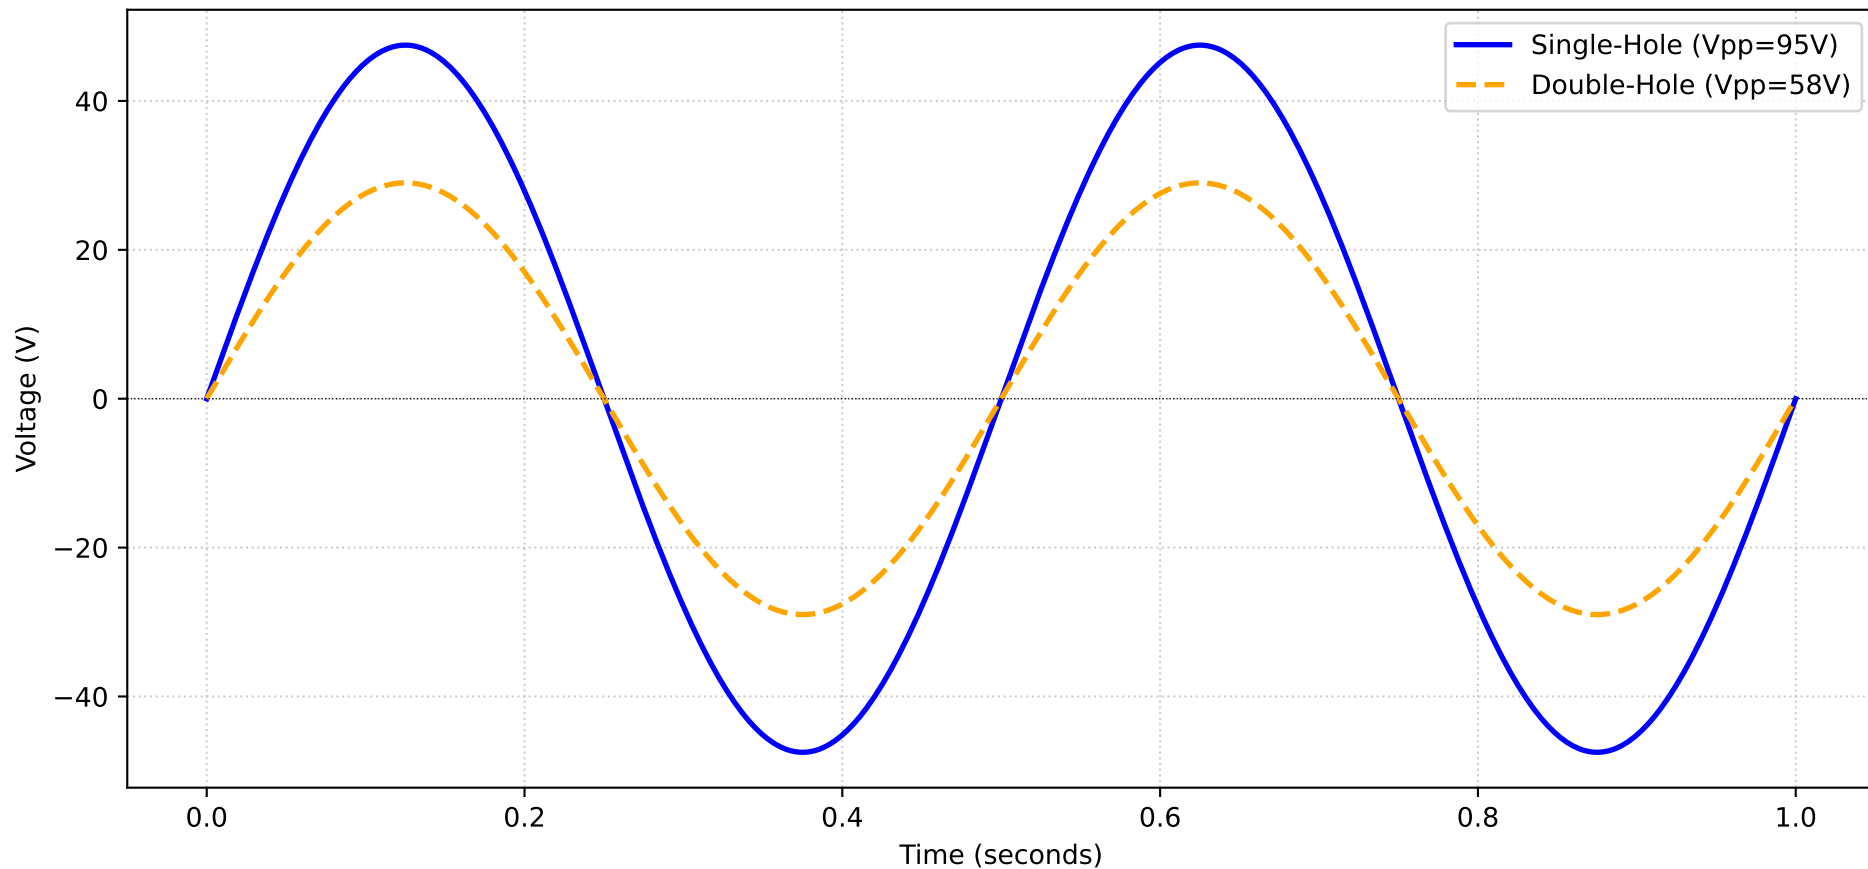


TENS Device Waveform Simulation - Mode 6 (3-19 Hz)

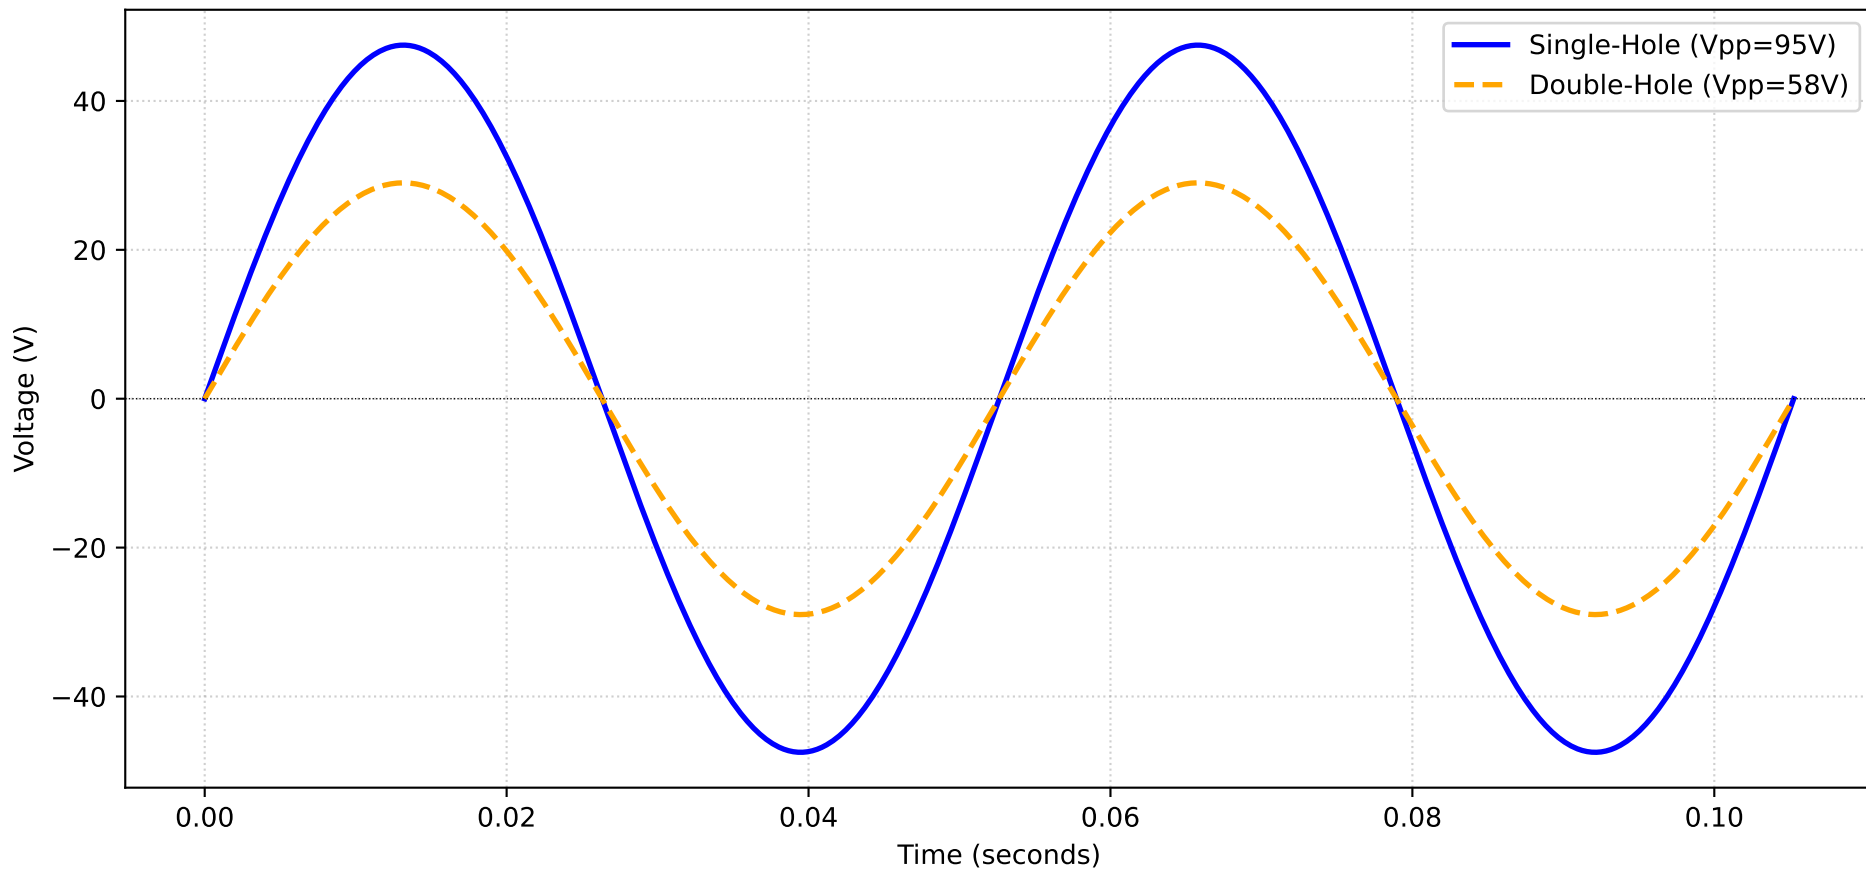

TENS Device Waveform Simulation - Mode 7 (8 Hz)

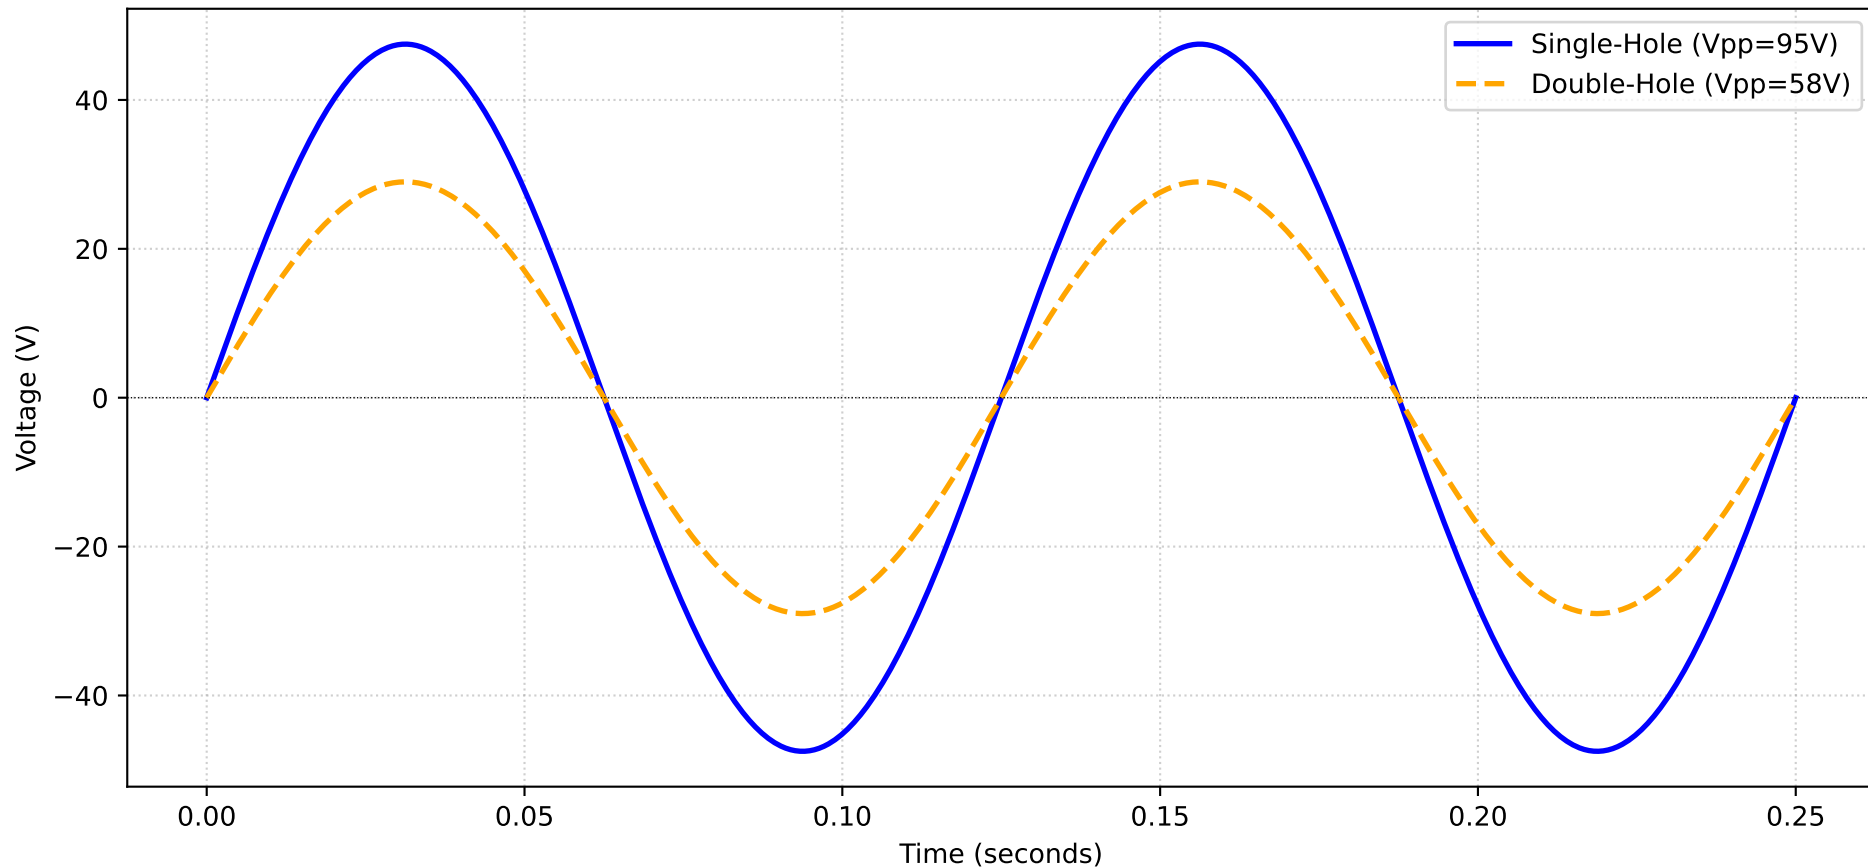


TENS Device Waveform Simulation - Mode 8 (56-22 Hz)

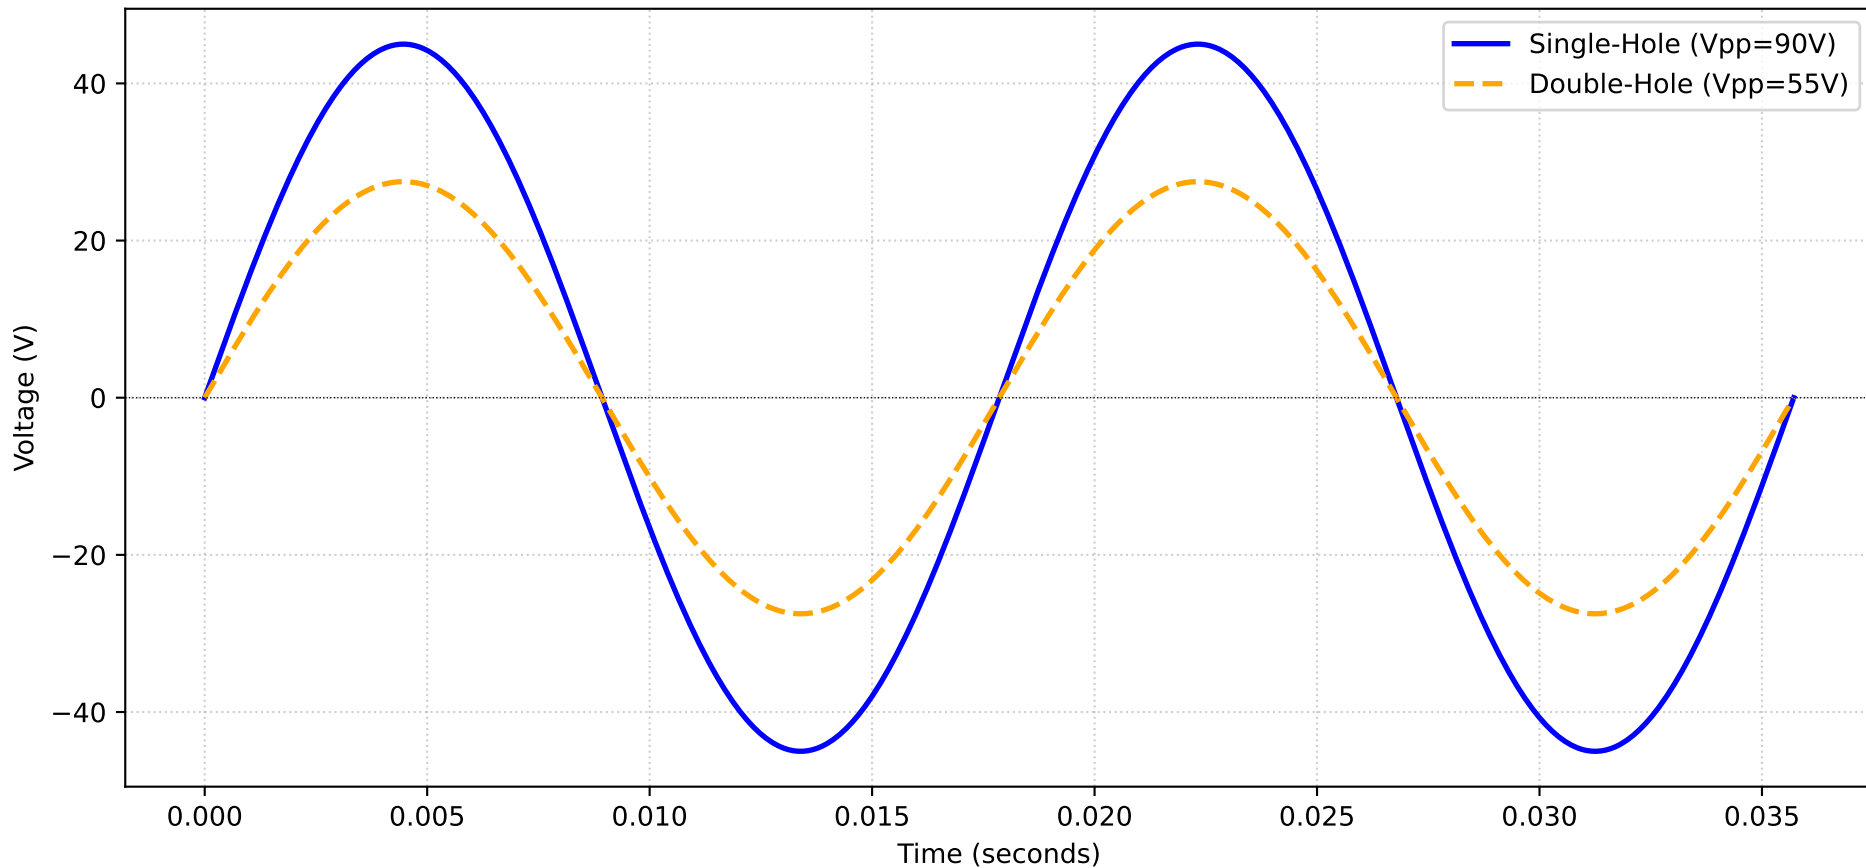





TENS Device Waveform Simulation - Mode 9 (8 Hz)

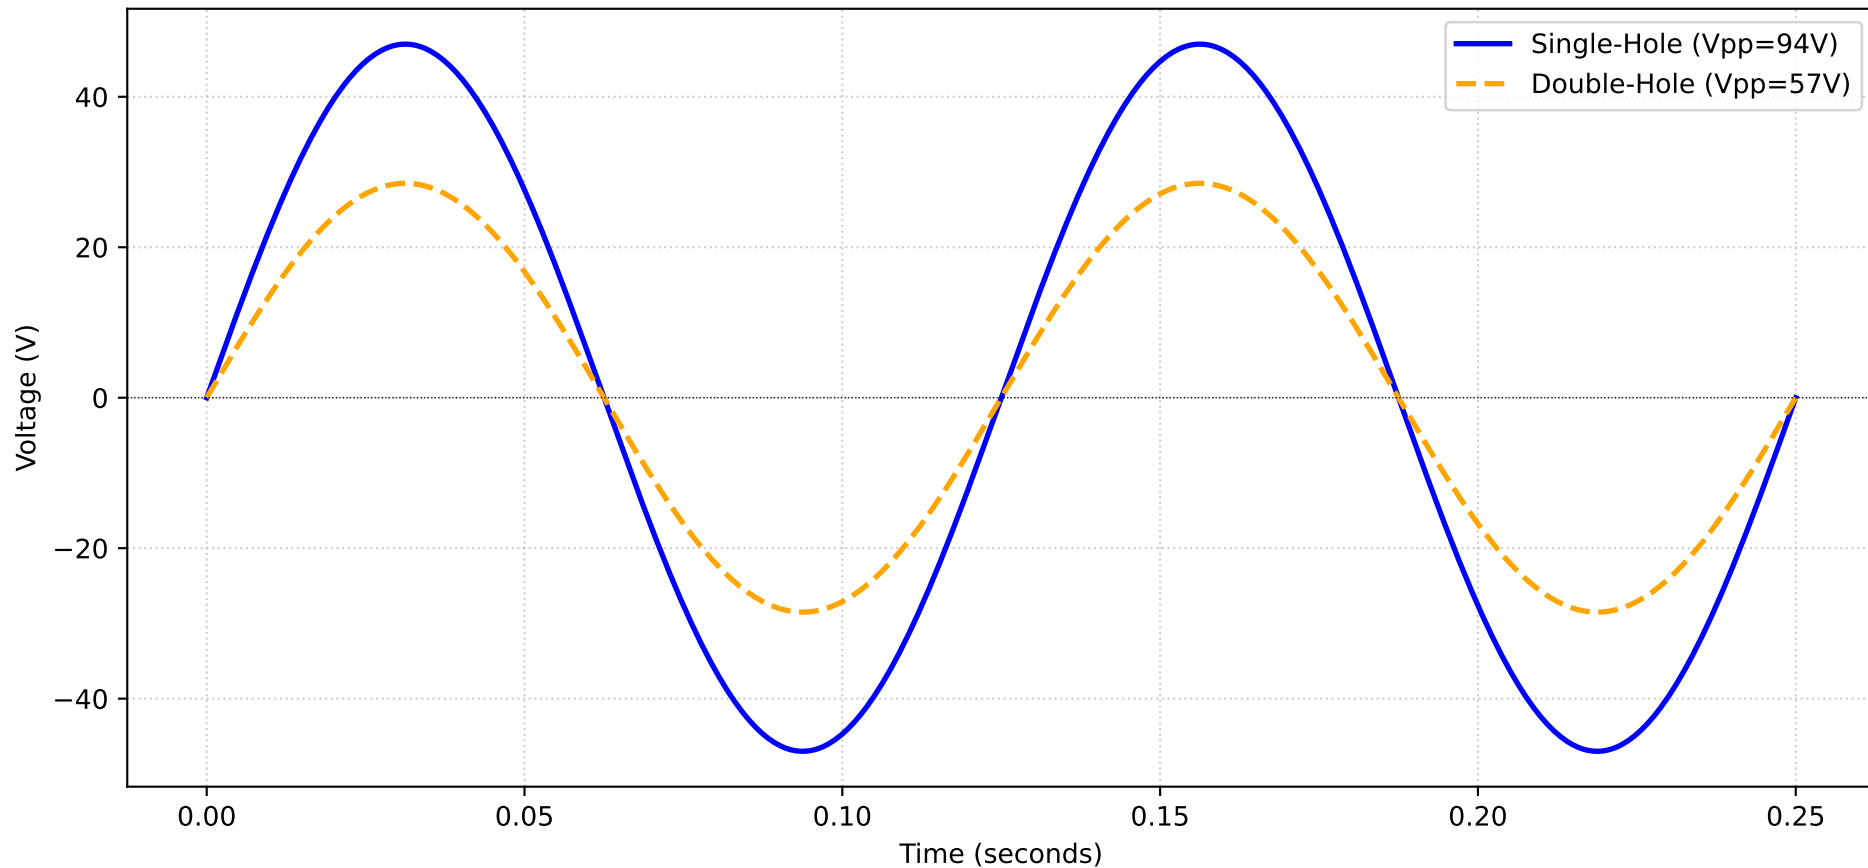


TENS Device Waveform Simulation - Mode 10 (38-24-38 Hz)

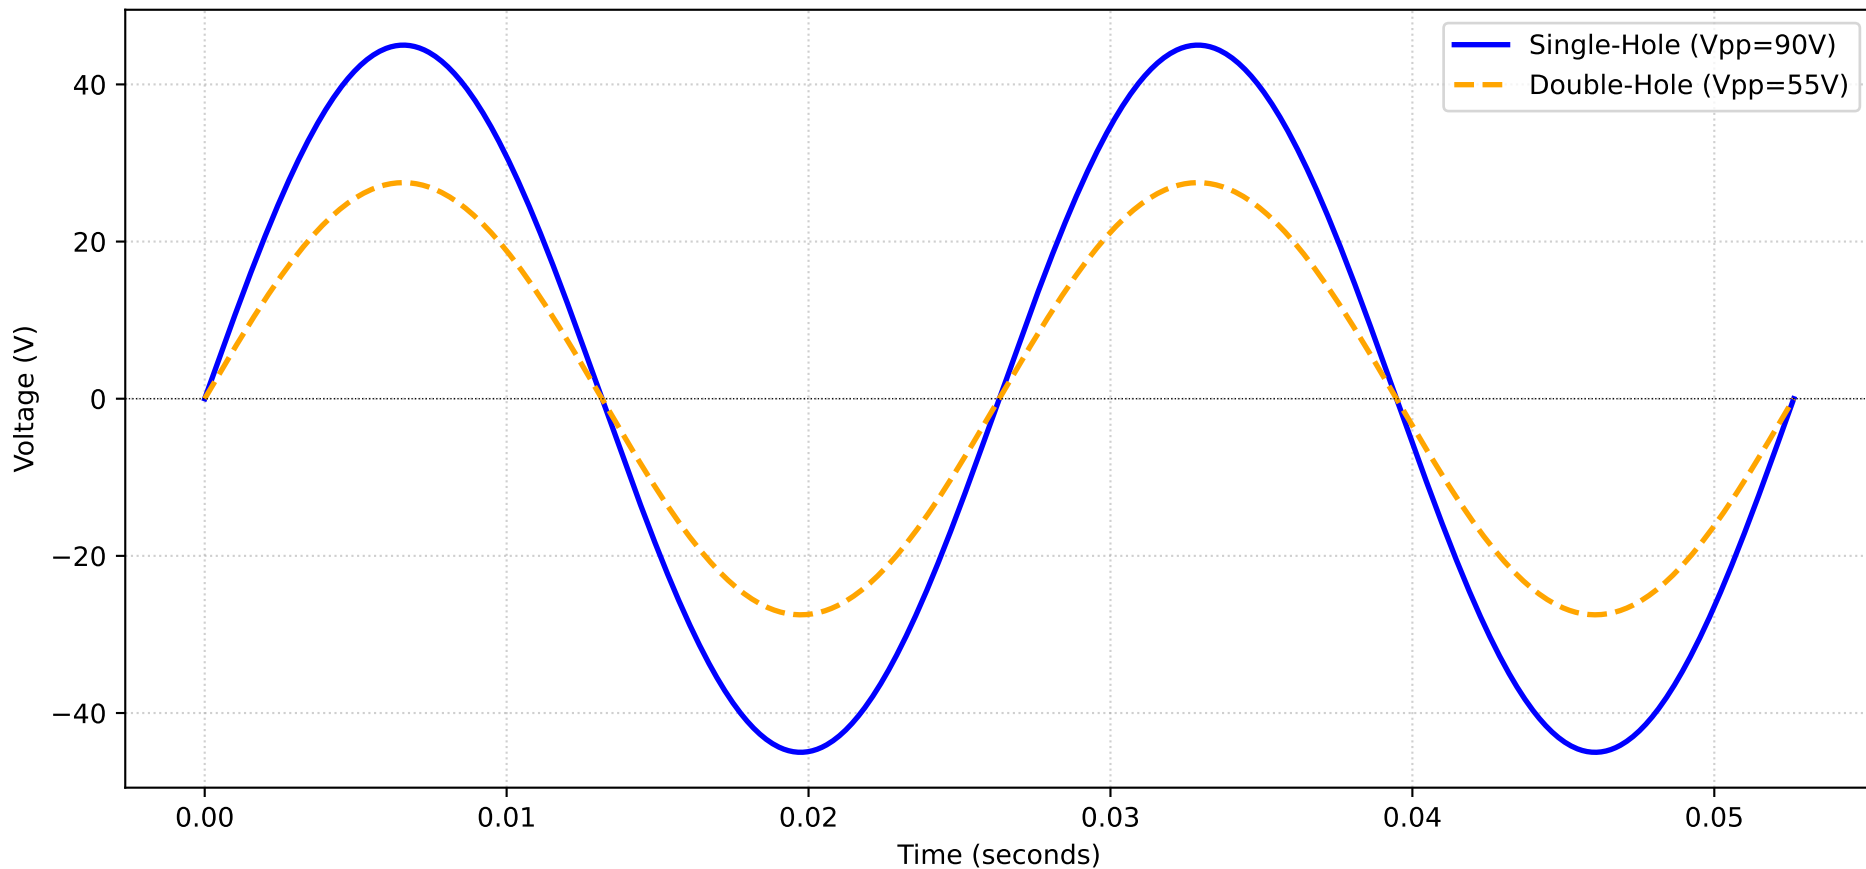


TENS Device Waveform Simulation - Mode 11 (35-22-35 Hz)

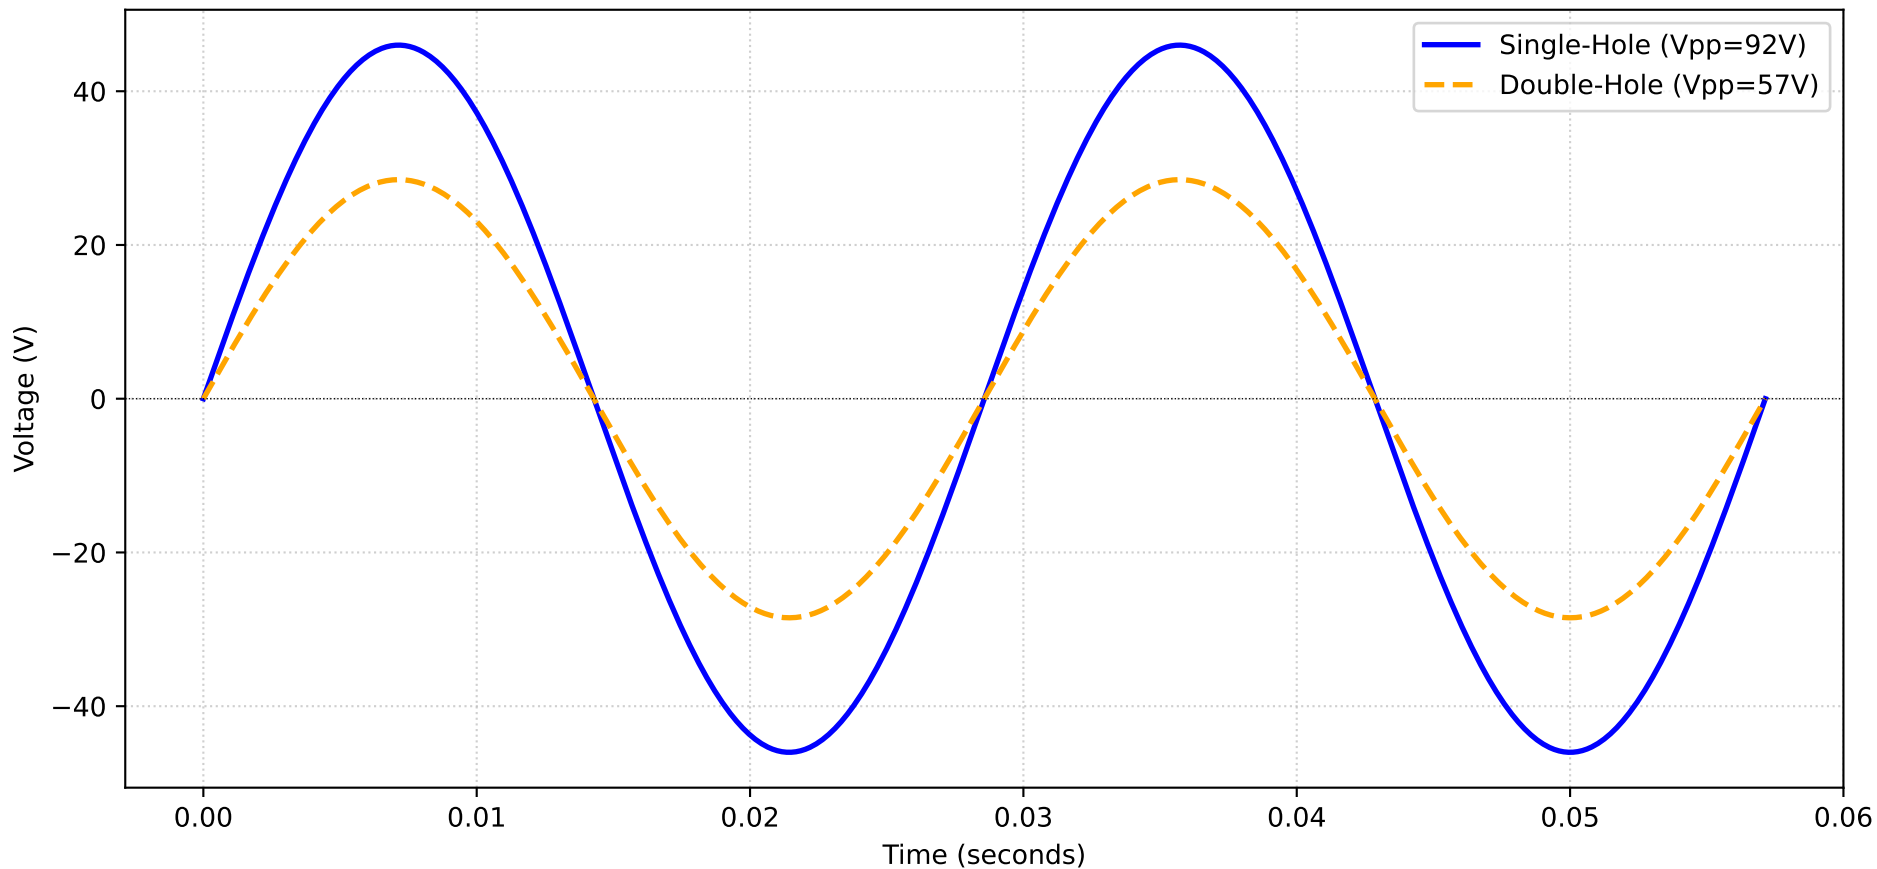


TENS Device Waveform Simulation - Mode 12 (45-22 Hz)

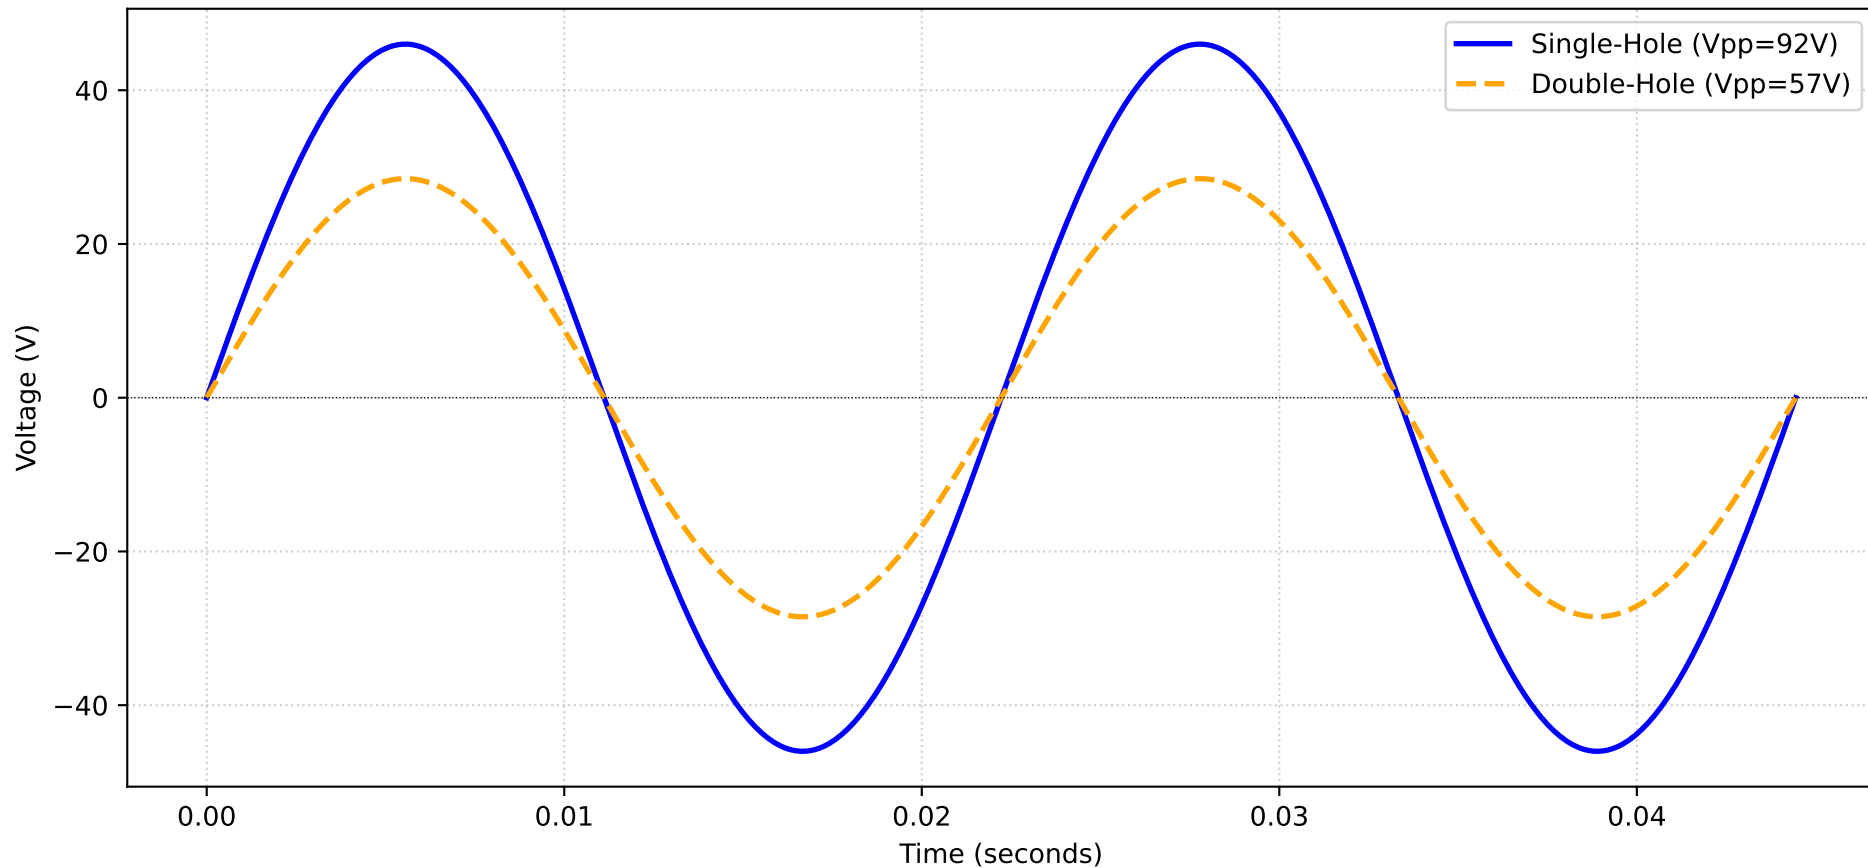


TENS Device Waveform Simulation - Mode 13 (20 Hz)

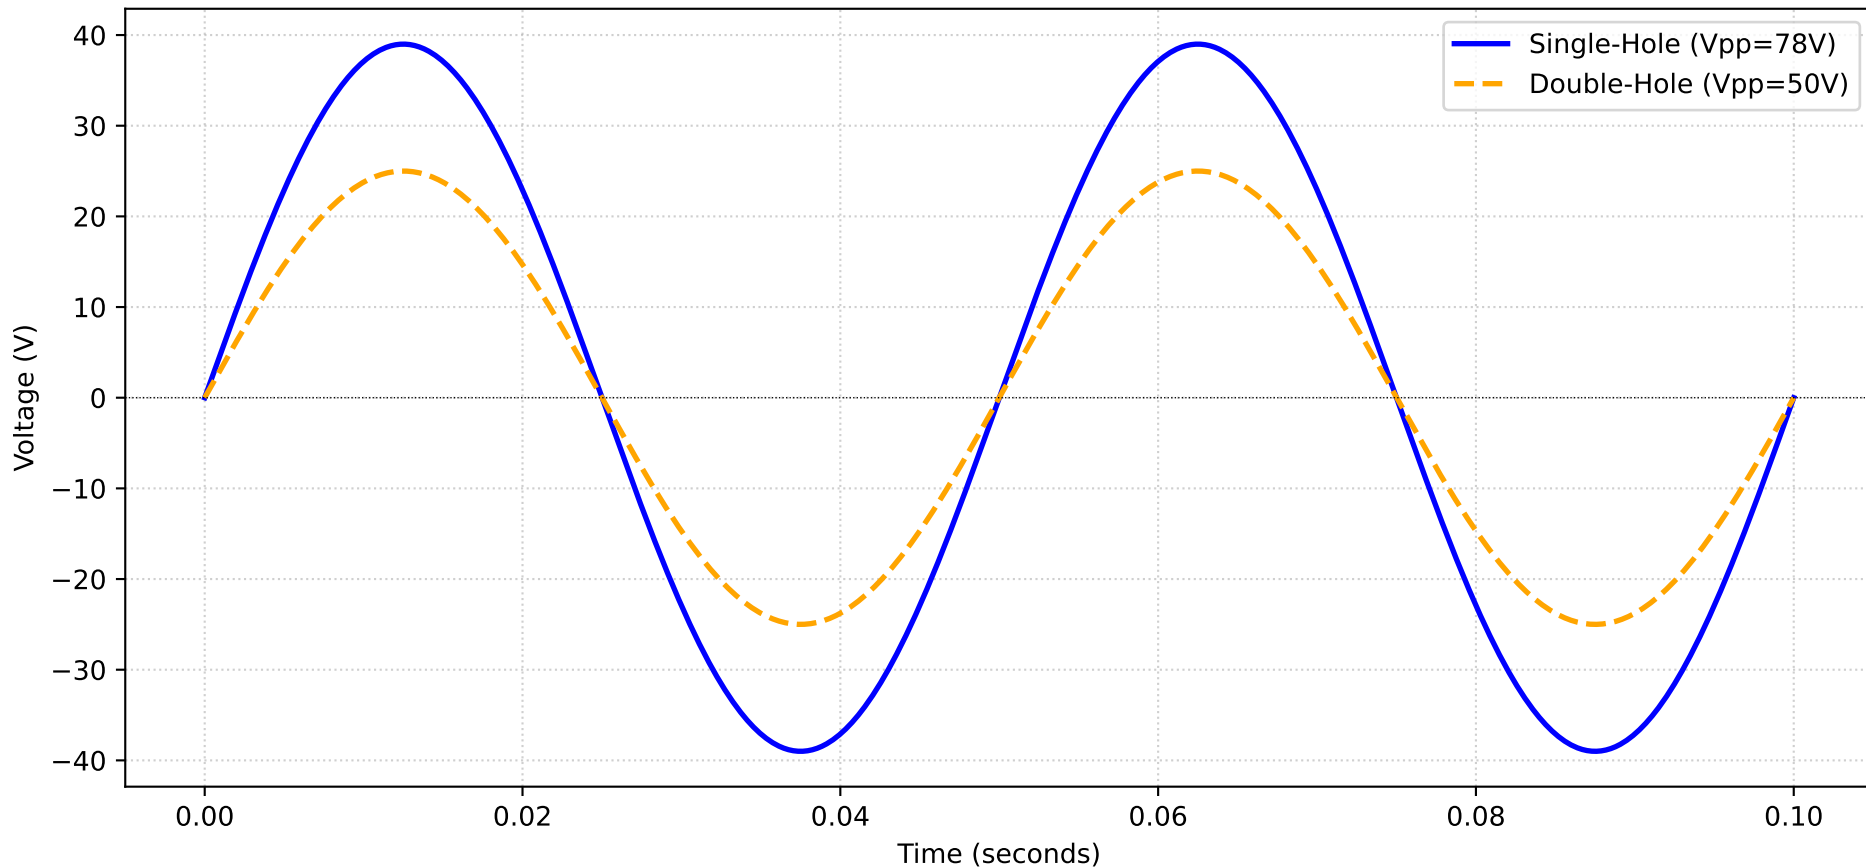


TENS Device Waveform Simulation - Mode 14 (35-22-35 Hz)

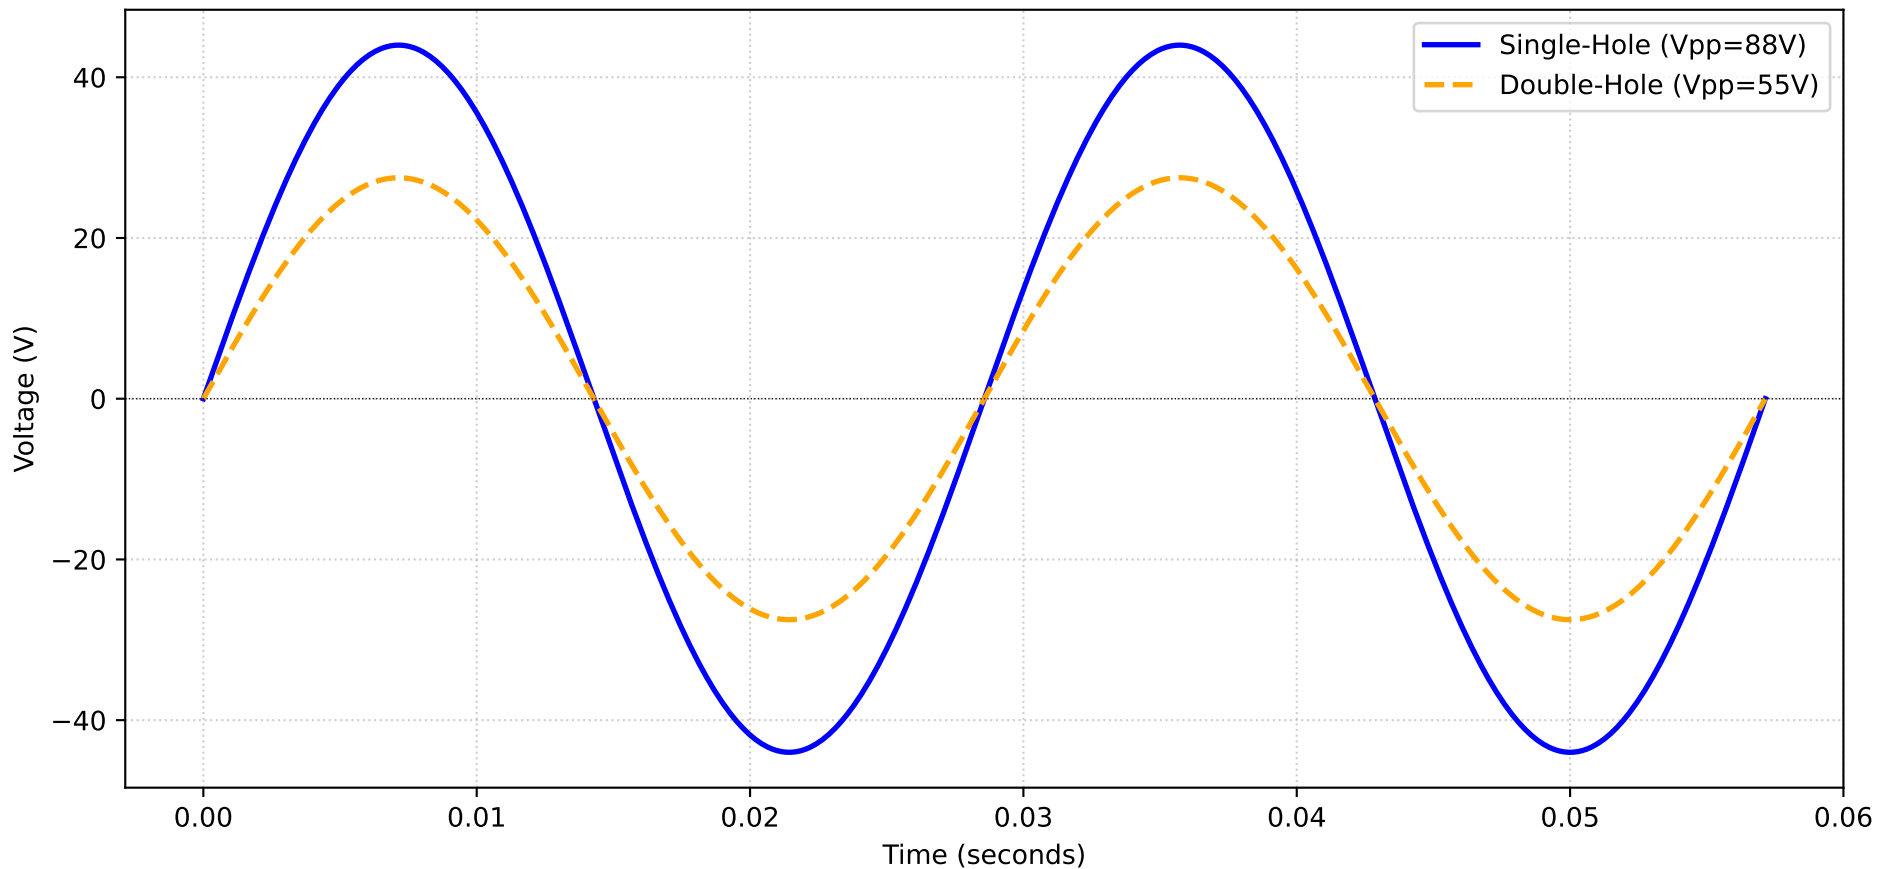

TENS Device Waveform Simulation - Mode 15 (33-25 Hz)

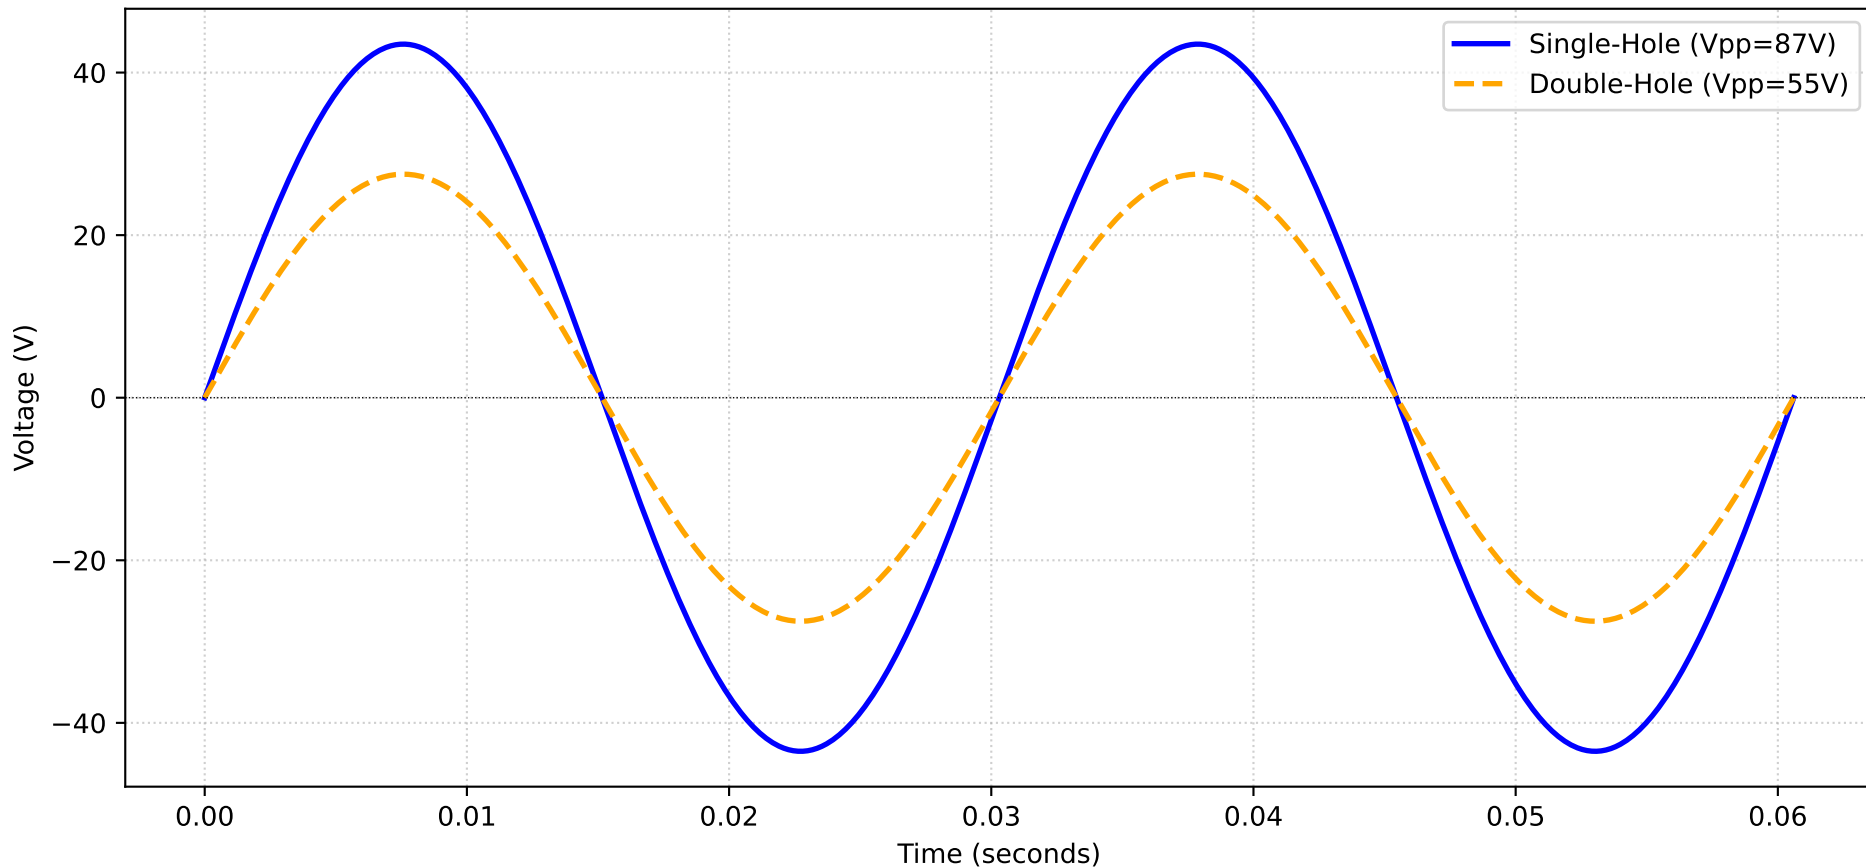


TENS Device Waveform Simulation - Mode 16 (29 Hz)

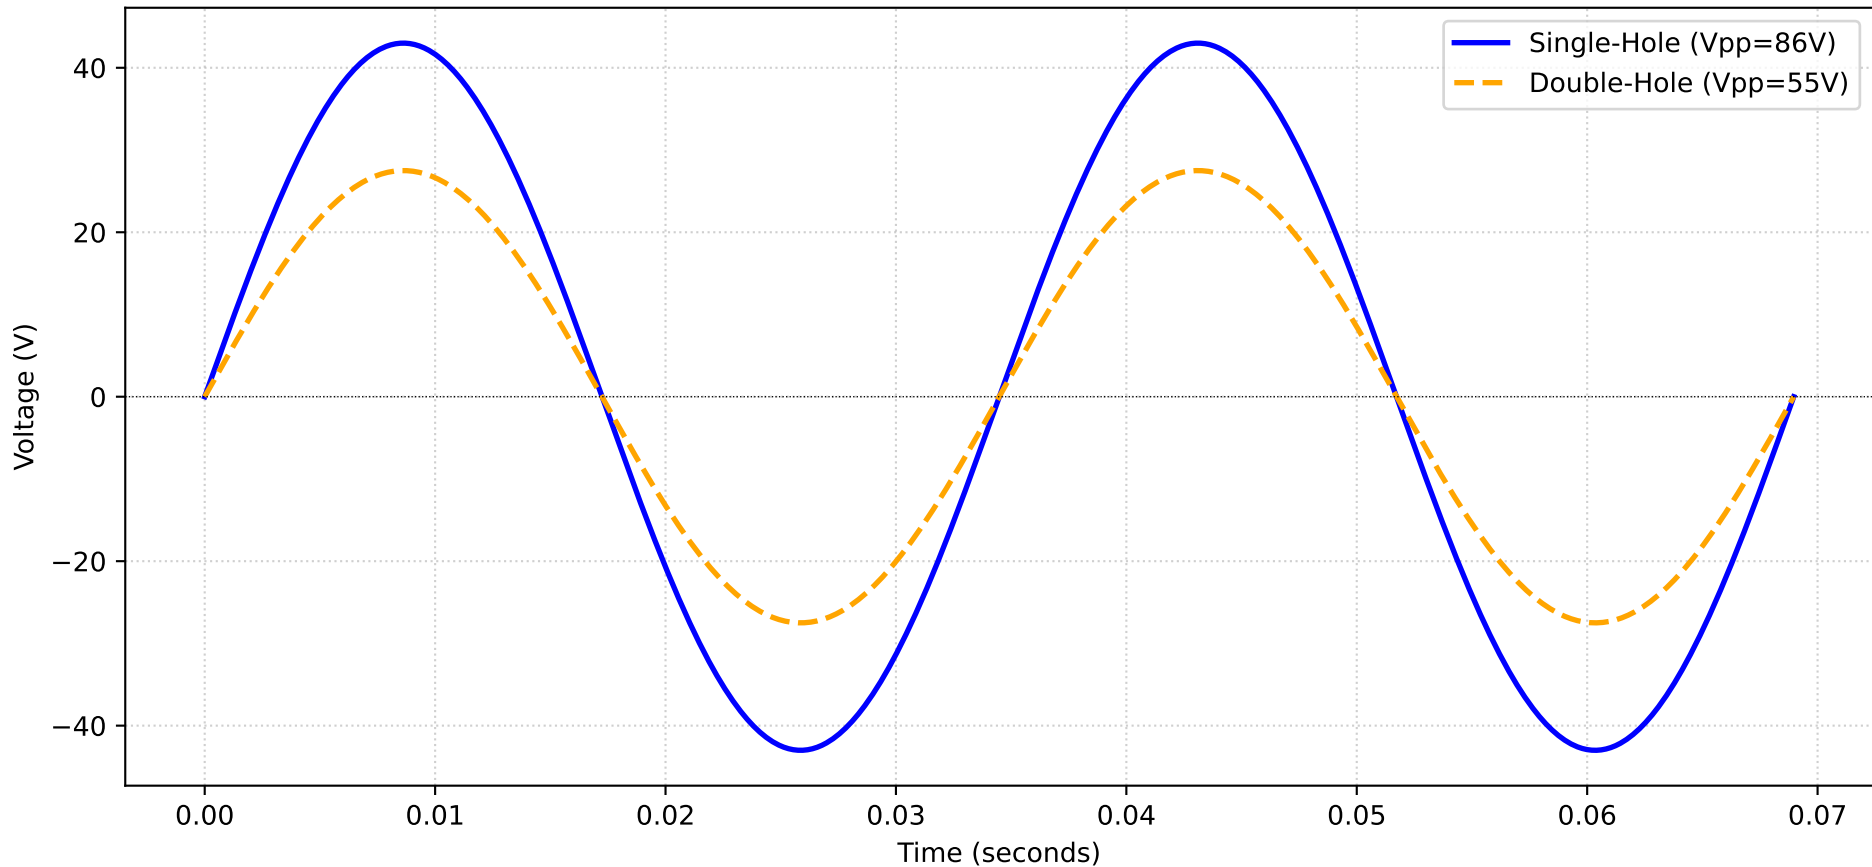





TENS Device Waveform Simulation - Mode 17 (6.5 Hz)

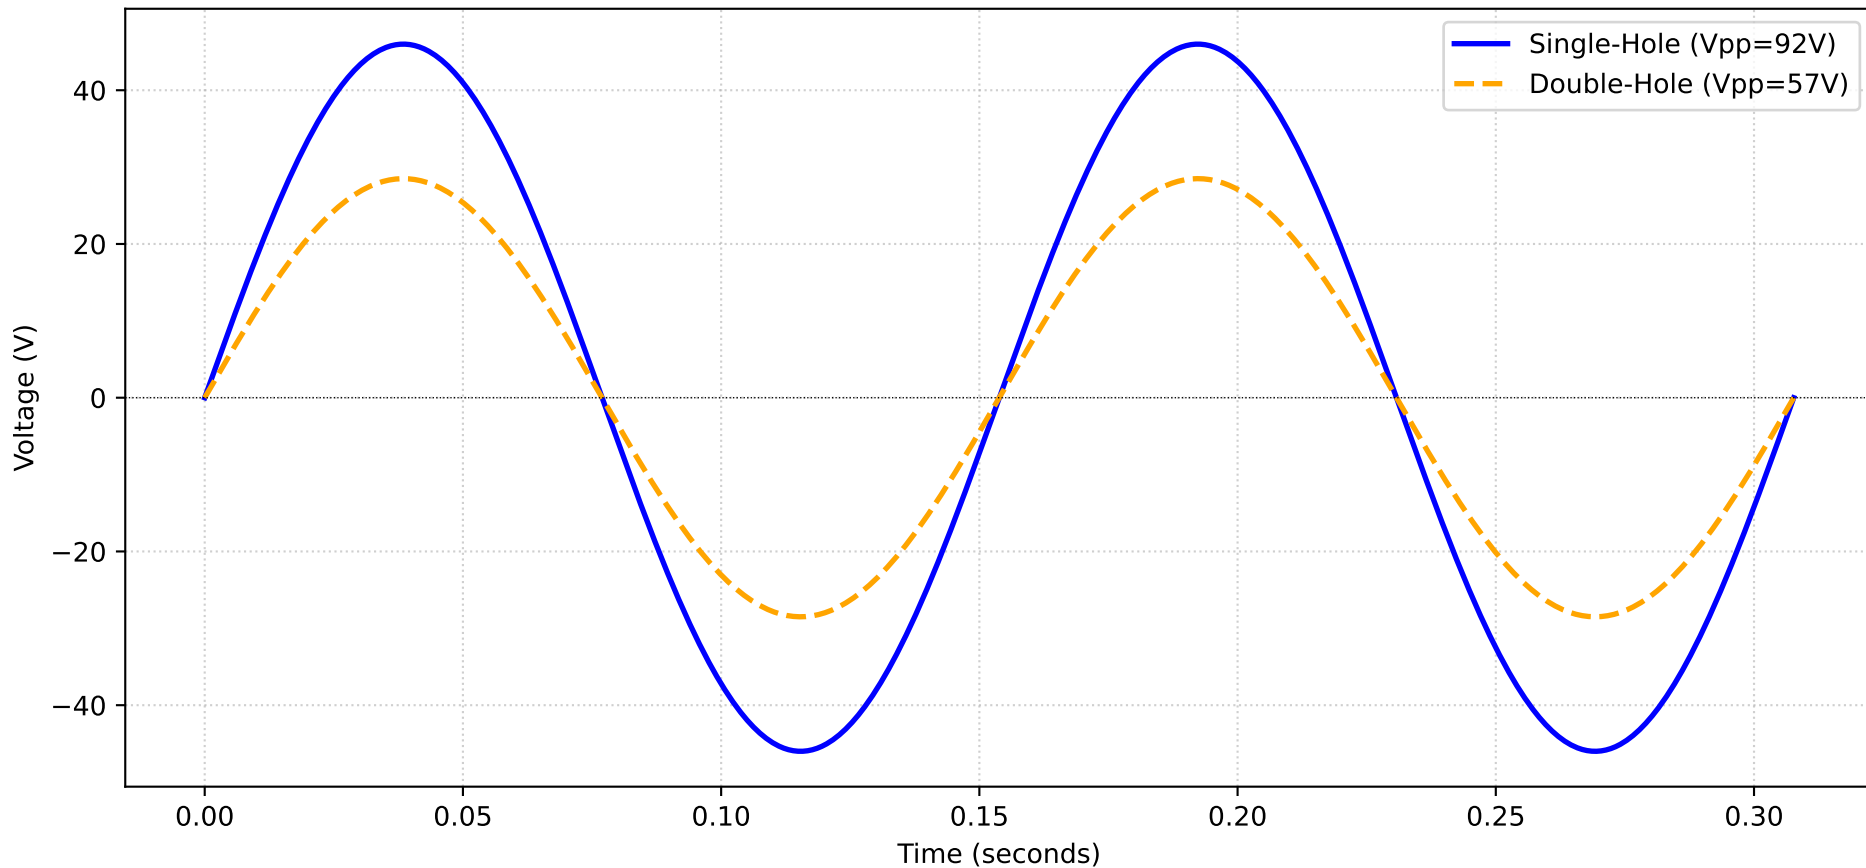


TENS Device Waveform Simulation - Mode 18 (38-23-38 Hz)

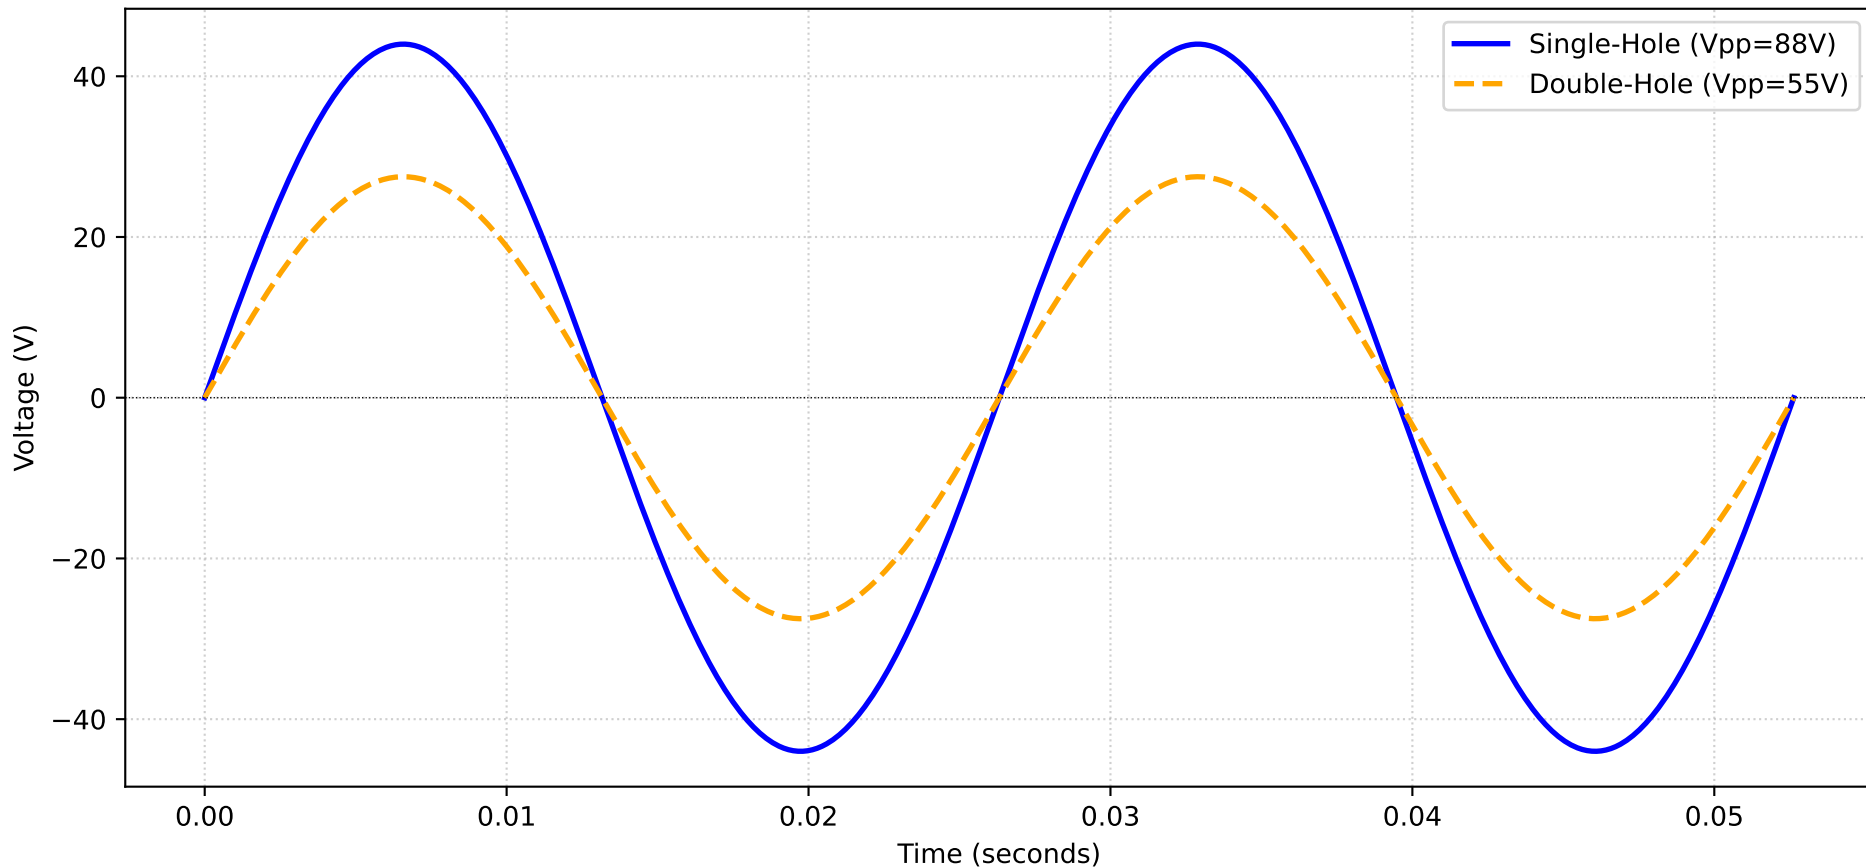


TENS Device Waveform Simulation - Mode 19 (20 Hz)

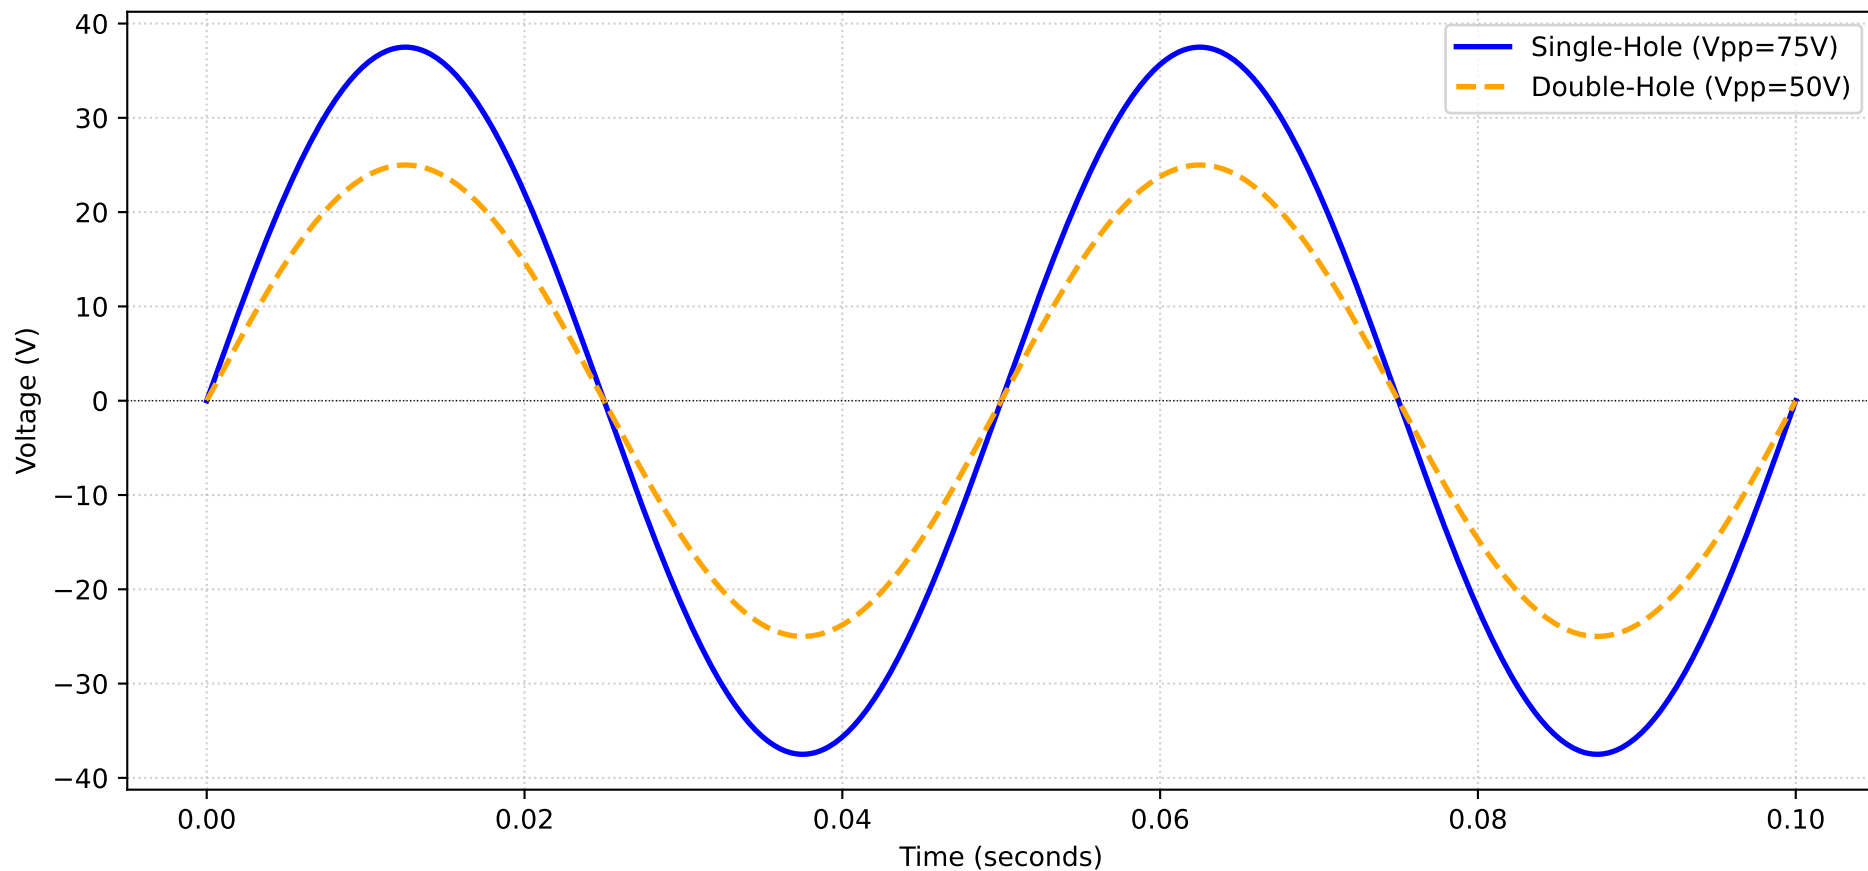


TENS Device Waveform Simulation - Mode 20 (3-22 Hz)

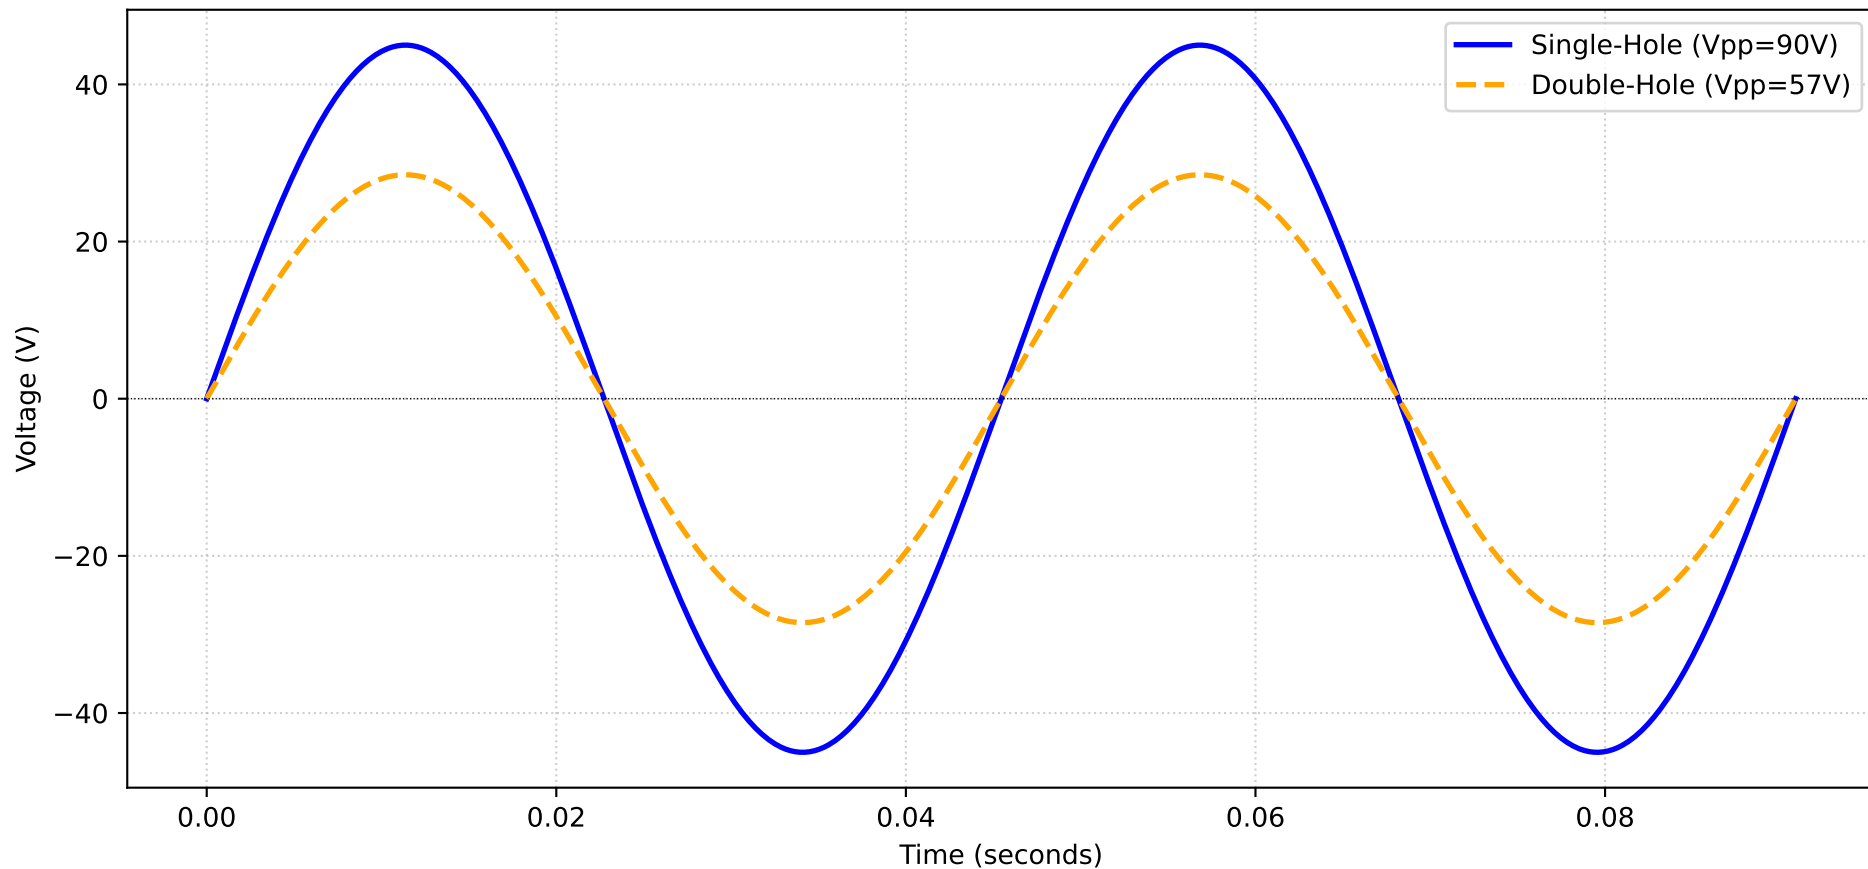


TENS Device Waveform Simulation - Mode 21 (20 Hz)

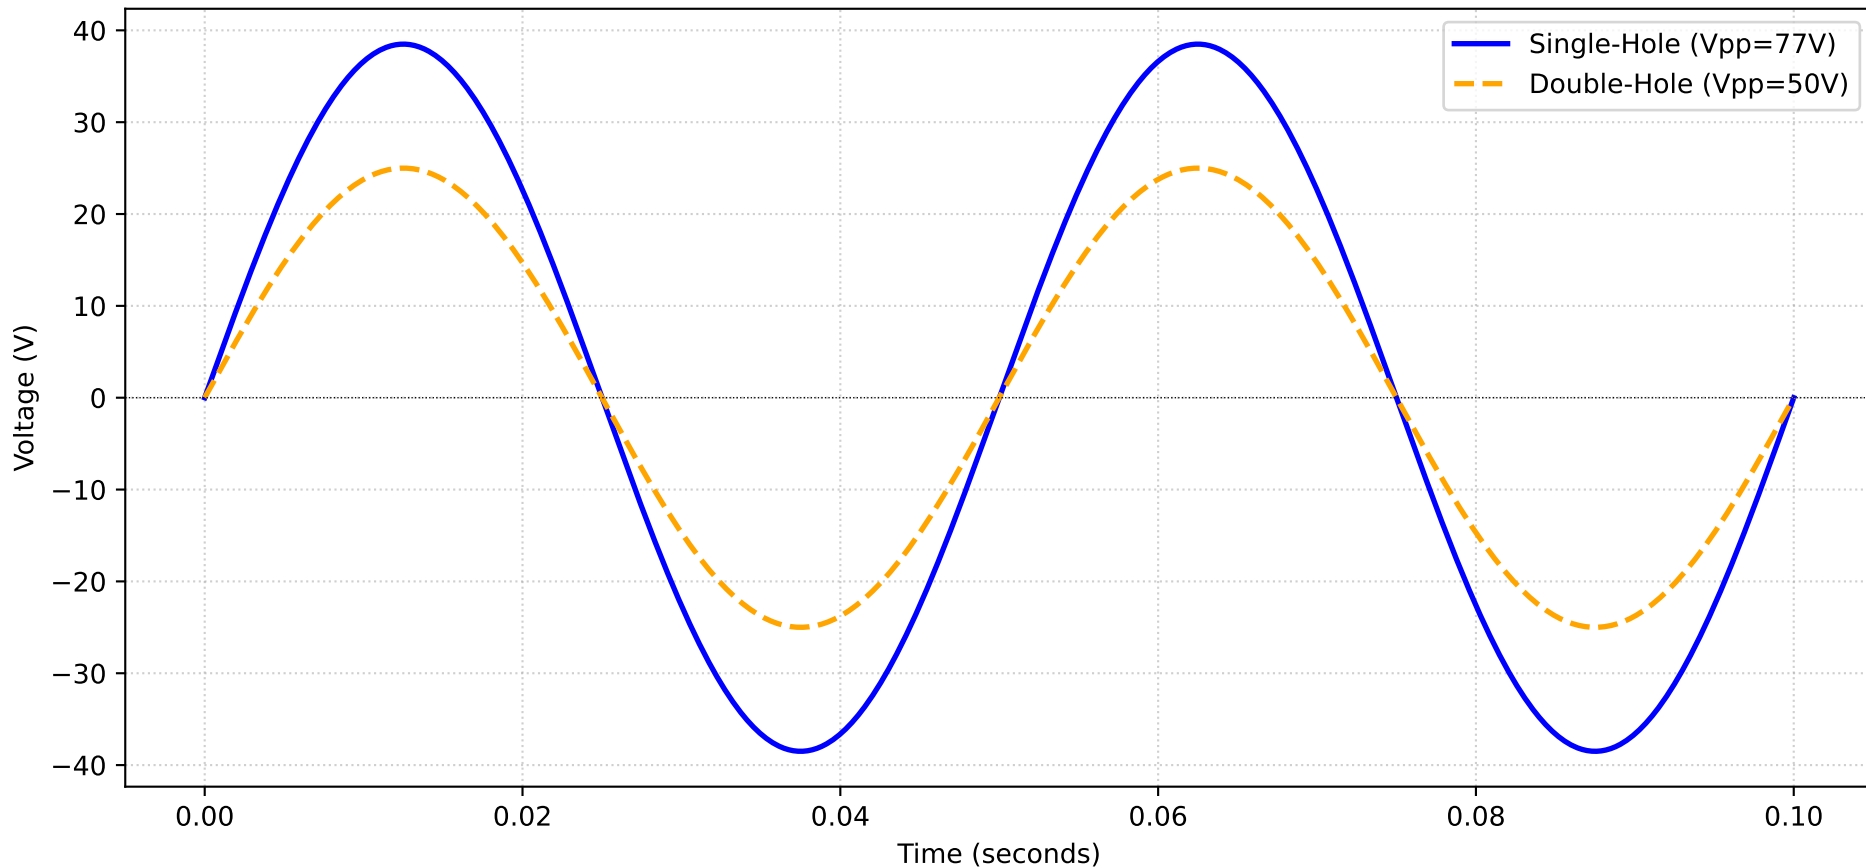

TENS Device Waveform Simulation - Mode 22 (38-22-38 Hz)

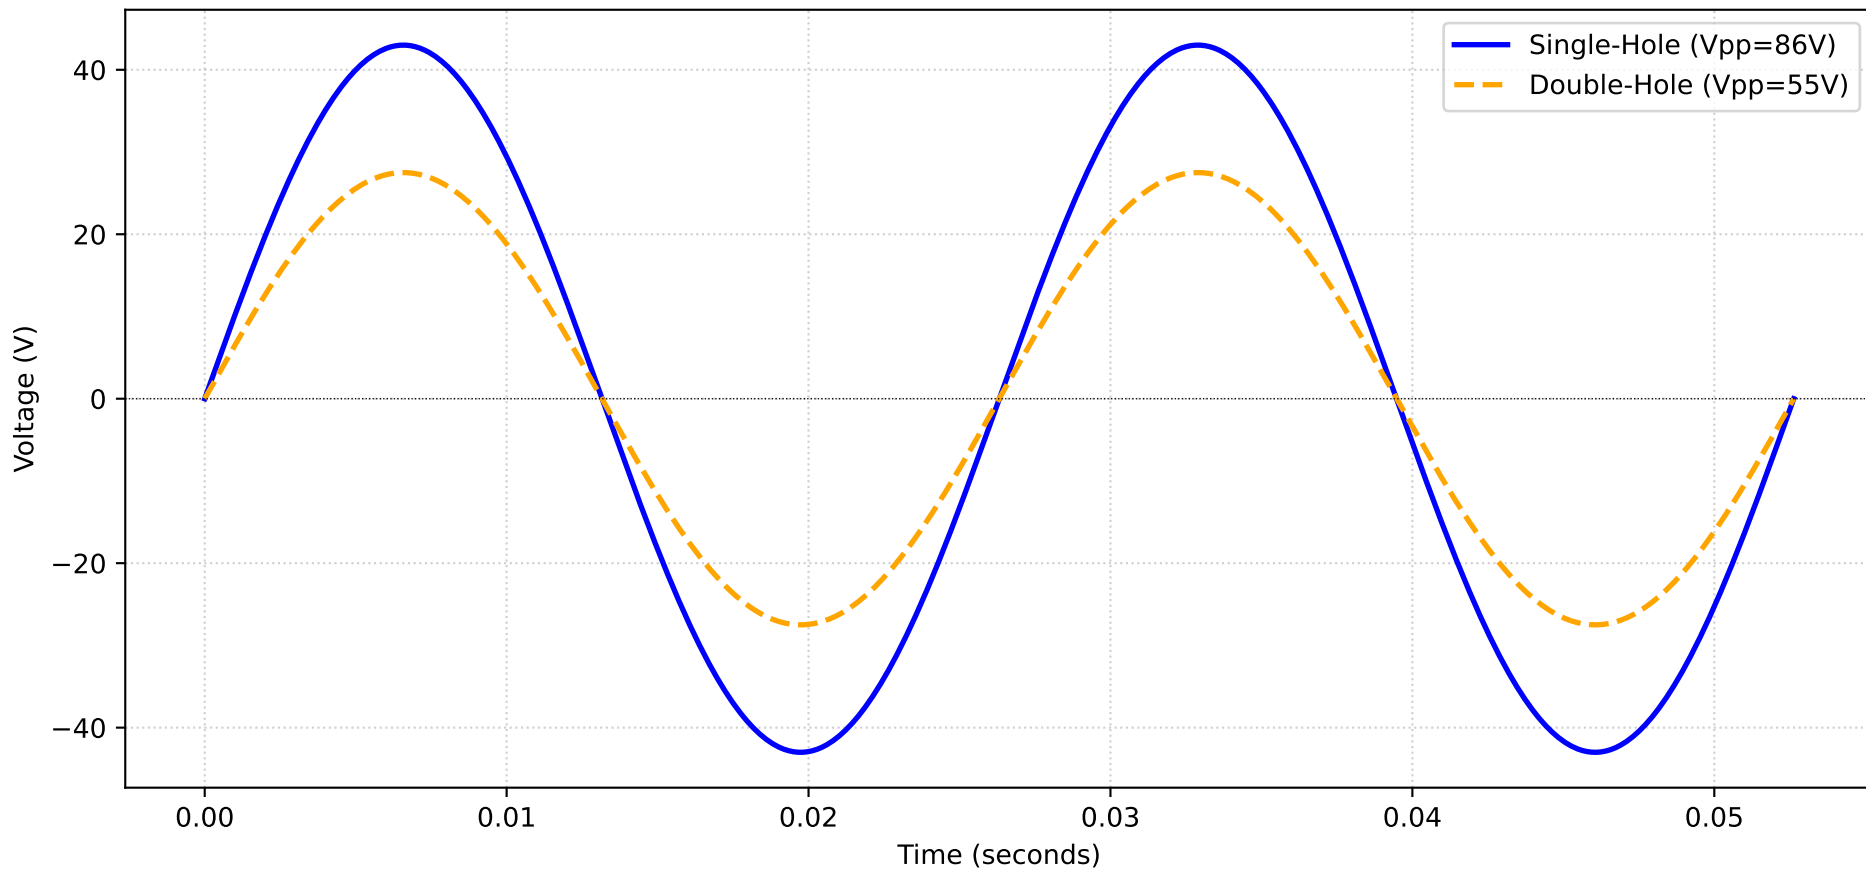

TENS Device Waveform Simulation - Mode 23 (20 Hz)

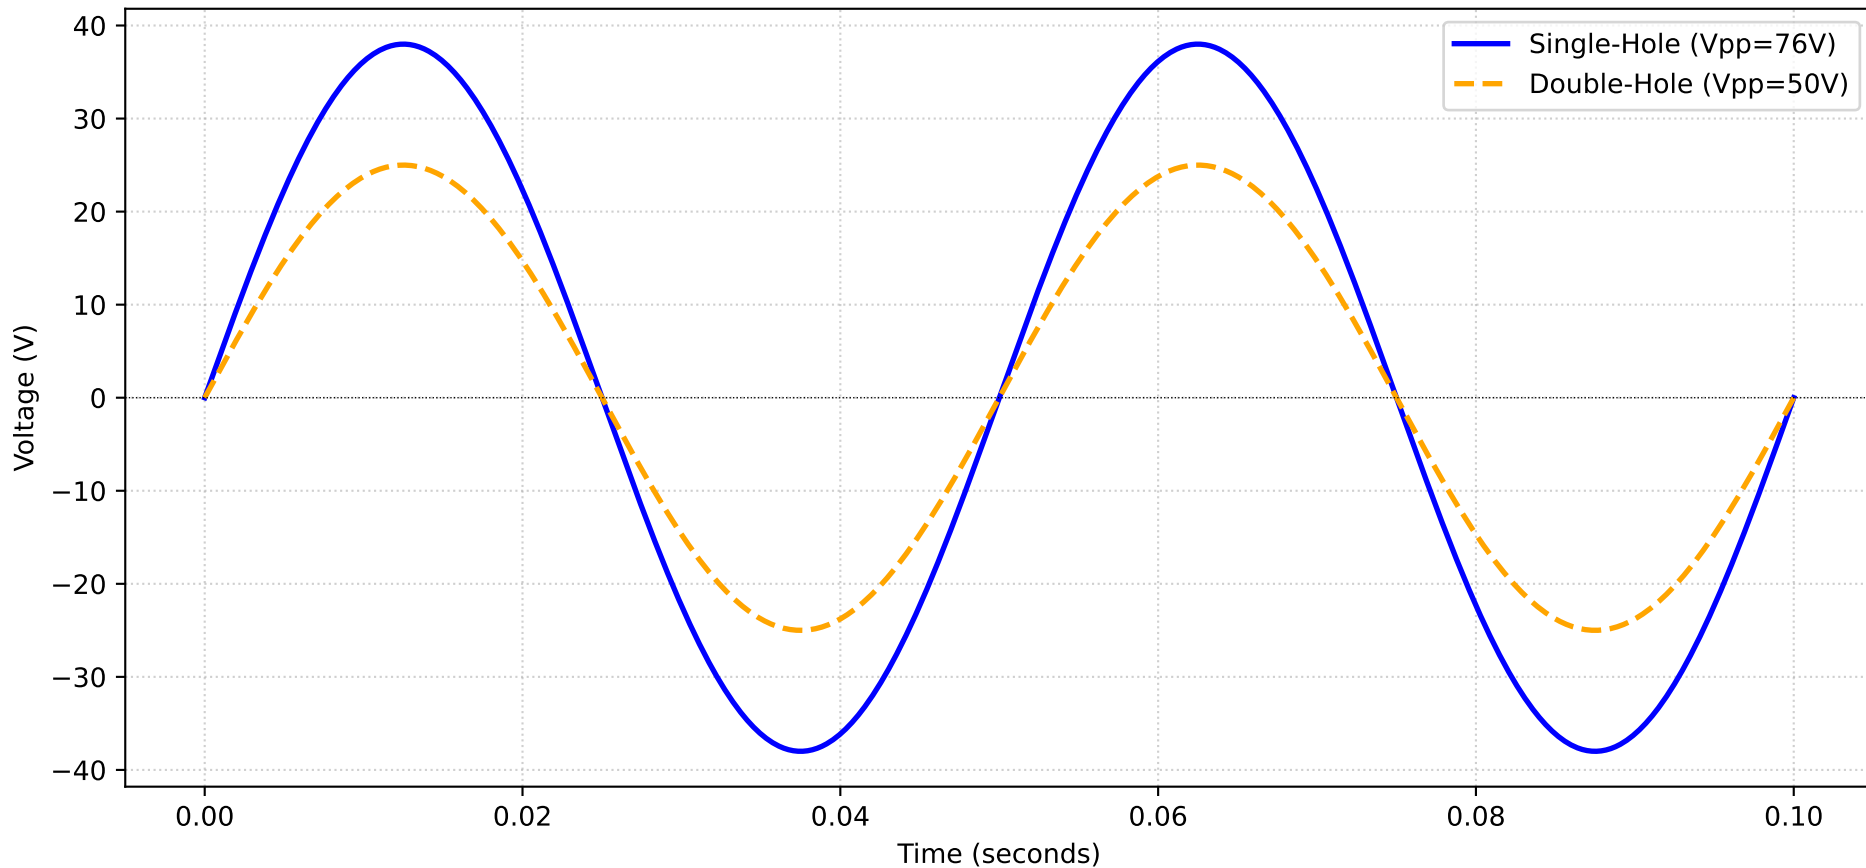

TENS Device Waveform Simulation - Mode 24 (41-25 Hz)

