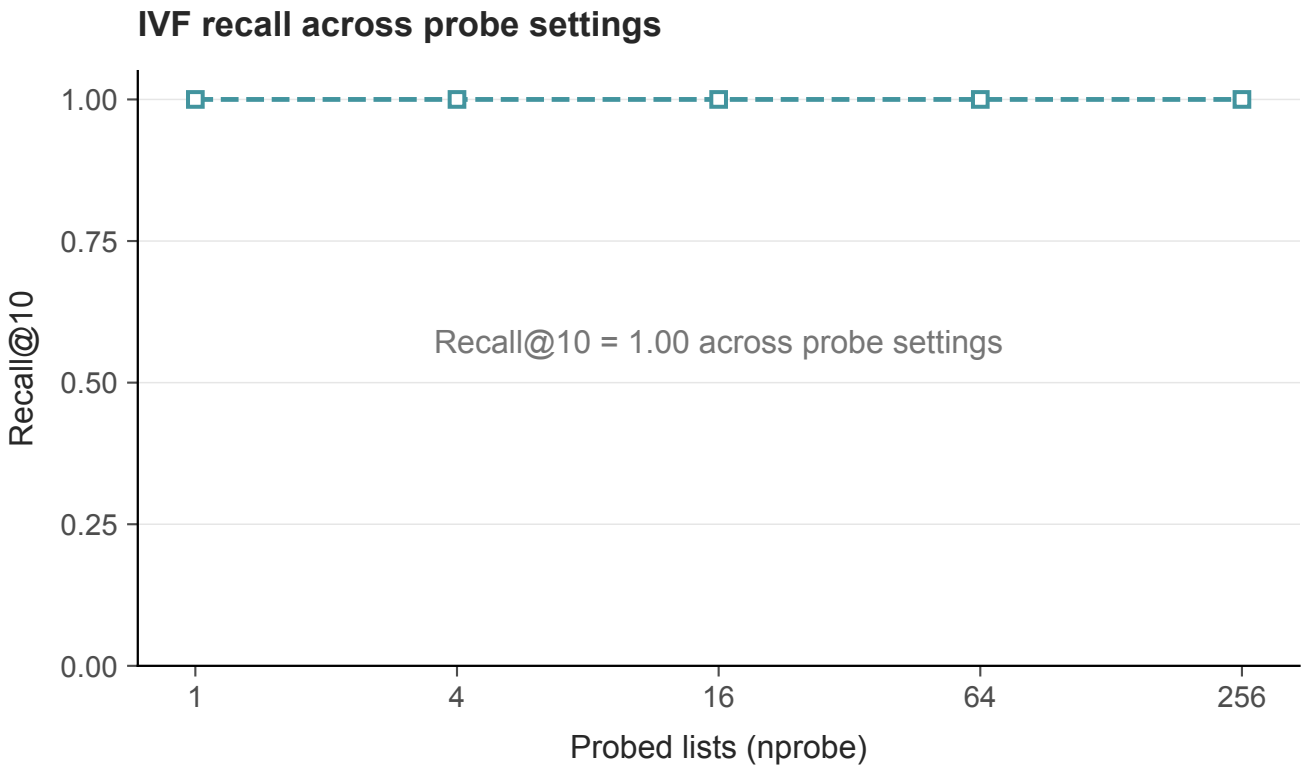
IVF recall across probe settings
1.00
0.75
0.50
0.25
0.00
Recall@10
Recall@10 = 1.00 across probe settings
1
4
16
64
256
Probed lists (nprobe)