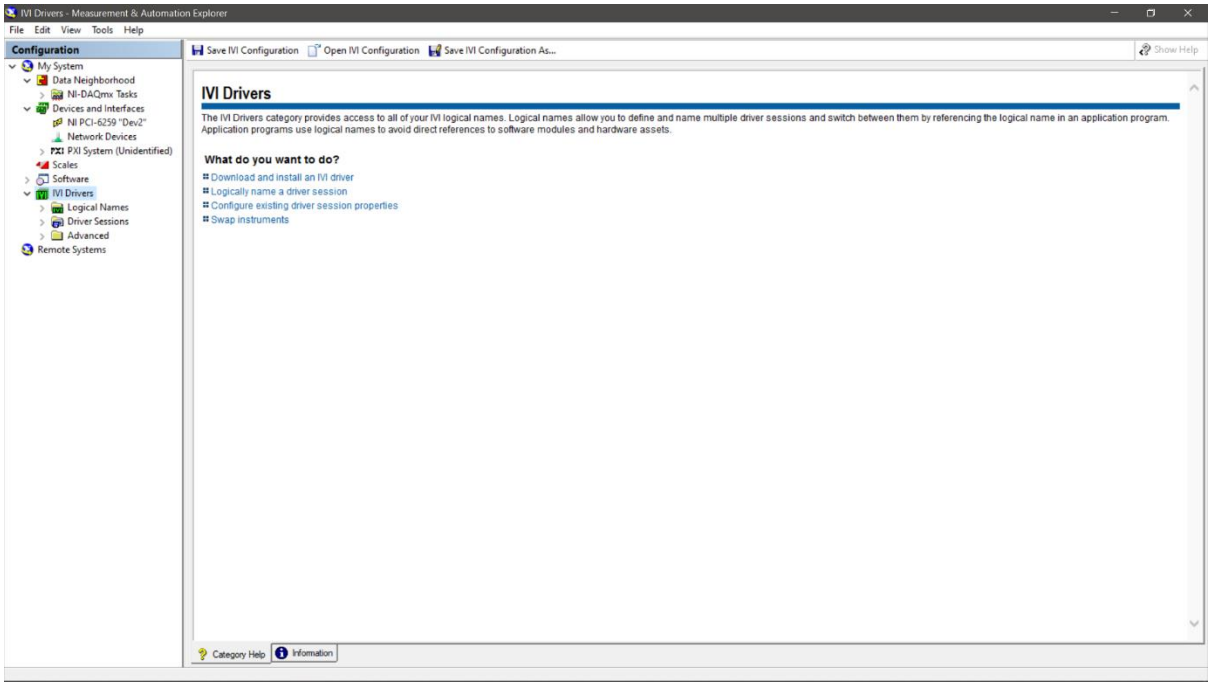
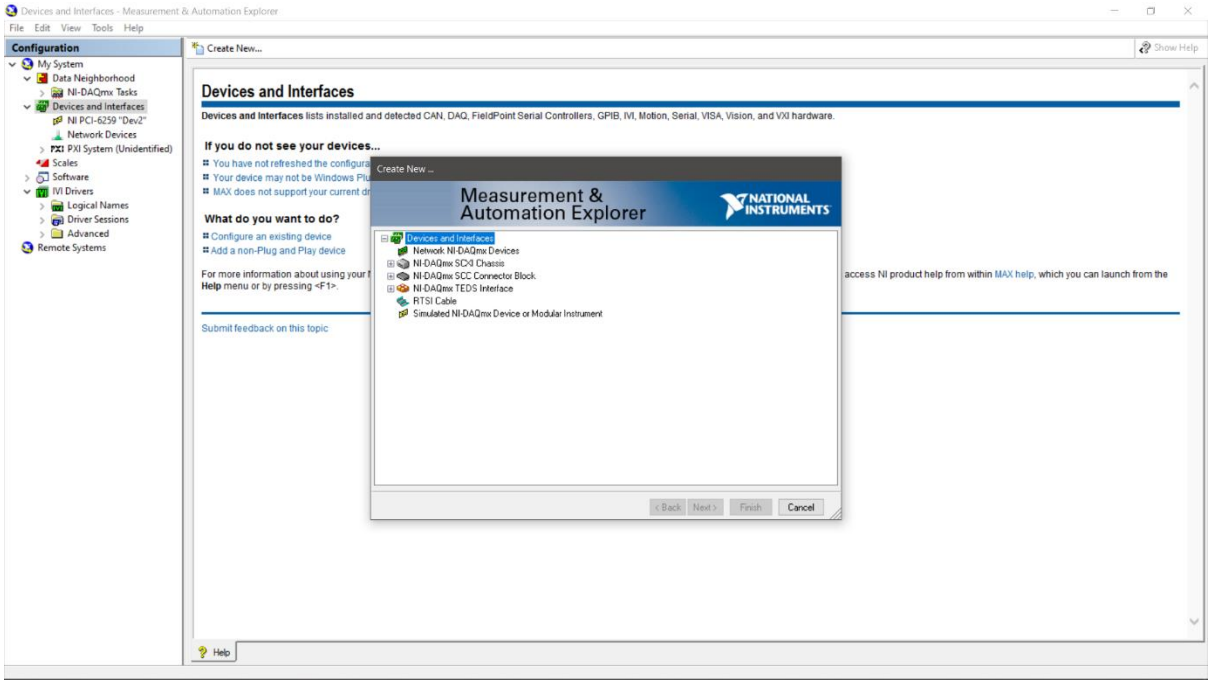
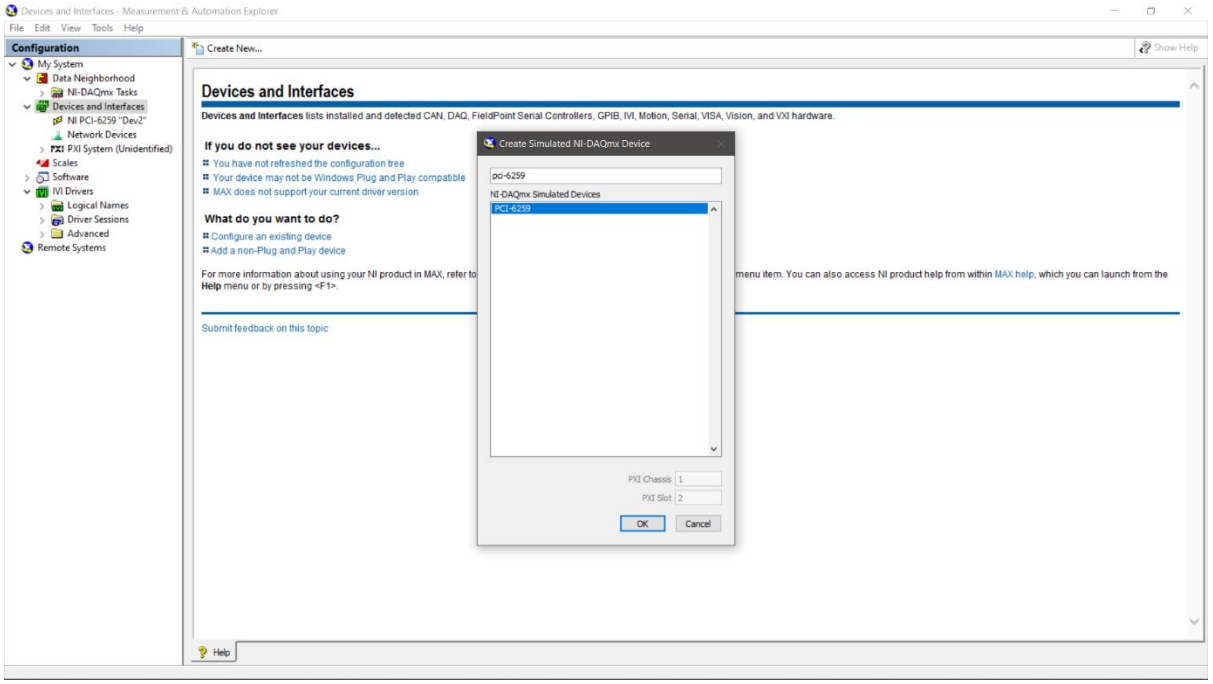
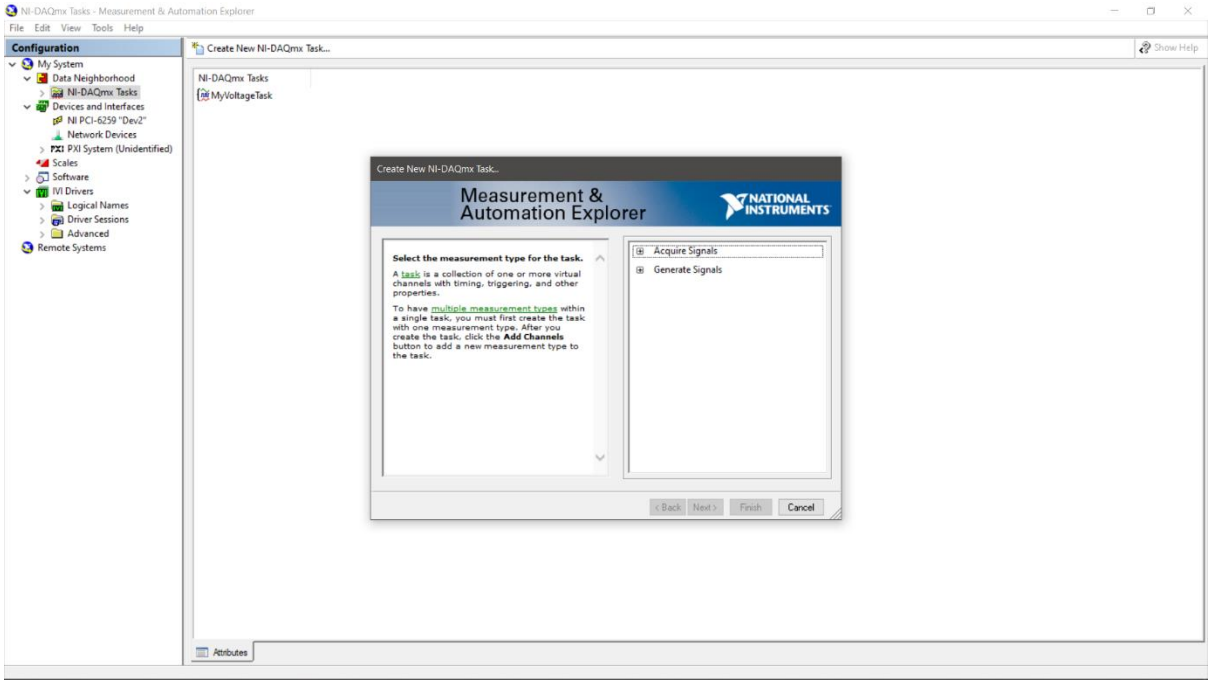
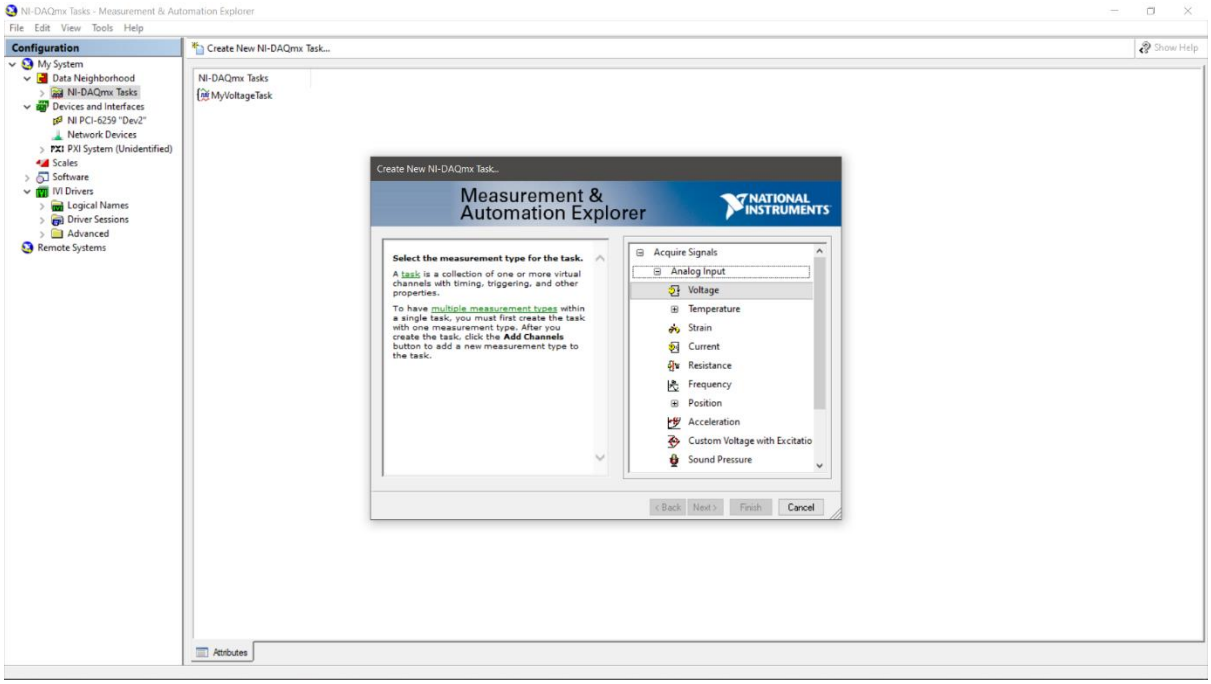
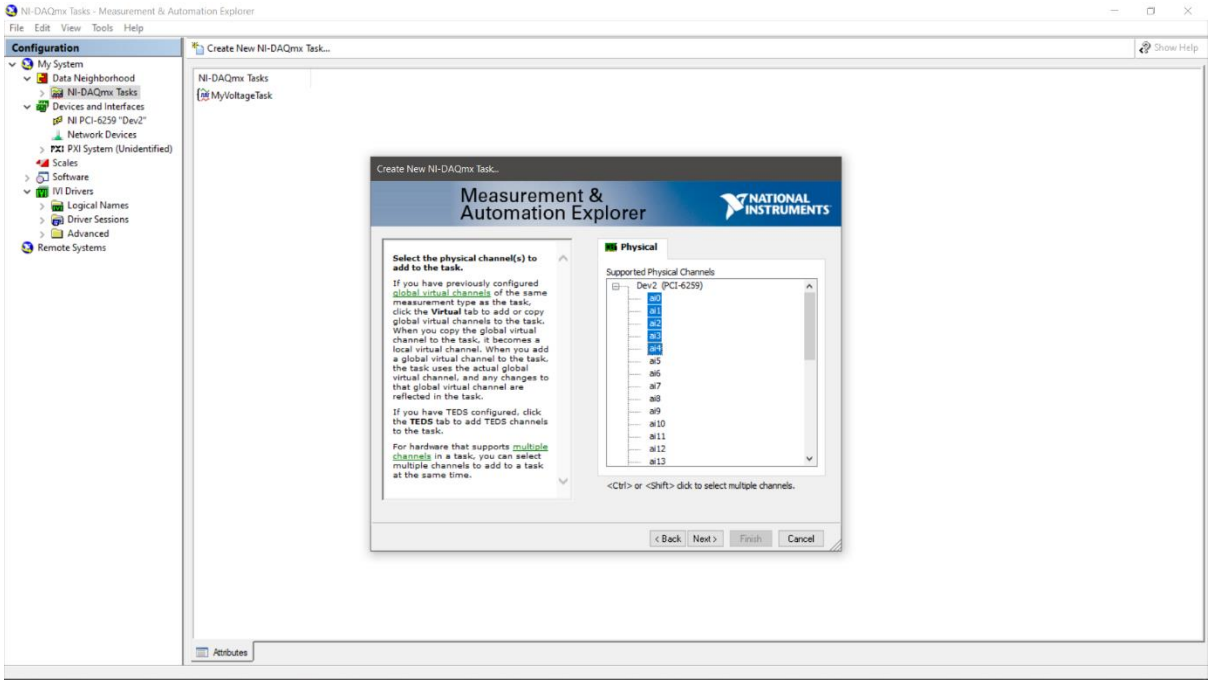

IVI Drivers - Measurement & Automation Explorer
File Edit View Tools Help
Configuration
My System
Data Neighborhood
NI-DAQmx Tasks
Devices and Interfaces
NI PCI-6259 "Dev2"
Network Devices
PXI System (Unidentified)
Scales
Software
IVI Drivers
Logical Names
Driver Sessions
Advanced
Remote Systems
Save IVI Configuration
Open IVI Configuration
Save IVI Configuration As...
Show Help
IVI Drivers
The IVI Drivers category provides access to all of your IVI logical names. Logical names allow you to define and name multiple driver sessions and switch between them by referencing the logical name in an application program. Application programs use logical names to avoid direct references to software modules and hardware assets.
What do you want to do?
Download and install an IVI driver
Logically name a driver session
Configure existing driver session properties
Swap instruments
Category Help
Information

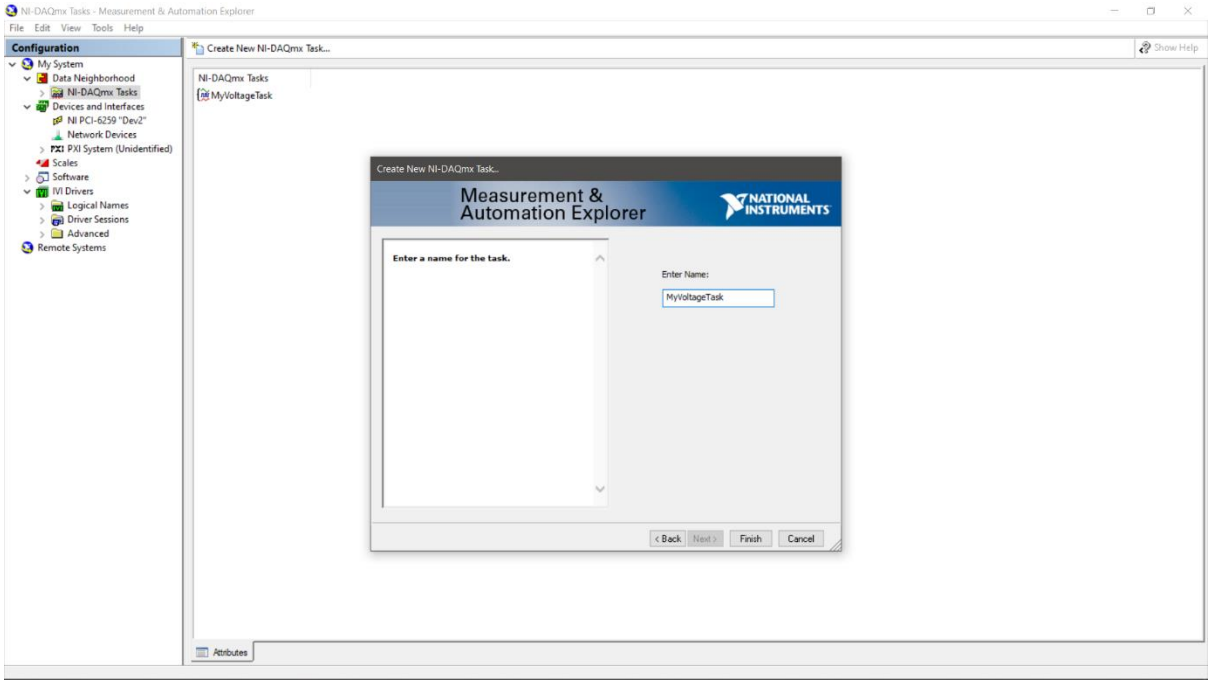

Devices and Interfaces - Measurement & Automation Explorer
File Edit View Tools Help
Configuration
My System
Data Neighborhood
NI-DAQmx Tasks
Devices and Interfaces
NI PCI-6259 "Dev2"
Network Devices
PXI System (Unidentified)
Scales
Software
IVI Drivers
Logical Names
Driver Sessions
Advanced
Remote Systems
Create New...
Show Help
Devices and Interfaces
Devices and Interfaces lists installed and detected CAN, DAQ, FieldPoint Serial Controllers, GPIB, IVI, Motion, Serial, VISA, Vision, and VXI hardware.
If you do not see your devices...
You have not refreshed the configura
Your device may not be Windows Plu
MAX does not support your current dr
What do you want to do?
Configure an existing device
Add a non-Plug and Play device
For more information about using your
Help menu or by pressing <F1>.
access NI product help from within MAX help, which you can launch from the
Submit feedback on this topic
Help
Create New ...
Measurement & Automation Explorer
NATIONAL INSTRUMENTS
Devices and Interfaces
Network NI-DAQmx Devices
NI-DAQmx SCXI Chassis
NI-DAQmx SCC Connector Block
NI-DAQmx TEDS Interface
RTSI Cable
Simulated NI-DAQmx Device or Modular Instrument
< Back
Next >
Finish
Cancel

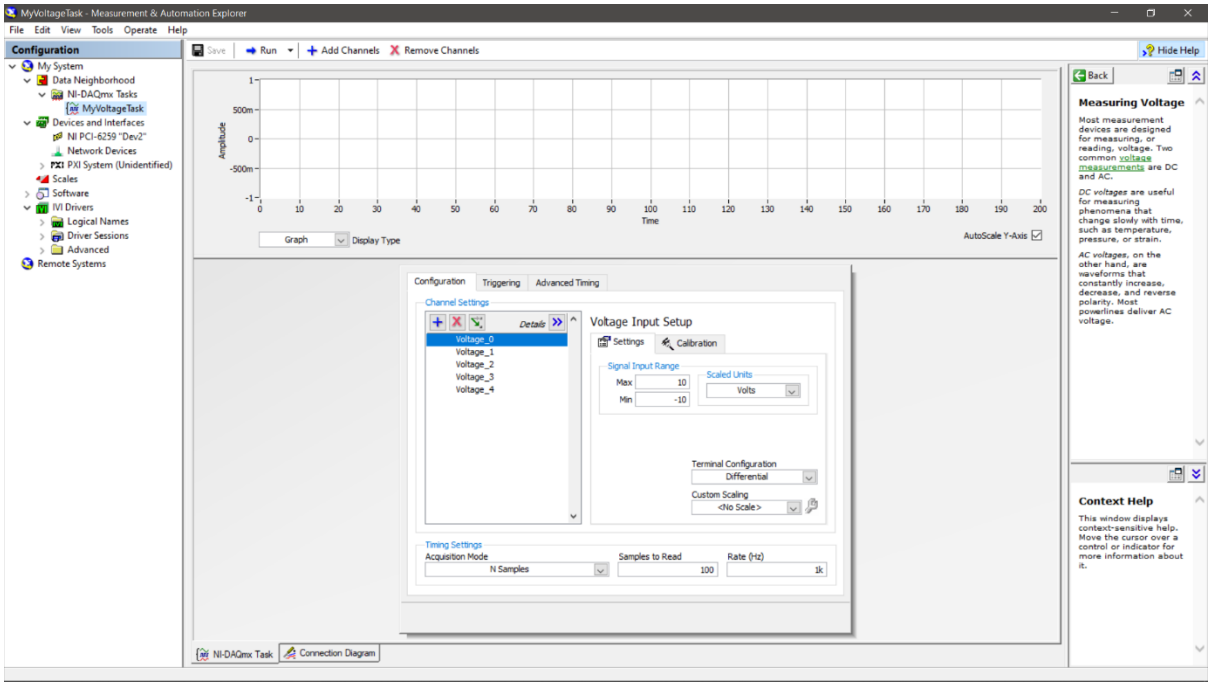

Devices and Interfaces - Measurement & Automation Explorer
File Edit View Tools Help
Configuration
My System
Data Neighborhood
NI-DAQmx Tasks
Devices and Interfaces
NI PCI-6259 "Dev2"
Network Devices
PXI System (Unidentified)
Scales
Software
IVI Drivers
Logical Names
Driver Sessions
Advanced
Remote Systems
Create New...
Show Help
Devices and Interfaces
Devices and Interfaces lists installed and detected CAN, DAQ, FieldPoint Serial Controllers, GPIB, IVI, Motion, Serial, VISA, Vision, and VXI hardware.
If you do not see your devices...
You have not refreshed the configuration tree
Your device may not be Windows Plug and Play compatible
MAX does not support your current driver version
What do you want to do?
Configure an existing device
Add a non-Plug and Play device
For more information about using your NI product in MAX, refer to
menu item. You can also access NI product help from within MAX help, which you can launch from the Help menu or by pressing <F1>.
Submit feedback on this topic
Create Simulated NI-DAQmx Device
pci-6259
NI-DAQmx Simulated Devices
PCI-6259
PXI Chassis 1
PXI Slot 2
OK
Cancel
Help

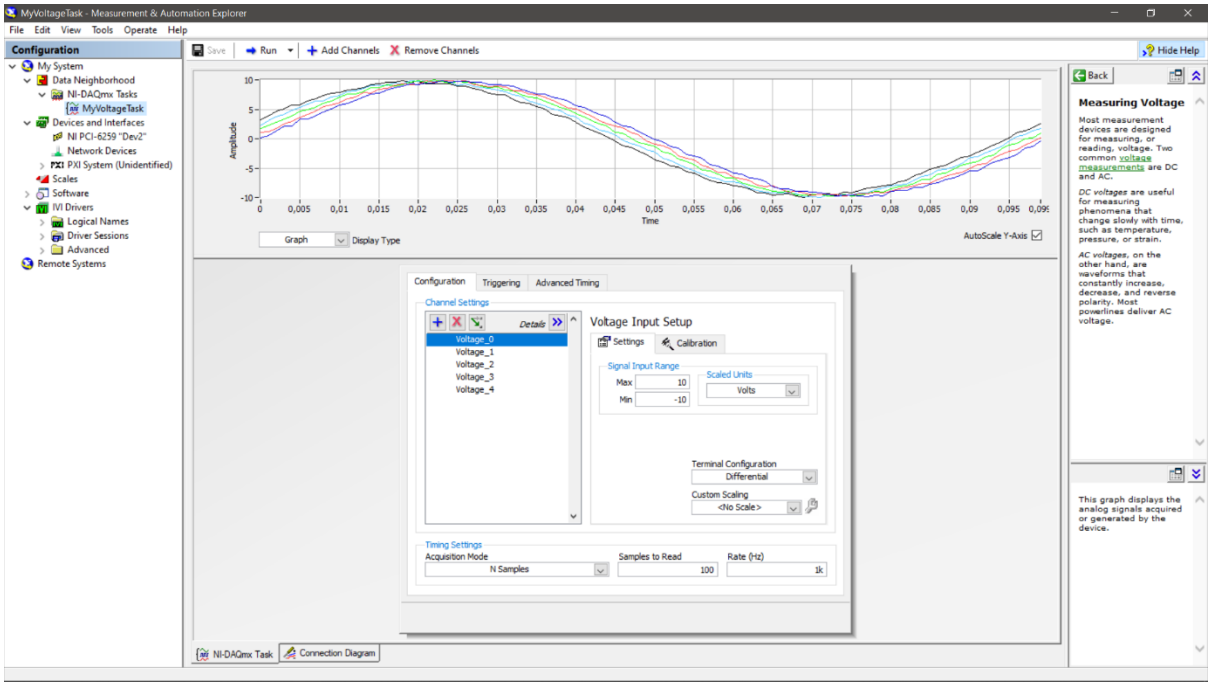

NI-DAQmx Tasks - Measurement & Automation Explorer
File Edit View Tools Help
Configuration
My System
Data Neighborhood
NI-DAQmx Tasks
Devices and Interfaces
NI PCI-6259 "Dev2"
Network Devices
PXI System (Unidentified)
Scales
Software
IVI Drivers
Logical Names
Driver Sessions
Advanced
Remote Systems
Create New NI-DAQmx Task...
Show Help
NI-DAQmx Tasks
MyVoltageTask
Create New NI-DAQmx Task...
Measurement & Automation Explorer
NATIONAL INSTRUMENTS
Select the measurement type for the task.
A task is a collection of one or more virtual channels with timing, triggering, and other properties.
To have multiple measurement types within a single task, you must first create the task with one measurement type. After you create the task, click the Add Channels button to add a new measurement type to the task.
Acquire Signals
Generate Signals
< Back
Next >
Finish
Cancel
Attributes

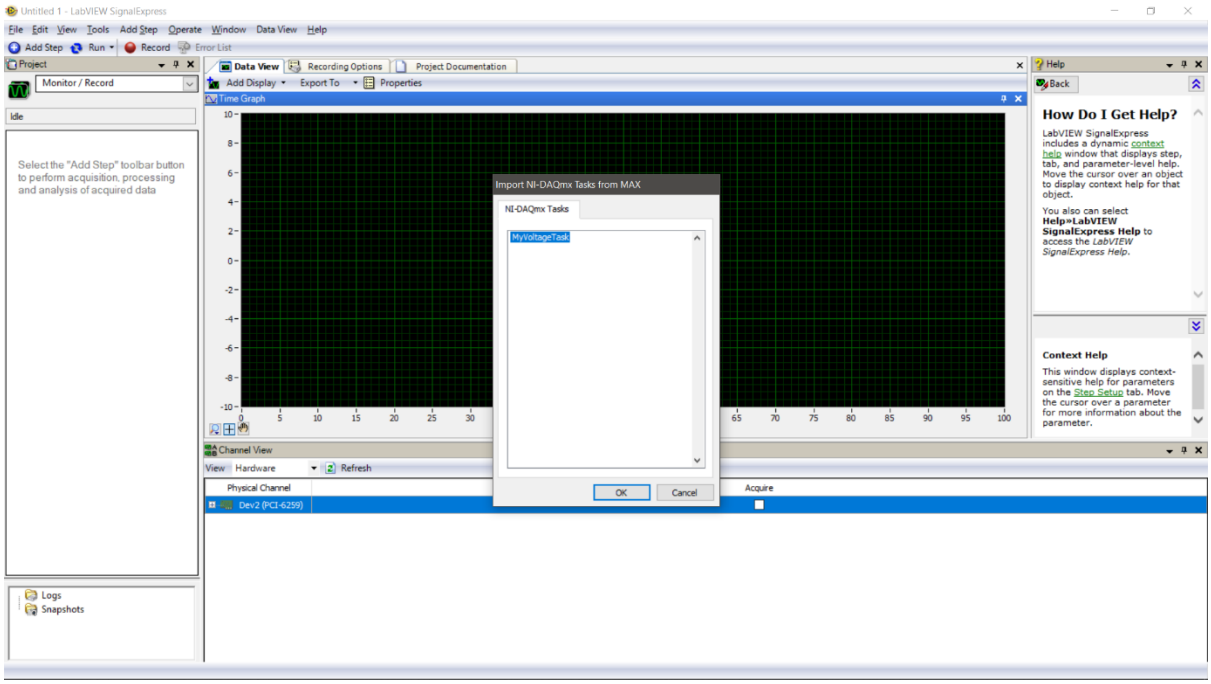

NI-DAQmx Tasks - Measurement & Automation Explorer
File Edit View Tools Help
Configuration
My System
Data Neighborhood
NI-DAQmx Tasks
Devices and Interfaces
NI PCI-6259 "Dev2"
Network Devices
PXI System (Unidentified)
Scales
Software
IVI Drivers
Logical Names
Driver Sessions
Advanced
Remote Systems
Create New NI-DAQmx Task...
Show Help
NI-DAQmx Tasks
MyVoltageTask
Create New NI-DAQmx Task...
Measurement & Automation Explorer
NATIONAL INSTRUMENTS
Select the measurement type for the task.
A task is a collection of one or more virtual channels with timing, triggering, and other properties.
To have multiple measurement types within a single task, you must first create the task with one measurement type. After you create the task, click the Add Channels button to add a new measurement type to the task.
Acquire Signals
Analog Input
Voltage
Temperature
Strain
Current
Resistance
Frequency
Position
Acceleration
Custom Voltage with Excitatio
Sound Pressure
< Back
Next >
Finish
Cancel
Attributes

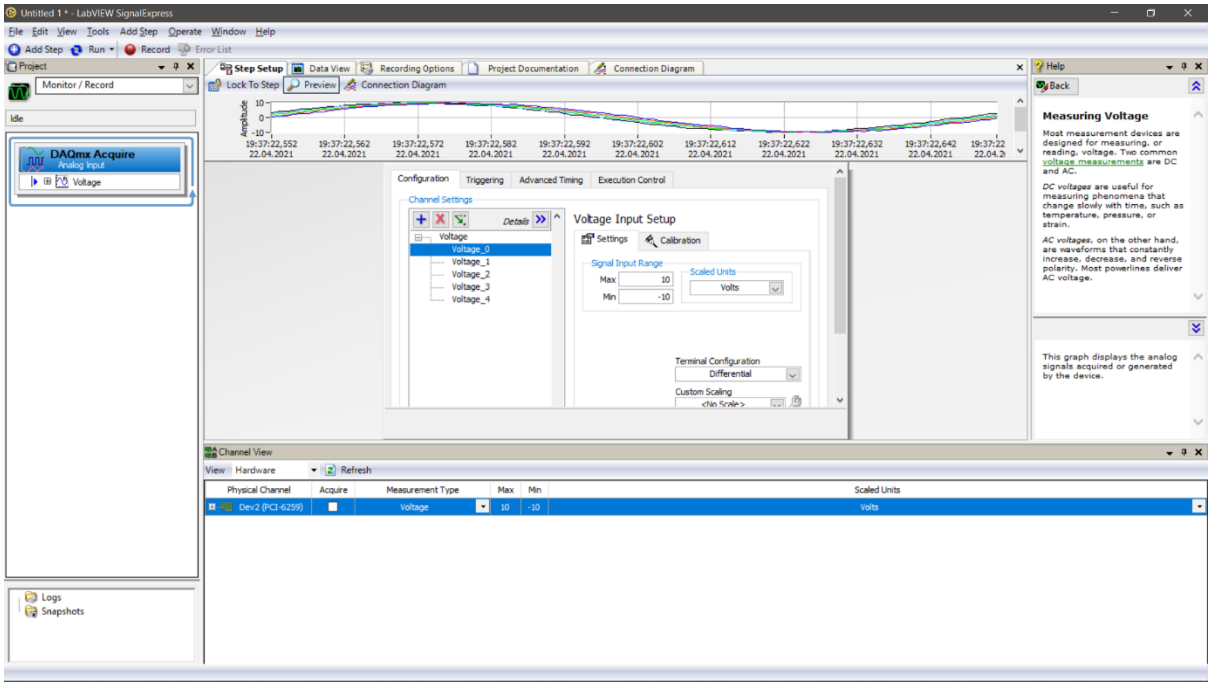

NI-DAQmx Tasks - Measurement & Automation Explorer
File Edit View Tools Help
Configuration
My System
Data Neighborhood
NI-DAQmx Tasks
Devices and Interfaces
NI PCI-6259 "Dev2"
Network Devices
PXI System (Unidentified)
Scales
Software
IVI Drivers
Logical Names
Driver Sessions
Advanced
Remote Systems
Create New NI-DAQmx Task...
Show Help
NI-DAQmx Tasks
MyVoltageTask
Create New NI-DAQmx Task...
Measurement & Automation Explorer
NATIONAL INSTRUMENTS
Select the physical channel(s) to add to the task.
If you have previously configured global virtual channels of the same measurement type as the task, click the Virtual tab to add or copy global virtual channels to the task. When you copy the global virtual channel to the task, it becomes a local virtual channel. When you add a global virtual channel to the task, the task uses the actual global virtual channel, and any changes to that global virtual channel are reflected in the task.
If you have TEDS configured, click the TEDS tab to add TEDS channels to the task.
For hardware that supports multiple channels in a task, you can select multiple channels to add to a task at the same time.
Physical
Supported Physical Channels
Dev2 (PCI-6259)
ai0
ai1
ai2
ai3
ai4
ai5
ai6
ai7
ai8
ai9
ai10
ai11
ai12
ai13
<Ctrl> or <Shift> click to select multiple channels.
< Back
Next >
Finish
Cancel
Attributes

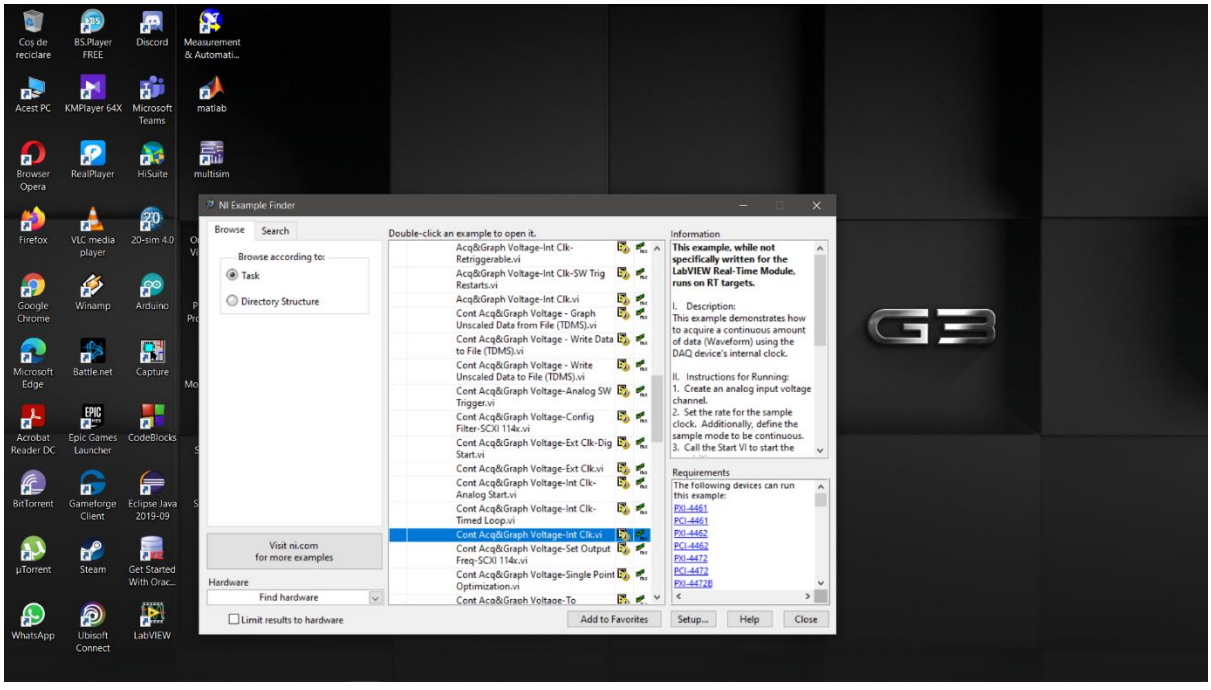

NI-DAQmx Tasks - Measurement & Automation Explorer
File Edit View Tools Help
Configuration
My System
Data Neighborhood
NI-DAQmx Tasks
Devices and Interfaces
NI PCI-6259 "Dev2"
Network Devices
PXI System (Unidentified)
Scales
Software
IVI Drivers
Logical Names
Driver Sessions
Advanced
Remote Systems
Create New NI-DAQmx Task...
Show Help
NI-DAQmx Tasks
MyVoltageTask
Create New NI-DAQmx Task...
Measurement & Automation Explorer
NATIONAL INSTRUMENTS
Enter a name for the task.
Enter Name:
MyVoltageTask
< Back
Next >
Finish
Cancel
Attributes

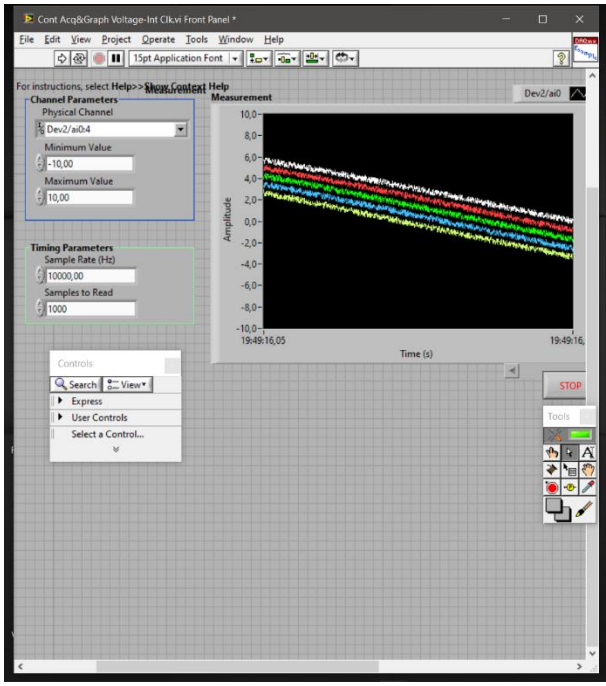

MyVoltageTask - Measurement & Automation Explorer
File Edit View Tools Operate Help
Configuration
My System
Data Neighborhood
NI-DAQmx Tasks
MyVoltageTask
Devices and Interfaces
NI PCI-6259 "Dev2"
Network Devices
PXI System (Unidentified)
Scales
Software
IVI Drivers
Logical Names
Driver Sessions
Advanced
Remote Systems
Save
Run
Add Channels
Remove Channels
Hide Help
Amplitude
Time
Graph
Display Type
AutoScale Y-Axis
Configuration
Triggering
Advanced Timing
Channel Settings
Details
Voltage_0
Voltage_1
Voltage_2
Voltage_3
Voltage_4
Voltage Input Setup
Settings
Calibration
Signal Input Range
Max
Min
Scaled Units
Volts
Terminal Configuration
Differential
Custom Scaling
<No Scale>
Timing Settings
Acquisition Mode
N Samples
Samples to Read
Rate (Hz)
NI-DAQmx Task
Connection Diagram
Back
Measuring Voltage
Most measurement devices are designed for measuring, or reading, voltage. Two common voltage measurements are DC and AC.
DC voltages are useful for measuring phenomena that change slowly with time, such as temperature, pressure, or strain.
AC voltages, on the other hand, are waveforms that constantly increase, decrease, and reverse polarity. Most powerlines deliver AC voltage.
Context Help
This window displays context-sensitive help. Move the cursor over a control or indicator for more information about it.

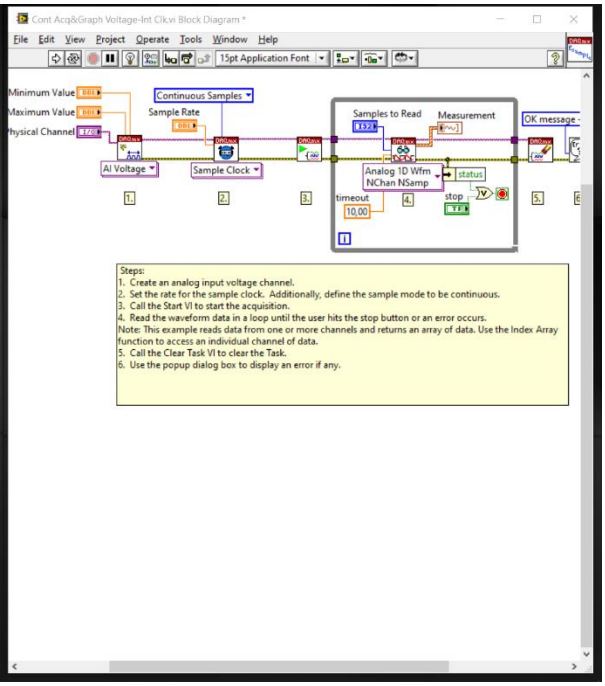

MyVoltageTask - Measurement & Automation Explorer
File Edit View Tools Operate Help
Configuration
My System
Data Neighborhood
NI-DAQmx Tasks
MyVoltageTask
Devices and Interfaces
NI PCI-6259 "Dev2"
Network Devices
PXI System (Unidentified)
Scales
Software
IVI Drivers
Logical Names
Driver Sessions
Advanced
Remote Systems
Save
Run
Add Channels
Remove Channels
Hide Help
Amplitude
Time
Graph
Display Type
AutoScale Y-Axis
Configuration
Triggering
Advanced Timing
Channel Settings
Details
Voltage_0
Voltage_1
Voltage_2
Voltage_3
Voltage_4
Voltage Input Setup
Settings
Calibration
Signal Input Range
Max
Min
Scaled Units
Volts
Terminal Configuration
Differential
Custom Scaling
<No Scale>
Timing Settings
Acquisition Mode
N Samples
Samples to Read
Rate (Hz)
NI-DAQmx Task
Connection Diagram
Back
Measuring Voltage
Most measurement devices are designed for measuring, or reading, voltage. Two common voltage measurements are DC and AC.
DC voltages are useful for measuring phenomena that change slowly with time, such as temperature, pressure, or strain.
AC voltages, on the other hand, are waveforms that constantly increase, decrease, and reverse polarity. Most powerlines deliver AC voltage.
This graph displays the analog signals acquired or generated by the device.

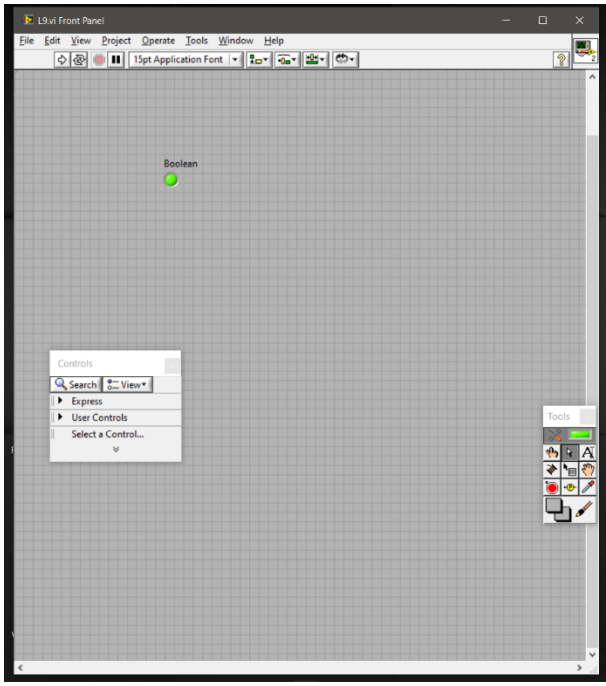

Untitled 1 - LabVIEW SignalExpress
File Edit View Tools Add Step Operate Window Data View Help
Add Step
Run
Record
Error List
Project
Monitor / Record
Idle
Select the "Add Step" toolbar button to perform acquisition, processing and analysis of acquired data
Logs
Snapshots
Data View
Recording Options
Project Documentation
Add Display
Export To
Properties
Time Graph
Import NI-DAQmx Tasks from MAX
NI-DAQmx Tasks
MyVoltageTask
OK
Cancel
Channel View
View
Hardware
Refresh
Physical Channel
Acquire
Dev2 (PCI-6259)
Help
Back
How Do I Get Help?
LabVIEW SignalExpress includes a dynamic context help window that displays step, tab, and parameter-level help. Move the cursor over an object to display context help for that object.
You also can select Help»LabVIEW SignalExpress Help to access the LabVIEW SignalExpress Help.
Context Help
This window displays context-sensitive help for parameters on the Step Setup tab. Move the cursor over a parameter for more information about the parameter.

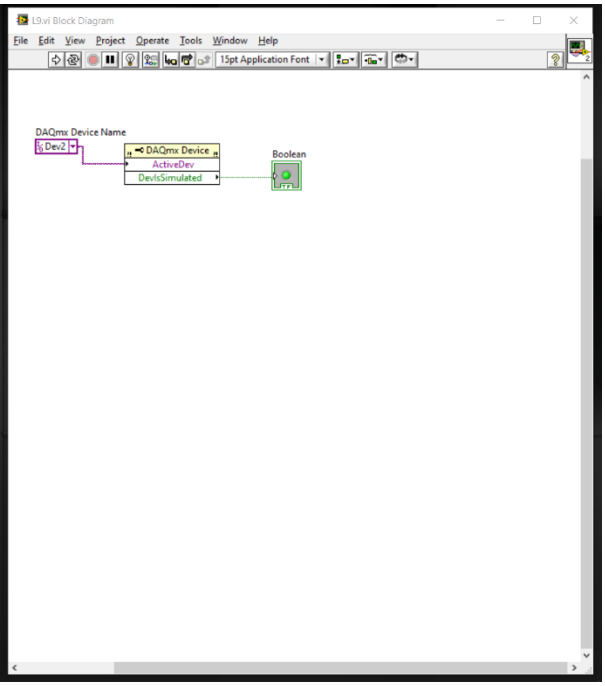

Untitled 1 * - LabVIEW SignalExpress
File Edit View Tools Add Step Operate Window Help
Add Step Run Record Error List
Project
Monitor / Record
Idle
DAQmx Acquire
Analog Input
Voltage
Logs
Snapshots
Step Setup
Data View
Recording Options
Project Documentation
Connection Diagram
Lock To Step
Preview
Connection Diagram
Amplitude
10
0
-10
19:37:22,552 22.04.2021
19:37:22,562 22.04.2021
19:37:22,572 22.04.2021
19:37:22,582 22.04.2021
19:37:22,592 22.04.2021
19:37:22,602 22.04.2021
19:37:22,612 22.04.2021
19:37:22,622 22.04.2021
19:37:22,632 22.04.2021
19:37:22,642 22.04.2021
Configuration
Triggering
Advanced Timing
Execution Control
Channel Settings
Details
Voltage
Voltage_0
Voltage_1
Voltage_2
Voltage_3
Voltage_4
Voltage Input Setup
Settings
Calibration
Signal Input Range
Max 10
Min -10
Scaled Units
Volts
Terminal Configuration
Differential
Custom Scaling
<No Scale>
Help
Back
Measuring Voltage
Most measurement devices are designed for measuring, or reading, voltage. Two common voltage measurements are DC and AC.
DC voltages are useful for measuring phenomena that change slowly with time, such as temperature, pressure, or strain.
AC voltages, on the other hand, are waveforms that constantly increase, decrease, and reverse polarity. Most powerlines deliver AC voltage.
This graph displays the analog signals acquired or generated by the device.
Channel View
View Hardware
Refresh
Physical Channel
Acquire
Measurement Type
Max
Min
Scaled Units
Dev2 (PCI-6259)
Voltage
10
-10
Volts


Coș de reciclare
BSPlayer FREE
Discord
Measurement & Automati...
Acest PC
KMPlayer 64X
Microsoft Teams
matlab
Browser Opera
RealPlayer
HiSuite
multisim
Firefox
VLC media player
20-sim 4.0
Google Chrome
Winamp
Arduino
Microsoft Edge
Battle.net
Capture
Acrobat Reader DC
Epic Games Launcher
CodeBlocks
BitTorrent
Gameforge Client
Eclipse Java 2019-09
µTorrent
Steam
Get Started With Orac...
WhatsApp
Ubisoft Connect
LabVIEW
NI Example Finder
Browse
Search
Browse according to:
Task
Directory Structure
Visit ni.com for more examples
Hardware
Find hardware
Limit results to hardware
Double-click an example to open it.
Acq&Graph Voltage-Int Clk-Retriggerable.vi
Acq&Graph Voltage-Int Clk-SW Trig Restarts.vi
Acq&Graph Voltage-Int Clk.vi
Cont Acq&Graph Voltage - Graph Unscaled Data from File (TDMS).vi
Cont Acq&Graph Voltage - Write Data to File (TDMS).vi
Cont Acq&Graph Voltage - Write Unscaled Data to File (TDMS).vi
Cont Acq&Graph Voltage-Analog SW Trigger.vi
Cont Acq&Graph Voltage-Config Filter-SCXI 114x.vi
Cont Acq&Graph Voltage-Ext Clk-Dig Start.vi
Cont Acq&Graph Voltage-Ext Clk.vi
Cont Acq&Graph Voltage-Int Clk-Analog Start.vi
Cont Acq&Graph Voltage-Int Clk-Timed Loop.vi
Cont Acq&Graph Voltage-Int Clk.vi
Cont Acq&Graph Voltage-Set Output Freq-SCXI 114x.vi
Cont Acq&Graph Voltage-Single Point Optimization.vi
Cont Acq&Graph Voltage-To
Information
This example, while not specifically written for the LabVIEW Real-Time Module, runs on RT targets.
I. Description:
This example demonstrates how to acquire a continuous amount of data (Waveform) using the DAQ device's internal clock.
II. Instructions for Running:
1. Create an analog input voltage channel.
2. Set the rate for the sample clock. Additionally, define the sample mode to be continuous.
3. Call the Start VI to start the
Requirements
The following devices can run this example:
PXI-4461
PCI-4461
PXI-4462
PCI-4462
PXI-4472
PCI-4472
PXI-4472B
Add to Favorites
Setup...
Help
Close


Cont Acq&Graph Voltage-Int Clk.vi Front Panel *
File Edit View Project Operate Tools Window Help
15pt Application Font
For instructions, select Help>>Show Context Help
Channel Parameters
Physical Channel
Dev2/ai0:4
Minimum Value
-10,00
Maximum Value
10,00
Timing Parameters
Sample Rate (Hz)
10000,00
Samples to Read
1000
Measurement
Dev2/ai0
Amplitude
Time (s)
19:49:16,05
Controls
Search
View
Express
User Controls
Select a Control...
STOP
Tools


Cont Acq&Graph Voltage-Int Clk.vi Block Diagram *
File Edit View Project Operate Tools Window Help
15pt Application Font
Minimum Value
Maximum Value
Physical Channel
Continuous Samples
Sample Rate
AI Voltage
Sample Clock
Samples to Read
Measurement
Analog 1D Wfm NChan NSamp
status
timeout
10,00
stop
OK message
Steps:
1. Create an analog input voltage channel.
2. Set the rate for the sample clock. Additionally, define the sample mode to be continuous.
3. Call the Start VI to start the acquisition.
4. Read the waveform data in a loop until the user hits the stop button or an error occurs.
Note: This example reads data from one or more channels and returns an array of data. Use the Index Array function to access an individual channel of data.
5. Call the Clear Task VI to clear the Task.
6. Use the popup dialog box to display an error if any.


L9.vi Front Panel
File Edit View Project Operate Tools Window Help
15pt Application Font
Boolean
Controls
Search
View
Express
User Controls
Select a Control...
Tools


L9.vi Block Diagram
File Edit View Project Operate Tools Window Help
15pt Application Font
DAQmx Device Name
Dev2
DAQmx Device
ActiveDev
DevIsSimulated
Boolean