



Test Scores

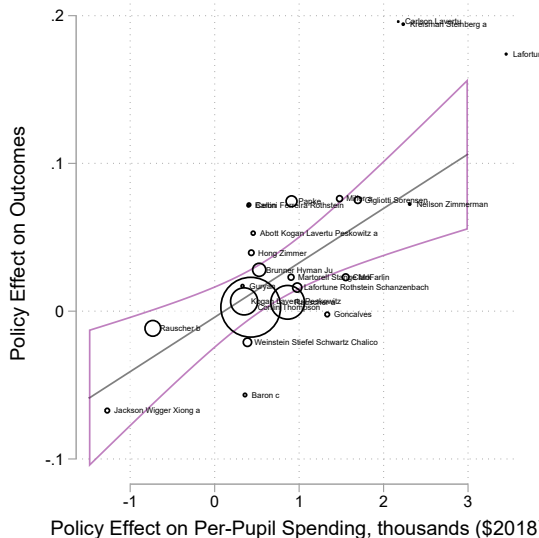

Precision-weighted linear slope: 0.0368 (p-value = 0.004),
 constant: -0.0041 (p-value = 0.635)
 Instrument overidentification test p-value: 0.4656
 Roy (2011) and Chaudhary (2009) not plotted for scale.

Educational Attainment

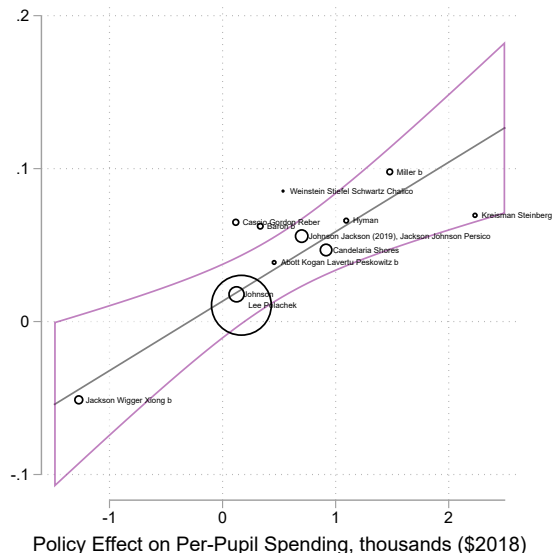

Precision-weighted linear slope: 0.0454 (p-value = 0.011)
 constant: 0.0133 (p-value = 0.165)
 Instrument overidentification test p-value: 0.4813