


Test Scores

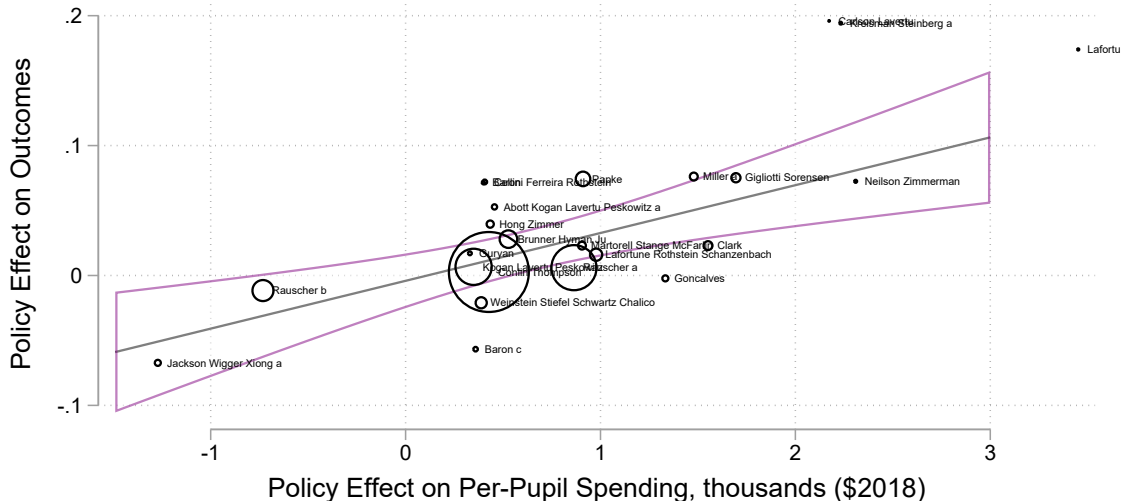

— Linear w/ 95% CI

Precision-weighted linear slope: 0.0368 (p-value = 0.004),
constant: -0.0041 (p-value = 0.635)

Instrument overidentification test p-value: 0.4656

Roy (2011) and Chaudhary (2009) not plotted for scale.