

# ATI Mini40 DAQ F/T sensor information and tips

Iris David Du Mutel

July 21, 2023

## Abstract

This document is meant to be a summary of all the relevant information I have found while working with the ATI Mini40 DAQ F/T sensor. It contains all the information and instructions to operate such sensor in various environments such as LabView, Python and MATLAB using the Keysight 34970A Data Acquisition Unit.

## 1 What kind of sensor is the ATI Mini40 DAQ F/T?

The transducer is a compact, durable, monolithic structure that converts force and torque into analog strain gage signals. The force applied to the transducer flexes three symmetrically placed beams using Hooke's law (from page 16 of the manual 9620-05-DAQ):

- $s = E \cdot e$
- $s$  = Stress applied to the beam ( $s$  is proportional to force)
- $E$  = Elasticity modulus of the beam
- $e$  = Strain applied to the beam

Semiconductor strain gages are attached to the beams and act as strain-sensitive resistors. The resistance of the strain gage changes as a function of the applied strain as follows:

- $\Delta R = S_a \cdot R_o \cdot e$
- $\Delta R$  = Change in resistance of strain gage
- $S_a$  = Gage factor of strain gage
- $R_o$  = Resistance of strain gage unstrained
- $e$  = Strain applied to strain gage

### 1.1 Load calculation

From page 18 of the manual:

Additionally to this, gain correction factor is only required when a customer amplifier is being used. Refer to page 20 of the manual for more information.

## 2 Wiring and connecting to a DAQ

There are two different wiring alternatives for the DAQ version of this sensor:

- Differential connections to DAQ (Figure ??)
- Single-ended connections to DAQ (Figure ??)

Figure 3.4—FT Matrix Calculations

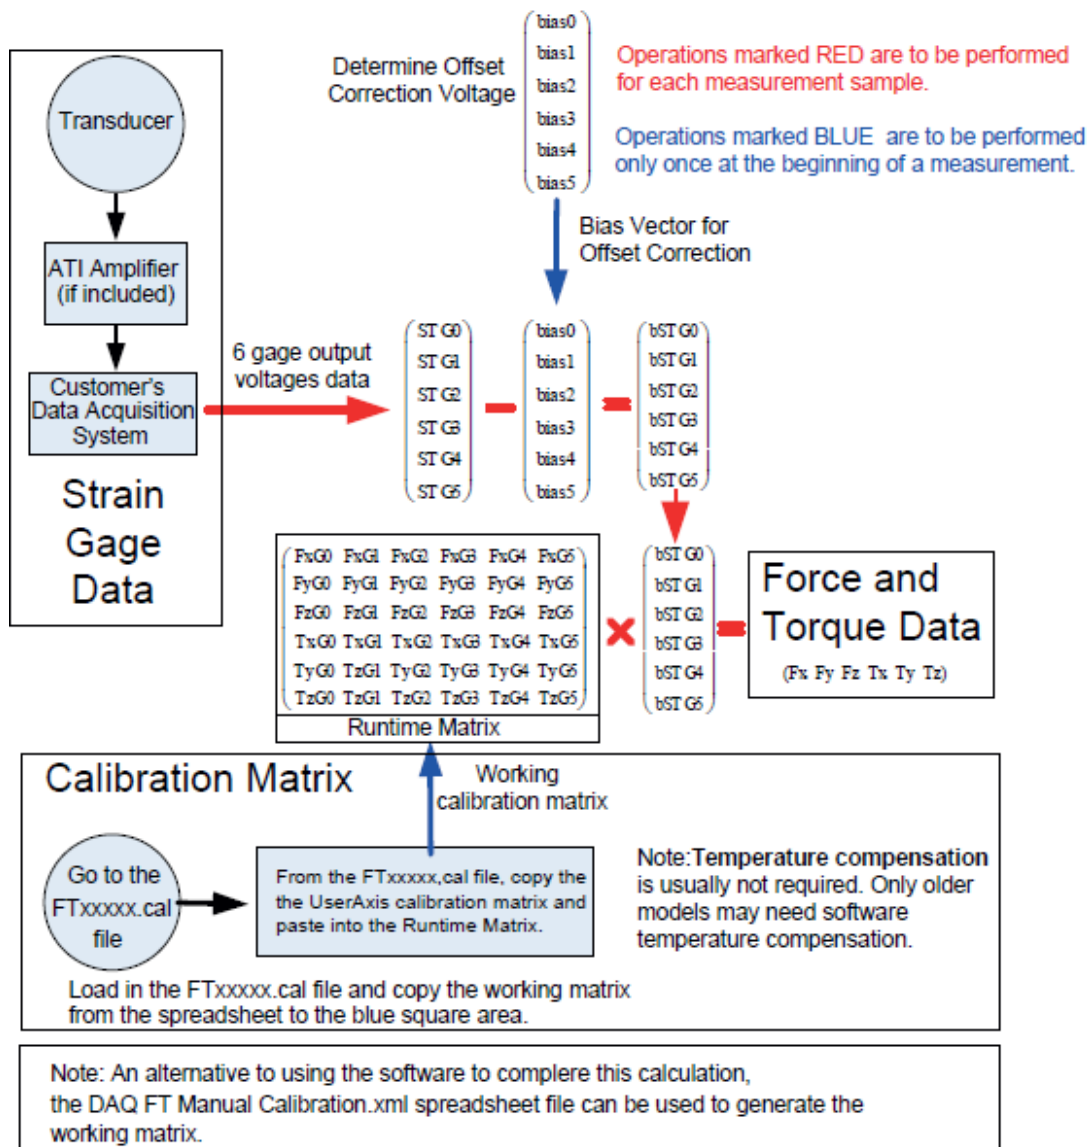


Figure 1: Load calculation process

A connection from the DAQ F/T's AGnd/AIGnd line to the data acquisition system's analog input ground or analog ground is required in most cases. This line allows the return of the small amount of current used by the data acquisition system. Noise can result if this current isn't returned via the AGnd/AIGnd path. For best noise performance, the cabling from the PS/IPFS connector should be shielded and each strain gage's signals in a twisted pair. The shielding should be connected to the PS/IPFS connector shell and to the shell of the data acquisition system's connector. If the data acquisition system has no connector or its connector shell is electrically floating, then the shield at the PS/IPFS connector should be connected to the AGnd/AIGnd signal.

## 2.1 Sampling

For best performance in all applications (page 37 from 9620-05-DAQ), the transducer electronics have bandwidth of 5kHz to 10kHz (depending on gain settings). This allows collection of all transducer frequency content. Note: that to satisfy the Nyquist Theorem, the data needs to be coupled at a rate

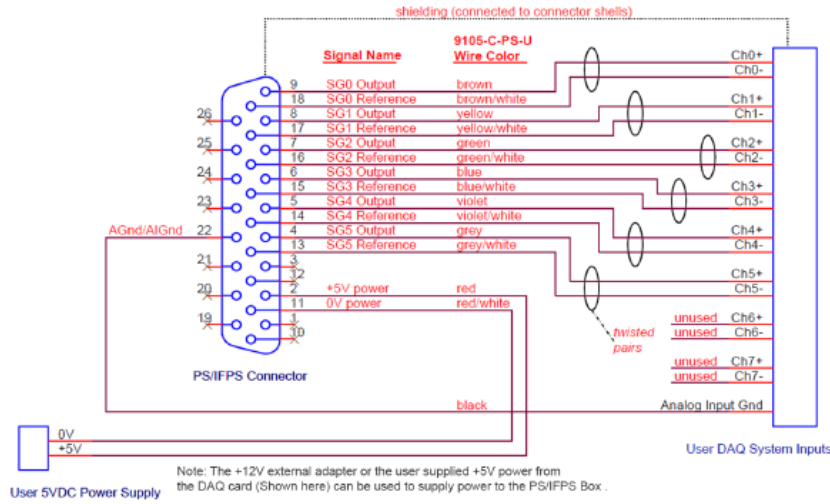


Figure 2: Differential wiring connections to data acquisition system (page 35 from 9620-05-DAQ)

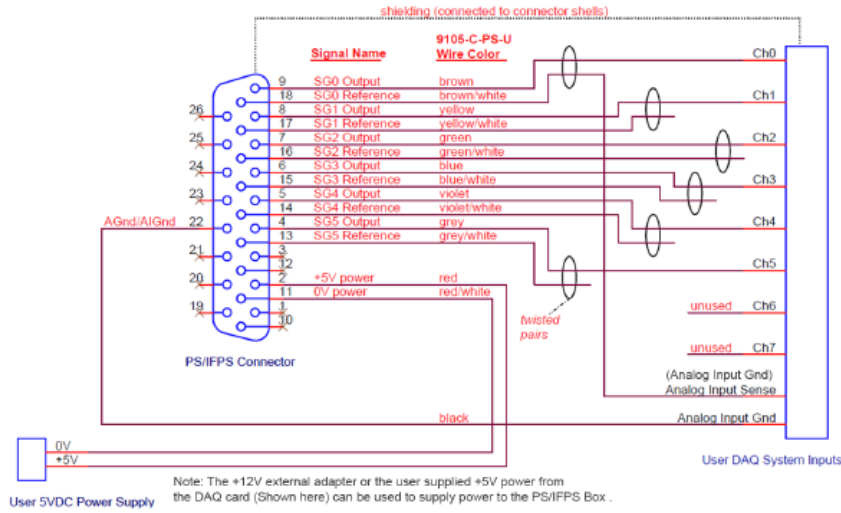


Figure 3: Single-ended wiring connections to data acquisition system (page 36 from 9620-05-DAQ)

greater than twice the highest frequency present, even if data at that frequency is not preferred. The forces and torques will be sampled at that frequency, not having anything to do with the sampling rate of the data acquisition unit.

The data acquisition unit on the other hand has a maximum ampertire time of  $400\mu s$ , meaning that's the smallest amount of time it needs for opening and reading from one channel. This aperture time is equivalent to an integration time of 0.02 PLC. The relationship between this two parameters is the following:

$$\frac{0.02PLC}{50Hz(instrumentpowerfrequency)} = 400\mu s \quad (1)$$

Using a differential wiring with 12 channels, we will need to multiply that aperture time by the number of channels:

$$400\mu s \cdot 12 = 4800\mu s \quad (2)$$

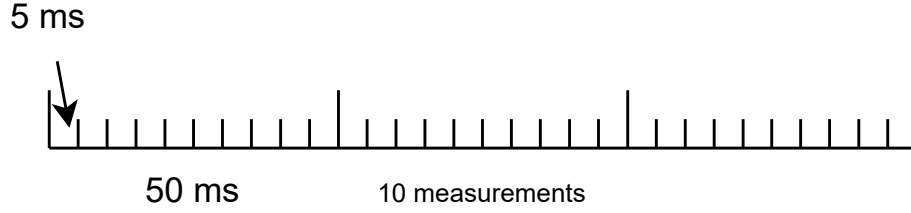


Figure 4: Representation of stuff

An aperture time of 4.8 ms is equivalent to a frequency of around 208 Hz. Rounding the aperture time to 5 ms per data volume (a vector containing one voltage value for each channel), we can obtain 10 measurements every 50 ms.

## 2.2 Range

As specified in the ATI site, the range of the sensor for the calibration US-20-40 is the following defined as the average of the worst and best case scenarios:

Table 1: Range values in imperial and metric systems

Fx, Fy	Fz	Tx,Ty	Tz
$\pm 20$ lbf	$\pm 60$ lbf	$\pm 40$ lbf-in	$\pm 40$ lbf-in
$\pm 88.9644$ N	$\pm 266.893$ N	$\pm 4.51939$ N-m	$\pm 4.51939$ N-m

## 2.3 Resolution

As specified in the ATI site, the resolution of the sensor for the calibration US-20-40 is the following defined as the average of the worst and best case scenarios:

Table 2: Resolution values in imperial and metric systems

Fx, Fy	Fz	Tx,Ty	Tz
1/200 lbf	1/100 lbf	1/200 lbf-in	1/200 lbf-in
0.022241108 N	0.0444822 N	0.000564924 N-m	0.000564924 N-m

## 2.4 Sensitivity and output range and resolution voltages

From page 54 of the transducer manual, we can obtain the analog  $\pm 10$  V sensitivity. Using the data from tables 1 and 2, we can obtain the following table:

Table 3: Sensitivity, range and resolution outputs voltages (imperial system)

	Fx, Fy	Fz	Tx,Ty,Tz
Analog $\pm 10$ V sensitivity	2 lbf/V	6 lbf/V	4 lbf-in/V
Range [V]	$\pm 10$	$\pm 10$	$\pm 10$
Resolution [V]	1/400	1/600	1/800

The minimum voltage that the DAQ must be able to measure is  $1/800$  V = 1.25 mV. The range must be  $\pm 10$  V.

Just for clarity purposes, Table 3 in metric system would be as follows:

Table 4: Sensitivity, range and resolution outputs voltages (metric system)

	Fx, Fy	Fz	Tx,Ty,Tz
Analog $\pm 10V$ sensitivity	8.89644 N/V	26.6893 N/V	17.7929 N/V
Range [V]	$\pm 10$	$\pm 10$	$\pm 10$
Resolution [V]	1/400	1/600	1/800

### 3 Keysight 34970A connection to PC

The connection is made via a GPIB-USB-HS cable. The GPIB-USB-HS is an IEEE 488 controller device for computers with USB slots. The GPIB-USB-HS achieves maximum IEEE 488.2 performance. The exact model can be found in Amazon. The differences with the original true version of this device are not the scope of this document.

There are various manuals for this DAQ. The most helpful one containing command examples is the Keysight 34970A/34972A Command Reference Manual. From this manual, the information from the following section was found.

#### 3.1 Important commands

**ROUT:SCAN** : This command selects the channels to be included in the scan list. This command is used in conjunction with the CONFigure commands to set up an automated scan. To start the scan, use the INITiate or READ? command.

**INStrument:DMM** : This command disables or enables the internal digital multimeter. When you change the state of the internal DMM, the instrument issues a Factory Reset (\*RST command).

**TRIGger:SOURce** : Select the trigger source to control the onset of each sweep through the scan list (a sweep is one pass through the scan list). The instrument will accept a software (bus) command, an immediate (continuous) scan trigger, an external TTL trigger pulse, an alarm-initiated action, or an internally paced timer. Usually used: TIMer = Internally paced timer trigger.

**TRIGger:TIMer** : This command sets the trigger-to-trigger interval (in seconds) for measurements on the channels in the present scan list. This command defines the time from the start of one trigger to the start of the next trigger, up to the specified trigger count.

### 4 LabView

LabView offers two main ways of interacting with the Keysight 34970A DAQ:

- General purpose Virtual Instrument Software Architecture (VISA) blocks. NI-VISA is an API that provides a programming interface to control Ethernet/LXI, GPIB, serial, USB, PXI, and VXI instruments in NI application development environments like LabVIEW, LabWindows/CVI, and Measurement Studio. The API is installed through the NI-VISA driver [1].
- Agilent Technologies / Keysight Technologies 34970A drivers. These block are based on the VISA blocks but offer a more user-friendly approach to configuring the instrument as well as reading data from it.

The example provided in this repository uses generic VISA blocks. In Figure 5, the block diagram of the VI can be seen:

Inside the while loop, the write and read blocks are interacting with the instrument. Every iteration, the *write* block sends the following commands to the DAQ:

- DISP OFF: This command turns off the display of the external instrument. This speeds up the sampling process.

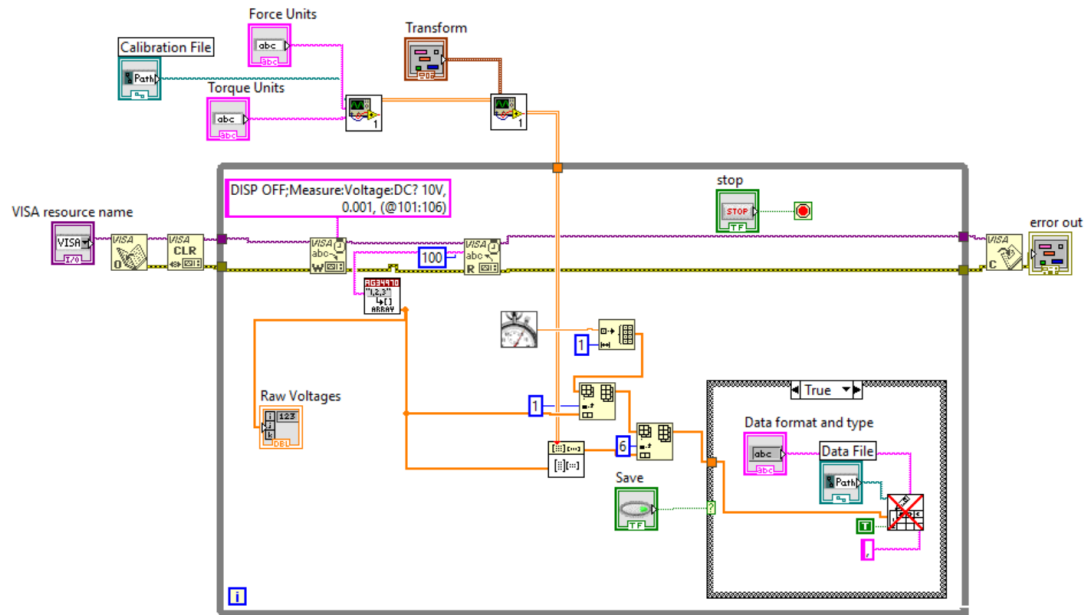


Figure 5: LabView block diagram

- MEASure:VOLTage:DC? 10V, 0.001, (@101:106): The first part of the command 'MEASure:VOLTage:DC?' is requesting the measurement of the voltage. The question mark indicates a query command. The two numbers following such query are the *range* and the *resolution*, respectively. There are alternative values for these parameters. See more in pages 211 to 217 from the manual.

## 5 Python

## 6 Resources

Keysight 34970A/34972A Command Reference Manual

## References

- [1] "Ni-visa overview - ni." [Online]. Available: <https://www.ni.com/en/support/documentation/supplemental/06/ni-visa-overview.html>
- [2] "Agilent technologies / keysight technologies 34970a data acquisition unit - instrument driver - national instruments." [Online]. Available: [http://sine.ni.com/apps/utf8/niid\\_web\\_display.model\\_page?p\\_model.id=5547](http://sine.ni.com/apps/utf8/niid_web_display.model_page?p_model.id=5547)