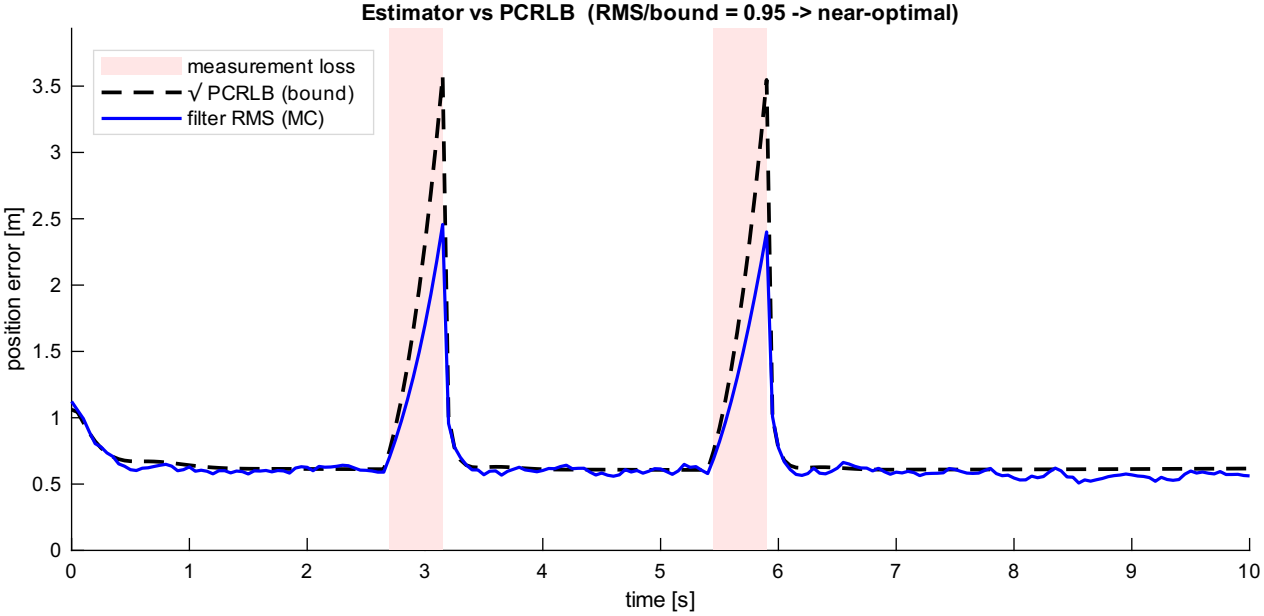
Estimator vs PCRLB (RMS/bound = 0.95 -> near-optimal)
measurement loss
√ PCRLB (bound)
filter RMS (MC)
position error [m]
time [s]
0
0.5
1
1.5
2
2.5
3
3.5
0
1
2
3
4
5
6
7
8
9
10