

1 Highlights

2 **A physics-informed digital twin for tube-life-aware operation of** 3 **industrial steam methane reformers under uncertainty**

4 Madina Sissenbay, Izbassar Orynbasar

- 5 • Open digital twin couples reformer kinetics, furnace, tube wall and
6 creep life
- 7 • Calibrated on published plant data: outlet T within 4 K, wall T within
8 12 K
- 9 • Firing, steam-to-carbon and excess air govern hot-spot temperature
10 and life
- 11 • Catalyst aging doubles tube-life cost; load-following changes it under 2
12 %
- 13 • Creep-curve scatter dominates life uncertainty; regime rankings survive
14 it

15 A physics-informed digital twin for tube-life-aware
16 operation of industrial steam methane reformers under
17 uncertainty

18 Madina Sissenbay^{a,*}, Izbassar Orynbassar^b

^a*Institute of Petrochemical Engineering and Ecology named after N.K. Nadirov, Safi
Utebayev Atyrau University of Oil and Gas, Atyrau, Kazakhstan*

^b*School of Information Studies, Syracuse University, 343 Hinds
Hall, Syracuse, 13244, NY, USA*

19 **Abstract**

20 Catalyst tubes are the life-limiting component of a steam methane reformer,
21 yet operating decisions are rarely taken with a quantified tube-life cost. A
22 digital twin is assembled from published data and open code, coupling a one-
23 dimensional Xu–Froment tube model, a long-furnace model of a top-fired
24 box furnace, a Larson–Miller creep-life module built on manufacturer rup-
25 ture curves with their printed scatter band, and Gaussian-process surrogates
26 with conformal prediction intervals. The tube model is verified against an
27 industrial simulation, and the coupled model is calibrated on three published
28 plant operating points with leave-one-case-out cross-validation, reproducing
29 outlet temperatures within 4 K and tube-wall temperatures within 12 K.
30 Firing intensity, steam-to-carbon ratio and excess air explain 82 % of the
31 hot-spot temperature variance with negligible interactions. Under outlet-
32 temperature control, load-following changes the tube-life cost per kmol of
33 hydrogen by less than 2 % in either direction, whereas catalyst aging under
34 a constant methane-slip target doubles it within four years. A Pareto knee

*Corresponding author.

Email addresses: m.sisenbay@aogu.edu.kz (Madina Sissenbay), iorynbas@syr.edu
(Izbassar Orynbassar)

URL: <https://orcid.org/0009-0009-8160-7472> (Madina Sissenbay),
<https://orcid.org/0009-0002-4224-3249> (Izbassar Orynbassar)

35 delivers 15 % more hydrogen at 17 % less fuel per kmol for 0.28 of the base
36 life cost, and creep-curve scatter dominates the life-prediction variance at
37 86 %. Regime rankings hold on four rupture curves; absolute lives do not.
38 *Keywords:* steam methane reforming, digital twin, creep life, uncertainty
39 quantification, multi-objective optimization, conformal prediction

40 1. Introduction

41 Steam methane reforming (SMR) supplies the large majority of the world's
42 hydrogen, close to 100 Mt per year and still produced predominantly from
43 natural gas without carbon capture [1]; it will remain the dominant route for
44 at least a decade while electrolytic capacity is built up. The core of an SMR
45 plant is a top-fired or side-fired furnace in which several hundred centrifu-
46 gally cast high-alloy tubes, filled with nickel catalyst, carry natural gas and
47 steam at 25–35 bar while their outer walls are heated to 1100–1200 K. The
48 tubes operate in the creep regime by design, and their remaining life is the
49 single most important maintenance variable of the plant: a tube failure forces
50 an unplanned shutdown, retubing costs about a tenth of the installed plant
51 cost [2], and service life varies between 30 000 and 180 000 h with material
52 quality and operating conditions [3]. Tube life is governed almost entirely
53 by the outer-wall temperature at the hottest elevation, because the rupture
54 time roughly halves for every 10–20 K of additional metal temperature [2, 4];
55 the rupture curve used here halves the life every 13 K at the stress of the
56 calibrated tube.

57 Operating decisions therefore trade hydrogen production, fuel consump-
58 tion and tube life against each other, but the trade-off is rarely quantified:

59 plants are run against a maximum tube-wall temperature limit read from py-
 60 rometer surveys, and the effect of a load, steam-to-carbon or burner change
 61 on tube life is left to experience. Two developments make a quantitative
 62 approach both necessary and possible. Hydrogen plants are increasingly
 63 expected to follow variable downstream demand or to operate alongside in-
 64 termittent electrolytic hydrogen, which raises the question of what tube life
 65 flexible operation costs; and validated models of the tube [2, 5–7] and fur-
 66 nace [8, 9] exist, surrogates make them fast enough for hourly simulation
 67 and optimization [10–13], and rupture data for the relevant alloys are docu-
 68 mented in public data sheets and manufacturers’ design curves [14, 15, 24].
 69 What is missing is a coupled, calibrated and uncertainty-aware chain from
 70 operating inputs to tube life, built entirely on published data and open code,
 71 so that its conclusions can be checked and its data replaced.

72 *1.1. Previous work*

73 The reformer tube has been modeled at every level of complexity. Xu
 74 and Froment [5] established the Langmuir–Hinshelwood–Hougen–Watson ki-
 75 netics of methane steam reforming and water-gas shift on a Ni/MgAl₂O₄
 76 catalyst that remains the standard intrinsic model, and in the compan-
 77 ion paper [6] simulated an industrial tube with a one-dimensional hetero-
 78 geneous model. The tube has since been coupled to a zone model of the
 79 furnace [8], to a unified top-fired model with three-dimensional zonal anal-
 80 ysis [9] and to a dynamic heterogeneous formulation [7]. Latham and co-
 81 workers [2, 17] calibrated a Hottel zone-method model of a top-fired box
 82 reformer on plant measurements including infrared tube-wall temperature
 83 surveys, and published the operating points and absolute tube-wall temper-

atures in the thesis appendix [17]; that data set is the basis of the present calibration. Computational-fluid-dynamics models of the furnace [18–20] resolve the temperature field but are used to balance tube temperatures rather than to quantify life, and the data-driven work of the last decade — furnace-balancing and smart-manufacturing frameworks [10, 19, 20], CFD-trained machine-learning surrogates [11, 13] and uncertainty-aware production optimization [12] — addresses production and efficiency: tube life, when it appears, enters as a constraint on a maximum temperature rather than as an objective with a quantified cost, and the uncertainty in kinetics, heat transfer and creep data is not propagated to the conclusions.

On the materials side, the creep behavior of the 25Cr–20Ni (HK40) and 25Cr–35Ni–Nb (HP-Nb) families of centrifugally cast tube alloys is characterized in the long-term data sheets of the National Institute for Materials Science [14, 15, 21] and in remaining-life studies of service-exposed tubes [3, 22, 23]. Yeh [24] combined a computed tube-wall temperature with a manufacturer’s Larson–Miller curve for a proprietary HP-Nb alloy to estimate life, and showed that evaluating the life at the average instead of the maximum tube temperature overstates it by two orders of magnitude. The Larson–Miller parameter [25] and the linear life-fraction rule of Robinson [26] remain the basis of design codes such as API 530 [4].

1.2. Contribution and research questions

This paper presents a physics-informed digital twin of an industrial top-fired SMR linking operating inputs to tube creep life through the module chain of Fig. 1, verified against Xu and Froment [6], calibrated on the plant data of Latham [17], and produced throughout by a versioned open pipeline

109 from published data. Four research questions are answered:

110 **RQ1** Which operating variables govern the hot-spot temperature and the
111 creep-life consumption of the tube, and how do they interact?

112 **RQ2** What is the tube-life cost, per unit of hydrogen produced, of flexible
113 operation (load-following, renewable-following, over-firing events) and
114 of catalyst aging, relative to steady operation?

115 **RQ3** Which operating regimes are Pareto-optimal in hydrogen production,
116 fuel consumption and life consumption, and how does the answer de-
117 pend on how steam is charged?

118 **RQ4** How uncertain are these answers, which uncertainty sources dominate,
119 and which conclusions survive the uncertainty?

120 **2. Methods**

121 The twin is implemented as a Python package (`rdt`) whose modules follow
122 the chain of Fig. 1b. All physical data (kinetic parameters, plant operating
123 points, creep curves) are read from annotated YAML and CSV files; no
124 number is hard-coded in the model code. Thermodynamic properties, heat
125 capacities and reaction equilibrium constants are taken from Cantera [27]
126 with the GRI-Mech 3.0 species data, so that kinetics and energy balance are
127 mutually consistent.

128 *2.1. Reactor tube model*

129 The tube is described by a steady one-dimensional pseudo-homogeneous
130 plug-flow model with axial coordinate z from the inlet (top) to the outlet.

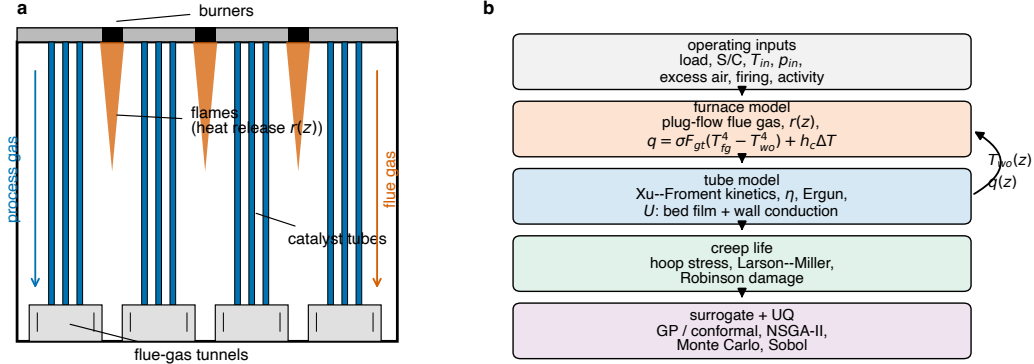


Figure 1: (a) Cross-section of a top-fired box reformer: burners in the roof between rows of catalyst tubes, flames releasing heat in the upper part of the firebox, flue gas flowing downward co-currently with the process gas and leaving through tunnels at the floor. (b) Module chain of the digital twin: operating inputs are mapped through the furnace and tube models, which exchange the outer-wall temperature profile and the heat flux, to the creep-life module; surrogates and uncertainty quantification wrap the chain.

131 The state consists of the molar flows F_i of CH_4 , H_2O , H_2 , CO , CO_2 and N_2 ,
 132 the process-gas temperature T and the pressure p . The intrinsic kinetics are
 133 those of Xu and Froment [5] for steam reforming (r_1), water-gas shift (r_2)
 134 and overall reforming to CO_2 (r_3):

$$r_1 = \frac{k_1}{p_{\text{H}_2}^{2.5}} \frac{p_{\text{CH}_4} p_{\text{H}_2\text{O}} - p_{\text{H}_2}^3 p_{\text{CO}} / K_1}{\text{DEN}^2}, \quad (1)$$

$$r_2 = \frac{k_2}{p_{\text{H}_2}} \frac{p_{\text{CO}} p_{\text{H}_2\text{O}} - p_{\text{H}_2} p_{\text{CO}_2} / K_2}{\text{DEN}^2}, \quad (2)$$

$$r_3 = \frac{k_3}{p_{\text{H}_2}^{3.5}} \frac{p_{\text{CH}_4} p_{\text{H}_2\text{O}}^2 - p_{\text{H}_2}^4 p_{\text{CO}_2} / K_3}{\text{DEN}^2}, \quad (3)$$

$$\text{DEN} = 1 + K_{\text{CO}} p_{\text{CO}} + K_{\text{H}_2} p_{\text{H}_2} + K_{\text{CH}_4} p_{\text{CH}_4} + K_{\text{H}_2\text{O}} p_{\text{H}_2\text{O}} / p_{\text{H}_2}, \quad (4)$$

135 with partial pressures in bar. The rate coefficients k_j and adsorption con-
 136 stants K_i follow the Arrhenius and van't Hoff forms with the activation en-

ergies, adsorption enthalpies and reference values of Table 5 of [5], reparameterised at the reference temperatures 648 K and 823 K used in that table so that the reported confidence intervals can be propagated directly (Section 2.7). The equilibrium constants K_1 – K_3 are computed from Gibbs energies of formation rather than from fitted expressions, which removes a source of inconsistency with the energy balance (Section S1).

The balances per tube are

$$\frac{dF_i}{dz} = A_{cs} \rho_b \sum_j \nu_{ij} \eta_j r_j, \quad (5)$$

$$\sum_i F_i c_{p,i} \frac{dT}{dz} = \pi d_i U (T_{wo}(z) - T) - A_{cs} \rho_b \sum_j \eta_j r_j \Delta H_j(T), \quad (6)$$

$$-\frac{dp}{dz} = \frac{1-\phi}{\phi^3} \left(1.75 + 150 \frac{1-\phi}{Re_p} \right) \frac{\rho_g v_s^2}{d_p}, \quad (7)$$

where A_{cs} is the cross-section, ρ_b the bed density, η_j the effectiveness factors, ϕ the bed voidage, d_p the equivalent particle diameter and Re_p the particle Reynolds number; Eq. (7) is the Ergun equation [28]. Rather than solving the pellet problem, constant effectiveness factors $\eta_j = 0.05$ in the first tenth of the tube and 0.1 thereafter are used, and higher alkanes in the feed (C_2 – C_5) are converted to CO and CH_4 at the inlet; both follow Latham et al. [2] and are set out in Section S1.

The overall heat-transfer coefficient referred to the inner surface combines the bed-side film coefficient α_i and the conduction through the tube wall,

$$\frac{1}{U} = \frac{1}{\alpha_i} + \frac{d_i}{2\lambda_t} \ln \frac{d_o}{d_i}, \quad T_{wi} = T_{wo} - q_o'' \frac{d_o}{2\lambda_t} \ln \frac{d_o}{d_i}, \quad (8)$$

with the tube conductivity $\lambda_t = 29.6 \text{ W m}^{-1} \text{ K}^{-1}$ of [17]. The film coefficient uses the Leva–Grummer correlation [30] in the form written by Latham et

al. [2], multiplied by a heat-transfer factor f_{htg} that is estimated from plant data (Section 2.5). The alternative chain of Xu and Froment [6], based on De Wasch and Froment [31] and Yagi and Kunii [32], is implemented as an option and discussed in Section 3.1. Equations (5)–(7) are integrated for a prescribed outer-wall profile $T_{\text{wo}}(z)$ (stand-alone mode) or as part of the coupled system below.

2.2. Furnace model and coupling

The furnace is a top-fired box with rows of burners in the roof between rows of tubes (Fig. 1a; the reference geometry has 7 rows of 48 tubes and 8 rows of 12 burners [2]). Instead of the zone method of Hottel and Sarofim [33] used by Plehiers and Froment [8] and Latham et al. [2], we use a one-dimensional long-furnace model in the sense of Roesler [34]: the flue gas is a plug flow travelling downward co-currently with the process gas, and the gas–tube radiative exchange is lumped into one effective exchange factor F_{gt} . Per unit height z (zero at the roof),

$$\dot{n}_{\text{fg}} c_{p,\text{fg}} \frac{dT_{\text{fg}}}{dz} = r(z) - q(z) \pi d_o N_t, \quad (9)$$

$$q(z) = \sigma F_{\text{gt}} (T_{\text{fg}}^4 - T_{\text{wo}}^4) + h_c (T_{\text{fg}} - T_{\text{wo}}), \quad (10)$$

$$q(z) = U (T_{\text{wo}} - T) \frac{d_i}{d_o}, \quad (11)$$

where N_t is the number of tubes, q the flux per unit outer tube area and h_c a furnace-side convective coefficient, which at furnace-gas temperatures is a minor correction to the radiative flux. The heat-release density $r(z)$ is a downward-opening parabola that vanishes at $z = L_q L$, with the dimensionless flame length L_q and the top-zone release fraction α_{top} as calibration

parameters. Because a pure plug flow starting from the mixed fuel–air inlet temperature would give an unphysical cold region before the first heat release, the top zone is treated as well mixed: the fraction α_{top} of the heat is released instantly at the roof. The release profile, the convective coefficient and the combustion calculation are given in Section S1.

Equations (10) and (11) close the system in T_{wo} at every z , so that furnace and tube are integrated together in one downward sweep (Section S1). The global energy closure of the coupled solution is verified to 10^{-5} of the combustion heat, and one coupled operating point takes about 0.3 s on a laptop.

2.3. Tube wall and creep life

The creep-life module converts the outer-wall temperature profile into a life estimate. The hoop stress is computed from the mean-diameter formula of API 530 [4], $\sigma_h = p(d_o - t)/(2t)$ with wall thickness t , at the process-gas pressure of each elevation; the thin-wall and Lamé variants differ from it by less than 12 % at the geometry used ($d_o = 146$ mm, $t = 15$ mm, 28 bar: 10.8, 12.2 and 12.4 MPa respectively). The wall thickness is not given by Latham; it is taken as 15 mm, consistent with the 15.3 mm wall of the industrial tube of Xu and Froment [6], and varied between 12 and 18 mm in the uncertainty analysis. The temperature entering the life calculation is the outer-wall temperature, which is conservative with respect to the mid-wall temperature; the difference is shown in Fig. 4.

The rupture time follows the Larson–Miller parameter [25],

$$\text{LMP} = 10^{-3} T (C + \log_{10} t_r), \quad \log_{10} \sigma = P_3(\text{LMP}), \quad (12)$$

198 with T in K, t_r in h and $C = 18.6$, the constant printed on the Centralloy G
 199 4852 data sheet, and P_3 a cubic master curve fitted separately to the Average
 200 and to the Lower Scatter Band curves of that sheet (Section 2.4). The sheet
 201 states the lower band as a 95 % confidence level, so the pair defines the scat-
 202 ter directly rather than by assumption: the median horizontal separation of
 203 the two curves at 1147 K is 0.298 decades of rupture time, a standard devi-
 204 ation of 0.181 decades on $\log_{10} t_r$. The three sheets do not share a constant
 205 ($C = 18.6$ for G 4852, 22.9 for G 4852 Micro, 19.3 for ET 45 Micro), so the
 206 constant must be taken from the sheet whose curve is used. Damage under
 207 a piecewise-constant history is accumulated with the linear life-fraction rule
 208 of Robinson [26], $D = \sum_k \Delta t_k / t_r(T_k, \sigma_k)$, and rupture is predicted at $D = 1$.
 209 Life is reported throughout as a consumption rate $1/t_r$ at the hot spot, or as
 210 damage per kmol of hydrogen relative to the calibrated base case, because
 211 ratios depend on the local slope of the master curve rather than on its ab-
 212 solute position; Section 3.5 shows on four curves that they are indeed far
 213 more stable than absolute lives. The rupture time so obtained is that of one
 214 average tube; the extension to the tube population is given in Section S10.

215 2.4. Data

216 *Verification data.* The industrial simulation of Xu and Froment [6] (Fig. 3 of
 217 that paper) provides axial profiles of methane and CO₂ conversion, process-
 218 gas, inner-wall and outer-wall temperatures and pressure for one operating
 219 point with the feed of their Table 2 (520 °C, 29 bar, steam-to-carbon 3.36,
 220 tube 0.1016 m inner and 0.1322 m outer diameter, 11.12 m heated length).
 221 The curves were digitized with WebPlotDigitizer with 120–260 points per
 222 curve and separate axis calibrations for conversion, pressure and temperature;

the calibration resolution is about 2 K and 0.005 in conversion. The data are stored as tidy CSV files with their metadata (Section S4 of the Supplementary material). The outer-wall curve serves as the boundary condition and the remaining curves as targets.

Plant data. Latham [17] reports, in Appendix H, four operating points of an industrial top-fired reformer (Plants A, B and two states of Plant C) with inlet conditions, feed and fuel compositions, outlet temperature and composition, flue-gas outlet temperature and the tube-wall temperatures measured by infrared pyrometer at two peep-hole elevations (3.66 and 8.53 m from the top of the 12.5 m heated length). Table 1 lists the cases. The instrument uncertainties stated in the thesis, 2 K for the outlet temperature, 3 K for the wall temperatures and 8 K for the flue gas, are treated as one-sigma weights in the calibration; the standard deviation of the wall temperature across the tube population at a given elevation is much larger, 15–22 K in the journal version of the data [2], and is used to interpret the residuals. Plant C1 is excluded from calibration because its feed flow is inconsistent with the other cases (it equals the reported combustion-air flow to four digits and exceeds the Plant A feed by 22 % at a lower plant rate), which we attribute to a transcription error in the source. The excess air of each case is derived from the reported fuel, off-gas and air flows and is 21.6 % for Plant A.

Creep data. The master curve is taken from the published material data sheets of Schmidt + Clemens for three centrifugally cast reformer alloys: Centralloy G 4852 (HP-Nb, the base case), G 4852 Micro (an HP micro-alloy) and ET 45 Micro (a 45Ni–35Cr grade, included as the high-alloy end

247 member; it is not an HK40 equivalent). Each sheet prints a parametric stress-
 248 rupture chart with an Average and a Lower Scatter Band curve over roughly
 249 1–100 MPa, so the hoop stress of the calibrated tube lies inside the plotted
 250 range rather than in extrapolation. Both curves of each sheet were extracted
 251 by an automated routine, from the vector paths where the chart is vector
 252 and by colour tracing of a 600 dpi rendering otherwise; the two independent
 253 paths agree to 0.06 % median and 1.6 % worst case over the six curves. The
 254 sheets themselves are not redistributed: the repository holds the extracted
 255 points, the fitted coefficients and the extraction script. The ingestion routine
 256 was validated on a synthetic data set with a known constant and scatter, re-
 257 covered to 0.17 % and 6.4 % respectively. They describe the manufacturer’s
 258 qualification population, not the heat-to-heat spread of the tubes in a partic-
 259 ular furnace, and the alloy of the reference plant is not stated. Rupture data
 260 resolved by heat, such as the long-term data sheets of the National Institute
 261 for Materials Science for the HK40 and HP40 alloys [14, 15], remain the nat-
 262 ural reference for heat-to-heat statistics, but they are served for interactive
 263 viewing only and their terms of use prohibit the assembly of consolidated
 264 data sets [16]; rupture points tabulated in the open literature [21, 22] are the
 265 accessible alternative.

266 2.5. Calibration and cross-validation

267 Four parameters of the coupled model cannot be taken from the literature:
 268 the exchange factor F_{gt} , the flame length L_q , the top-zone release fraction
 269 α_{top} and the heat-transfer factor f_{htg} . They are estimated by weighted non-
 270 linear least squares on the three plant cases against nine residuals per case,
 271 each scaled by its measurement uncertainty; the residual set, the optimizer,

the multi-start procedure and the covariance estimate are given in Section S1. Predictive performance is assessed by leave-one-case-out cross-validation: the parameters are refitted on two cases and the held-out case is predicted. The four-parameter fit places α_{top} at its bound with a correlation of 0.985 to L_q , so the adopted configuration fixes $\alpha_{\text{top}} = 0.182$, the value fitted by Latham et al. [2] to the same furnace with the zone method, and estimates the remaining three; the increase in χ^2 is reported in Section 3.1.

2.6. Surrogates and conformal prediction

The coupled model takes about 0.3 s per operating point, which is adequate for calibration and sensitivity analysis but not for hourly annual histories, evolutionary optimization or Monte Carlo over histories. Surrogates are trained on a Latin-hypercube design of 2000 points over the seven operating inputs (Table S1) for eight outputs, and the model with the lowest five-fold cross-validated error is selected per target and evaluated on an independent Saltelli design of 4096 points. The targets, the three model families compared, their hyperparameters and the two physics-derived features are given in Section S3. Prediction intervals are obtained by the cross-conformal (CV+) method [37] as implemented in MAPIE [38], which provides finite-sample marginal coverage without a distributional assumption; the Gaussian-process native intervals are reported for comparison.

2.7. Sensitivity, scenarios, optimization and uncertainty propagation

RQ1. Global sensitivity uses the variance-based Sobol indices [39] estimated with SALib [40] on the Saltelli design evaluated with the physics model, together with an open-loop Latin-hypercube campaign and a closed-loop grid

296 in steam-to-carbon ratio and load in which the firing is solved so that the
297 outlet temperature equals the Plant A value (1105.55 K).

298 *RQ2.* Annual histories of 8760 hourly quasi-steady states are evaluated through
299 the surrogates, with every 24th hour and every hour outside the training
300 bounds re-evaluated by the physics model. Two control modes are repre-
301 sented by inverting the surrogates for the firing factor with a vectorised bi-
302 section: holding the outlet temperature at its base value, or holding the dry
303 methane slip. Six scenarios cover steady operation, daily and renewable-
304 following load variation, over-firing events, four years of catalyst aging under
305 each control mode, and two steam-to-carbon settings; their definitions are
306 given in Table S2. Damage is accumulated hourly by Eq. (12) and Robin-
307 son’s rule, and each scenario is also evaluated at its annual-mean inputs to
308 quantify the error of a steady-state assessment. Start-up and shutdown tran-
309 sients, thermal fatigue and creep–fatigue interaction are outside the scope.

310 *RQ3.* The non-dominated sorting genetic algorithm NSGA-II [41] in py-
311 moo [42] maximizes net hydrogen per tube and minimizes firebox fuel per
312 kmol H₂ and life consumption per kmol H₂ over five decision variables (load,
313 steam-to-carbon ratio, inlet temperature, excess air, firing) subject to a
314 methane slip not above the base value, a hot-spot temperature not above
315 1193 K and an outlet temperature not above 1125 K, using the Gaussian-
316 process surrogates (population 200, 300 generations); the basis of the 1193 K
317 limit is given in Section S2. Every Pareto member is re-evaluated with the
318 physics model and the constraints are re-checked. Because firebox fuel per
319 kmol H₂ ignores the cost of raising the additional steam, a steam credit α is
320 introduced: the total fuel counts firebox fuel plus a fraction $(1 - \alpha)$ of the

321 heat needed to raise the process steam and to preheat the dry feed (enthalpy
 322 basis in Section S2), so that $\alpha = 1$ recovers the firebox-only objective and
 323 $\alpha = 0$ charges steam in full. The iso-production front (hydrogen within 1 %
 324 of the base) is recomputed for α from 0 to 1.

325 *RQ4.* Uncertain inputs are grouped into kinetics, heat transfer, creep and
 326 measurement, with the distributions of Table S3; the creep group carries the
 327 scatter of the rupture band, a normal 0.181 decades on $\log_{10} t_r$ measured
 328 as described in Section 2.3. A scrambled Sobol design of 2048 samples is
 329 propagated through the physics model at eight operating points taken from
 330 RQ2 and RQ3; the same sample is used at every point so that ratios between
 331 points are paired. A digitized curve is already a function of the Larson–
 332 Miller parameter, so C enters only the conversion from that parameter to
 333 a rupture time and the polynomial is carried over unchanged. Variance is
 334 decomposed by varying one group at a time (1024 samples per group) and,
 335 independently, by Sobol indices computed on a Gaussian-process surrogate
 336 of the joint sample. Finally, the fraction of paired samples for which each
 337 qualitative conclusion of RQ2 and RQ3 holds is reported, both with the
 338 calibrated flame length and over a sweep of a structural variant in which the
 339 flame length shrinks with load as $L_q \text{load}^p$, for p from 0 to 1; the two ends of
 340 that range are discussed in Section 4.2; the variant is a bound rather than
 341 an expectation, for the reasons set out in Section S2. The complete pipeline
 342 from design to figures runs in 35 minutes on a laptop.

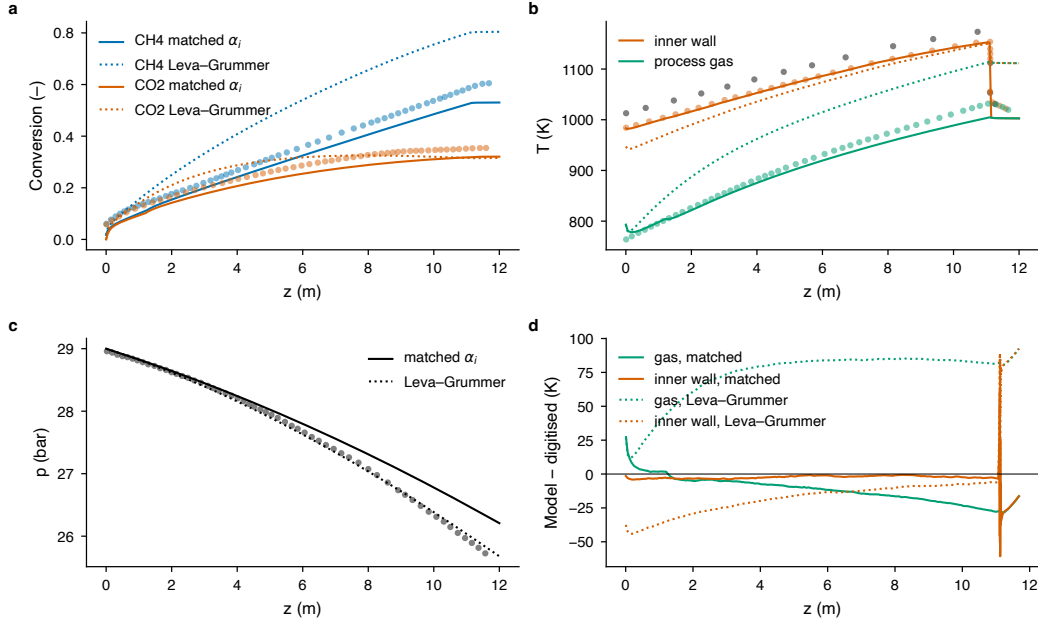


Figure 2: Verification against the digitized industrial case of Xu and Froment [6] (symbols) with the digitized outer-wall temperature as boundary condition: (a) methane and CO₂ conversion, (b) process-gas and inner-wall temperatures, (c) pressure and (d) temperature residuals, for the matched film coefficient (solid lines) and for the Leva-Grummer correlation with $f_{\text{htg}} = 1$ (dotted).

3. Results

3.1. Verification and validation

With the digitized outer-wall temperature prescribed, the response of the tube model is controlled almost entirely by the bed-side film coefficient, and the first finding of the study is that the heat-transfer chain printed in Part II of Xu and Froment [6] does not reproduce their own figure. Evaluated as printed, the De Wasch-Froment wall coefficient with the Yagi-Kunii dynamic terms gives $\alpha_i \approx 3100\text{--}3700 \text{ W m}^{-2} \text{ K}^{-1}$ at the particle Reynolds number

351 of the case ($Re_p \approx 4000$), and the Leva–Grummer correlation gives 940–
 352 $1580 \text{ W m}^{-2} \text{ K}^{-1}$; the value back-calculated from the digitized wall and gas
 353 temperatures and the wall conduction is $348 \text{ W m}^{-2} \text{ K}^{-1}$ (interquartile range
 354 313–363). Used as printed, the correlations overpredict the gas temperature
 355 by 70–115 K and the conversion by 0.14–0.22, an RMSE of 75.4 K and 0.160
 356 against 14.0 K and 0.039 for the adopted configuration (Table S5). Both
 357 dynamic terms are linear in $Re Pr$ and were established for air an order of
 358 magnitude below industrial Reynolds numbers [31, 32], so the extrapolation
 359 drives the effective radial conductivity of the bed to some $50 \text{ W m}^{-1} \text{ K}^{-1}$,
 360 which no measurement supports. A displaced decimal in the printed effective-
 361 conductivity coefficient (0.014 instead of 0.14) would bring the chain to within
 362 30 % of the back-calculated value, but this is a hypothesis rather than a
 363 correction.

364 The Xu–Froment case is therefore used as a verification of the tube model
 365 with a matched film coefficient rather than as a validation of the heat-transfer
 366 correlation. With $\alpha_i = 348 \text{ W m}^{-2} \text{ K}^{-1}$ and Latham’s inlet effectiveness pro-
 367 file, the model reproduces the digitized profiles with an RMSE of 14.0 K
 368 in gas temperature, 16.7 K in inner-wall temperature and 0.015 in the con-
 369 version increment along the tube (Fig. 2, Table S5). The residual offset of
 370 about 0.04 in absolute conversion originates in the first half metre and re-
 371 flects an ambiguity in the digitized inlet that the increment metric removes
 372 (Section S4). This verifies the kinetics, the thermodynamics, the energy bal-
 373 ance and the wall-conduction chain. The pressure RMSE rises from 0.04 bar
 374 with the Leva–Grummer run to 0.25 bar with the matched coefficient, for
 375 the reason given in Section S5.

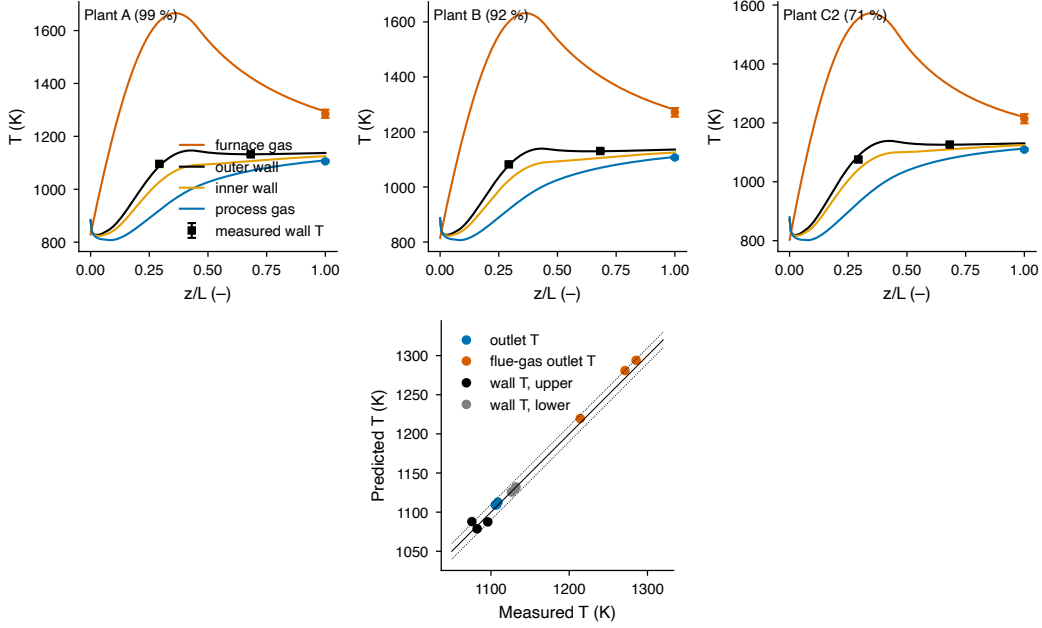


Figure 3: Coupled furnace–tube model after calibration (α_{top} fixed) on the plant cases of Latham [17]: axial profiles of furnace-gas, outer-wall, inner-wall and process-gas temperatures for Plants A, B and C2 with the measured wall temperatures at the two peep-hole elevations, the outlet temperature and the flue-gas outlet temperature (error bars $\pm 1.96\sigma$), and the parity of predicted against measured temperatures (dotted lines ± 10 K).

376 The bed-side coefficient is validated instead on the plant data, where the
 377 furnace model supplies the outer-wall condition and f_{htg} is a free parameter.
 378 Fig. 3, Table 1 and Table S6 summarize the calibration. The adopted fit
 379 (α_{top} fixed) gives $F_{\text{gt}} = 0.323$ [0.309, 0.338], $L_q = 0.456$ [0.434, 0.478] and
 380 $f_{\text{htg}} = 1.83$ [1.617, 2.052] as 95% intervals, a χ^2 of 34.9 on 24 degrees of
 381 freedom (reduced χ^2 1.46), and reproduces the outlet temperatures of all
 382 three cases within 4 K, the lower wall temperatures within 1.1 K and the
 383 upper wall temperatures within 12.2 K. The four-parameter fit lowers χ^2 to
 384 30.5 but is degenerate in L_q and α_{top} (Table S6); fixing α_{top} raises χ^2 by

Table 1: Plant cases of Latham [17] (Appendix H, absolute temperatures) and calibration results: measured inlet and outlet conditions, model errors (predicted minus measured) of the all-cases fit with α_{top} fixed, and leave-one-case-out held-out errors. Plant C1 is excluded from the fit (inconsistent feed flow). Per-tube feed; steam-to-carbon ratio on total hydrocarbon carbon; upper and lower wall temperatures at 3.66 and 8.53 m of 12.5 m.

Case	Rate (%)	T_{in} (K)	p_{in} (bar)	Feed (kmol h^{-1})	S/C	T_{out} (K)	$T_{\text{w,u}}$ (K)	$T_{\text{w,l}}$ (K)	ΔT_{out}	$\Delta T_{\text{w,u}}$	$\Delta T_{\text{w,l}}$	CV $\Delta T_{\text{w,u}}$	CV $\Delta T_{\text{w,l}}$
Plant A	99	884.5	30.06	23.5	2.89	1105.5	1095.9	1132.0	+3.6	-8.4	+0.2	-12.8	+0.7
Plant B	92	887.0	29.44	21.1	2.79	1107.2	1082.3	1130.8	+2.2	-3.6	-1.1	-5.4	-1.7
Plant C1	96	890.9	30.27	28.7	2.85	1122.0	1111.2	1151.5	-	-	-	-	-
Plant C2	71	879.9	28.09	15.9	2.86	1108.9	1075.7	1126.2	+3.9	+12.2	-0.5	+18.2	-0.1

14 %, and the three-parameter fit is adopted for all subsequent work because its parameters are identifiable and its cross-validation folds return nearly the same values (F_{gt} 0.321–0.326, L_q 0.449–0.465, f_{htg} 1.79–1.85). The heat-transfer factor of 1.83 is within 9 % of the 1.68 obtained by Latham et al. [2] with a different furnace model on the same plant, and corresponds to a bed-side coefficient of about $1400 \text{ W m}^{-2} \text{ K}^{-1}$ at mid-height of the Plant A tube, i.e. between the two literature correlations and four times the value that reproduces the Xu–Froment figure; the range $300\text{--}3000 \text{ W m}^{-2} \text{ K}^{-1}$ is the epistemic span carried into the uncertainty analysis through f_{htg} .

Leave-one-case-out cross-validation (last two columns of Table 1) shows that the held-out upper-wall temperature is predicted within 5–18 K and the lower within 2 K. The upper-wall error is systematic: Plant C2, at 71 % rate, is predicted too hot at the upper elevation and Plant A too cold. The upper peep hole lies in the flame zone, where a single parabolic release profile with a load-independent flame length cannot follow the change in flame shape with firing rate. This is the main structural limitation of the furnace model; the residuals are nevertheless within the 15–22 K standard deviation

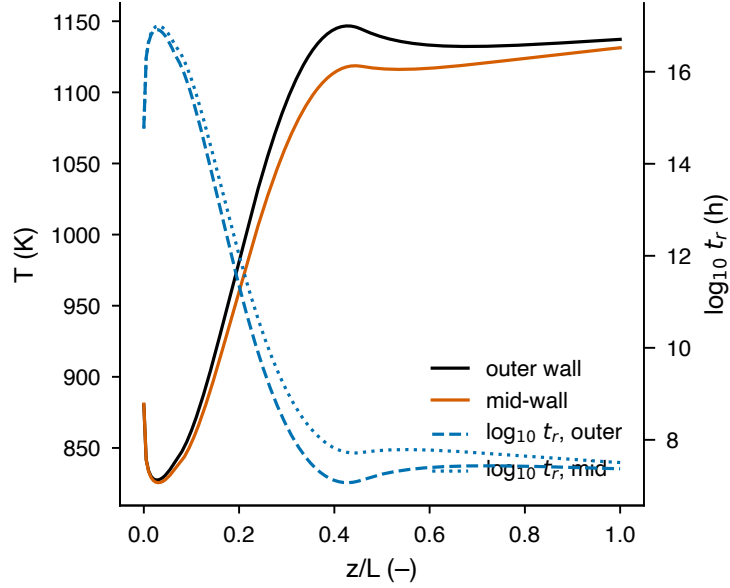


Figure 4: Outer-wall and mid-wall temperature profiles of the calibrated Plant A tube and the corresponding local rupture time from the Centralloy G 4852 lower scatter band at the local hoop stress; the hot spot governs the life.

of the wall temperature across the tube population at that elevation [2]. The consequence for the conclusions is examined in Section 3.5.

Fig. 4 shows the life profile of the calibrated Plant A tube. The hot spot lies at about 0.43 of the heated length, where the outer wall reaches 1147 K at a hoop stress of 12.9 MPa; the rupture time from the lower scatter band is 10^7 h at this point, and evaluating the life at the length-averaged outer-wall temperature instead of at the hot spot overstates it by a factor of about 57. The same effect is reported by Yeh [24], there of the order of two hundred; it is smaller here because the master curve of the present alloy is flatter. The absolute value is not credible as a tube life — the model represents one average tube under creep alone, and the design band of a manufacturer is

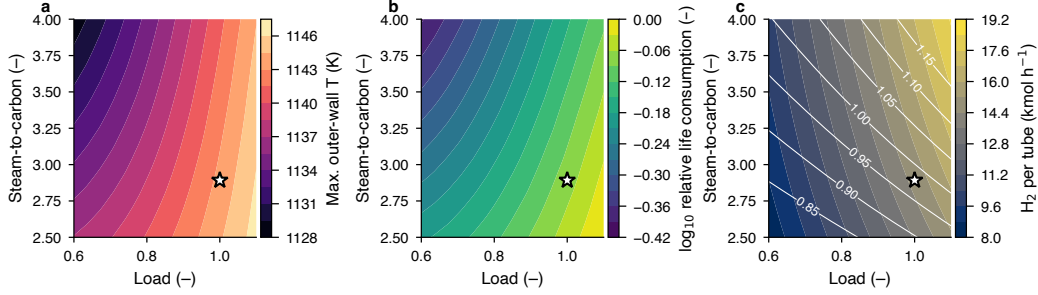


Figure 5: Closed-loop operating maps in load and steam-to-carbon ratio at constant outlet temperature: (a) hot-spot temperature, (b) $\log_{10}$ of the life consumption relative to the base case and (c) net hydrogen per tube with contours of the firing factor required. The star marks the calibrated Plant A base.

not the scatter of an installed tube population — which is why all results below are expressed as ratios.

3.2. RQ1: what governs hot-spot temperature and life

The closed-loop maps (Fig. 5) show the structure of the operating space when the outlet temperature is held by the firing controller. Across the whole grid the hot spot spans only 1128–1146 K. It rises mildly with load: the duty per tube is proportional to the load, and the bed-side coefficient rises almost proportionally with it ($\alpha_i \propto Re^{0.9}$ in the Leva–Grummer correlation), so the film temperature difference is nearly load-independent and only the conduction drop across the wall grows with the flux. It falls with steam-to-carbon ratio because, at the same outlet temperature, the larger process-gas flow raises the bed-side coefficient, the additional steam increases the gas heat capacity, and the equilibrium shift lets the same methane slip be reached with a slightly lower gas temperature, all of which reduce the wall-to-gas temperature difference despite the higher firing needed. The life map (panel b) is

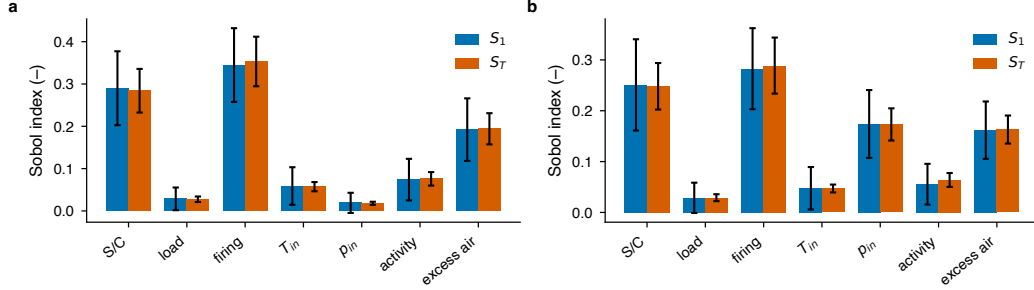


Figure 6: First-order (S_1) and total-effect (S_T) Sobol indices with 95 % confidence intervals for (a) the hot-spot temperature and (b) $\log_{10} t_r$ at the hot spot, from the Saltelli design of Table S8.

the image of the temperature map through the Larson–Miller relation and spans about half a decade across the space. Hydrogen production (panel c) increases with both load and steam-to-carbon ratio, the latter through the shift of equilibrium, at the cost of a higher firing factor.

The Sobol analysis over all seven inputs (Fig. 6, Table S8) ranks the drivers of the hot-spot temperature as the specific firing factor ($S_T = 0.35$), the steam-to-carbon ratio (0.28) and the excess air (0.19), together 82 % of the variance, with the inlet pressure entering $\log_{10} t_r$ at $S_T = 0.17$ through the hoop stress, where it is invisible in the temperature; the remaining indices, the weakness of the interactions and the drivers of the methane slip are given in Section S7.

The surrogates that make the following campaigns possible are summarized in Fig. S1 and Table S4. The Gaussian process is selected for seven of the eight targets, and the physics features improve the hot-spot temperature, outlet temperature and slip. The test RMSE is 0.11 K for the hot-spot temperature and 0.0049 decades for $\log_{10} t_r$, two orders of magnitude below

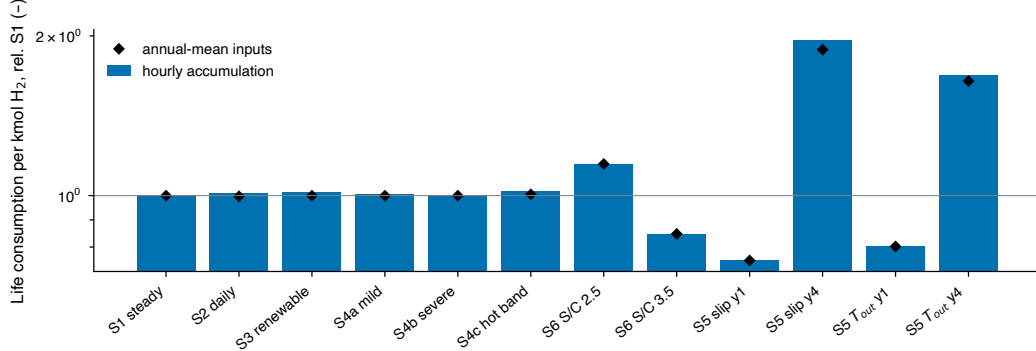


Figure 7: Annual life consumption per kmol of hydrogen relative to the steady base S1 for the RQ2 scenarios, from hourly accumulation (bars) and from a single evaluation at the annual-mean inputs (diamonds).

the calibration residuals, at a speed-up of about 4700 relative to the physics model. The position of the hot spot is not learnable ($R^2 = 0.64$) because it is bimodal, an interior maximum near 0.43 of the length for most inputs and an outlet plateau for others; the plateau appears at high firing, where the process gas has caught up with the wall and the local flux at the outlet is small (Section S11), and it is not needed for the life calculation. The CV+ intervals over-cover: at a nominal level of 0.90 the empirical coverage is 0.94–0.97 for all targets. Over-coverage is expected for CV+, whose guarantee is one-sided, and is conservative; the interval widths are nevertheless small enough (0.25 K for the hot-spot temperature) that surrogate error is immaterial to the conclusions.

3.3. RQ2: life cost of flexible operation and aging

Table 2 and Fig. 7 answer RQ2 for one year of operation at the calibrated base. Under the outlet-temperature controller, load-following is life-neutral: the daily profile (S2) and the renewable-following profile (S3) consume 1.010

Table 2: RQ2 scenario summary for one year of the Plant A twin at the calibrated excess air: hydrogen per tube, Robinson damage D , life consumption per kmol H_2 relative to S1, ratio of the annual-mean-condition damage estimate to the hourly-accumulated damage, mean and maximum hot-spot temperature and mean firing factor. Life uses the Centralloy G 4852 lower scatter band ($C = 18.6$).

Scenario	H_2 (10^3 kmol)	D (-)	Rel. life cost	Avg.-cond. ratio	$T_{wo,max}$ (K)	max $T_{wo,max}$ (K)	Firing
S1 steady base	128.5	6.30×10^{-4}	1.000	1.000	1143	1143	0.978
S2 daily load-following	115.7	5.72×10^{-4}	1.010	0.987	1141	1143	0.944
S3 renewable-following	109.7	5.44×10^{-4}	1.013	0.987	1140	1146	0.927
S4a mild over-firing (48 h)	128.6	6.34×10^{-4}	1.006	0.994	1144	1157	0.979
S4b severe over-firing (6 h)	128.5	6.32×10^{-4}	1.003	0.997	1143	1179	0.978
S4c hot band +40 K (24 h)	128.5	6.41×10^{-4}	1.018	0.988	1144	1183	0.978
S6 steam-to-carbon 2.5	119.9	6.74×10^{-4}	1.147	1.000	1144	1144	0.897
S6 steam-to-carbon 3.5	139.8	5.80×10^{-4}	0.847	1.000	1142	1142	1.092
S5 aging, hold slip, year 1	128.5	4.77×10^{-4}	0.756	0.998	1138	1139	0.974
S5 aging, hold slip, year 4	128.5	1.23×10^{-3}	1.959	0.961	1156	1164	0.989
S5 aging, hold T_{out} , year 1	129.0	5.08×10^{-4}	0.803	0.999	1139	1140	0.982
S5 aging, hold T_{out} , year 4	127.4	1.05×10^{-3}	1.686	0.975	1153	1159	0.969

and 1.013 of the S1 life per kmol H_2 . Two effects nearly cancel. The hot-spot temperature falls with load at constant outlet temperature (Fig. 5a), so the hours at reduced load save life, while the hours at overload cost it; which one wins is decided by the local slope of the master curve, and the margin is smaller than the uncertainty on that slope. The statement that S2 costs no more than S1 holds in 0.43 of the Monte Carlo samples (Table 5) and its sign changes with the alloy (Section 3.5), so the defensible statement is that smooth load variation changes the life cost per kmol by less than 2 % in either direction and that the sign is not resolved. Hydrogen output falls by 10 % and 15 % respectively, so the absolute annual damage falls in proportion. A steady-state assessment at the annual-mean inputs reproduces the hourly accumulation within 2 % for every scenario without discrete events (ratio 0.987 for S3), which means that the non-linearity of the Larson–Miller

472 relation is not strong enough over this load range to make time-resolved sim-
 473 ulation necessary for smooth load changes. The conclusion is conditional on
 474 the controller: without outlet-temperature (or slip) control, a load reduction
 475 at unchanged firing raises the hot spot sharply, and the open-loop design
 476 shows life-consumption ratios of up to 40 times the base when high firing co-
 477 incides with a hot inlet; the operating discipline of controlling on the outlet
 478 is itself the main protection of the tubes.

479 Discrete over-firing events are different in kind. During a mild event
 480 (+10% firing) the damage rate is 2.1 times the base rate, during a severe
 481 event (+25%) it is 4.9 times, and a 40 K hot band raises it by a factor
 482 of 7.4; but because the events are short, their share of the annual damage
 483 is 0.3–1.7% and the annual life cost per kmol rises by at most 2%. The
 484 annual-mean evaluation underestimates the event scenarios (diamonds below
 485 bars in Fig. 7), as it must for a convex damage law, but the error is small at
 486 these event frequencies. The steam-to-carbon ratio has a larger steady effect:
 487 operating at 2.5 costs 1.15 and at 3.5 costs 0.85 of the S1 life per kmol H₂,
 488 because the higher ratio both cools the hot spot and raises the hydrogen
 489 yield.

490 Catalyst aging dominates every operational effect. With the activity
 491 falling from 0.30 to 0.10 over four years, a range that brackets the mid-
 492 campaign value of 0.20 fitted to the plant and is consistent with the rapid
 493 initial deactivation followed by a slow decline observed for fresh catalyst [5]
 494 and with the four-year catalyst life of the reference plant [2], and with the
 495 controller holding the methane slip, the life cost per kmol H₂ rises from 0.76
 496 in the first year (fresh catalyst) to 1.96 in the fourth as the hot spot climbs

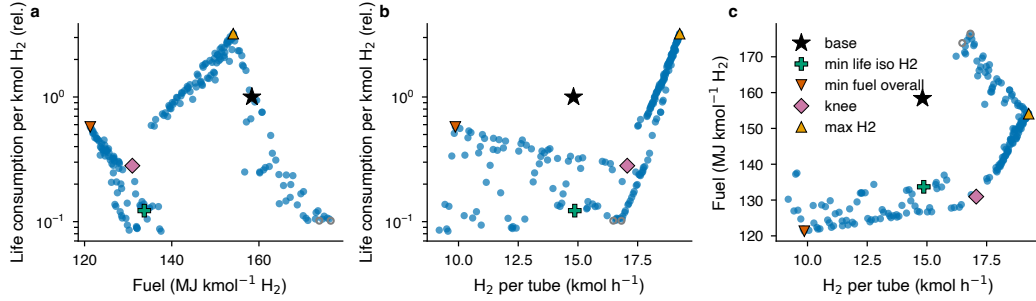


Figure 8: Physics-verified NSGA-II Pareto set in (a) firebox fuel per kmol H₂ against life consumption per kmol H₂, (b) net hydrogen per tube against life consumption and (c) hydrogen against fuel; open circles are members infeasible under the physics model, and the marked regimes are listed in Table 3.

from 1138 to 1164 K; holding the outlet temperature instead gives 1.69 in the fourth year because the slip is allowed to rise. Over the campaign the life consumed in year 4 is two and a half times that in year 1, and the question of when to change the catalyst is therefore also a tube-life question. The ranking here is by creep-life cost alone. Rainflow counting of the hourly wall-gradient histories (Section S11) shows a year of daily load-following matching one start-up and shutdown only for a fatigue exponent below about 4.2, against the two to six cool-downs a plant undergoes each year; thermal cycling does not overturn the ranking, although creep-fatigue interaction remains outside the model.

3.4. RQ3: Pareto-optimal regimes and the steam credit

The Pareto set (Fig. 8, Table 3) contains 200 members, of which 198 remain feasible under the physics model; the maximum discrepancy between surrogate and physics on the set is 0.03 in relative life and below 0.1 MJ kmol⁻¹ in fuel. The calibrated base is dominated by 37 members.

Table 3: RQ3 representative regimes, physics-verified, from the NSGA-II Pareto set. Fuel is firebox fuel per kmol H_2 ; life is the consumption rate per kmol H_2 relative to the base (G 4852 lower scatter band).

Regime	Load	S/C	T_{in} (K)	Excess air (%)	Firing	H_2 (kmol h^{-1})	Fuel (MJ kmol $^{-1}$)	Rel. life cost	$T_{\text{wo,max}}$ (K)	CH_4 slip (%)
base	1.00	2.89	885	21.6	1.000	14.82	158.4	1.000	1147	7.81
min life, iso- H_2	0.97	4.00	897	17.6	0.872	14.87	133.7	0.123	1108	7.80
knee	1.10	4.00	893	5.4	0.866	17.06	131.0	0.281	1127	7.42
max H_2	1.10	4.00	900	5.0	1.150	19.26	154.1	3.220	1177	3.89
min fuel overall	0.60	4.00	900	5.0	0.850	9.87	121.3	0.575	1128	5.72
min life overall	0.62	4.00	823	24.5	0.897	9.56	137.5	0.084	1092	7.80

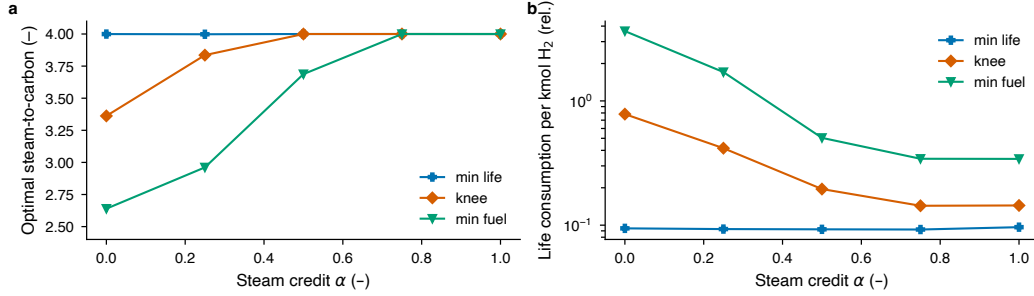


Figure 9: Iso-production front as a function of the steam credit α : (a) optimal steam-to-carbon ratio and (b) life consumption per kmol H_2 relative to the base for the minimum-life, knee and minimum-fuel regimes. The full sweep is given in Table S7.

512 The knee of the front raises hydrogen by +15 % while cutting fuel per kmol
513 by -17% and life consumption per kmol to 0.28 of the base; it does so by
514 running at 110 % load with the minimum excess air, a high inlet temperature
515 and a lower firing factor. At constant production the life cost falls to 0.12 of
516 the base, an eightfold reduction obtained purely by reducing the firing and
517 letting the hot spot fall from 1147 to 1108 K, at -16% fuel. The maximum-
518 hydrogen corner (+30 %) costs 3.2 times the base life per kmol and runs close
519 to the wall-temperature limit.

520 Every member of the front sits at the upper bound of the steam-to-carbon
521 ratio (3.96–4.00). This is an artefact of the objective: with firebox fuel alone,

522 additional steam is free, and the equilibrium shift and the cooling of the hot
 523 spot both favor maximum steam. The steam-credit sweep (Fig. 9, Table S7)
 524 shows how the answer changes when steam raising and feed preheat are
 525 charged. With steam fully charged ($\alpha = 0$) the minimum-fuel regime moves
 526 to a steam-to-carbon ratio of 2.64 and the knee to 3.4, while the minimum-
 527 life regime stays at 4.0 but now costs +4.1 % more total fuel than the base
 528 for a life cost of 0.094. For $\alpha \geq 0.75$ the ratio of 4.0 is optimal for all three
 529 regimes, and already at $\alpha = 0.5$ the minimum-fuel regime sits at 3.7, close to
 530 the bound. In a hydrogen plant the process steam is raised in the waste-heat
 531 boiler on the reformer effluent and in the flue-gas convection section, and the
 532 surplus is exported, so the marginal steam for a higher ratio mostly displaces
 533 export steam rather than requiring extra fuel; this corresponds to α between
 534 about 0.5 and 1 depending on the value the site attaches to export steam,
 535 and places most plants in the region where tube life and fuel economy pull
 536 in the same direction. The plant's own steam balance, not the reformer,
 537 therefore decides whether running steam-rich is a life-saving measure or a
 538 fuel penalty, and the twin makes the dependence explicit.

539 3.5. *RQ4: uncertainty and robustness*

540 Table 4 and Fig. 10 give the propagated uncertainty. At the base point the
 541 90 % interval of the hot-spot temperature is 42 K wide and that of $\log_{10} t_r$
 542 spans 5.94–8.20, i.e. a factor of about 180 in absolute rupture time. The
 543 paired ratios are much tighter: the knee regime costs 0.21–0.56 of the base
 544 life per kmol and the fourth aging year 1.7–6.2 times, so the ranking of
 545 regimes survives an uncertainty that makes the absolute life meaningless.
 546 The nominal result lies inside the 90 % interval at every point, and the end-

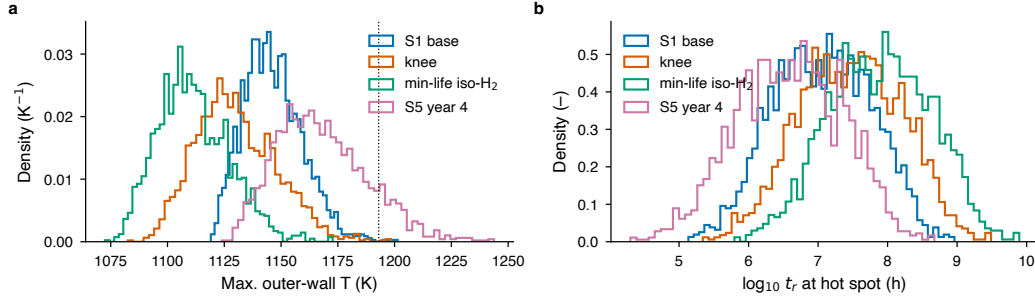


Figure 10: Monte Carlo distributions of all uncertainty groups through the physics model: (a) the hot-spot temperature, with the design limit, and (b) $\log_{10} t_r$ at the hot spot, at the S1 base, the RQ3 knee, the iso-H₂ minimum-life regime and the end of the fourth aging year.

of-campaign hot spot exceeds the 1193 K limit in about 8 % of the samples.

The variance decomposition (Fig. S2, Table S9) attributes 86 % of the variance of $\log_{10} t_r$ to the creep group, dominated by the scatter of the rupture band and the Larson–Miller constant, 9 % to the kinetics, 3 % to the wall-temperature measurement and 2 % to the calibrated heat-transfer parameters. For the hot-spot temperature the kinetics group dominates (51 %), followed by the measurement offset and the wall thickness; that decomposition is identical to every printed digit on all four rupture curves tested, because the alloy enters the thermal problem only through the wall thickness and the tube conductivity. The one-at-a-time shares sum to within 0.04 of one and the Sobol total effects on the surrogate confirm the ranking, so the groups act almost additively.

The robustness fractions (Table 5) state which conclusions hold across the joint uncertainty. That the knee regime halves the life cost holds in 0.89 of the samples, that steam-to-carbon 3.5 is cheaper in life than 2.5 in

Table 4: RQ4 Monte Carlo (scrambled Sobol design, all uncertainty groups) through the physics model: median and 5–95 % interval of the hot-spot temperature, of $\log_{10} t_r$ and of the paired life consumption per kmol H_2 relative to the base.

Operating point	$T_{\text{wo,max}}$ (K)	$\log_{10} t_r$ (h)	Rel. life cost
S1 base	1145 [1127, 1169]	7.06 [5.94, 8.20]	1.000 (paired)
RQ3 knee	1128 [1103, 1161]	7.47 [6.26, 8.63]	0.329 [0.213, 0.561]
RQ3 min-life, iso- H_2	1110 [1088, 1138]	7.90 [6.69, 9.06]	0.143 [0.107, 0.212]
S5 year 4, hold slip	1165 [1138, 1203]	6.60 [5.34, 7.79]	2.823 [1.657, 6.242]
S/C 2.5	1146 [1129, 1166]	7.03 [5.93, 8.18]	1.140 [0.941, 1.315]
S/C 3.5	1144 [1127, 1172]	7.11 [5.94, 8.25]	0.857 [0.623, 1.083]
load 0.70	1138 [1123, 1156]	7.20 [6.09, 8.34]	1.034 [0.732, 1.384]
load 0.85	1141 [1124, 1162]	7.13 [6.02, 8.28]	0.989 [0.841, 1.170]

0.86, and that the fourth aging year costs more than twice the S1 life per kmol in 0.82; repeating the analysis on the other three curves leaves all three between 0.82 and 0.94, so they are properties of the process rather than of the alloy. The flexibility statements are different in kind. At the calibrated flame length they already hold in fewer than half of the samples, 0.43 and 0.48, and Table 5 shows how quickly that support goes: an exponent of 0.1, barely distinguishable from a constant flame length, cuts both by a third; by 0.3 they are 0.03 and 0.06, and at 0.5 neither survives. The material conclusions are untouched across the range — the knee strengthens from 0.885 to 0.997 — and hold on all four rupture curves, while the flexibility fractions cross 0.5 with the curve too (0.55 and 0.62 on the two with the higher Larson–Miller constant). The flame-length response to load (Section 4.2) and the local slope of the master curve, neither identifiable from the published data, decide the sign of an effect whose magnitude is under 2 %.

Table 5: Robustness of the RQ2/RQ3 conclusions: fraction of paired Monte Carlo samples supporting each statement, as a function of the exponent p in a structural variant where the flame length shrinks with load as $L_q \text{ load}^p$. The calibrated model is $p = 0$; $p = 0.5$ is the bound discussed in Section 4.2. The first and third rows involve only full-load operating points, where $\text{load}^p = 1$, so they cannot move with p and serve as a check on the sampling.

Statement	$p = 0$	0.1	0.2	0.25	0.5	1.0
aging year 4 costs $> 2 \times$ S1 life per kmol	0.819	0.819	0.819	0.819	0.819	0.819
knee regime $< 0.5 \times$ base	0.885	0.911	0.928	0.936	0.974	0.997
S/C 3.5 cheaper in life than S/C 2.5	0.856	0.856	0.856	0.856	0.856	0.856
S2 daily $\leq$ S1	0.425	0.265	0.116	0.067	0.000	0.000
S3 renewable $\leq$ S1	0.484	0.320	0.168	0.105	0.000	0.000

576 All of the above describes one average tube. Because damage is convex in
577 wall temperature, spreading a per-tube offset over the 336 tubes of the ref-
578 erence furnace (Section S10) raises the population-mean damage rate above
579 the average tube's by 1.29 to 1.75 for a population standard deviation of
580 15 to 22 K; the hottest decile consumes life 3.9 to 7.4 times faster and the
581 hottest tube by an order of magnitude. The correction varies little between
582 regimes, leaving the ranking by life per kmol H_2 unchanged.

583 4. Discussion

584 4.1. Industrial implications

585 Three results have direct operational consequences. First, of the three
586 drivers identified in Section 3.2, excess air is the least appreciated: at fixed
587 fuel it lowers the hot-spot temperature by shifting heat release down the
588 tube. Its efficiency penalty, the larger flue-gas flow and stack loss, enters

589 through the firing required to hold the outlet temperature, so the optimizer
590 weighs it against life rather than ignoring it. Excess air is also the cheapest
591 variable to move on an operating plant, and its effect can be verified with
592 the existing pyrometer survey.

593 Second, whether the gains of the knee regime are realizable depends on
594 constraints outside the twin: preheat-coil metallurgy at 900 K inlet temper-
595 ature, pressure-swing-adsorption capacity at 110 % load and the downstream
596 steam balance. The steam-credit sweep shows the recommended steam-to-
597 carbon ratio moving from 4.0 to about 2.7 depending on how the plant values
598 steam; the twin cannot decide this, but it makes the dependence explicit.

599 Third, provided the outlet temperature is controlled, a plant that must
600 follow demand should not fear the tube-life consequences of smooth load
601 changes in either direction, but should watch the end-of-campaign hot-spot
602 temperature under a methane-slip target. That the load-following conclu-
603 sions are the least robust of the study reflects the size of the nominal effect
604 (a factor of 2.0 against 1 %), not a difference in modeling quality, and we
605 recommend that digital-twin studies report robustness fractions alongside
606 nominal results so that small nominal effects are not mistaken for findings.

607 *4.2. The flame-length response to load as a measurement need*

608 The one structural assumption that changes a conclusion is how the heat-
609 release profile of the burners responds to the firing rate. The calibrated model
610 uses a single dimensionless flame length, and the cross-validation residuals
611 at the upper peep hole (Section 3.1) already show that this is the weakest
612 element of the model: the partially loaded Plant C2 is predicted too hot at
613 the top and the fully loaded Plant A too cold. When the flame is allowed

614 to shorten with load, the flexible-operation conclusion reverses because the
 615 hot spot at reduced load moves into a hotter part of the furnace. The two
 616 hypotheses correspond to two ways of turning a furnace down: reducing the
 617 fuel flow through all burners, which leaves the length of a turbulent diffusion
 618 flame nearly unchanged [35], or taking burner rows out of service, which
 619 redistributes the heat release; the three published operating points cannot
 620 separate them. What would settle the question is a pyrometer survey at
 621 three or four elevations at two or three firing rates on one furnace, which
 622 most plants already perform in part during turnaround planning; a digital
 623 twin of the kind presented here turns such a survey into an estimate of the
 624 flame-length response with its uncertainty. The requirement is demanding:
 625 the sweep of Table 5 shows that an exponent of 0.1 already changes the
 626 answer materially, and the wall-temperature signature of that difference is
 627 about 9 K at the upper peep hole at 70 % load and below 0.1 K at the lower,
 628 in both cases smaller than the 15–22 K spread of the tube population, so a
 629 single elevation at a single firing rate cannot resolve it however accurate the
 630 instrument. Such a survey would not rescue the flexibility conclusions — at
 631 the calibrated flame length they already sit below even odds — but it would
 632 replace an unresolved sign with a quantified one, and it would do so for the
 633 two statements that the present data cannot decide. We regard this as the
 634 single most valuable measurement for tube-life-aware operation of top-fired
 635 reformers.

636 *4.3. Limitations*

637 The model represents one average tube. Tube-to-tube variation, from
 638 burner imbalance, row position and flow maldistribution, has a standard de-

639 viation of 15–22 K across the population at a given elevation in the reference
640 furnace [2]. Section S10 propagates that scatter through the rupture curve:
641 the population mean exceeds the average tube by about 1.5 in damage rate
642 and the hottest of 336 tubes — the one that decides when the furnace is
643 retubed — by 16.5 at $\sigma = 18.5$ K, without changing the ranking of the
644 scenarios or the regimes.

645 The life model covers creep only. Thermal fatigue, creep–fatigue interac-
646 tion and carburisation are not modeled, and the hoop stress is the pressure
647 stress alone, although the elastic thermal stress from the radial gradient is
648 close to an order of magnitude above it and drives damage during thermal cy-
649 cling (Section S1). The scenario results are therefore creep-life costs, not total
650 life costs; the screening of Section S11 finds the cyclic exposure of smooth
651 load variation small against the start-up cycles a plant already accepts, so
652 the ranking is unlikely to change if thermal cycles were counted.

653 The rupture curve is a manufacturer design band, not a heat-resolved
654 data set (Section 2.4). Absolute rupture times therefore remain implausible
655 as tube lives (10^7 h at the calibrated hot spot) and all results are reported
656 as ratios, which keep their direction on all four curves tested; replacing the
657 band by a measured scatter distribution is the remaining step towards any
658 absolute statement.

659 The scenarios are quasi-steady: each hour is a steady state of the twin,
660 and the thermal inertia of the tube, the catalyst and the furnace refractory is
661 neglected. The tube follows hourly load changes essentially instantaneously
662 while the refractory lags them (Section S1); for load ramps of 0.1 per hour
663 and events of one hour or longer the quasi-steady approximation is reasonable

664 for the tube, but it excludes the transient overshoot of the wall temperature
665 during a fast firing step, which would increase the cost of the over-firing
666 events. Finally, the calibration rests on three operating points of one furnace,
667 so the parameter intervals are conditional on that furnace and transfer to
668 another reformer requires recalibration on its own survey data.

669 5. Conclusions

670 A physics-informed digital twin of an industrial top-fired steam methane
671 reformer has been built from published kinetics, plant data and creep curves,
672 coupling a one-dimensional tube model, a long-furnace model, a Larson–
673 Miller life module, Gaussian-process surrogates with conformal prediction
674 intervals and Monte Carlo uncertainty propagation in one open, versioned
675 pipeline.

- 676 • The tube model reproduces the industrial case of Xu and Froment
677 within 14 K in gas temperature, and the heat-transfer correlations
678 printed in that paper overpredict the film coefficient by an order of
679 magnitude at industrial Reynolds numbers. Calibrated on three plant
680 operating points, the coupled model reproduces outlet temperatures
681 within 4 K and wall temperatures within 12 K, with a systematic resid-
682 ual at the upper elevation that points to the flame-length response to
683 load.
- 684 • Firing intensity, steam-to-carbon ratio and excess air explain 82 % of
685 the variance of the hot-spot temperature with negligible interactions;
686 inlet pressure enters the life only through the hoop stress.

- 687 • Under outlet-temperature control, load-following and renewable-following
688 change the life cost per kmol of hydrogen by less than 2 %, short over-
689 firing events by at most 2 %, and the steam-to-carbon ratio by ± 15 %;
690 catalyst aging under a methane-slip target doubles the life cost in four
691 years; the cyclic thermal exposure of smooth load variation is small
692 against the plant's own start-up cycles.
- 693 • The calibrated base is Pareto-dominated: a knee regime gives +15 %
694 hydrogen at -17 % fuel per kmol and 0.28 of the life cost, and 0.12 at
695 constant production. The optimal steam-to-carbon ratio moves from
696 4.0 to 2.7 when steam raising is charged in full.
- 697 • The 90 % uncertainty on the absolute rupture time spans a factor of
698 about 180, dominated by creep-curve scatter (86 %), while paired ratios
699 remain tight. The aging, knee and steam-to-carbon conclusions hold in
700 82 % to 88 % of samples on the base curve and 82 % to 94 % across four
701 rupture curves; the flexible-operation conclusion is supported in fewer
702 than half even at the calibrated flame length, and disappears under any
703 appreciable load dependence of the flame length or a change of rupture
704 curve.

705 The sign of the life cost of flexible operation is decided jointly by the flame-
706 length response to load and by the local slope of the rupture curve, neither
707 of which the published data identify. Two measurements would settle them,
708 in that order of priority: a multi-elevation pyrometer survey at several firing
709 rates, and rupture data resolved by heat for the HP-Nb and HK40 families.

710 **Data and code availability**

711 The model code (`rdt` package), the pipeline entry point (`python -m`
712 `rdt.pipeline -stage all -version v3`), the transcribed literature data
713 with their provenance annotations, the digitized verification curves, all v3
714 result files and the scripts that generate every figure, table and number in this
715 manuscript are available at <https://github.com/Izbassar0/reformer-digital-twin>
716 and archived at <https://doi.org/10.5281/zenodo.22666191>. The litera-
717 ture PDFs are not redistributed. Transcribed data are released under CC BY 4.0
718 and code under the MIT license. Questions about the code, the data and the
719 pipeline should be addressed to Izbassar Orynbassar (iorynbas@syr.edu).

720 **CRedit authorship contribution statement**

721 **Madina Sissenbay:** Conceptualization, Methodology, Validation, Inves-
722 tigation, Resources, Supervision, Project administration, Writing – review &
723 editing. **Izbassar Orynbassar:** Conceptualization, Methodology, Software,
724 Formal analysis, Data curation, Visualization, Writing – original draft, Writ-
725 ing – review & editing.

726 **Declaration of generative AI and AI-assisted technologies in the** 727 **writing process**

728 During the preparation of this work the authors used Claude (Anthropic)
729 in order to assist with code development, data transcription checks, figure and
730 table generation and drafting of the text. After using this tool, the authors
731 reviewed and edited the content as needed and take full responsibility for the
732 content of the published article.

733 **Declaration of competing interest**

734 The authors declare that they have no known competing financial inter-
735 ests or personal relationships that could have appeared to influence the work
736 reported in this paper. M.S. is employed in the industrial gas sector; the
737 work uses exclusively published data and no proprietary information from
738 any employer.

739 **Funding**

740 This research did not receive any specific grant from funding agencies in
741 the public, commercial, or not-for-profit sectors.

742 **Acknowledgements**

743 I.O. acknowledges the support of the Bolashak International Scholarship
744 of the Republic of Kazakhstan during the preparation of this work. The
745 authors thank D. A. Latham for the publicly archived thesis appendix that
746 made the plant-scale calibration possible.

747 **References**

- 748 [1] International Energy Agency, Global Hydrogen Review 2024, IEA, Paris,
749 2024.
- 750 [2] D. A. Latham, K. B. McAuley, B. A. Peppley, T. M. Raybold, Math-
751 ematical modeling of an industrial steam-methane reformer for on-
752 line deployment, Fuel Process. Technol. 92 (2011) 1574–1586. [https:](https://doi.org/10.1016/j.fuproc.2011.04.001)
753 /doi.org/10.1016/j.fuproc.2011.04.001

- 754 [3] A. K. Ray, S. K. Sinha, Y. N. Tiwari, J. Swaminathan, G. Das, S. Chaud-
755 huri, R. Singh, Analysis of failed reformer tubes, *Eng. Fail. Anal.* 10
756 (2003) 351–362. [https://doi.org/10.1016/S1350-6307\(02\)00029-8](https://doi.org/10.1016/S1350-6307(02)00029-8)
- 757 [4] American Petroleum Institute, API Standard 530: Calculation of
758 Heater-Tube Thickness in Petroleum Refineries, 7th ed., API, Wash-
759 ington, DC, 2015.
- 760 [5] J. Xu, G. F. Froment, Methane steam reforming, methanation and
761 water-gas shift: I. Intrinsic kinetics, *AIChE J.* 35 (1989) 88–96. <https://doi.org/10.1002/aic.690350109>
- 762 [6] J. Xu, G. F. Froment, Methane steam reforming: II. Diffusional lim-
763 itations and reactor simulation, *AIChE J.* 35 (1989) 97–103. <https://doi.org/10.1002/aic.690350110>
- 764 [7] G. Pantoleontos, E. S. Kikkinides, M. C. Georgiadis, A heteroge-
765 neous dynamic model for the simulation and optimisation of the steam
766 methane reforming reactor, *Int. J. Hydrogen Energy* 37 (2012) 16346–
767 16358. <https://doi.org/10.1016/j.ijhydene.2012.02.125>
- 768 [8] P. M. Plehiers, G. F. Froment, Coupled simulation of heat transfer and
769 reaction in a steam reforming furnace, *Chem. Eng. Technol.* 12 (1989)
770 20–26. <https://doi.org/10.1002/ceat.270120105>
- 771 [9] A. Zamaniyan, H. Ebrahimi, J. S. S. Mohammadzadeh, A unified model
772 for top fired methane steam reformers using three-dimensional zonal
773 analysis, *Chem. Eng. Process.* 47 (2008) 946–956. <https://doi.org/10.1016/j.cep.2007.03.005>
- 774 [10] A. Kumar, M. Baldea, T. F. Edgar, O. A. Ezekoye, Smart manufactur-
775 ing approach for efficient operation of industrial steam-methane reform-
776 ing approach for efficient operation of industrial steam-methane reform-
777 ing approach for efficient operation of industrial steam-methane reform-
778 ing approach for efficient operation of industrial steam-methane reform-

- ers, Ind. Eng. Chem. Res. 54 (2015) 4360–4370. <https://doi.org/10.1021/ie504087z>
- [11] A. Jafarizadeh, M. Panjepour, M. D. Emami, Advanced modelling and optimization of steam methane reforming: from CFD simulation to machine learning-driven optimization, Int. J. Hydrogen Energy 96 (2024) 1262–1280. <https://doi.org/10.1016/j.ijhydene.2024.11.352>
- [12] L. E. Yerimah, M. Mehana, R. P. Singh, P. Sharan, Uncertainty-aware hydrogen production optimization from a steam methane reformer with a water gas shift reactor and pressure swing adsorption, Ind. Eng. Chem. Res. 64 (2025) 18298–18314. <https://doi.org/10.1021/acs.iecr.5c01681>
- [13] S. R. Nabavi, Z. Guo, Z. Wang, Machine learning-assisted surrogate modeling with multi-objective optimization and decision-making of a steam methane reforming reactor, arXiv:2507.07641 (2025). <https://arxiv.org/abs/2507.07641>
- [14] National Institute for Materials Science, Data sheets on the elevated-temperature properties of centrifugally cast 25Cr-20Ni-0.4C steel tubes for use in reformer furnaces (SCH 22-CF), NIMS Creep Data Sheet No. 16B, Tsukuba, Japan. <https://doi.org/10.11503/nims.1020>
- [15] National Institute for Materials Science, Data sheets on the elevated-temperature properties of centrifugally cast tubes and cast block of 25Cr-35Ni-0.4C steel for reformer furnaces (SCH 24), NIMS Creep Data Sheet No. 38A, Tsukuba, Japan. <https://doi.org/10.11503/nims.1042>
- [16] National Institute for Materials Science, MatNavi Service Terms of

804 Use, NIMS, Tsukuba, Japan. [https://mits.nims.go.jp/agreement/](https://mits.nims.go.jp/agreement/MatNavi_agreement_en.pdf)
805 [MatNavi_agreement_en.pdf](https://mits.nims.go.jp/agreement/MatNavi_agreement_en.pdf)

806 [17] D. A. Latham, Mathematical modelling of an industrial steam methane
807 reformer, M.Sc.E. thesis, Department of Chemical Engineering, Queen's
808 University, Kingston, Ontario, Canada, 2008. [http://hdl.handle.](http://hdl.handle.net/1974/1650)
809 [net/1974/1650](http://hdl.handle.net/1974/1650)

810 [18] L. Lao, A. Aguirre, A. Tran, Z. Wu, H. Durand, P. D. Christofides, CFD
811 modeling and control of a steam methane reforming reactor, Chem. Eng.
812 Sci. 148 (2016) 78–92. <https://doi.org/10.1016/j.ces.2016.03.038>

813 [19] A. Tran, A. Aguirre, M. Crose, H. Durand, P. D. Christofides,
814 Temperature balancing in steam methane reforming furnace via an
815 integrated CFD/data-based optimization approach, Comput. Chem.
816 Eng. 104 (2017) 185–200. [https://doi.org/10.1016/j.compchemeng.](https://doi.org/10.1016/j.compchemeng.2017.04.013)
817 [2017.04.013](https://doi.org/10.1016/j.compchemeng.2017.04.013)

818 [20] A. Kumar, M. Baldea, T. F. Edgar, A physics-based model for indus-
819 trial steam-methane reformer optimization with non-uniform tempera-
820 ture field, Comput. Chem. Eng. 105 (2017) 224–236. [https://doi.org/](https://doi.org/10.1016/j.compchemeng.2017.01.002)
821 [10.1016/j.compchemeng.2017.01.002](https://doi.org/10.1016/j.compchemeng.2017.01.002)

822 [21] M. Whittaker, B. Wilshire, J. Brear, Creep fracture of the centrifugally-
823 cast superaustenitic steels, HK40 and HP40, Mater. Sci. Eng. A 580
824 (2013) 391–396. <https://doi.org/10.1016/j.msea.2013.05.041>

825 [22] G. N. Haidemenopoulos, A. D. Zervaki, H. Kamoutsis, K. Poly-
826 chronopoulou, Creep rupture in HP-Nb refractory steel tubes due to
827 short-term overheating, Eur. J. Mater. 1 (2021) 1–22. [https://doi.](https://doi.org/10.1080/26889277.2021.1994841)
828 [org/10.1080/26889277.2021.1994841](https://doi.org/10.1080/26889277.2021.1994841)

- [23] K. Guguloth, N. Roy, Creep life estimation of reformer alloy using θ -projection method – a neuro fuzzy approach, Int. J. Press. Vessels Piping 203 (2023) 104938. <https://doi.org/10.1016/j.ijpvp.2023.104938>
- [24] C.-L. Yeh, Effect of burner operation on the catalyst tube lifetime of a steam methane reformer: a numerical study, Appl. Sci. 11 (2021) 231. <https://doi.org/10.3390/app11010231>
- [25] F. R. Larson, J. Miller, A time-temperature relationship for rupture and creep stresses, Trans. ASME 74 (1952) 765–775.
- [26] E. L. Robinson, Effect of temperature variation on the long-time rupture strength of steels, Trans. ASME 74 (1952) 777–781.
- [27] D. G. Goodwin, H. K. Moffat, I. Schoegl, R. L. Speth, B. W. Weber, Cantera: an object-oriented software toolkit for chemical kinetics, thermodynamics, and transport processes, version 3.1, 2024. <https://doi.org/10.5281/zenodo.14455267>
- [28] S. Ergun, Fluid flow through packed columns, Chem. Eng. Prog. 48 (1952) 89–94.
- [29] M. H. Wesenberg, H. F. Svendsen, Mass and heat transfer limitations in a heterogeneous model of a gas-heated steam reformer, Ind. Eng. Chem. Res. 46 (2007) 667–676.
- [30] M. Leva, M. Grummer, Heat transfer to gases through packed tubes: effect of particle characteristics, Ind. Eng. Chem. 40 (1948) 415–419. <https://doi.org/10.1021/ie50459a012>
- [31] A. P. De Wasch, G. F. Froment, Heat transfer in packed beds, Chem. Eng. Sci. 27 (1972) 567–576. [https://doi.org/10.1016/0009-2509\(72\)87012-X](https://doi.org/10.1016/0009-2509(72)87012-X)

- [32] S. Yagi, D. Kunii, Studies on heat transfer near wall surface in packed beds, *AIChE J.* 6 (1960) 97–104. <https://doi.org/10.1002/aic.690060119>
- [33] H. C. Hottel, A. F. Sarofim, *Radiative Transfer*, McGraw-Hill, New York, 1967.
- [34] F. C. Roesler, Theory of radiative heat transfer in co-current tube furnaces, *Chem. Eng. Sci.* 22 (1967) 1325–1336. [https://doi.org/10.1016/0009-2509\(67\)80023-X](https://doi.org/10.1016/0009-2509(67)80023-X)
- [35] W. R. Hawthorne, D. S. Weddell, H. C. Hottel, Mixing and combustion in turbulent gas jets, *Third Symposium on Combustion and Flame and Explosion Phenomena* 3 (1949) 266–288.
- [36] F. Pedregosa, G. Varoquaux, A. Gramfort, V. Michel, B. Thirion, O. Grisel, M. Blondel, P. Prettenhofer, R. Weiss, V. Dubourg, J. Vanderplas, A. Passos, D. Cournapeau, M. Brucher, M. Perrot, É. Duchesnay, Scikit-learn: machine learning in Python, *J. Mach. Learn. Res.* 12 (2011) 2825–2830.
- [37] R. F. Barber, E. J. Candès, A. Ramdas, R. J. Tibshirani, Predictive inference with the jackknife+, *Ann. Stat.* 49 (2021) 486–507. <https://doi.org/10.1214/20-AOS1965>
- [38] V. Taquet, V. Blot, T. Morzadec, L. Lacombe, N. Brunel, MAPIE: an open-source library for distribution-free uncertainty quantification, *arXiv:2207.12274* (2022). <https://arxiv.org/abs/2207.12274>
- [39] A. Saltelli, P. Annoni, I. Azzini, F. Campolongo, M. Ratto, S. Tarantola, Variance based sensitivity analysis of model output. Design and estimator for the total sensitivity index, *Comput. Phys. Commun.* 181

- 879 (2010) 259–270. <https://doi.org/10.1016/j.cpc.2009.09.018>
- 880 [40] J. Herman, W. Usher, SALib: an open-source Python library for sensi-
881 tivity analysis, J. Open Source Softw. 2 (2017) 97. [https://doi.org/](https://doi.org/10.21105/joss.00097)
882 [10.21105/joss.00097](https://doi.org/10.21105/joss.00097)
- 883 [41] K. Deb, A. Pratap, S. Agarwal, T. Meyarivan, A fast and elitist mul-
884 tiobjective genetic algorithm: NSGA-II, IEEE Trans. Evol. Comput. 6
885 (2002) 182–197. <https://doi.org/10.1109/4235.996017>
- 886 [42] J. Blank, K. Deb, pymoo: multi-objective optimization in Python, IEEE
887 Access 8 (2020) 89497–89509. [https://doi.org/10.1109/ACCESS.](https://doi.org/10.1109/ACCESS.2020.2990567)
888 [2020.2990567](https://doi.org/10.1109/ACCESS.2020.2990567)