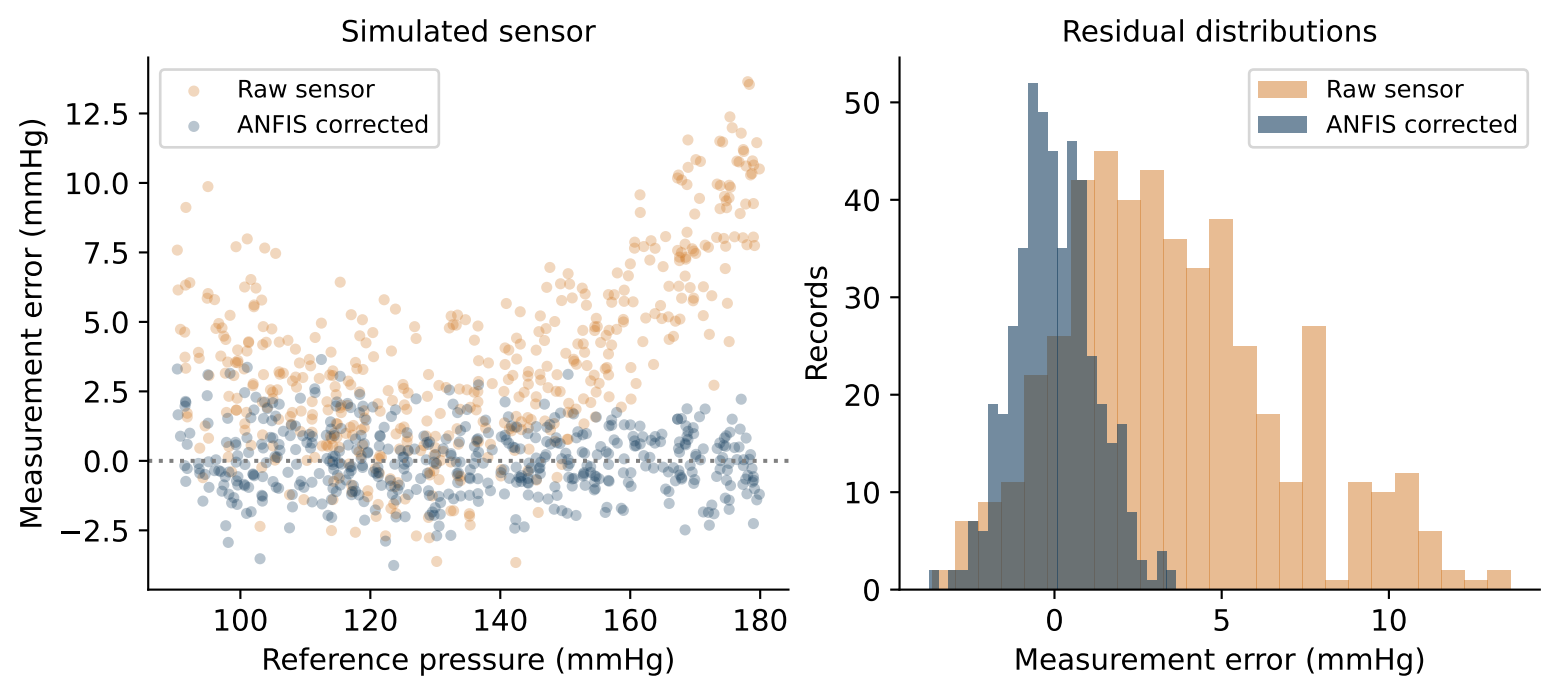
Simulated sensor
Raw sensor
ANFIS corrected
Measurement error (mmHg)
12.5
10.0
7.5
5.0
2.5
0.0
−2.5
100
120
140
160
180
Reference pressure (mmHg)
Residual distributions
Raw sensor
ANFIS corrected
Records
50
40
30
20
10
0
0
5
10
Measurement error (mmHg)