


Measurement: Impedance Adapter

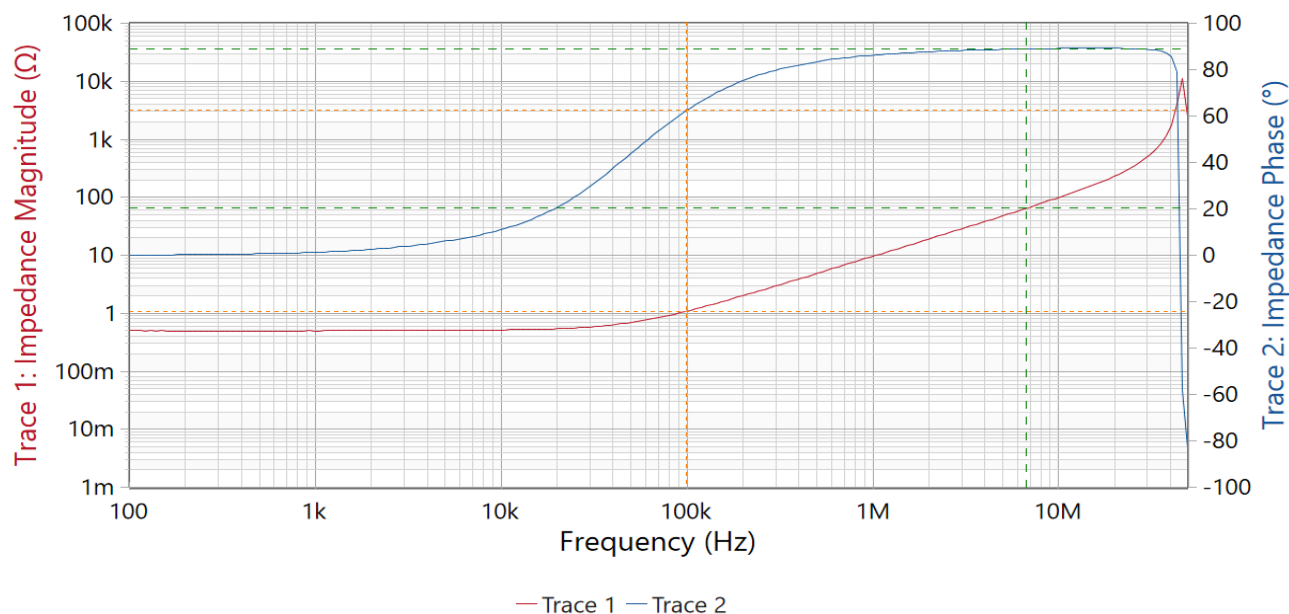

	Cursor 1	Cursor 2	Delta C2-C1
Frequency	6,79 MHz	100 kHz	-6,69 MHz
Trace 1	Magnitude	Magnitude	Magnitude
Measurement	64,915 Ω	1,086 Ω	-63,829 Ω
Trace 2	Phase (°)	Phase (°)	Phase (°)
Measurement	88,96 °	62,373 °	-26,587 °
Trace 3	Ls	Ls	Ls
Measurement	1,521 μH	1,532 μH	10,362 nH
Trace 4	Rs	Rs	Rs
Measurement	1,179 Ω	503,576 mΩ	-675,032 mΩ
Trace 5	Q	Q	Q
Measurement	55,084	1,912	-53,172

Sweep

Start frequency:	100 Hz
Stop frequency:	50 MHz
Center frequency:	25 MHz
Span:	50 MHz
Sweep mode:	Logarithmic
Numer of points:	201

Calibration

Calibration	Full-Range	User-Range
-------------	------------	------------

Impedance

Active

-

Averaging

Averaging	Compl. Sweeps	Factor
-----------	---------------	--------

Impedance

OFF

10

Hardware setup

Device type:	Bode100R1
Serial number:	NM128G
Receiver bandwidth:	300 Hz
Output level:	13 dBm
DUT settling time:	0 ms

Comments: