



Filename: 2021-01-08 - 15.29.13.D5000

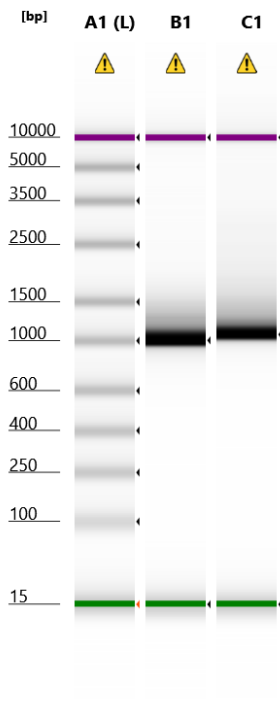

Default image (Contrast 100%)

Sample Info


Well	Conc. [ng/ul]	Sample Description	Alert	Observations
A1	47.9	Ladder	⚠	Caution! Expired ScreenTape device; Ladder
B1	56.1	AQ Poc mtORF 1	⚠	Caution! Expired ScreenTape device
C1	60.4	AQ Poc mtORF 2	⚠	Caution! Expired ScreenTape device

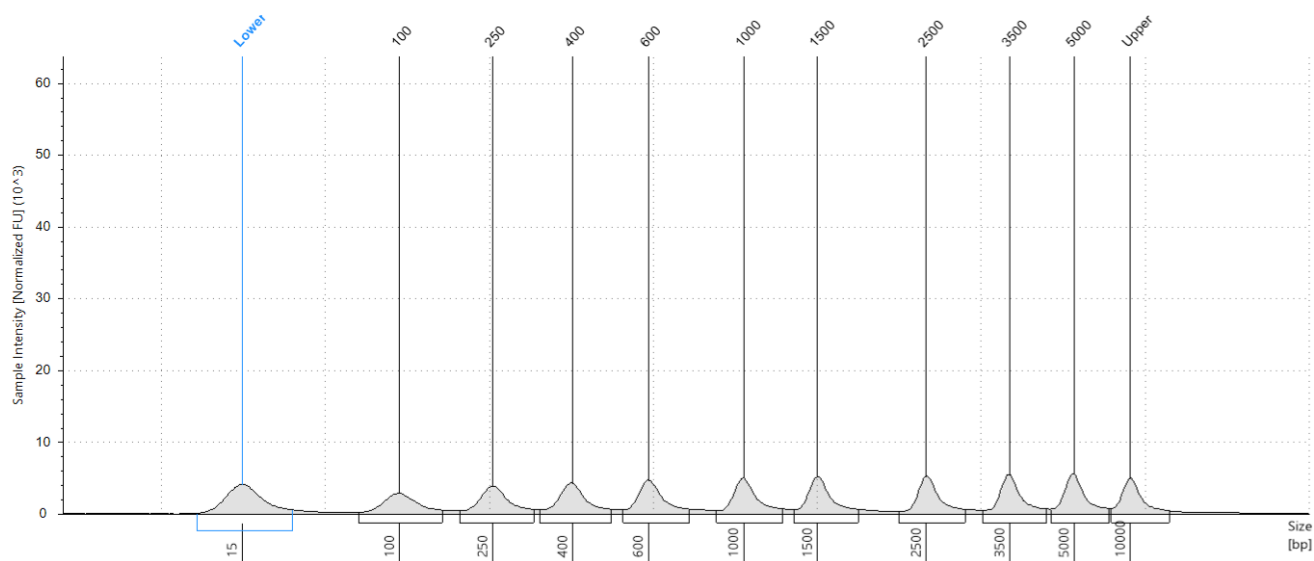A1: Ladder**Sample Table**

Well	Conc. [ng/μl]	Sample Description	Alert	Observations
A1	47.9	Ladder		Caution! Expired ScreenTape device; Ladder

Peak Table

Size [bp]	Calibrated Conc. [ng/μl]	Assigned Conc. [ng/μl]	Peak Molarity [nmol/l]	% Integrated Area	Peak Comment	Observations
15	5.75	-	590	-		Lower Marker
100	4.56	-	70.2	9.52		
250	5.22	-	32.1	10.89		
400	5.46	-	21.0	11.39		
600	5.49	-	14.1	11.46		
1000	5.46	-	8.40	11.40		
1500	5.48	-	5.62	11.44		
2500	5.30	-	3.26	11.06		
3500	5.48	-	2.41	11.43		
5000	5.46	-	1.68	11.40		
10000	3.25	3.25	0.500	-		Upper Marker

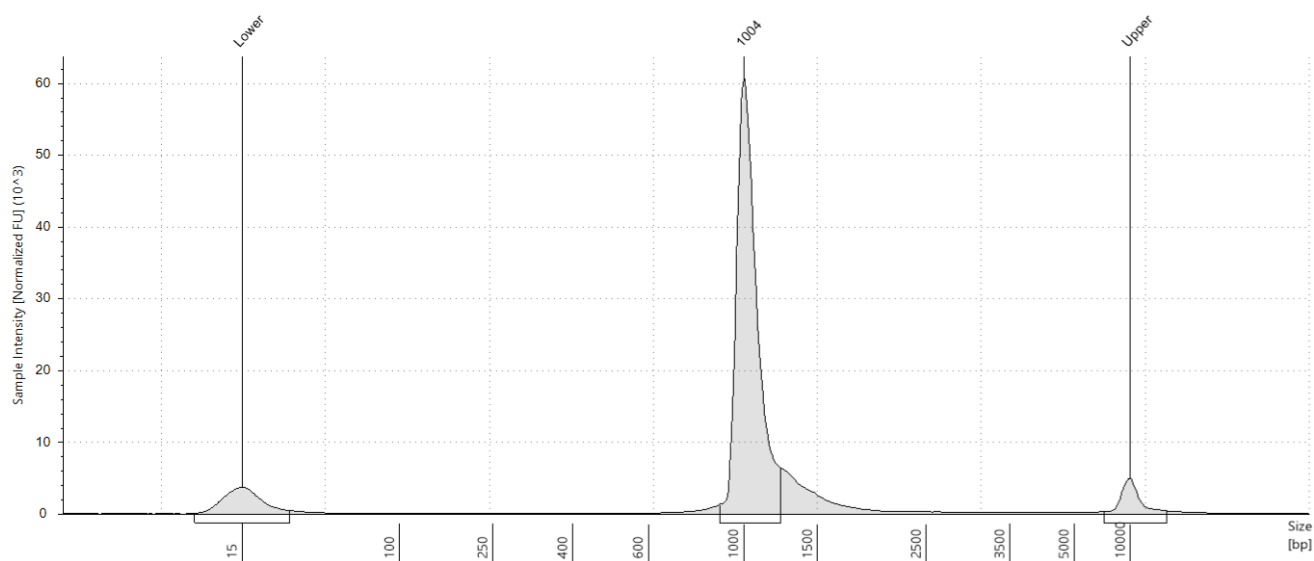
B1: AQ Poc mtORF 1**Sample Table**

Well	Conc. [ng/μl]	Sample Description	Alert	Observations
B1	56.1	AQ Poc mtORF 1	⚠	Caution! Expired ScreenTape device

Peak Table

Size [bp]	Calibrated Conc. [ng/μl]	Assigned Conc. [ng/μl]	Peak Molarity [nmol/l]	% Integrated Area	Peak Comment	Observations
15	5.42	-	556	-		Lower Marker
1004	56.1	-	85.9	100.00		
10000	3.25	3.25	0.500	-		Upper Marker

C1: AQ Poc mtORF 2

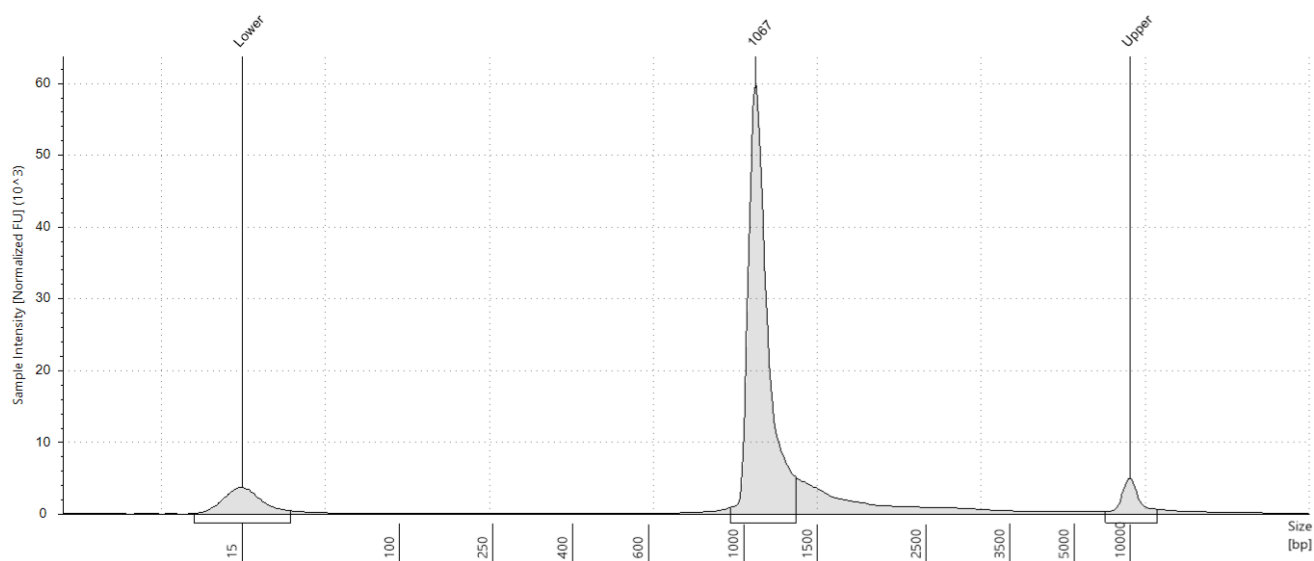

Sample Table

Well	Conc. [ng/μl]	Sample Description	Alert	Observations
C1	60.4	AQ Poc mtORF 2	⚠	Caution! Expired ScreenTape device

Peak Table

Size [bp]	Calibrated Conc. [ng/μl]	Assigned Conc. [ng/μl]	Peak Molarity [nmol/l]	% Integrated Area	Peak Comment	Observations
15	6.25	-	641	-		Lower Marker
1067	60.4	-	87.1	100.00		
10000	3.25	3.25	0.500	-		Upper Marker