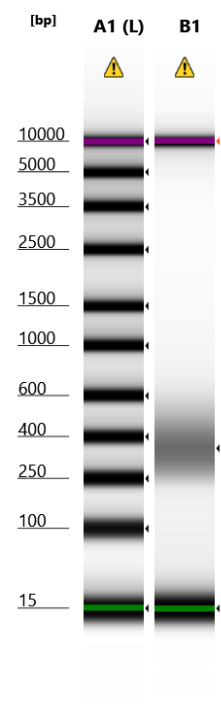


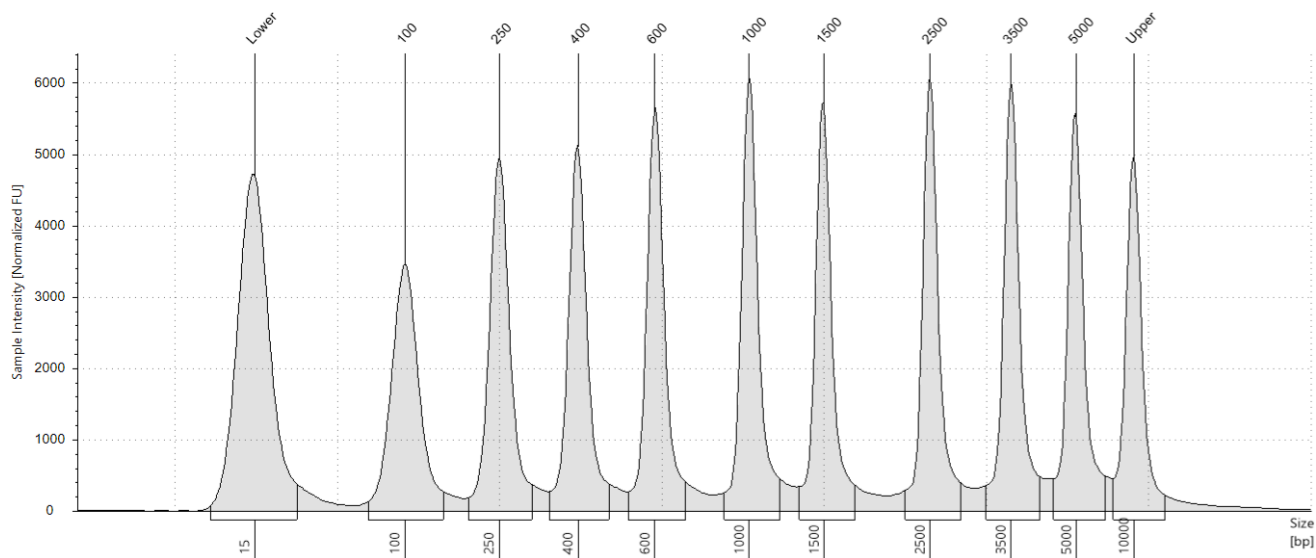
Filename: 2019-09-06 - 17.03.12.D5000



Default image (Contrast 100%)

Sample Info

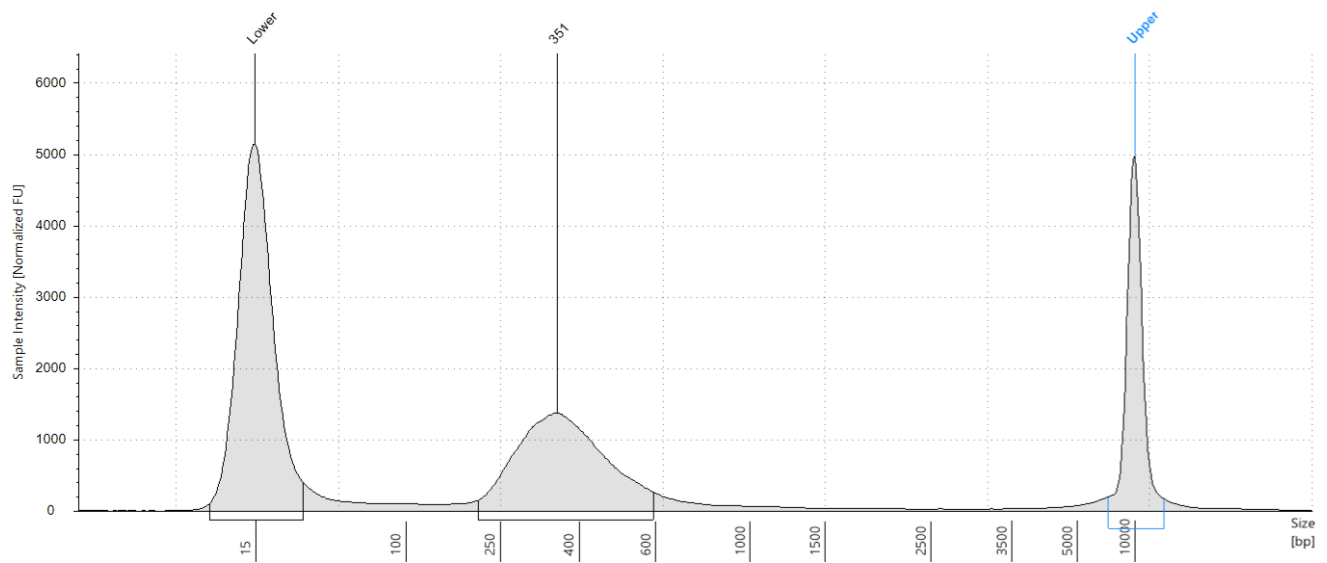
Well	Conc. [ng/ul]	Sample Description	Alert	Observations
A1	44.2	Ladder		Caution! Expired ScreenTape device (used after two weeks of first use); Ladder
B1	5.80	T A Hot 2 Ribo-free RNA lib test		Caution! Expired ScreenTape device (used after two weeks of first use)

**A1: Ladder****Sample Table**

Well	Conc. [ng/μl]	Sample Description	Alert	Observations
A1	44.2	Ladder		Caution! Expired ScreenTape device (used after two weeks of first use); Ladder

**Peak Table**

Size [bp]	Calibrated Conc. [ng/μl]	Assigned Conc. [ng/μl]	Peak Molarity [nmol/l]	% Integrated Area	Peak Comment	Observations
15	6.64	-	681	-		Lower Marker
100	4.71	-	72.5	10.67		
250	5.12	-	31.5	11.58		
400	4.86	-	18.7	11.00		
600	5.06	-	13.0	11.46		
1000	5.16	-	7.93	11.67		
1500	4.74	-	4.87	10.74		
2500	4.93	-	3.03	11.16		
3500	4.96	-	2.18	11.23		
5000	4.63	-	1.43	10.49		
10000	3.25	3.25	0.500	-		Upper Marker

**B1: TA Hot 2 Ribo-free RNA lib test****Sample Table**

Well	Conc. [ng/μl]	Sample Description	Alert	Observations
B1	5.80	TA Hot 2 Ribo-free RNA lib test	⚠	Caution! Expired ScreenTape device (used after two weeks of first use)

**Peak Table**

Size [bp]	Calibrated Conc. [ng/μl]	Assigned Conc. [ng/μl]	Peak Molarity [nmol/l]	% Integrated Area	Peak Comment	Observations
15	7.55	-	774	-		Lower Marker
351	5.80	-	25.4	100.00		
10000	3.25	3.25	0.500	-		Upper Marker