Contents

MeltR

Automated fitting of RNA/DNA absorbance melting curves and fluorescence binding isotherms in R

1 Overview

MeltR is a R package that fits nucleic acid folding data to molecular models to obtain thermodynamic parameters. MeltR automates the trivial but time-consuming tasks associated with fitting nucleic acids thermodenaturation data, leading to facile conversion of raw data into useful thermodynamic parameters.

MeltR was inspired by Meltwin.[1] MeltR and Meltwin have the same utility: easy and consistent fitting to obtain thermodynamic parameters. The main drawback of MeltR is that it is ran from your R console, whereas Meltwin has a graphical-user-interface. However, the MeltR syntax is not complicated, and MeltR has other advantages: (1) A current versions of MeltR can be downloaded from GitHub by entering two lines of code in your R consol, whereas Meltwin has been out of support for years. (2) MeltR supports fitting fluorescence binding isotherms to obtain thermodynamic parameters. (3) MeltR can be ran in bulk. (4) Anecdotally, MeltR is more robust than Meltwin and requires less input from the user.

The core of MeltR is the "meltR.A" function for fitting absorbance melting curves and the "meltR.F" function for fitting fluorescence binding isotherms.

2 MeltR installation

```
install.packages("devtools")
devtools::install_github("JPSieg/MeltR")
```

3 Theory

3.1 Fitting fluorescence isotherms

MeltR can obtains thermodynamic parameters from fluorescence binding isotherms for heteroduplex DNA and RNA using the non-linear regression function in base R, "nls". In this strategy, a quencher labeled strand is titrated, at about 1 to 1000 nM concentrations, into different wells in a qPCR plate containing a constant concentration of fluorophore labeled strand. The fluorophore labeled strand binds to the quencher labeled strand, reducing the fluorescence emmission (E) and resulting in an apparant fluorescence binding isotherm, where the shape of the curve is determined by Equation 1.

$$E = F_{max} + (F_{min} - F_{max}) * F(K_D, [A]_T, [B]_T) \qquad (1)$$

Where Fmax is the fluorescence emission of unbound fluorophore labeled strand (A), Fmin is the fluorescence emission of the fluorophore labeled strand completely bound to a quencher labeled strand (B), and F(K_D, $[A]_T$, $[B]_T$) is the mole fraction of the bound fluorophore labeled strand to the total fluorophore labeled strand.

$$F(K_D, [A]_T, [B]_T) = \frac{[AB]}{[A]_T} \qquad (2)$$

F(K$_D$, [A]$_T$, [B]$_T$) is a function controled experimental variables, the total fluorophore labled strandd ([A]$_T$) and the total quenceher labeled strand ([B]$_T$), and the K$_D$ is given by the the expression:

$$K_D = \frac{[A][B]}{[AB]} \qquad (3)$$

F(K$_D$, [A]$_T$, [B]$_T$) can be determined by solving the K$_D$ expression to obtain:

$$F(K_D, [A]_T, [B]_T) = \frac{(K_D + [A]_T + [B]_T) - \sqrt{(K_D + [A]_T + B]_T)^2 - 4[A]_T[B]_T}}{2[A]_T} \qquad (4)$$

Thus, the K$_D$ at each temperature was determined by fitting isotherms at each temperature to equation 5, obtained by plugging Equation 4 into Equation 1.

$$E = F_{max} + (F_{min} - F_{max}) \frac{(K_D + [A]_T + [B]_T) - \sqrt{(K_D + [A]_T + B]_T)^2 - 4[A]_T[B]_T}}{2[A]_T} \qquad (5)$$

Thermodynamic parameters for helix formation were extracted by the Van't hoff relationship (Equation 6) between the K$_D$ the temperature using the two methods described below.

$$ln(K_D) = \frac{dS}{R} - \frac{dH}{RT} \qquad (6)$$

For a single experiment, all samples should be diluted from the same fluorophore and quencher stocks, so that MeltR can deal with systematic uncertainty in strand concentrations.

3.1.1 Fluorescence data preprocessing

MeltR performs the following data preprocessing steps before fitting:

1.) The fluorophore labeled strand concentration is optomized using the concentration optimization algorithm, described in more detail in section 3.1.3.

2.) The T$_m$ of each sample is estimated using the first derivative of fluorescence emission as a function of temperature. First derivatives are calculated using

polynomial regression, where the data are approximated with a 20th order polynomial. Then, the analytical first derivative of the polynomial was determined using calculus. The approximate T_m (where 50% of the nucleic acid is single stranded) is calculated by finding the maximum of the first derivative curve to a precision of less than 0.1 °C. This T_m is unreliable because fluorecence baselines vary wildly with temperature. However, the T_m is useful for qualitative comparison of stability between conditions.

2.) Isotherms are fit to Equation 5 to determine K_D and error in the K_D at each temperature using "nls" in base R. Initial values for F_{max} and F_{min} are estimated by taking the mean of the 20% highest readings in each isotherm and the 20% lowest readings respecyively. Initial values for the K_D are provided by the user.

3.) K_Ds are filtered by K_D magnitude and error according to the users specifications to determine which isotherms are most reliable. First, K_Ds outside of a user specified range (10 to 1000 nM by default) are thrown out. Second, K_Ds are ranked by the error in the K_D. K_Ds that are below a user specified error quantile are thrown out. The default K_D error quantile file is 0.25, meaning the algorithem with keep the to 25% most accurate K_Ds.

4.) The most reliable K_Ds and temperatures are passed to Method 1 to make Van't Hoff plots and to calculate helix formation energies.

5.) Fluorescence data from the most reliable K_Ds and temperatures are passed to Method 2 for global fitting and to calculate helix formation energies.

3.1.2 Concentration optimization algorithm.

We have determined that the accuracy of fit results is highly dependent on errors in the predicted concentration of fluorophore and quencher RNA strands in stock solutions. Fit accuracy is dependent on the mole ratio of fluorophore and quencher labeled RNA in stock solutions, but not dependent on the total magnitude of both fluorophore and quencher labeled RNA concentrations in the stocks. Thus, the concentration optimization algorithm in MeltR does not need to find exact concentration to generate accurate helix formation energis, just the mole ratio (R) of fluorophore and quencher labeled RNA in samples that should have equal concentrations of fluorophore and quencher, for example predicted 200 nM FAM-RNA and 200 nM RNA-BHQ1.

MeltR uses a fluorecence binding isotherm from a temperature where the K_D is more than 10 times less than the fluorophore labeled strand concentration. Under these conditions, the shape of the curve will be independent of the K_D , and the isotherm can be used as a Job plot. For example, at a 200 nM fluorophore labeled strand concentration, the shape of the binding curve will be indendent of K_D if the K_D is less than 10 nM. The curve will resemble a hockey stick (Figure 1A) composed of two straint lines. The first line, where $[A]_T > [B]_T$, will decrease as the $[B]_T$ is increased and the fluorophore labeled strand is saturated.

The second line, where $[A]_T < [B]T_T$, will be horizontal as the $[B]_T$ is increased because the fluorphore labeled strand is saturated. The intersection of the first and second line will occure at:
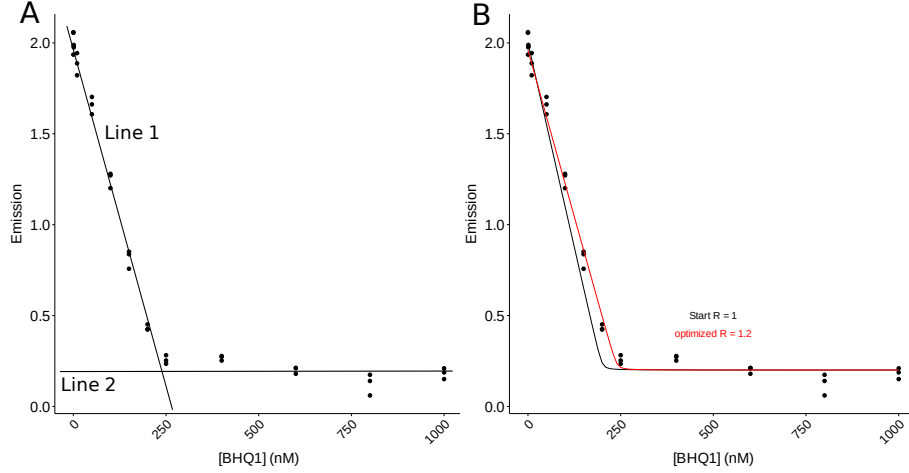
$$[A]_T = [B]_T \qquad (7)$$

Figure 1: Job_plot

The absolute concentration of $[A]_T$ and $[B]_T$ cannot be known with precicion. However, the mole ratio of the error (X) in the fluorophore and quencher stocks can be estimated from this data point at equation 8.

$$\frac{[A]_{T-estimated}}{X} = [B]_T \qquad (8)$$

Where $[A]_{T\text{-estimated}}$ is the estimated total A concentration, or the predicted concentration based on of the stock, and X is given by Equation 9 based on the actual concentration determined from the experiment.

$$X = \frac{[A]_T}{[B]_T} \qquad (9)$$

MeltR fits an overdetermined isotherm to a binding curve (selected by the user but by default the isotherm collected at the lowest temperature) to a modified version of Equation 5 to determine X (Figure 1 B).

$$E = F_{max} + (F_{min} - F_{max}) * \frac{(K_D + [A]_{T-estimated} + [B]_T X) - \sqrt{(K_D + [A]_{T-estimated} + B]_T X)^2 - 4[A]_{T-estim}}}{2[A]_{T-estimated}}$$

5

By default, the fit to determine X allows R and K_D to float. The user should also use an argument called "low_K", to set the Kd in the optimization fit to several K_D that are more than 10 times less than the fluorophore labeled strand concentrations. They should then inspect the R from several iterations of the optimization algorithm set to different "low_K" values to make sure it is similar to the iteration that allows the K_D to float.

$[A]_T$ is then corrected with Equation 11.

$$[A]_T = \frac{[A]_{T-estimated}}{X} \qquad (11)$$

3.1.3 Method 1 Van't Hoff plot

Method 1 fits K_Ds that were passed from the preprocessing steps to Equation 6. Initial estimates for the dH and dS of helix formation are provided by the user in kcal as a list using the "vh_start" argument. The default is -70 kcal/mol and 0.180 kcal/mol/K for the enthalpy and entropy respectively, and will work for most helices. The free energy of helix formation at 37 °C (dG) was calculated from the dH and dS values provided by the fit.

The standard error of the dG was propagated from the standartd error of dH and the dS from the fit, and the covariation between the two values.

$$SE_{dG} = \sqrt{SE_{dH}^2 + \left(310.15 * \frac{SE_{dS}}{dS}\right)^2 + 2 * 310.15 * \frac{Covar_{dH,dS}}{dH * dS}} \qquad (12)$$

Helix formation energies are traditionally reported in terms of the association constant.

$$K = \frac{[AB]}{[A][B]} = 1/K_D \qquad (13)$$

Thus, dHs and dSs reported by MeltR are also reported in terms of the association constant, which is obtained by multiplying helix formation energies from fitting K_D by negative one.

3.1.4 Method 2 Global fit

Method 2 globally fits fluorescence data that were passed from the preprocessing to equation x, obtained by plugging equation y into equation z. Fmax and Fmin was allowed to float between temperatures and dH and dS were constant. Starting values for F_{max}, F_{min}, dH, and dS are obtained from the results for individual fits.

$$E = F_{max}+(F_{min}-F_{max})*\frac{(\exp\frac{dS}{R} - \frac{dH}{RT} + [A]_T + [B]_T) - \sqrt{(\exp\frac{dS}{R} - \frac{dH}{RT} + [A]_T + B]_T)^2 - 4[A]_T[B]_T}}{2[A]_T}$$ (1

The dG and the error in the dG were calculated as in method 1.

3.2 Fitting abosorbance melting curves

3.2.1 Absorbance data preprocessing

MeltR can obtain thermodynamic parameters from absorbance melting curves for heteroduplex, homoduplex (selfcomplementary), and monomolecular self-structured DNA and RNA using the method pioneered by Tinoco and colleagues and refined by Turner and colleagues.[1-3]

MeltR performs the following data preprocessing steps before fitting:

1.) RNA and DNA extinction coefficients are calculated from the sequence using the data from Tinoco and colleagues.[2]

2.) The background absorbance of a user specified blank is scaled to the pathlength of the cuvette and subtracted from each curve.

3.) The total strand concentration (C_t) is calculated at a user specified temperature (Default = 90 °C).

4.) High and low temperature data are trimmed (to the users specification) to ensure linear baselines.

5.) First and second derivatives are taken using polynomial regression. First, the data are approximated using a 20th order polynomial. Then, the first and second derivatives of the polynomial are determined analystically using calculus. The approximate $T_{0.5}$ (the approximate melting temperature T_m where 50% of the nucleic acid is single stranded) is calculated by finding the maximum of the first derivative curve and the $T_{0.75}$ (the approximate temperature where 75% of the nucleic acid is single stranded) is calculated by finding the minimum of the first derivative (Figure 2), to a precision of less than 0.1 °C.

6.) Initial parameter estimates are calculated for each curve. The initial values for slopes and intercepts of the baselines are estimated by fitting absorbance values that are greater than the 75th quantile for the uper baselines, and fitting aborbance values that are lower than the 25th quantile for the lower baseline, to y = mx + b. Initial values for the enthalpy are determined using the $T_{0.5}$ and $T_{0.75}$ (in Kelvin) from first and second derivative curves. MeltR uses equation 15, equation 16, and equation 17, for heteroduplex, homoduplex, and monomolecular self-structured DNA and RNA melting curves.

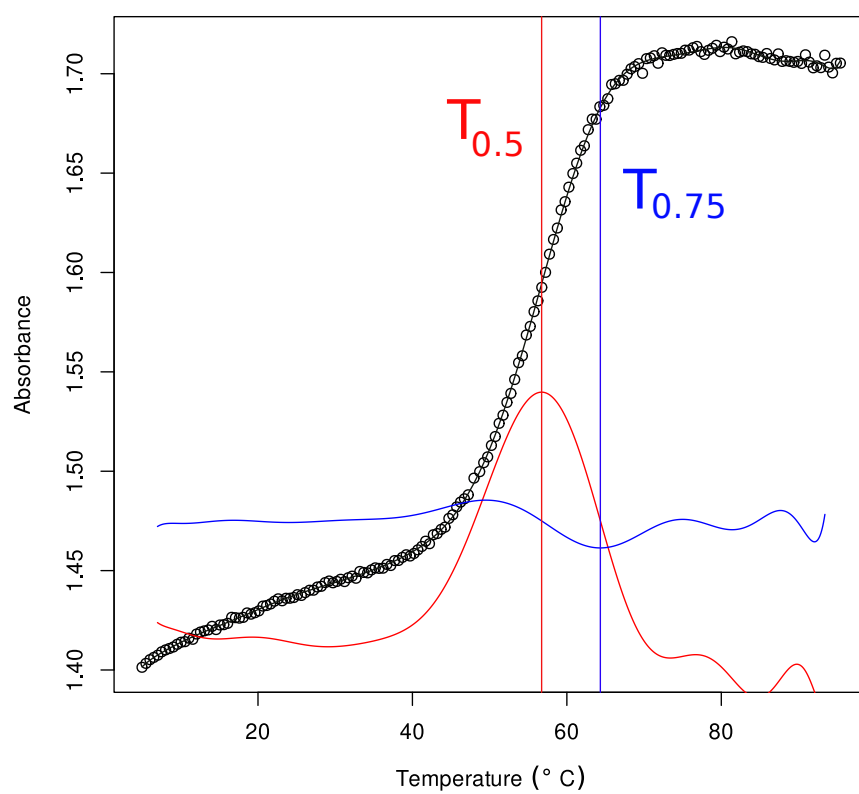$$dH = -0.007 * (\frac{1}{T_{0.5}} - \frac{1}{T_{0.75}})$$ (15)

Figure 2: Melt_curve_derivative

$$dH = -0.0044 * (\frac{1}{T_{0.5}} - \frac{1}{T_{0.75}}) \qquad (16)$$

$$dH = -0.0032 * (\frac{1}{T_{0.5}} - \frac{1}{T_{0.75}}) \qquad (17)$$

The initial $T_{m</sub}$ is estimated from the $T_{0.5}$, determined in step 5.

3.2.2 Thermodynamic models for duplex formation

Thermo-dynamic parameters for helix formation are obtained using a Van't Hoff model:

$$lnK = \frac{dS}{R} - \frac{dH}{RT} \qquad (18)$$

where dS is the entropy change, dH is the enthalpy change, R is the gas constant in kcal/mol, T is the temperature in Kelvin, and K is the equillibrium constant given by Equation 19, Equation 20, and Equation 21 for heteroduplexes, homoduplexes, and monomolecular self-structured RNA respectively.

$$K = \frac{[AB]}{[A][B]} \qquad (19)$$

$$K = \frac{[AA]}{[A]^2} \qquad (20)$$

$$K = \frac{[F]}{[U]} \qquad (21)$$

For Equation 19 and Equation 20, [A] and [B] are the concentration of different strands, [AB] is the concentration of strand A in a duplex with strand B, and [AA] is the concentration of a self complementary strand A in a duplex with another self complementary strand A. For Equation 21, [F] is the concentration of a monomolecular self-structured RNA in the folded state and [U] is the concentration of a monomolecular sel-structured RNA in the unfolded state.

MeltR uses three methods based on the Van't Hoff equation to calculate thermodynamic parameters: (1) fitting melting curves individually, (2) fitting the thermodenaturation point as a function of temperature, and (3) Global fitting melting curves.

3.2.3 Method 1 fitting melting curves individually

Method 1 fits the absorbtion as a function of temperature for each sample individually. Base lines are modeled as y= mx + b for the absorbance of the unfolded-single standed and folded-duplex states (Equation 22).

$$E = mT + b \qquad (22)$$

The absrorbtion of each sample as a function of temperature is also a function of the fraction of RNA in the folded-duplex state (DS), as a function of temperature f(T), given by Equation 23. SS represents the RNA in the single-stranded state.

$$E = (m_{DS}T + b_{DS})f(T) + (m_{SS}T + b_{SS})(1 - f(T)) \qquad (23)$$

f(t) is variable, calculated by the analytic solution of the binding constant. MeltR uses Equation 24 for heteroduplexes, Equation 25 for homoduplexes, and Equation 26 monomolecular self-structured RNA.

$$f(T) = \frac{\frac{2}{K(T)*Ct} + 2 - \sqrt{(\frac{2}{K(T)*Ct} + 2)^2 - 4}}{2} \qquad (24)$$

$$f(T) = \frac{\frac{1}{2*K(T)*Ct} + 2 - \sqrt{(\frac{1}{2*K(T)*Ct} + 2)^2 - 4}}{2} \qquad (25)$$

$$f(T) = \frac{K(T)}{1 + K(T)} \qquad (26)$$

Where C_t is the total strand concentration. K(T) is the equillibrium constant as a function of temperature, given by Equation 27 for heteroduplexes, Equation 28 for homoduplexes, and Equation 29 for monomolecular self-structured RNA.

$$K(T) = \exp\left(\frac{dH}{R}\left(\frac{1}{T_m} - \frac{1}{T}\right) + ln\left(\frac{4}{Ct}\right)\right) \qquad (27)$$

$$K(T) = \exp\left(\frac{dH}{R}\left(\frac{1}{T_m} - \frac{1}{T}\right) + ln\left(\frac{1}{Ct}\right)\right) \qquad (28)$$

$$K(T) = \exp\left(\frac{dH}{R}\left(\frac{1}{T_m} - \frac{1}{T}\right)\right) \qquad (29)$$

Note, K(T) has solved in terms of T_m and C_t, instead of the dS, to increase the ease of estimating initial parameters for non-linear regression and to increase

the robustness of the nls algorithm. Briefly, the dS is replaced with T_m and C\textsubscript{t by solving Equation 18 for the dS at the T_m, where f(t) = 0.5.

Thus, method 1 fits absorbtion versus temperature for each sample to equations 30, 31, and 32 to determine thermodynamic prameters for heteroduplexes, homoduplexes, and monomolecular self-structured RNA respectively.

$$E = (m_{DS}T + b_{DS})\frac{\frac{2}{\exp\left(\frac{dH}{R}\left(\frac{1}{T_m} - \frac{1}{T}\right) + ln(\frac{4}{Ct})\right)*Ct} + 2 - \sqrt{\left(\frac{2}{\exp\left(\frac{dH}{R}\left(\frac{1}{T_m} - \frac{1}{T}\right) + ln(\frac{4}{Ct})\right)*Ct} + 2\right)^2 - 4}}{2} + (m_{SS}T + b_{SS})(1 -$$

$$E = (m_{DS}T + b_{DS})\frac{\frac{1}{2*\exp\left(\frac{dH}{R}\left(\frac{1}{T_m} - \frac{1}{T}\right) + ln(\frac{1}{Ct})\right)*Ct} + 2 - \sqrt{\left(\frac{1}{2*\exp\left(\frac{dH}{R}\left(\frac{1}{T_m} - \frac{1}{T}\right) + ln(\frac{1}{Ct})\right)*Ct} + 2\right)^2 - 4}}{2} + (m_{SS}T + b_{SS})($$

$$E = (m_{DS}T + b_{DS})\frac{\exp\left(\frac{dH}{R}\left(\frac{1}{T_m} - \frac{1}{T}\right)\right)}{1 + \exp\left(\frac{dH}{R}\left(\frac{1}{T_m} - \frac{1}{T}\right)\right)} + (m_{SS}T + b_{SS})(1 - \frac{\exp\left(\frac{dH}{R}\left(\frac{1}{T_m} - \frac{1}{T}\right)\right)}{1 + \exp\left(\frac{dH}{R}\left(\frac{1}{T_m} - \frac{1}{T}\right)\right)}) \qquad (32)$$

Free energy at 37 degC (dG) is calculated from the dH and entropy (dS) of helix formation

$$dG = dS - 310.15 * dS \qquad (33)$$

The dS of helix formation is calculated from the dH and the Tm.

For heteroduplexes:

$$dS = \frac{dH}{Tm} + Rln(\frac{4}{Ct}) \qquad (34)$$

For homoduplexes:

$$dS = \frac{dH}{Tm} + Rln(\frac{1}{Ct}) \qquad (35)$$

For monomolecular self-structured RNA/DNA:

$$dS = \frac{dH}{Tm} \qquad (36)$$

Error in the dS and dG is calculated by propagating error in the fit terms dH and T_m.

$$SE_{dS} = |dS| \sqrt{(\frac{SE_{dH}}{dH})^2 + (\frac{SE_{Tm}}{Tm})^2 - 2\frac{Covar_{dH,Tm}}{dH * Tm}} \qquad (37)$$

$$SE_{dG} = \sqrt{SE_{dH}{}^2 + (310.15 * \frac{SE_{dH}}{dH})^2 + (310.15 * \frac{SE_{Tm}}{Tm})^2 - 2 * 310.15\frac{Covar_{dH,Tm}}{dH * Tm}} \qquad (38)$$

3.2.4 Method 2 fitting the T_m as a function of C_t

Method 2 fits the relationship between $1/T_m$ and the total strand concentration C_t. To avoid inaccuracies in T_m determination from first derivative plots or covariation with the dH terms in method 1, T_ms were determined for Method 2 using a semi-quantitative method. Slopes and intercepts from method 1 were used to calculate F(T) at each experimental temperature using the absorbance.

$$F(T) = \frac{A - (m_{SS}T + b_{SS})}{(m_{DS}T + b_{DS}) + (m_{SS}T + b_{SS})} \qquad (39)$$

F(T) is approimatelty linear in the range of 0.4 to 0.6. Thus, F(T in {0.4 to 0.6}) was fit with y = mT + b, and solved using y = 0.5 to accurately determine the melting temperature for each C_t. To determine thermodynamic parameters, the relationship between $1/T_m$ and the total strand concentration was then fit to Equations 40, and 41, for heteroduplexes and homoduplexes respectively. The T_m of monomolecular, self-structured RNA is independent of C_t so Method 2 cannot be used.

$$\frac{1}{T_m} = \frac{R}{dH} * lnC_t + \frac{dS}{dH} - R * ln(4) \qquad (40)$$

$$\frac{1}{T_m} = \frac{R}{dH} * lnC_t + \frac{dS}{dH} \qquad (41)$$

Free energy at 37 °C (dG) is calculated from the dH and entropy (dS) of helix formation directly from the fit.

$$dG = dS - 310.15 * dS \qquad (42)$$

Error in the dG is calculated by propagating error in the fit terms dH and dS.

$$SE_{dG} = \sqrt{SE_{dH}{}^2 + (310.15 * \frac{SE_{dS}}{dS})^2 - 2 * 310.15 * \frac{Covar_{dH,dS}}{dH * dS}} \qquad (43)$$

12

3.2.5 Method 3 Global fitting

Method 3 fits all curves to Equations 44, 45, and 46, simultaneously in a global fit, for heteroduplexes, homoduplexes, and mono-molecular self-structured RNA/DNA respectively. In this global fit, Equations 30, 31, and 31, are rearranged to be in terms of the dS instead of the Tm.

$$
E = (m_{DS}T + b_{DS})\frac{\frac{2}{\exp\left(\frac{dS}{R} - \frac{dH}{RT}\right)*Ct} + 2 - \sqrt{\left(\frac{2}{\exp\left(\frac{dS}{R} - \frac{dH}{RT}\right)*Ct} + 2\right)^2 - 4}}{2} + (m_{SS}T + b_{SS})(1 - \frac{\frac{2}{\exp\left(\frac{dS}{R} - \frac{dH}{RT}\right)*Ct} + 2 -
$$

$$
E = (m_{DS}T + b_{DS})\frac{\frac{1}{2\exp\left(\frac{dS}{R} - \frac{dH}{RT}\right)*Ct} + 2 - \sqrt{\left(\frac{1}{2*\exp\left(\frac{dS}{R} - \frac{dH}{RT}\right)*Ct} + 2\right)^2 - 4}}{2} + (m_{SS}T + b_{SS})(1 - \frac{\frac{1}{2*\exp\left(\frac{dS}{R} - \frac{dH}{RT}\right)*Ct} +
$$

$$
E = (m_{DS}T + b_{DS})\frac{\exp\left(\frac{H}{R*Tm} - \frac{1}{Tm}\right)}{1 + \exp\left(\frac{dS}{R} - \frac{dH}{RT}\right)} + (m_{SS}T + b_{SS})(1 - \frac{\exp\left(\frac{dS}{R} - \frac{dH}{RT}\right)}{1 + \exp\left(\frac{dS}{R} - \frac{dH}{RT}\right)}) \qquad (46)
$$

The baselines are allowed to vary but dHs and dSs are constrained to a single value for all curves. For global fitting, the slopes and intercepts of the fits from Method 1 are used as initial parameter estimates for the slopes and intercepts of the global fit, and the average of the dHs and dSs from Method 1 are used as initial parameter estimates for the dH and dS.

The dG and error in the dG is calculated using the same equations as Method 2.

4 Running MeltR

In this section, we cover how to use MeltR in your R console. If you have not already, read section 3 to understand the theory underlying the results of MeltR. In constrast, section 4 will cover MeltR usage and how to avoid pitfalls. The most common error with MeltR is a user attempting to fit data that is inconsistent with the underlying model, either a fluorescence isotherm or a absorbance melting curve with a non-standard shape or specifying an incorrect molecular model. In the case of data-with a non-standard shape, the aberrant data will need to be subsetted out data set prior to fitting the set with MeltR. While MeltR has no dependencies other than base R 4.1.3, data wrangling and plotting functions in the "tidyverse" package[4] are highly recommended, along with the "ggrepel" package[5], for data quality checks and filtering. To begin, open a new R session in the proper directory. Load relevant packages into your memory.

```
library(MeltR)
library(tidyverse)
library(ggrepel)
```

Help documentation for MeltR functions can be pulled up using standard R commands.

```
?meltR.F
?meltR.A
```

4.1 Fitting fluorescence binding isotherms

4.1.1 Formatting fluorescence data for MeltR

Data should be formatted into a comma separated value ("csv") text file with carefully labeled columns (Figure 3). There should be a "Well" column where numbers or character strings specify what well in a microplate the data came from, a "Reading" column that specifies the reading a data point comes from, a "Temperature" column that specifies the temperature where the data was recorded, a "B" column which specifies an approximate quencher labeled strand concentration in nM, an "A" column which specifies an approximate fluorophore labeled strand concentration in nM, and an "Emission" column containing the fluorescence emission intensity.

Helix	Well	Reading	Temperature	B	A	Emission
B	A3	1	20.0076	0	200	1.42
B	B7	1	20.0069	0	200	1.48
B	C12	1	19.9922	0	200	1.59
B	A3	2	20.5069	0	200	1.42
B	B7	2	20.4986	0	200	1.49
B	C12	2	20.4957	0	200	1.60
B	A3	3	20.9964	0	200	1.42

Figure 3: Formatting fluorescence binding isotherm datat in a csv file for MeltR with Excel

Two common pitfalls occur when formatting data for MeltR, usually in Excel. The first is incorrect column names, even incorperation of an extra space, so that MeltR cannot recognize relevant data when it is read into R. The second is incorperation of characters into data columns when values are missing. If a data point is missing, leave the cell blank. Do not write something like "NA".

4.2.3 Reading data into a R data frame

Comma separated value ("csv") data can be read into a R data frame for MeltR using the "read.csv" function that is included in base R.

```
df = read.csv("path/file_name.csv")
```

Data can be checked with the "View" function.

```
View(df)
```

Note, the columns in "df" must be named correctly. If the columns are not named correctly, MeltR cannot recognize them. You can rename the columns of a data frame using:

```
colnames(df) = c("Helix", "Well", "Reading", "Temperature", "B", "A", "Emission")
```

4.1.3 Applying "meltR.F" to obtain thermodynamic parameters

For this tutorial, we will use sample data included in MeltR. First check that MeltR is in your memory and find out what is in the sample data.

```
?df.fluor.data
df = df.fluor.data
```

In general, it is a good idea to plot your data before you start fitting. First, I want to check the quality of low temperature isotherms. Using the tidyverse and ggrepel.

```
head(df)
ggplot(df %>% filter(Reading == 1), aes(x = B, y = Emission, label = Well)) +
  geom_point() +
  geom_text_repel()
```

The result is a really nice binding isotherm (Figure 4). One should check a few more readings by changing the value in the filter command, for example 20, 60, 80, etc...

If you observe one or two ovious outliers in the data set, it is reasonable to remove them using the filter. However, this data is excellent and needs no filtering.

```
df %>% filter(!Well %in% c("A1", "C3"))
```

If you are satified with the the data, we can move on to fitting. I will first inspect the help file for meltR.F.

```
?meltR.F
```

The only argument that needs set is data frame.

```
meltR.F(df)
```

You will see the following output in your console.

```
> meltR.F(df)
[1] "Van't Hoff"
[1] "accurate Ks = 16"
      Method         H     SE.H        S      SE.S        G      SE.G
1   1 VH plot -48.37473 1.048500 -121.6157  3.357021 -10.65562 0.01033199
```
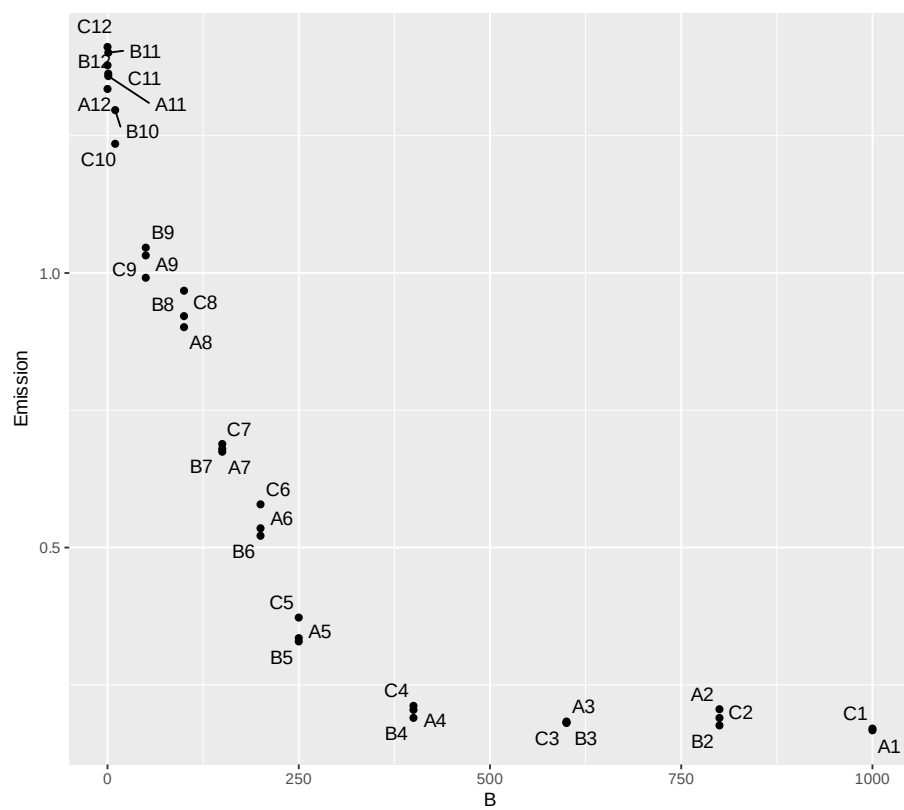
Figure 4: Isotherm_example

```
2 2 Global fit -48.88546 6.302188 -123.2438 20.157522 -10.66140 0.06564137
    K_error         R    Kd.opt
1 0.2916302 0.7797618 6.165553
2 0.2916302 0.7797618 6.165553
[1] "Fractional error between methods"
            H         S         G
1 0.01050236 0.013298 0.000542719
```

Note, the concentration optimization algorithm, by default allowing the Kd.opt to float, identified an optimal R of ~0.78. Since the FAM-RNA strand in each well is estimated at 200 nM, the concentration optimization algorith will adjust the concentration to $200/0.78 = 256$ nM. We will test the robustness of this estimate by constrianing the Kd.op range of KDs that are more than 10 times less than the FAM-RNA concentraion, using the "low_K" argument. For example, 1, 0.5, 0.1, and 0.05 nM. Note, the mole ratio "R" was labeled "X" in the theory section to avoid confusion with the gas constant.

```
> meltR.F(df, low_K = 1)
[1] "Van't Hoff"
[1] "accurate Ks = 14"
        Method          H        SE.H          S        SE.S          G          SE.G   K_error
1     1 VH plot -60.00212 0.7271876 -158.3742   2.317695 -10.88235 0.009438972 0.345963 0.7231
2 2 Global fit -60.25007 8.9451153 -159.1598  28.490520 -10.88665 0.120521827 0.345963 0.7231
[1] "Fractional error between methods"
            H          S          G
1 0.004123788 0.004947968 0.0003951875
> meltR.F(df, low_K = 0.5)
[1] "Van't Hoff"
[1] "accurate Ks = 14"
        Method          H        SE.H          S        SE.S          G          SE.G   K_error
1     1 VH plot -62.21273 0.6849323 -165.3667   2.179732 -10.92425 0.009800243 0.3552451 0.715
2 2 Global fit -62.39456 9.1846917 -165.9409  29.214906 -10.92800 0.134594527 0.3552451 0.715
[1] "Fractional error between methods"
            H          S          G
1 0.002918411 0.003466106 0.0003430056
> meltR.F(df, low_K = 0.1)
[1] "Van't Hoff"
[1] "accurate Ks = 14"
        Method          H        SE.H          S       SE.S          G          SE.G   K_error
1     1 VH plot -63.08832 0.6549918 -168.1096   2.08445 -10.94912 0.009371838 0.3609151 0.7080
2 2 Global fit -63.28360 9.3633293 -168.7267  29.78152 -10.95302 0.137643619 0.3609151 0.7080
[1] "Fractional error between methods"
            H          S          G
1 0.003090634 0.003664033 0.0003556102
> meltR.F(df, low_K = 0.05)
[1] "Van't Hoff"
[1] "accurate Ks = 14"
```

```
       Method       H      SE.H       S      SE.S       G        SE.G   K_error
1    1 VH plot -63.21087 0.6507751 -168.4935  2.07103 -10.95260 0.009311504 0.3617203 0.7070
2 2 Global fit -63.40791 9.3886281 -169.1162 29.86176 -10.95651 0.138076127 0.3617203 0.7070
[1] "Fractional error between methods"
            H          S           G
1 0.003112448 0.003688944 0.0003572172
```

The concentration with constrained Kds optomization algorithm adjusts the FAM-RNA concentration to at most 281, about 10% difference between constrained K_ds and a floating K_D. Thus, the default concentration optimization is robust. Note that there is considerable variance in the enthalpies, entropies, and free energies from the various constrained K_Ds and the unconstrained fit (about 20 kcal/mole in terms of the enthalpy). We will demonstrate how to refine these thermodynamic parameters independent of the concentration optimization algorithm in section 4.1.5.

4.1.4 Saving meltR.F outputs

meltR.F results can be saved to the disk using the "Save_results" argument.

```
meltR.F(df,
        Save_results = "all")
```

The "file_prefix" argument can be used to add a custom file name to the outputs.

```
meltR.F(df,
        Save_results = "all",
        file_prefix = "Helix_J")
```

This will create three pre-canned outputs. The first output, corresponding to Method 1, is a Van't Hoff plot (Figure 5A). Points represent the Kd and error from fitting isotherms individually. The red line represents the fit to Equation 6 that provides thermodynamic parameters. The blue line and orange line represents the lower and upper limit of the range of Kd values included in the fit. The second output, corresponding to Method 2, is a depiction of the global fit, where points represent raw data and red lines represent the global fit (Figure 5B). The third output is a .csv file containing the thermodynamic parameters from each method Figure 5 C. Note that the fit line (red) in Figure 5A does not follow the trend at high temperatures and the helix folding energies from this line are thus unreliable. We will cover refining the fits in the next section.

4.1.5 Refining meltR.F fits

Two arguments are important for refining meltR.F fits. The first is, "Kd_range", which is the range of K_Ds in nM that will be fit to obtain thermodynamic parameters. By default, the "Kd_range" is set to 10 to 1000. The second is, "Kd_error_quantile", which controls the amount of error that is included in the K_Ds that will be fit to obtain thermodynamic parameters. By default, the
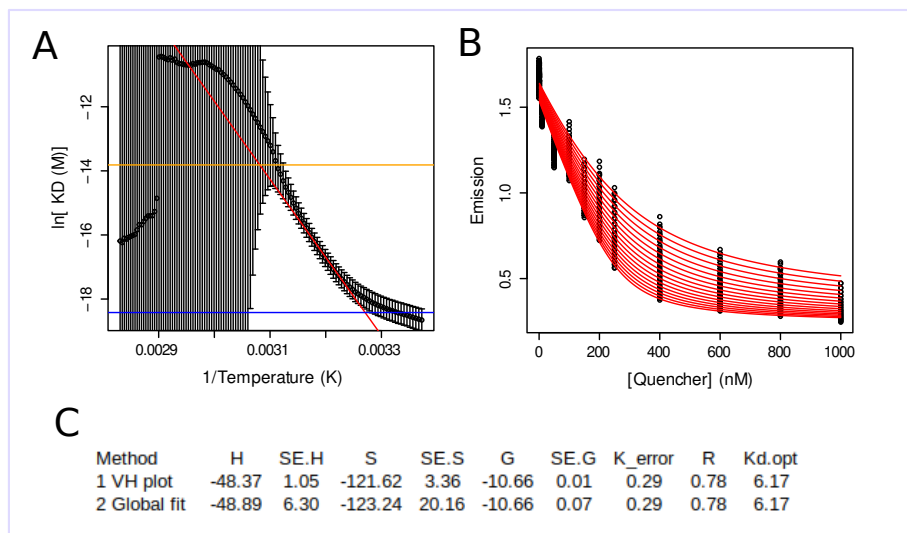
Figure 5: Pre-canned meltR.F outputs

"Kd_error_quantile" is 0.25, meaning only the 25% most accurate KDs in the "K_range" will be fit to obtain thermodynamic parameters.

As a first guess, the K_D range should start about 10 times less than the Fluorophore labeled RNA strand concentration and end at about 10 times more than the Fluorophore labeled RNA strand, and the "Kd_error_quantile" should be conservative, near 0.25. After this, the Van't Hoff plot should be inspected, for how well the fit matches the linear range. In general, constraining the "Kd_range" and loostening the "Kd_error_quantile" results in the best fits. For example, a "Kd_range" of 40 to 500 nM and a "Kd_error_quantile" of 0.5 works well for the sample data (Figure 6).

```
meltR.F(df,
        Kd_range = c(40, 500),
        Kd_error_quantile = 0.5,
        Save_results = "all")
```

with an output of:

```
[1] "Van't Hoff"
[1] "accurate Ks = 18"
        Method          H       SE.H          S        SE.S          G         SE.G
1    1 VH plot -60.60235 0.964952 -160.5832   3.057177 -10.79747 0.01834264
2 2 Global fit -59.90460 6.321305 -158.3554 20.049234 -10.79066 0.11245376
   K_error         R    Kd.opt
1 6.182951 0.7797618 6.165553
2 6.182951 0.7797618 6.165553
```

19

```
[1] "Fractional error between methods"
            H          S          G
1 0.01158036 0.01397017 0.0006300081
>
```

Note two things: (1) the refined fit uses more isotherms than the original iterations
of the program, where we were checking the concentration optimization algorithm
in Section 4.1.3, with an "accurate Ks" count of 18 instead of 14. (2) The the
thermodynamic parameters are closer to the fits with constrained "low_Ks",
with a difference of about 5% in terms of the enthalpy and 1% in terms of the
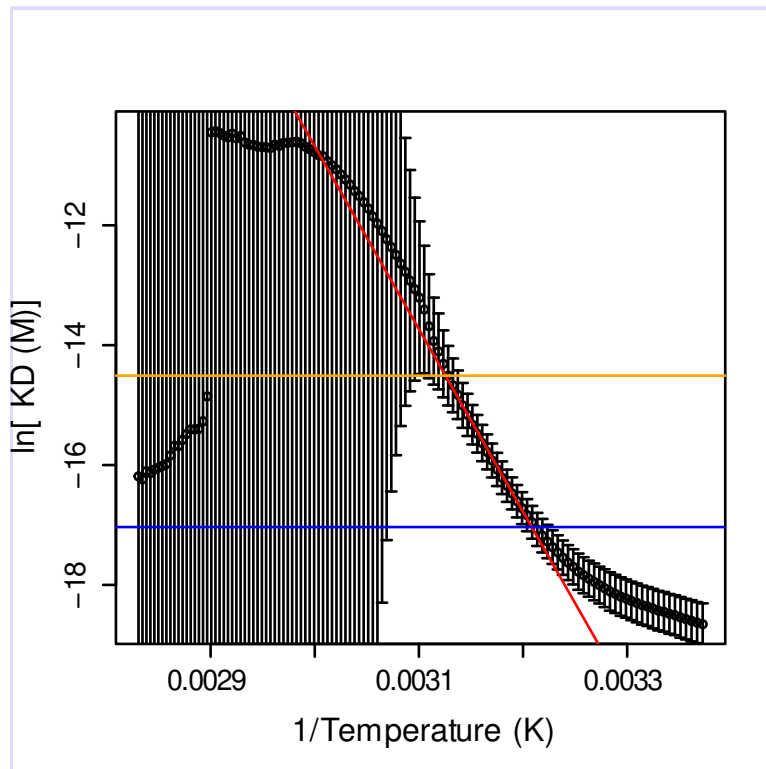free energy.

Figure 6: Refined Van't Hoff plot

4.1.6 Advanced analysis of meltR.F outputs in R

meltR.F can pass a more extensive output to an object in R.

```
MeltR.fit = meltR.F(df,
        Kd_range = c(40, 500),
        Kd_error_quantile = 0.5,
        Save_results = "all")
```

20

The object, "MeltR.fit" is now a list of objects that can be passed to plotting functions.

```
names(MeltR.fit)
```

Which will print the names of the list "MeltR.fit".

```
[1] "VantHoff"                          "K"
[3] "VH_method_1_fit"                   "VH_method_2_fit"
[5] "Raw_data"                          "First_derivative"
[7] "Tms"                               "R"
[9] "Fractional_error_between_methods"
```

[1] VantHoff: is a data frame containing the duflex formation energies. It can be called using:

```
MeltR.fit$VantHoff
```

[2] K: is a data frame containing the results from fitting each isotherm individually. It can be called using:

```
MeltR.fit$K
```

[3] VH_method_1_fit: is a nls object containing the fit obtained from the Van't Hoff plot. It can be called using:

```
MeltR.fit$VH_method_1_fit
```

[4] VH_method_2_fit: is a nls object containing the fit obtained from the global fit. It can be called using:

```
MeltR.fit$VH_method_2_fit
```

[5] Raw_data: The raw data passed back out of MeltR.F with no modifications. It can be called using:

```
MeltR.fit$Raw_data
```

[6] First derivative: The dirst derivative of each sample. Useful for qualitative comparison of data between conditions. It can be called using:

```
MeltR.fit$First_derivative
```

[7] Tms: The approximate T_m of each sample obtained from the maximum of the first derivative. Useful for qualitative comparison of data between solution conditions. It can be called using:

```
MeltR.fit$Tms
```

[8] R: the mole ratio of fluorophore and quencher labeled RNA, used in the concentration optimization algorithm. The mole ratio "R" was labeled "X" in the theory section to avoid confusion with the gas constant. It can be called using:

```
MeltR.fit$R
```

[9] Fractional error between Methods: The amount thermodynamic parameters vary between methods. It can be called using:

```
MeltR.fit$Fractional_error_between_methods
```

4.2 Fitting Absorbance Melting Curves in MeltR

4.2.1 Formatting absorbance data for MeltR

Data should be formatted into a comma separated value (".csv") text file with carefully labeled columns (Figure 7). There should be a "Sample" column where numbers or character strings specify what sampe the absorbance data was collected on. There should be one buffer blank in the data set for background subtraction. If no blank is availible, add data with an absorbance of 0 recorded at each temperature. A "Pathlength" column specifies the pathlength in cm of the cuvette the data was collected in. A "Temperature" column specifies the temperature in °C where the data was recorded. Lastly, a "Absorbance" column specifies the absorbance collected at each temperature.

Sample	Pathlength	Temperature	Absorbance
1	1	4.78	0.004394531
1	1	5.5	-0.000579834
1	1	6.03	7.78E-04
1	1	6.52	0.001037598
1	1	7.03	0.001068115
1	1	7.53	0.001678467
1	1	8.02	0.001800537

Figure 7: Formatting absorbance melting curve data in a csv in Excel

Two common pitfalls occur when formatting data for MeltR, usually in Excel. The first is incorrect column names, even incorperation of an extra space, so that MeltR cannot recognize data when it is read into R. The second is incorperation of characters into data columns when values are missing. If a data point is missing, leave the cell blank. Do not write something like "NA".

4.2.2 Reading data into a R data frame

Comma separated value (".csv") data can be read into a R data frame for MeltR using the "read.csv" function that is included in base R.

```
df = read.csv("path/file_name.csv")
```

Data can be checked with the "View" function.

```
View(df)
```

Note, the columns in "df" must be named correctly. If the columns are not named correctly, MeltR cannot recognize them. You can rename the columns of a data frame using:

```
colnames(df) = c("Sample", "Pathlength", "Temperature", "Absorbance")
```

4.2.3 Applying meltR.A to obtain thermodynamic parameters

Sample data is included in MeltR and can be loaded into your memory and checked.

```
?df.abs.data
df = df.abs.data
```

In general, it is a good idea to plot your data before you start fitting. First, I want to check the quality of low temperature isotherms. Using the tidyverse.

```
head(df)
ggplot(df, aes(x = Temperature, y = Absorbance, color = factor(Sample))) +
  geom_point() +
  theme_classic()
```

This data looks good (Figure 8), with a small and consistent blank absorbance and sigmoidal RNA melting curves. If one of the RNA melting curves does not resemble a sigmoid, it should be removed from the data set using:

```
df %>% filter(Sample != "Sample you want to remove")
```

Data can now be fit using meltR.A. First we need to define the nucleic acid sequence using a vector that specifies the RNA or DNA sequences used in the experiment.

```
helix = c("RNA", "CGAAAGGU", "ACCUUUCG")
```

meltR.A requires information from 4 user defined arguments to fit the data: the data frame the absorbance data is stored in, the blank sample, the nucleic acid sequences, and the molecular model. Three molecular models are availible in MeltR, "Monomolecular.2State", "Heteroduplex.2State", and "Homoduplex.2State". The absorbance sample data included in MeltR was collected on a heteroduplex.

```
?meltR.A
meltR.A(data_frame = df,
        blank = 1,
        NucAcid = helix,
        Mmodel = "Heteroduplex.2State")
```

The output looks like this.

```
[1] "Individual curves"
  Sample          Ct      H       S      G   Tm
1      2 2.832690e-06 -63.5 -0.1725  -9.9 43.1
2      3 4.718659e-06 -71.2 -0.1969 -10.1 44.6
```
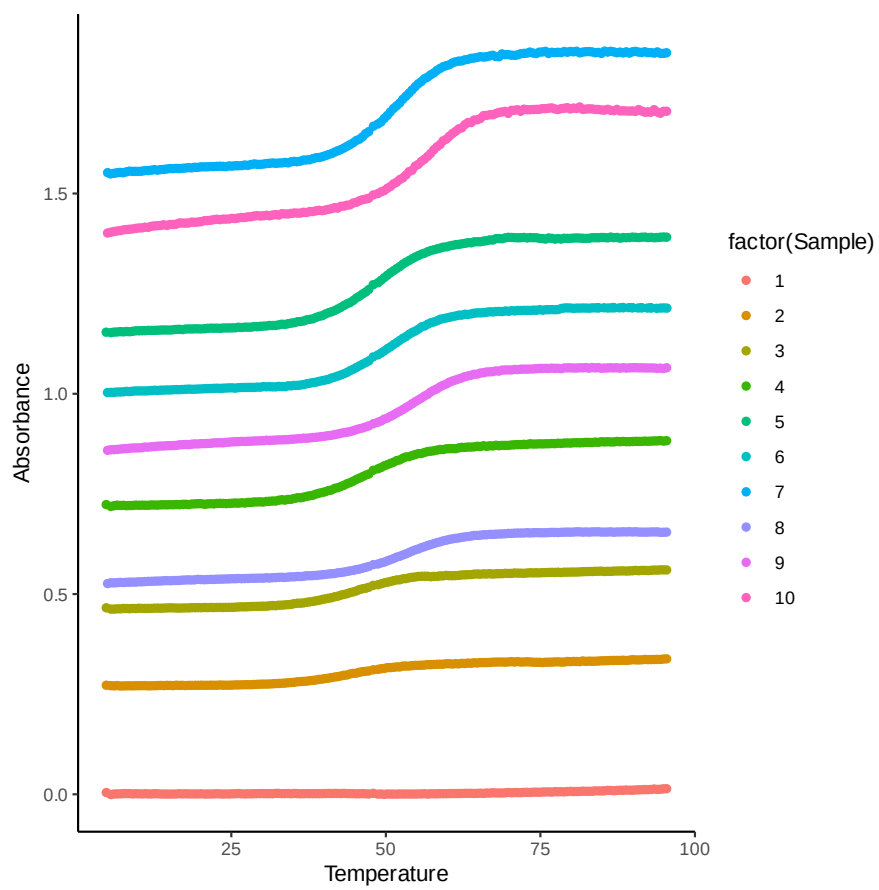
23

Figure 8: Check absorbance data

```
3       4 7.439046e-06 -64.8 -0.1764 -10.0 46.4
4       5 1.173670e-05 -64.5 -0.1752 -10.1 48.4
5       6 2.049582e-05 -70.9 -0.1952 -10.4 50.0
6       7 3.131297e-05 -74.3 -0.2055 -10.5 51.4
7       8 5.533500e-05 -71.6 -0.1974 -10.4 53.0
8       9 8.990554e-05 -74.8 -0.2069 -10.7 54.8
9      10 1.439218e-04 -76.7 -0.2121 -11.0 57.0
[1] "Summary"
              Method       H SE.H       S SE.S      G SE.G
1  1 individual fits -70.3  4.9 -193.1 14.9 -10.4  0.3
2 2 Tm versus ln[Ct] -60.4  1.2 -163.0  3.8  -9.9  0.1
3        3 Global fit -69.7  0.3 -191.3  1.0 -10.4  0.0
[1] "fractional error between methods"
          H         S         G
1 0.1482036 0.1649616 0.04885993
```

Note that the fractional error between the methods is over about 15% in terms of the enthalpy. Section X.X discusses how to refine the fits by trimming the absorbance baselines.

4.2.4 Saving meltR.A outputs

meltR.F results can be saved to the disk using the "Save_results" argument.

```
meltR.A(data_frame = df,
        blank = 1,
        NucAcid = helix,
        Mmodel = "Heteroduplex.2State",
        Save_results = "all")
```

The "file_prefix" argument can be used to add a custom file name to the outputs

```
meltR.A(data_frame = df,
        blank = 1,
        NucAcid = helix,
        Mmodel = "Heteroduplex.2State",
        Save_results = "all",
        file_prefix = "Helix")
```

This will create seven pre-canned outputs. The first and second outputs are depictions of the fits in method Method 1, with the individual fits (red lines) overlayed on raw data (Figure 9A) and normalized data generated by calculating the absorbtivity (extinction coefficient) at each temperature (Figure 9B). The third output is a depiction of the fit in Method 2, with the fit overlayed on the Tm data at each strand concentration (Figure 9C). The fourth and fifth outputs are depictions of the fit in method Method 3, with the global fits (red lines) overlayed on raw data (Figure 9D) and normalized data generated by calculating the absorbtivity (extinction coefficient) at each temperature (Figure 9E). The

sixth output is a .csv file containing the thermodynamic parameters generated by individual fits (Figure 9F). The seventh output is a .csv file containing the thermodynamic parameters from each method (Figure 9G).
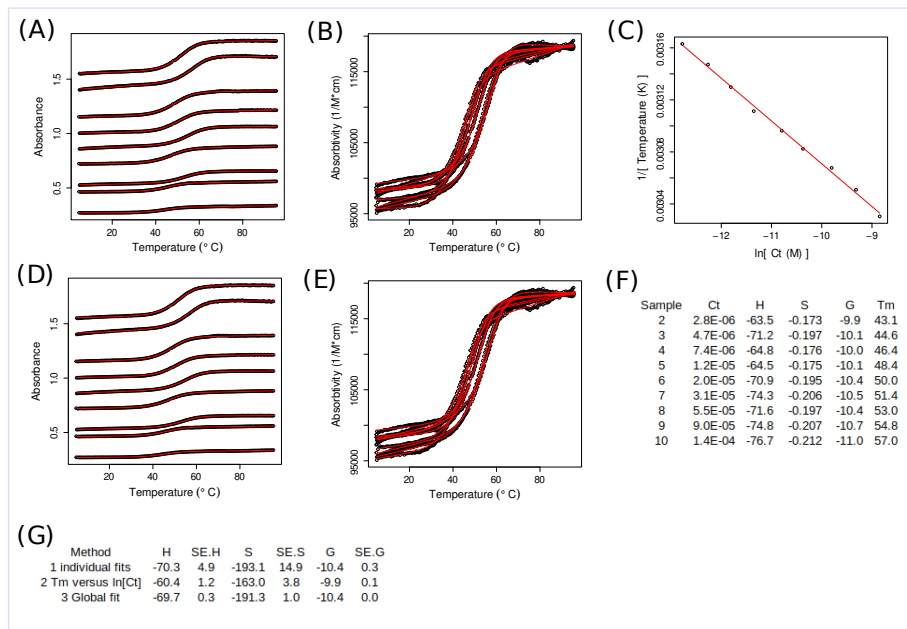

Figure 9: Absorbance outputs

4.2.5 Refining MeltR.A fits by trimming fluorescence baselines.

MeltR approximates absorbance baselines using a line (y = mx+b). Real absorbance data deviates from this linear behavior over wide temperature ranges. MeltR fits are thus improved by trimming the baselines so that baselines better approximate a line. First, the raw data should be inspected for linear baselines one sample at a time using the tidyverse.

```
ggplot(df %>% filter(Sample == 10), #Only plot sample 10
aes(x = Temperature, y = Absorbance, color = factor(Sample))) +
  geom_point() +
  theme_classic() +
  geom_vline(xintercept = c(15, 70)) #will add horizontal lines to the plot at 15 and 70
```

Thus, for Sample 2, baselines are approximately linear above 15 °C and below 70 °C (Figure X).

This should be repeated for each sample that contains RNA). After identifying ranges where baselines are linear, ranges can be supplied to the "fitTs" argument as a list of vectors (in the order of the samples in the data set). Note, do not
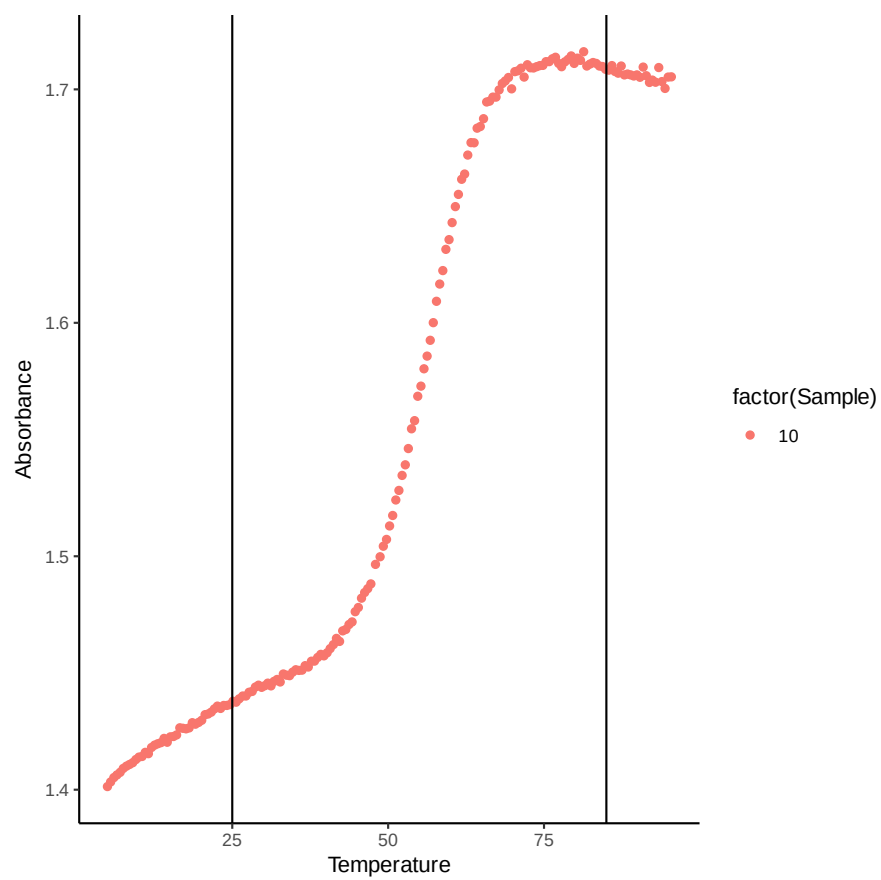
Figure 10: Baseline trimming on Sample 10

provide a temperature range for the blank.

```
list.T.range = list(c(15, 70), #Sample 2
                    c(15, 70), #Sample 3
                    c(15, 80), #Sample 4
                    c(15, 85), #Sample 5
                    c(20, 78), #Sample 6
                    c(20, 85), #Sample 7
                    c(20, 85), #Sample 8
                    c(25, 85), #Sample 9
                    c(25, 85)) #Sample 10

meltR.A(data_frame = df,
        blank = 1,
        NucAcid = helix,
        Mmodel = "Heteroduplex.2State",
        Save_results = "all",
        file_prefix = "Trimmed",
        fitTs = list.T.range)
```

Which will produce:

```
[1] "Individual curves"
  Sample            Ct      H       S      G   Tm
1      2 2.832690e-06 -67.2 -0.1849  -9.9 42.4
2      3 4.718659e-06 -71.6 -0.1984 -10.1 44.5
3      4 7.439046e-06 -65.3 -0.1783 -10.0 46.1
4      5 1.173670e-05 -61.9 -0.1676 -10.0 47.9
5      6 2.049582e-05 -66.3 -0.1813 -10.0 49.3
6      7 3.131297e-05 -71.2 -0.1964 -10.3 50.8
7      8 5.533500e-05 -68.9 -0.1894 -10.1 52.3
8      9 8.990554e-05 -68.4 -0.1879 -10.1 53.9
9     10 1.439218e-04 -71.0 -0.1952 -10.4 56.1
[1] "Summary"
              Method     H SE.H      S SE.S      G SE.G
1  1 individual fits -68.0  3.2 -186.6  9.9 -10.1  0.2
2 2 Tm versus ln[Ct] -62.2  1.4 -168.9  4.5  -9.9  0.1
3        3 Global fit -67.4  0.3 -184.7  0.9 -10.1  0.0
[1] "fractional error between methods"
           H          S          G
1 0.08805668 0.09829693 0.01993355
```

The fitting trimmed baselines reduces the fractional error between the methods from 15% to 9% in terms of the enthalpy.

4.2.6 Advanced plotting meltR.A outputs using the "tidyverse"

meltR.A can pass a more extensive output to an object in R.

```
MeltR.fit = meltR.A(data_frame = df,
        blank = 1,
        NucAcid = helix,
        Mmodel = "Heteroduplex.2State",
        Save_results = "all",
        file_prefix = "Trimmed",
        fitTs = list.T.range)
```

The object, "MeltR.fit" is now a list of objects that can be passed to plotting functions.

```
names(MeltR.fit)
```

Which will print a list of fit names:

```
 [1] "Summary"          "Method.1.indvfits" "Range"
 [4] "Derivatives.data"  "Method.1.data"     "Method.1.fit"
 [7] "Method.2.data"     "Method.2.fit"      "Method.3.data"
[10] "Method.3.fit"
```

[1] Summary: A data frame containing the thermodynamic parameters from each method. It can be called using:

```
MeltR.fit$Summary
```

[2] Method.1.indfits: A data frame containint the thermodynamic parameters from the individual fits.It can be called using:

```
MeltR.fit$Method.1.indvfits
```

[3] Fractional error between Method 1, 2, and 3. It can be called using:

```
MeltR.fit$Range
```

[4] Derivatives.data: Contains the first and second derivatives for each sample containing RNA. It can be called and plotted using:

```
MeltR.fit$Derivatives.data
ggplot(MeltR.fit$Derivatives.data, aes(x = Temperature, y = dA.dT/(Pathlength*Ct), color = 1
  geom_point() +
  theme_classic()
```

[5] Method.1.data: Contains the raw data from method 1 and the model. It can be called and plotted using:

```
MeltR.fit$Method.1.data
ggplot(MeltR.fit$Method.1.data, aes(x = Temperature, color = factor(Sample), group = factor(
  geom_point(mapping = aes(y = Absorbance/(Pathlength*Ct))) +
  geom_line(mapping = aes(y = Model/(Pathlength*Ct)), color = "black") +
  theme_classic()
```

[6] MeltR.fit$Method.1.fit: A list of nls objects containing the fits obtained from fitting melting curves individually. It can be called using:

```
MeltR.fit$Method.1.fit
```

[7] MeltR.fit$Method.2.data: Contains the raw data from method 1 and the model. It can be called and plotted using:

```
MeltR.fit$Method.2.data
ggplot(MeltR.fit$Method.2.data, aes(x = lnCt)) +
  geom_point(mapping = aes(y = invT)) +
  geom_line(mapping = aes(y = Model)) +
  theme_classic()
```

[8] Method.2.fit: A nls object containing the fit obtained from fitting the relationship of Tm and Ct. It can be called using:

```
MeltR.fit$Method.2.fit
```

[9] Method 3 data: Contains the raw data from method 2 and the model. It can be called and plotted using:

```
MeltR.fit$Method.3.data
ggplot(MeltR.fit$Method.3.data, aes(x = Temperature, color = factor(Sample), group = factor(
  geom_point(mapping = aes(y = Absorbance/(Pathlength*Ct))) +
  geom_line(mapping = aes(y = Model/(Pathlength*Ct)), color = "black") +
  theme_classic()
```

[10] Method.3.fit: A nls object containing the fit obtained from fitting the raw data. It can be called using:

```
MeltR.fit$Method.3.fit
```

5 References

[1] Biochemistry 1996, 35 (45), 14077–14089. [2] Methods in Enzymology, 1989; Vol. 180, pp 304-325. [3] Biochemistry 1998, 37 (42), 14719–14735. [4] Welcome | R for Data Science https://r4ds.had.co.nz/ (accessed 2022 -05 -02). [5] ggrepel: An R package https://ggrepel.slowkow.com/index.html (accessed 2022 -05 -02).