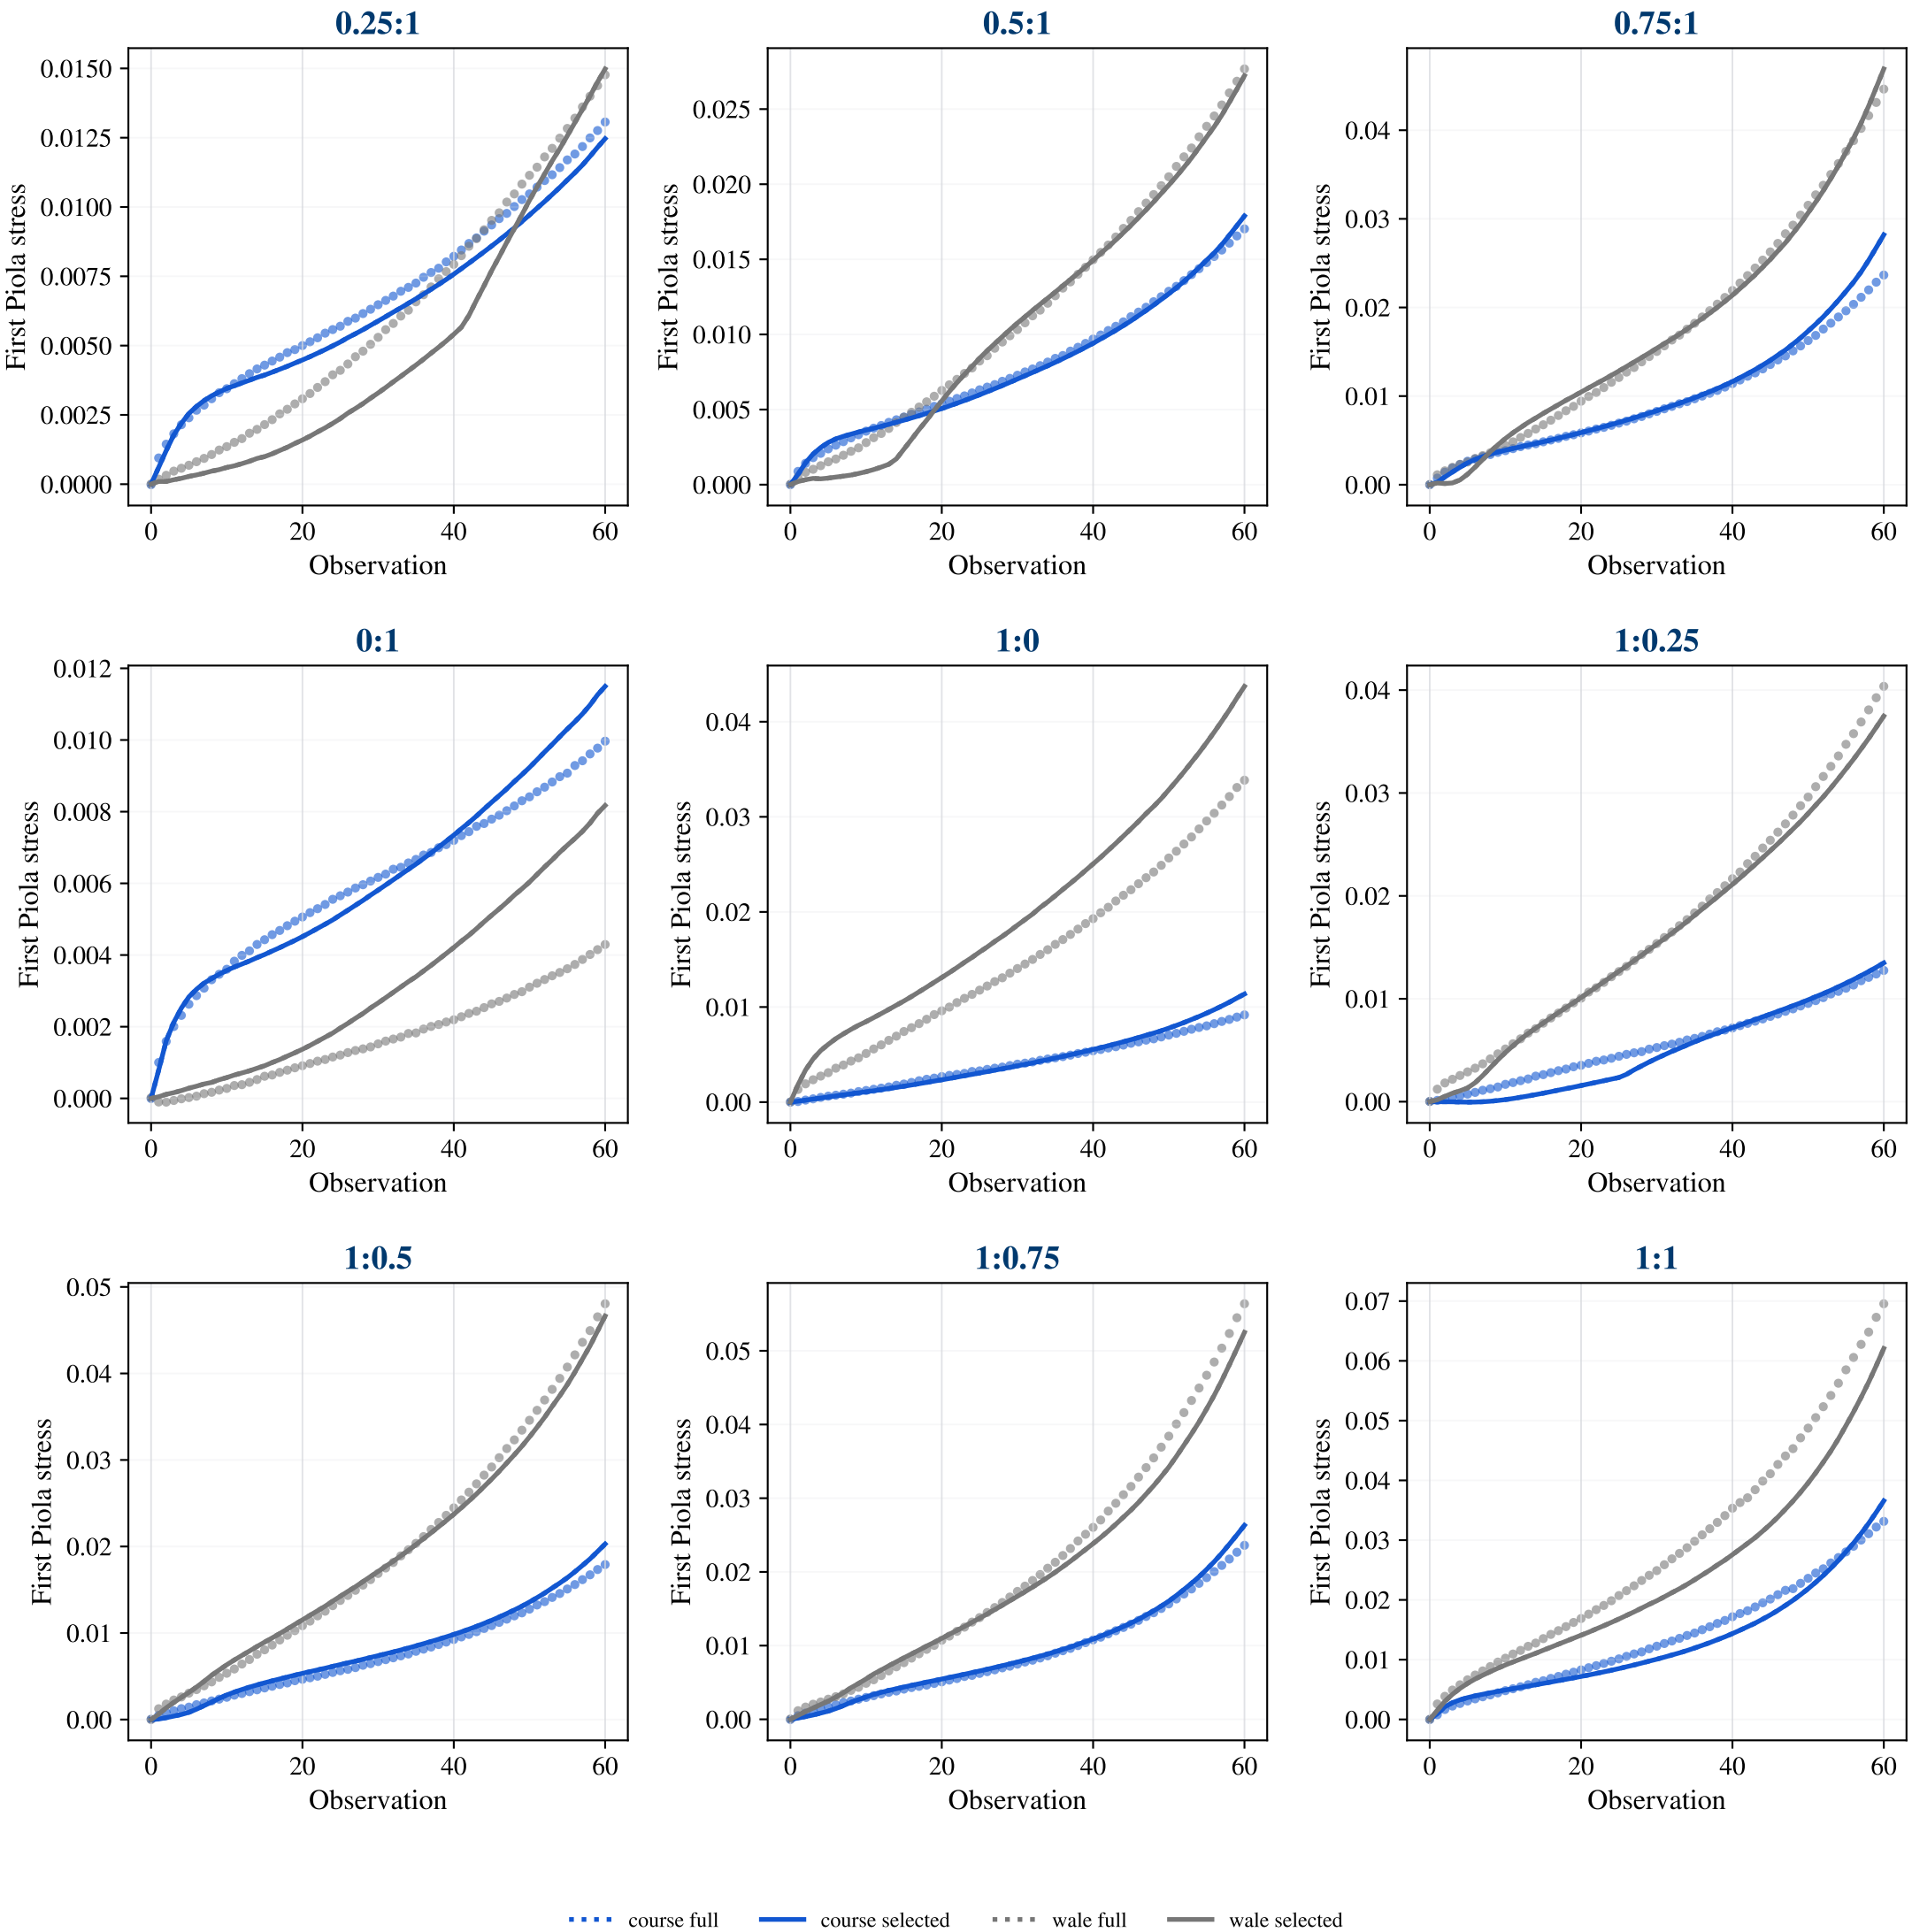Interlock: full versus selected all-nine calibration