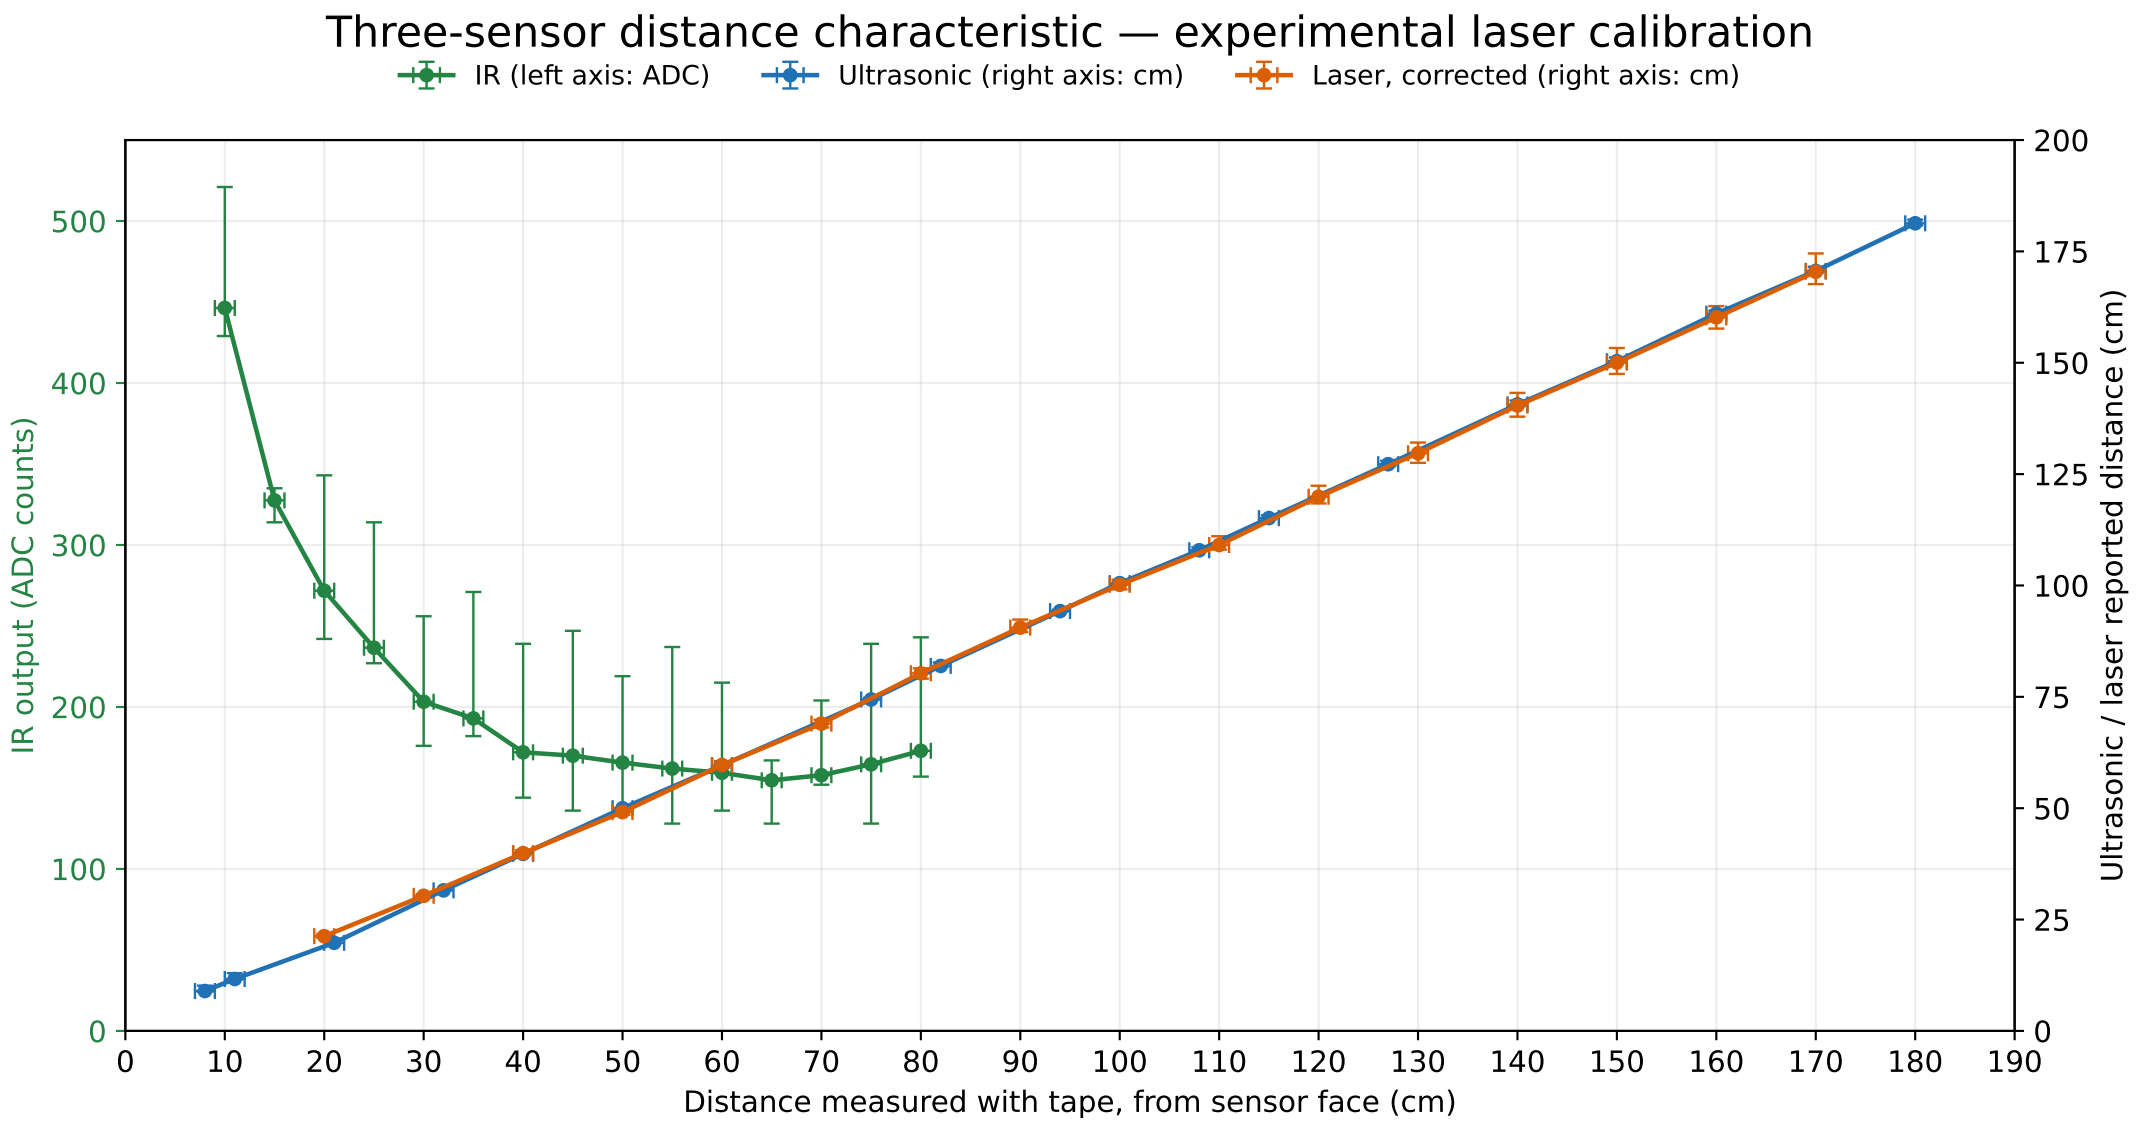

Points: mean of 3 accepted repeats. Vertical bars: minimum–maximum of all accepted samples.
Horizontal bars: ±1 cm tape-measure uncertainty (2 cm total width).
US uses existing calibration; IR remains in ADC counts. Laser: corrected = 0.96924 × reported − 0.699 cm.
Laser mounting changed around 60 cm; this curve retains the original run.
The two y-axes use independent scales; curve intersections do not imply equal outputs.