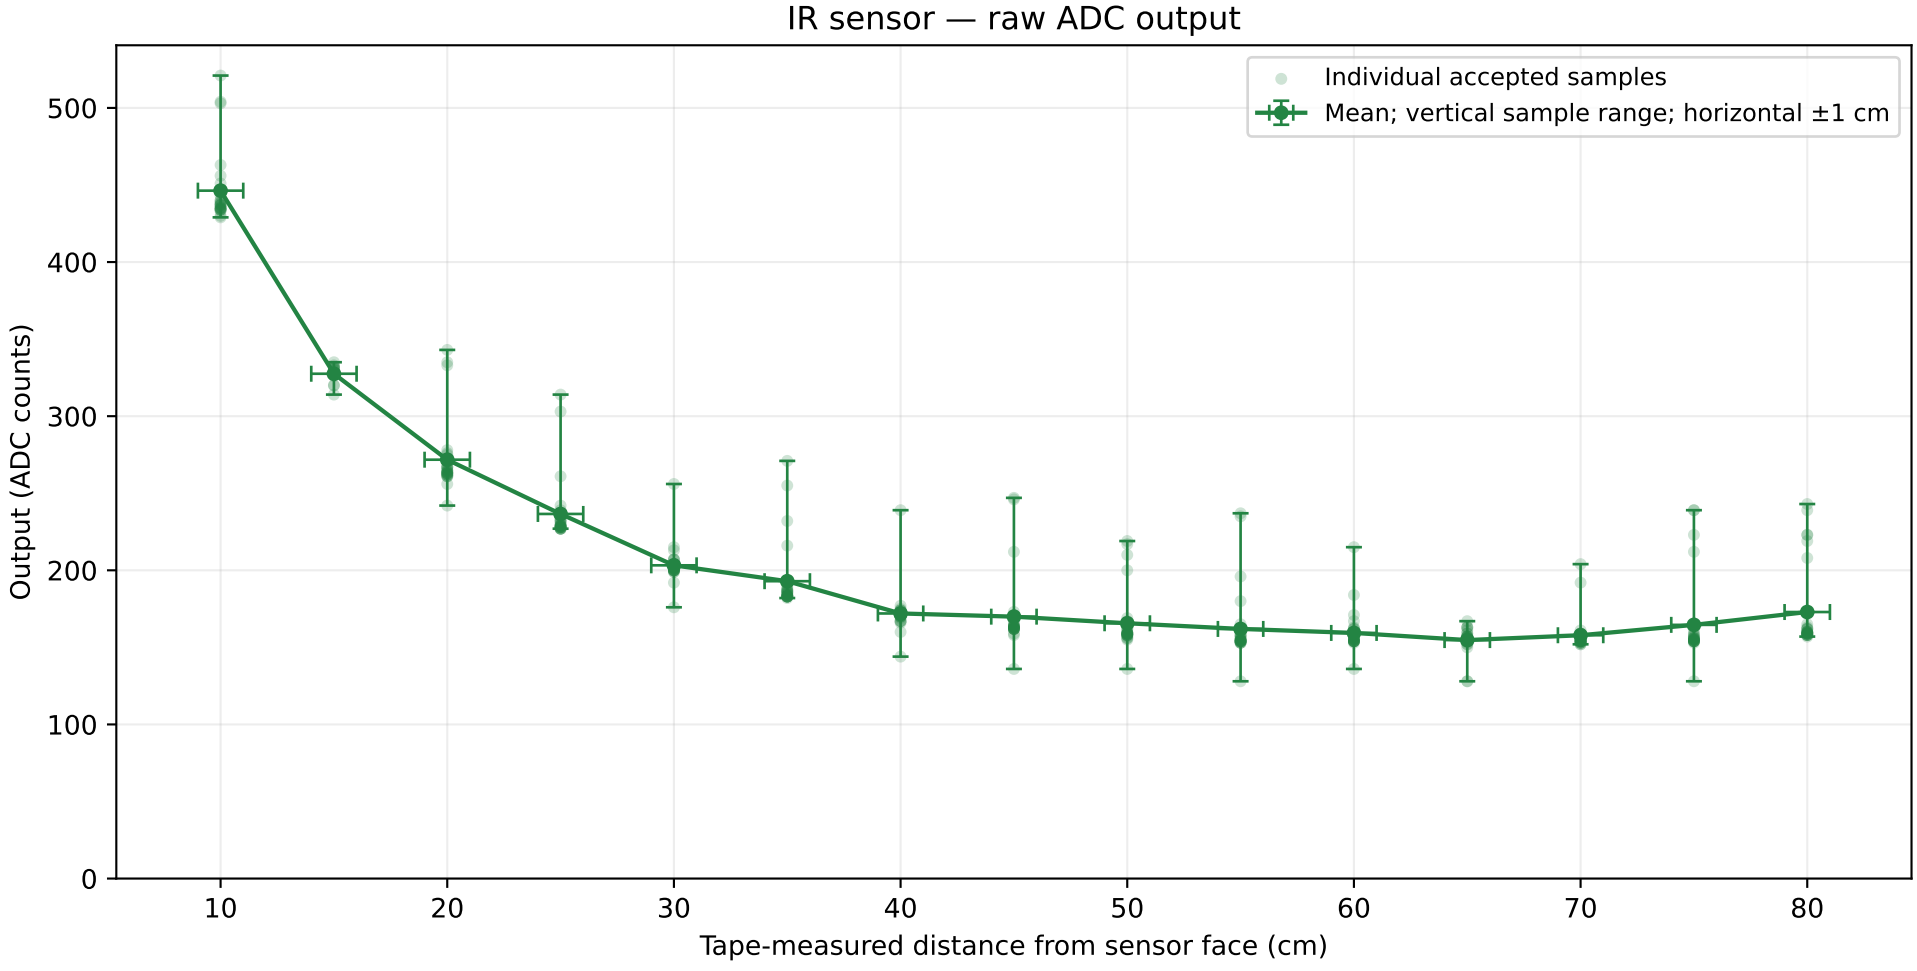

Points: equally weighted mean of 3 accepted repeats; faint dots: individual raw samples.
Vertical bars: minimum–maximum of accepted samples. Horizontal bars: ±1 cm (2 cm total).
Raw ADC counts; no distance conversion. The ambiguous far-distance response is retained.

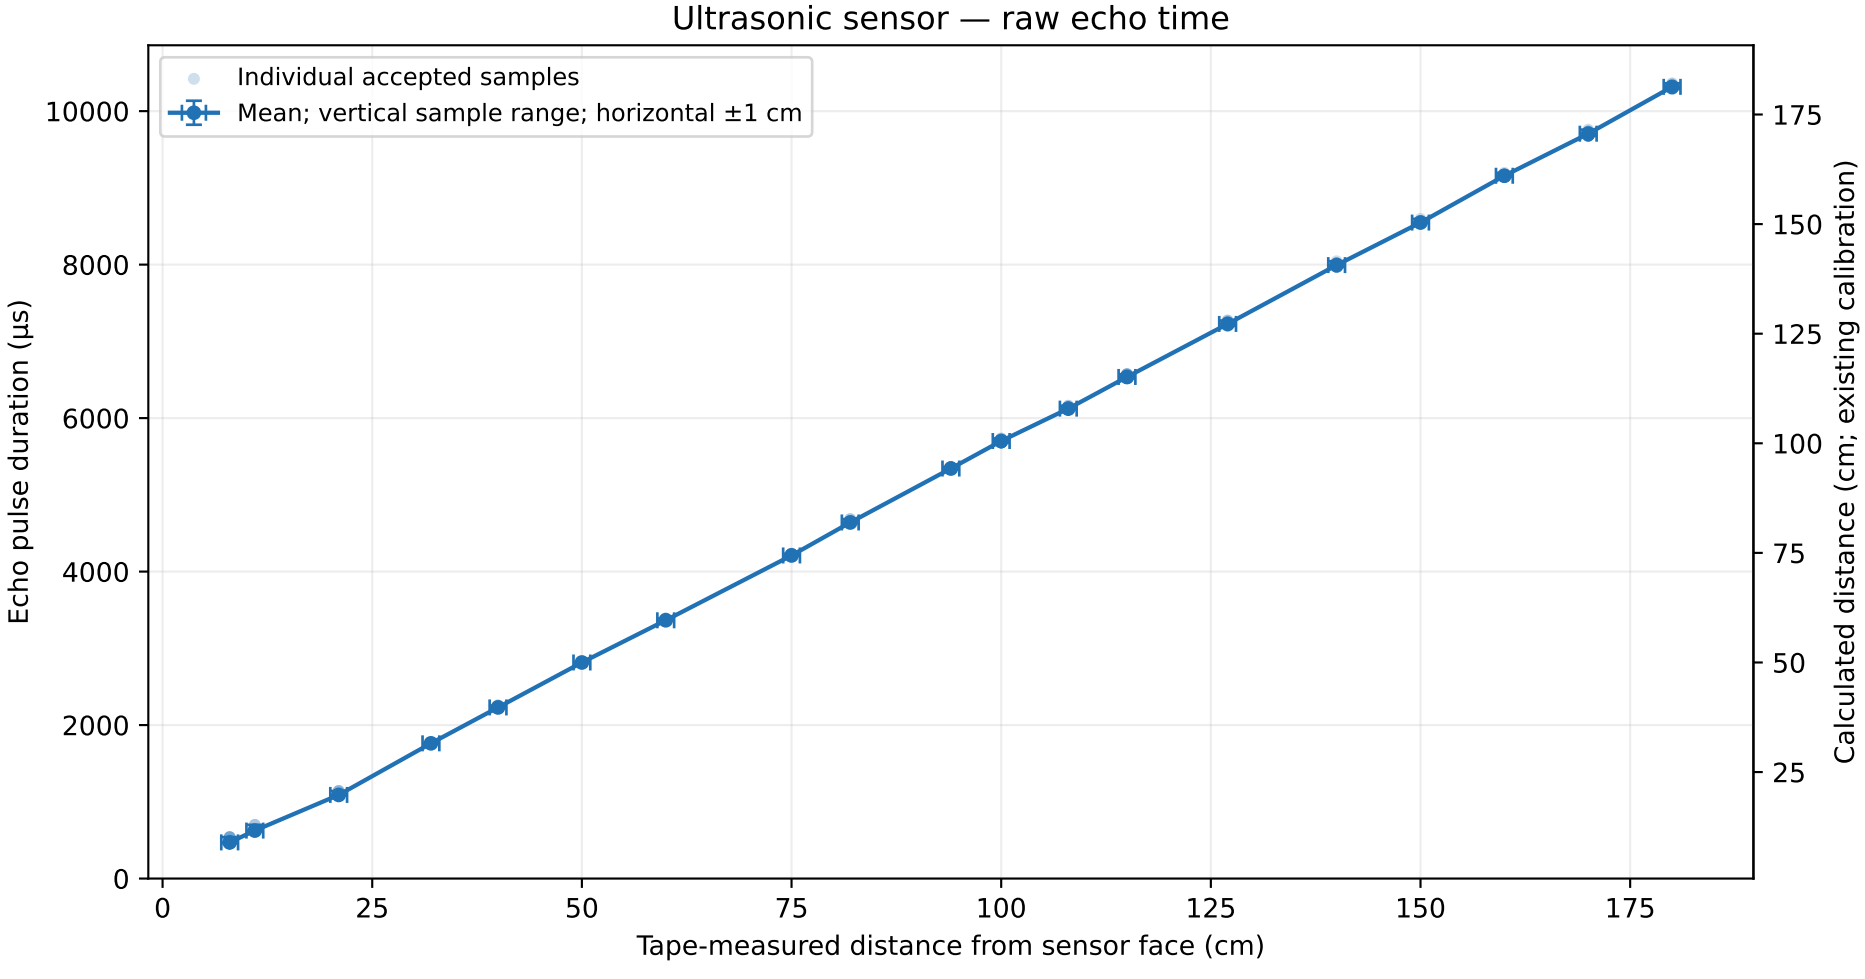

Points: equally weighted mean of 3 accepted repeats; faint dots: individual raw samples.
Vertical bars: minimum–maximum of accepted samples. Horizontal bars: ±1 cm (2 cm total).
Right axis: cm = (echo µs / 58) × 1.01535 + 0.7091. The same points and bars use both scales.

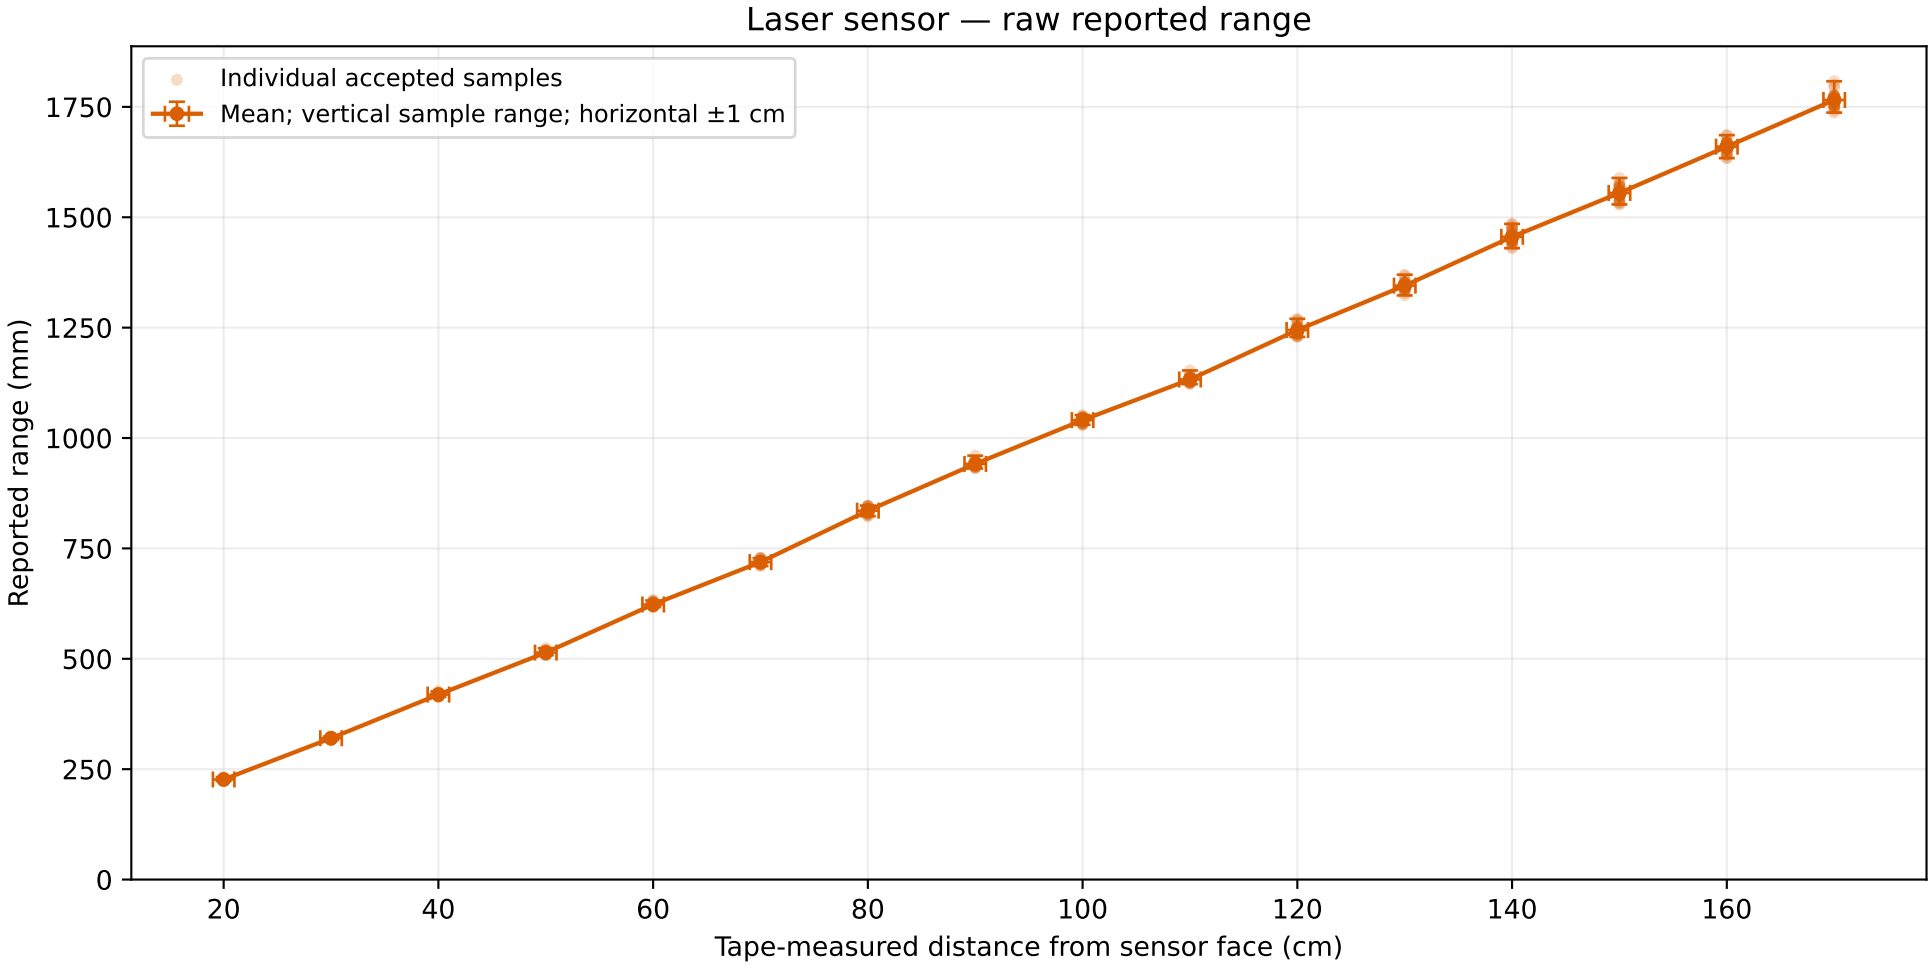

Points: equally weighted mean of 3 accepted repeats; faint dots: individual raw samples.
Vertical bars: minimum–maximum of accepted samples. Horizontal bars: ±1 cm (2 cm total).
Raw device-reported millimetres; no empirical laser correction applied.
Mounting was adjusted around 60 cm in this original run; separate follow-up data are excluded.