


Fluorescence-activated microfluidic droplet screening

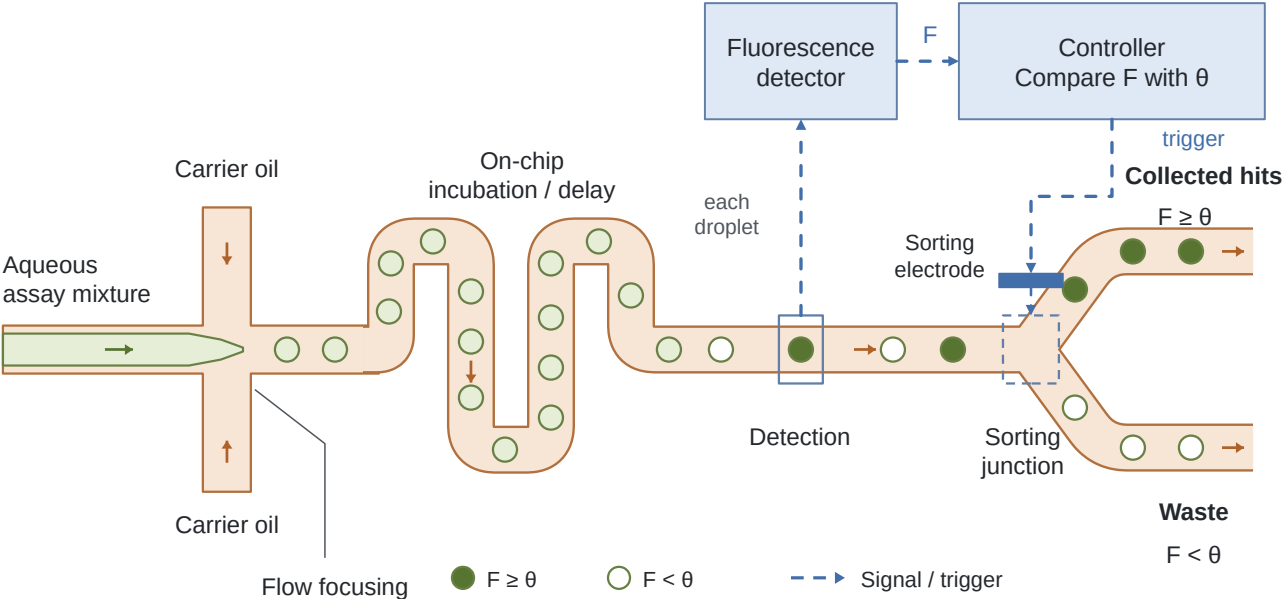

Hypothetical workflow. Droplets and channel geometry are schematic.