



Random-circuit null (50 circuits, interchange ablation)


Accuracy (pct 0.0, p 1.000)

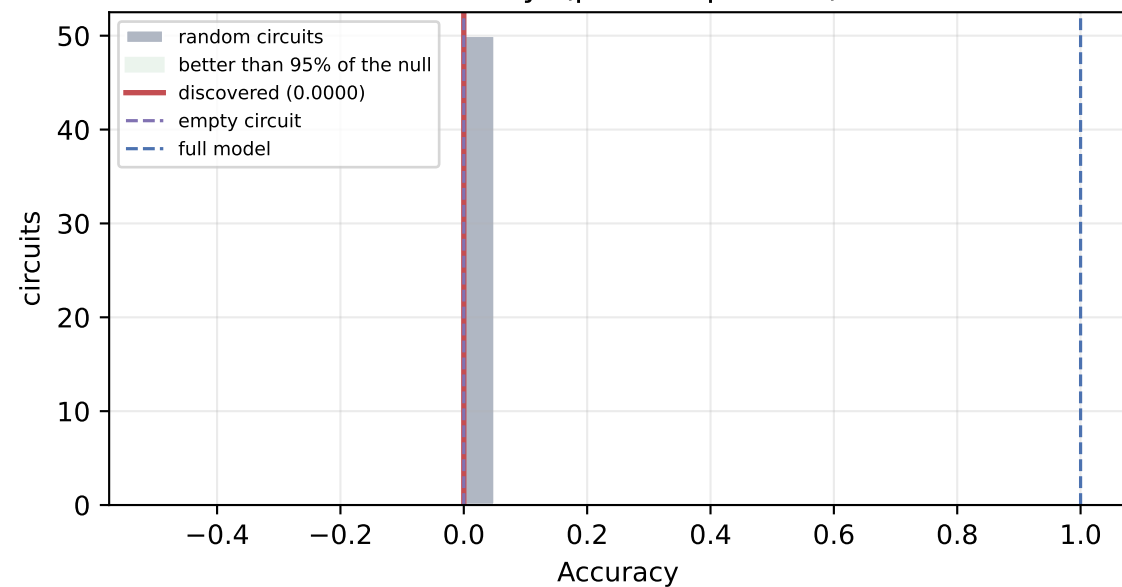

Logit Diff (pct 100.0, p 0.020)

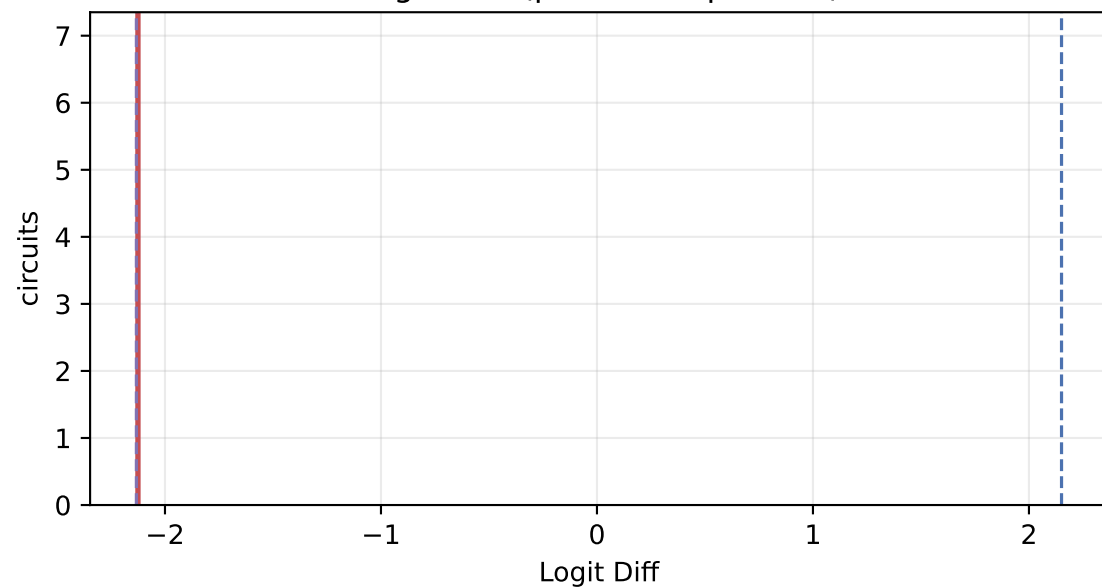

KL Div (pct 100.0, p 0.020)

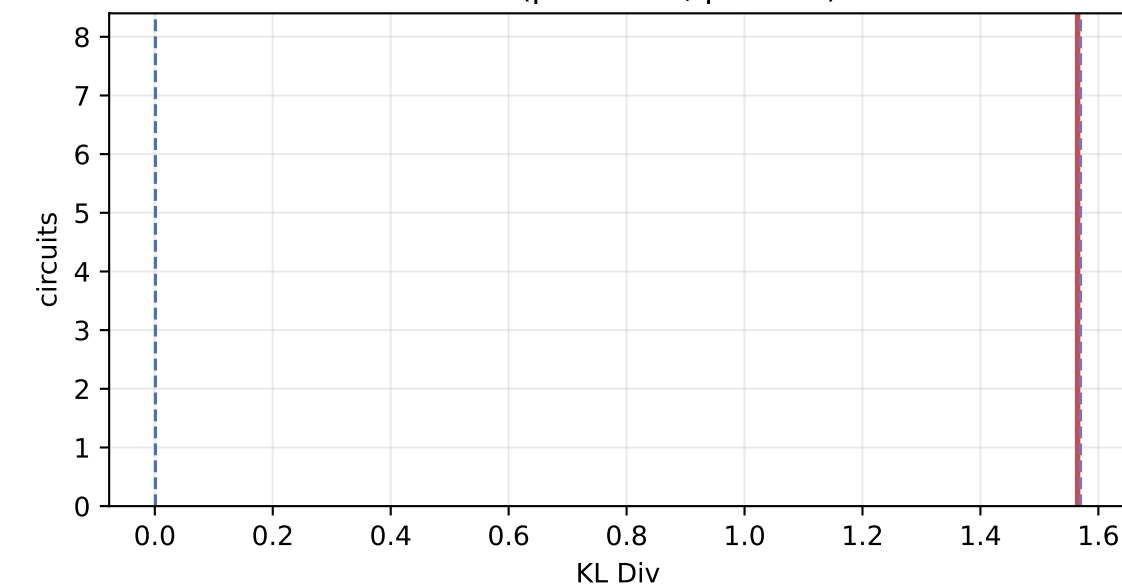

Exact Match (pct 0.0, p 1.000)

