



Random-circuit null (50 circuits, interchange ablation)


Accuracy (pct 0.0, p 1.000)

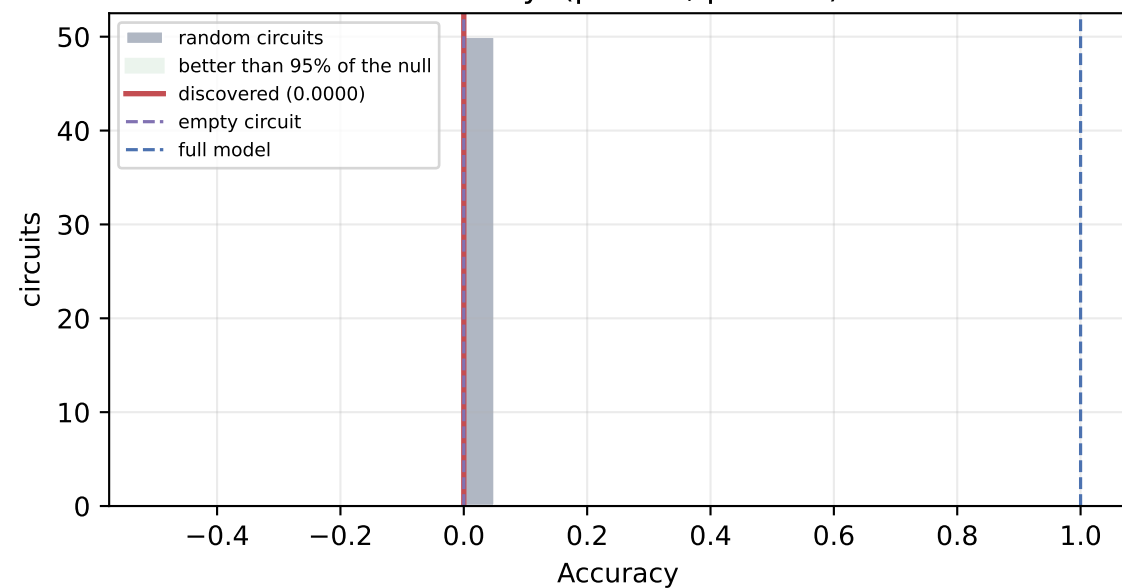

Logit Diff (pct 92.0, p 0.098)

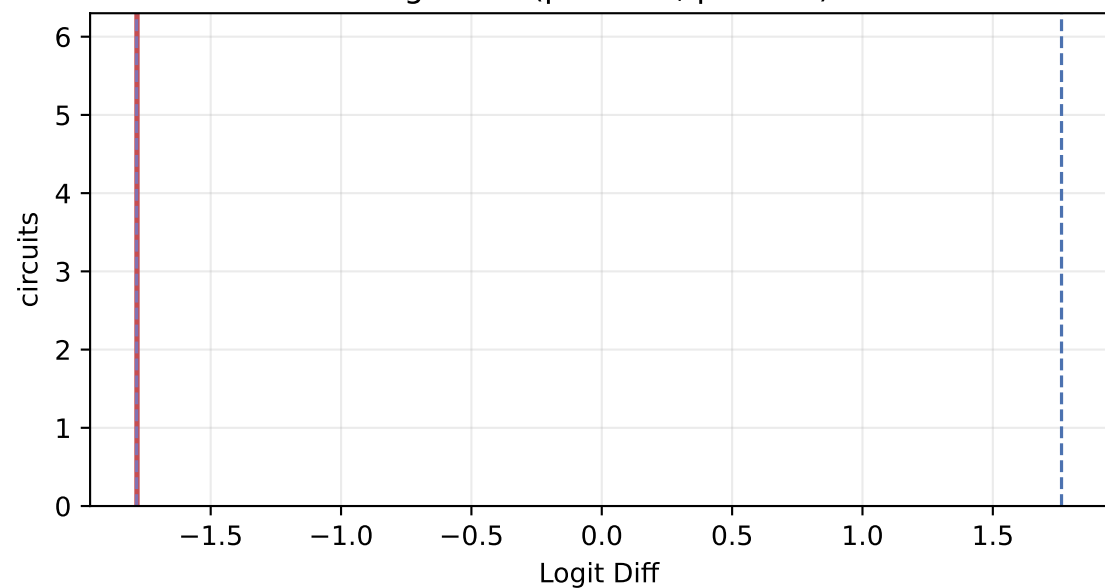

KL Div (pct 80.0, p 0.216)

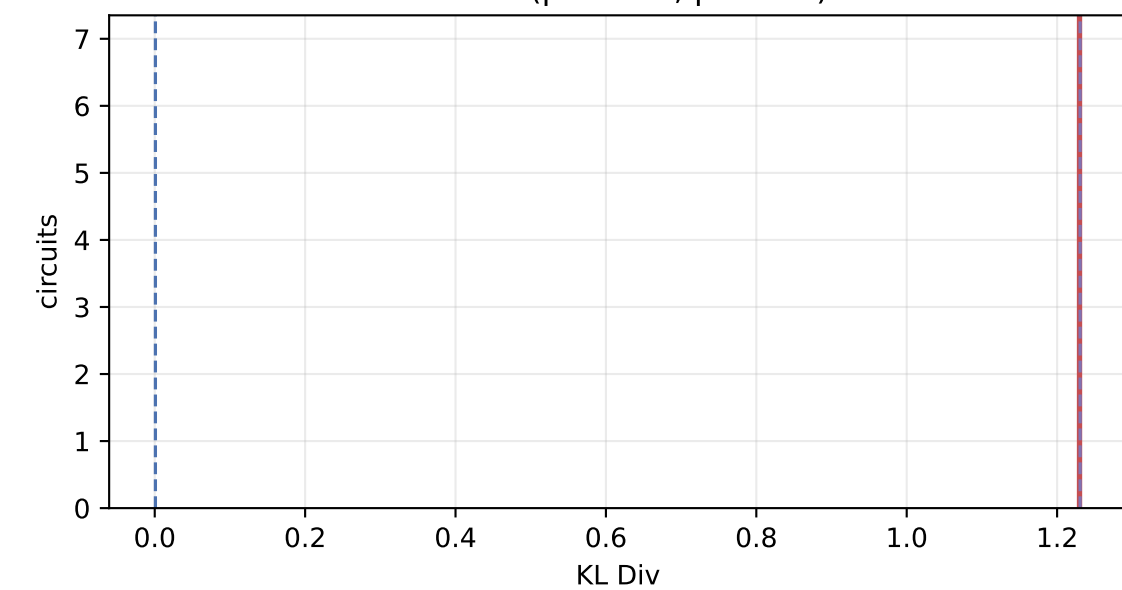

Exact Match (pct 0.0, p 1.000)

