



Random-circuit null (50 circuits, interchange ablation)


Accuracy (pct 100.0, p 0.020)

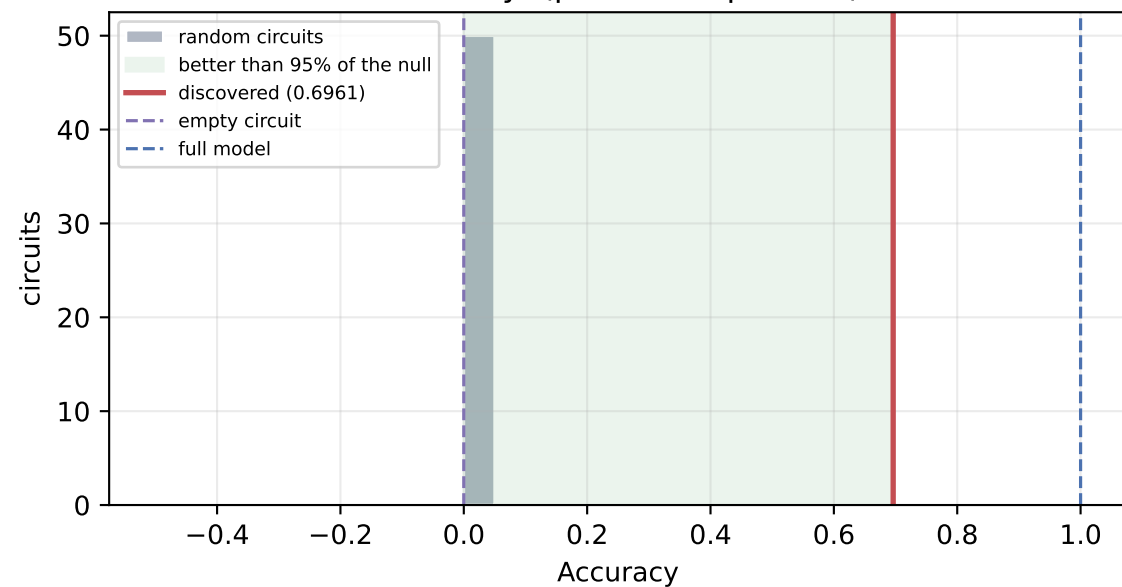

Logit Diff (pct 100.0, p 0.020)

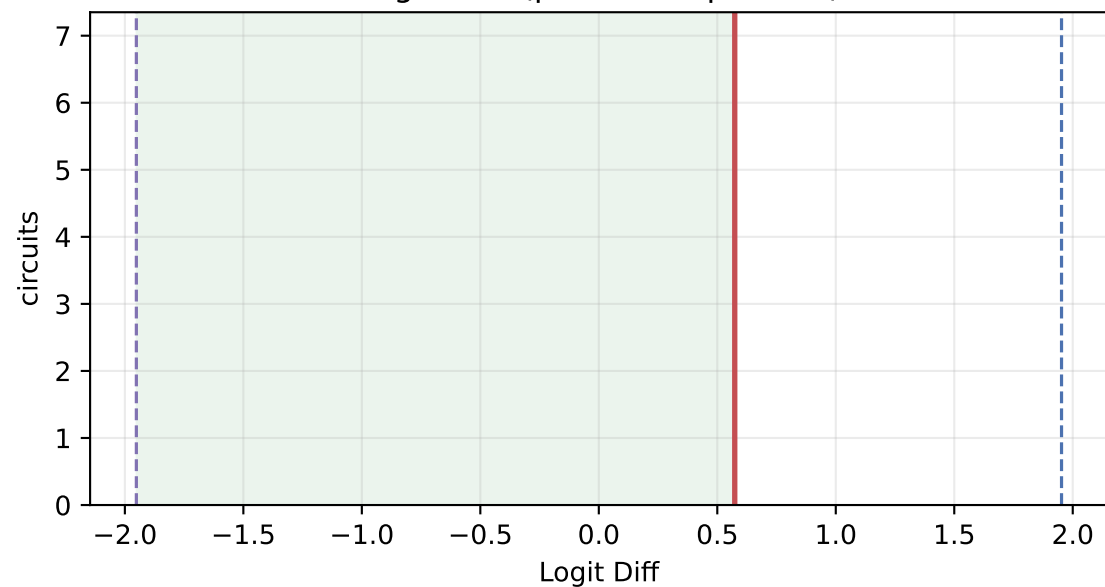

KL Div (pct 100.0, p 0.020)

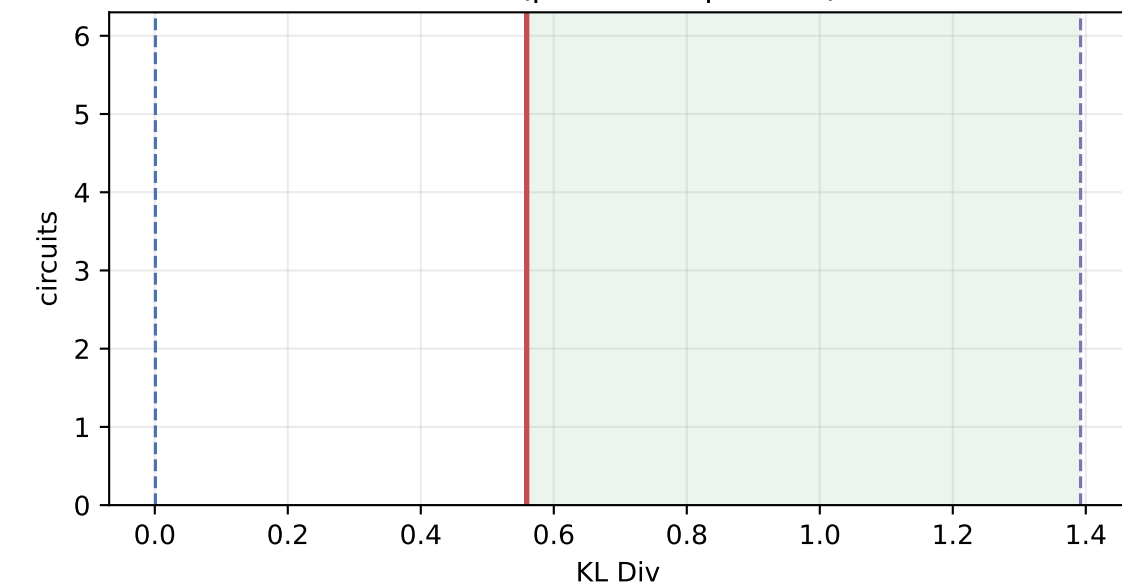

Exact Match (pct 100.0, p 0.020)

