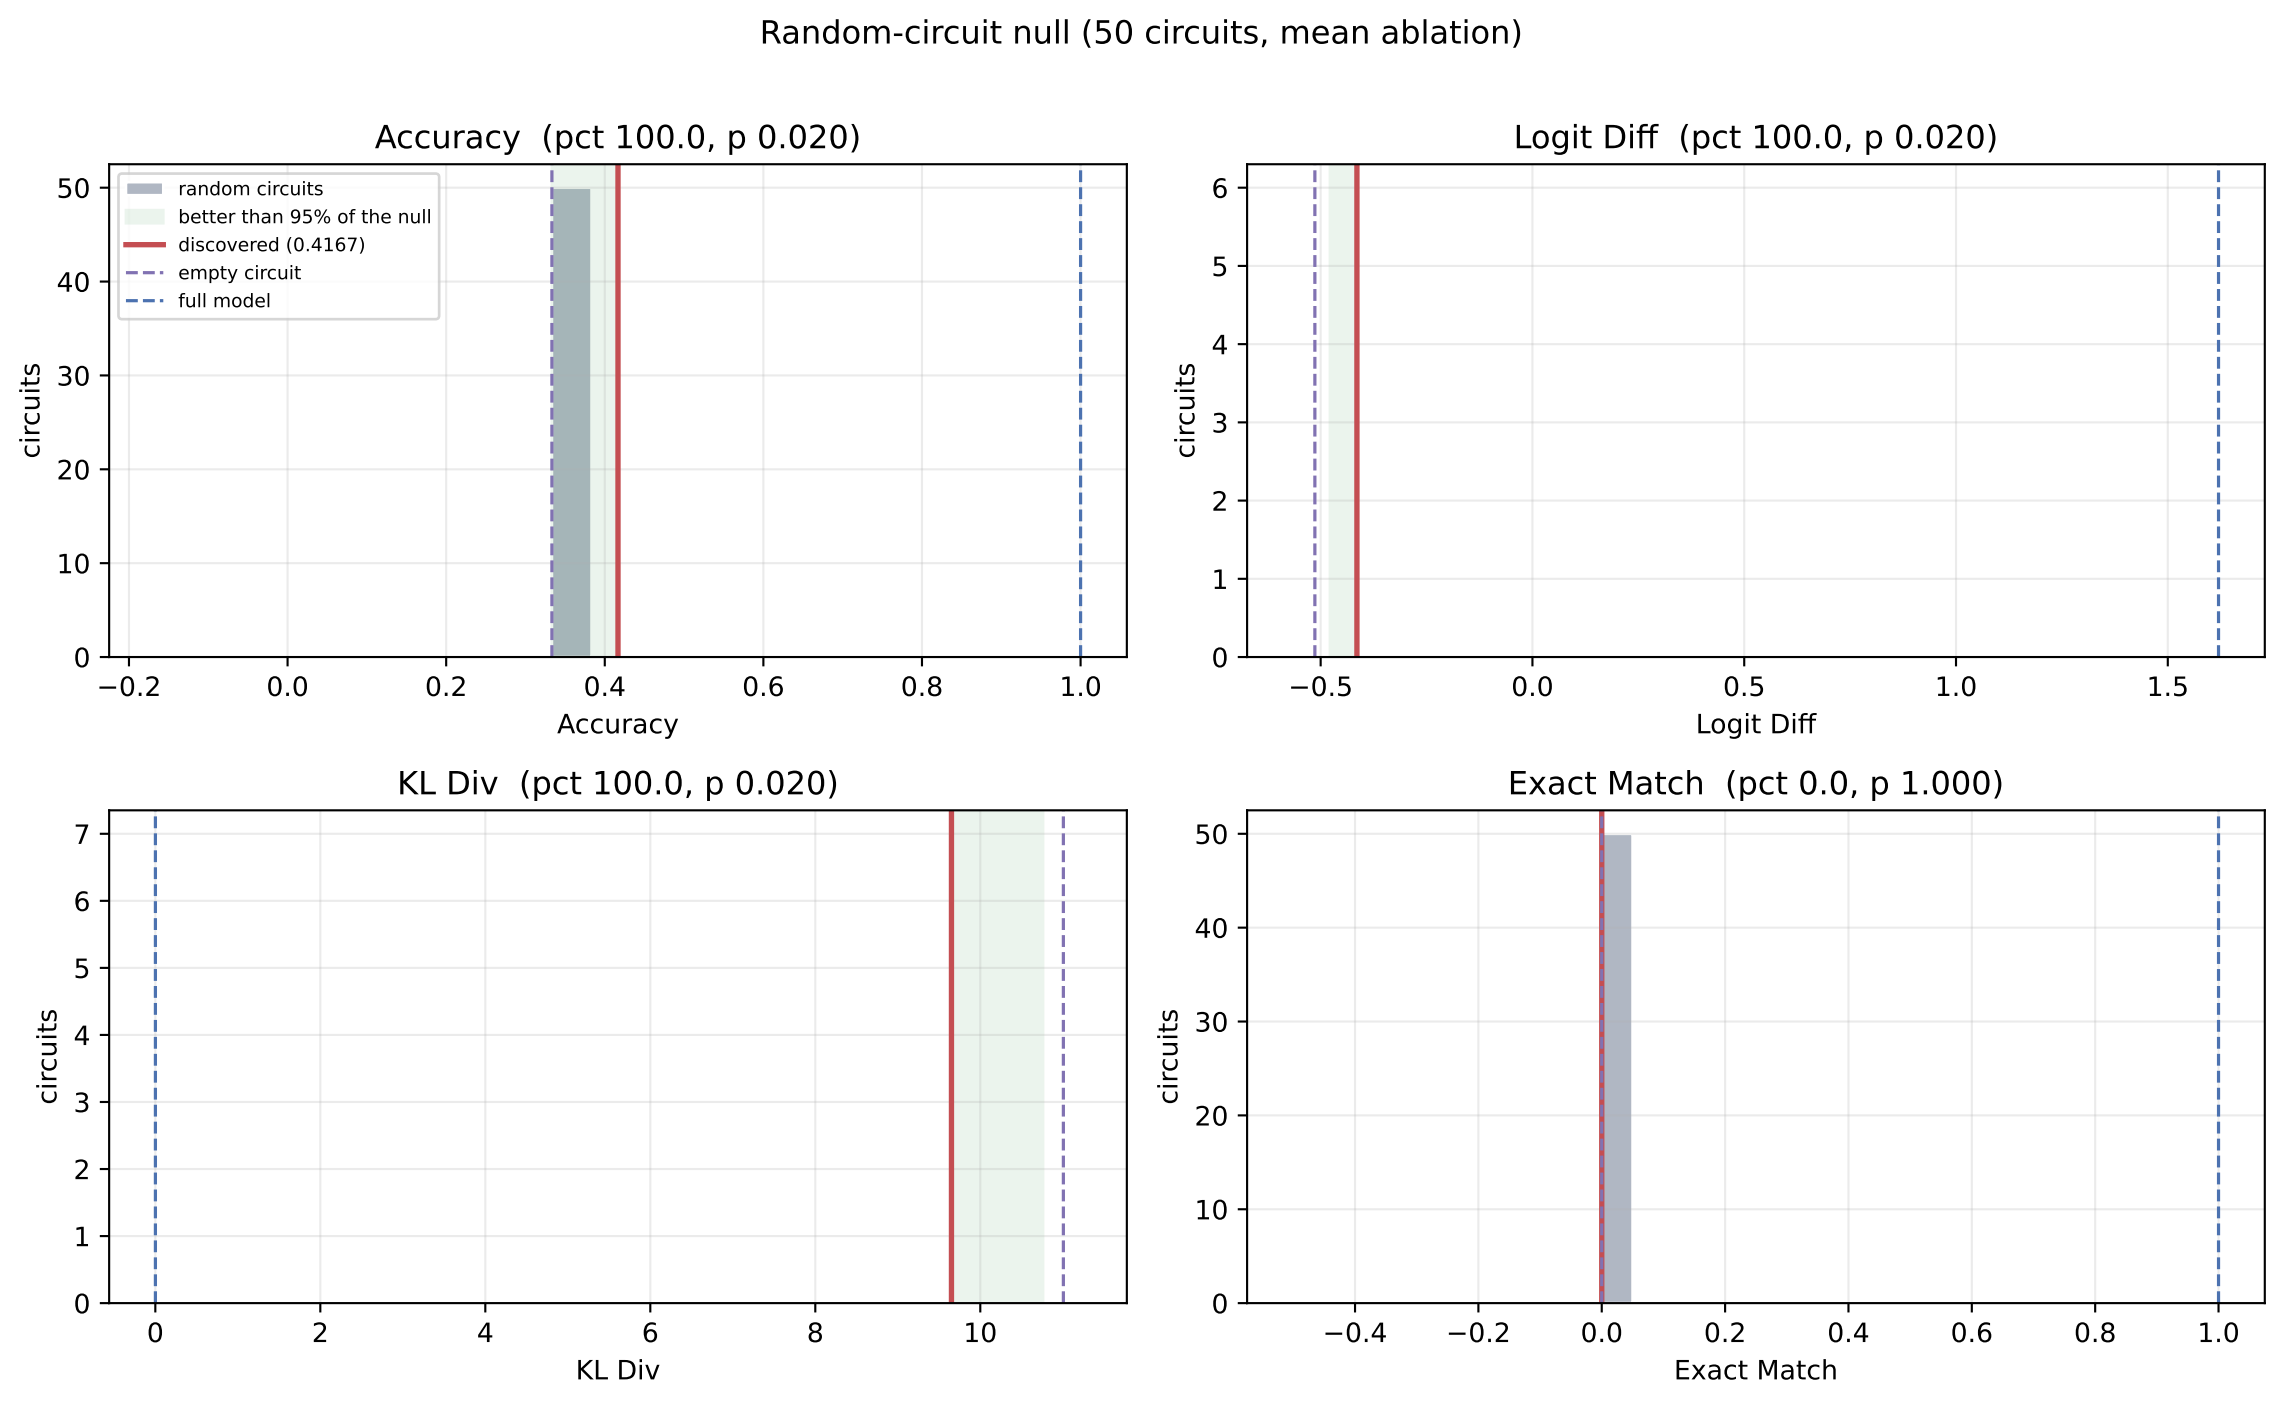
Random-circuit null (50 circuits, mean ablation)
Accuracy (pct 100.0, p 0.020)
random circuits
better than 95% of the null
discovered (0.4167)
empty circuit
full model
circuits
Accuracy
Logit Diff (pct 100.0, p 0.020)
Logit Diff
KL Div (pct 100.0, p 0.020)
KL Div
Exact Match (pct 0.0, p 1.000)
Exact Match