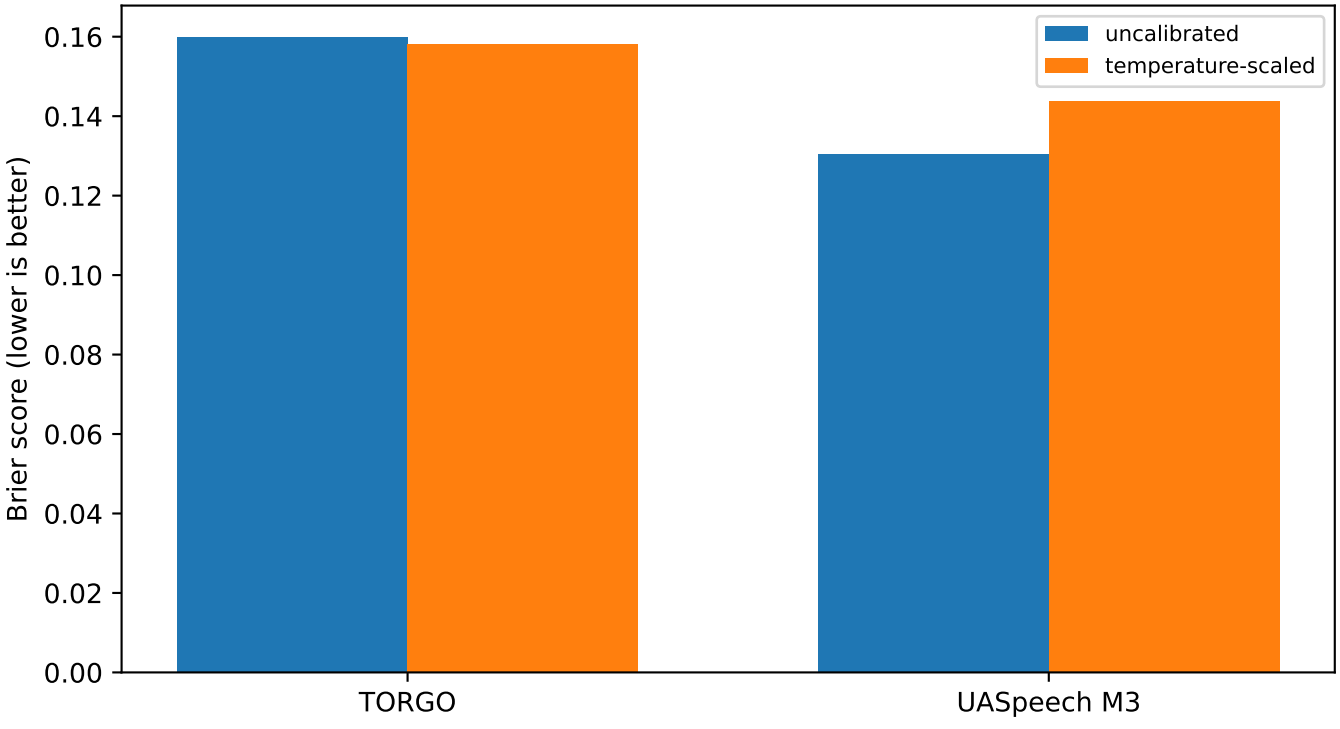
Locked TORGO calibration and M3 transfer
uncalibrated
temperature-scaled
Brier score (lower is better)
0.16
0.14
0.12
0.10
0.08
0.06
0.04
0.02
0.00
TORGO
UASpeech M3