



ECG experiment: 10% labeled training patients
PTB-XL diagnostic proxy; not student screening validation


Primary label sample (seed 42)

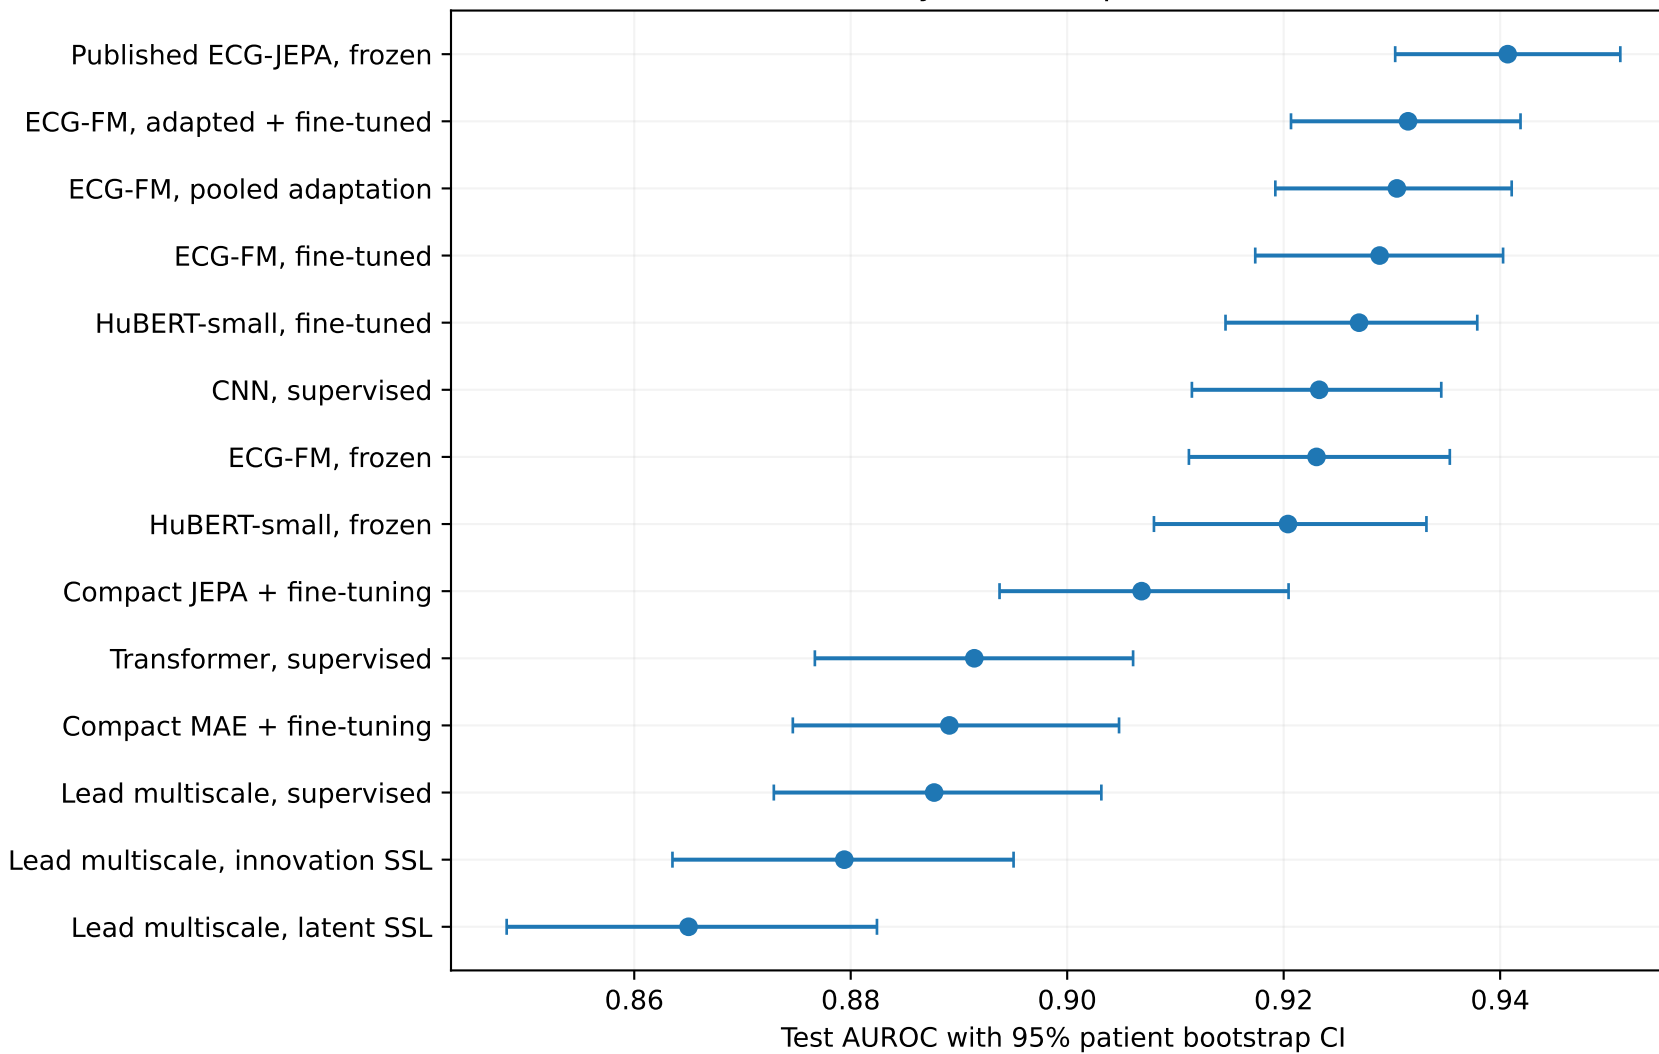

Threshold fixed on calibration patients

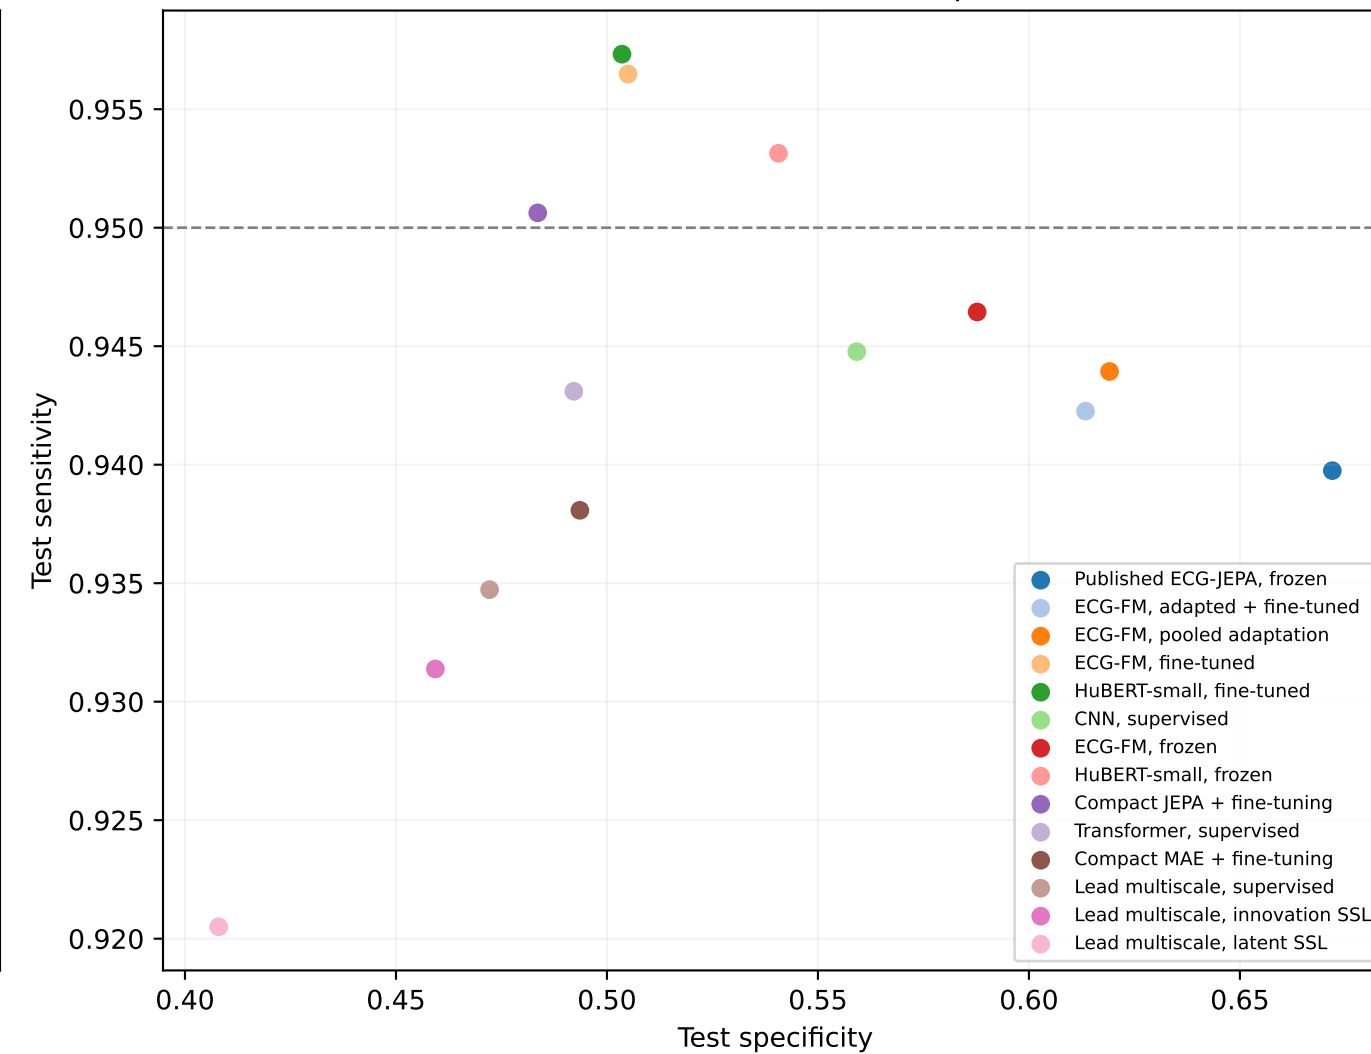

Test ROC curves

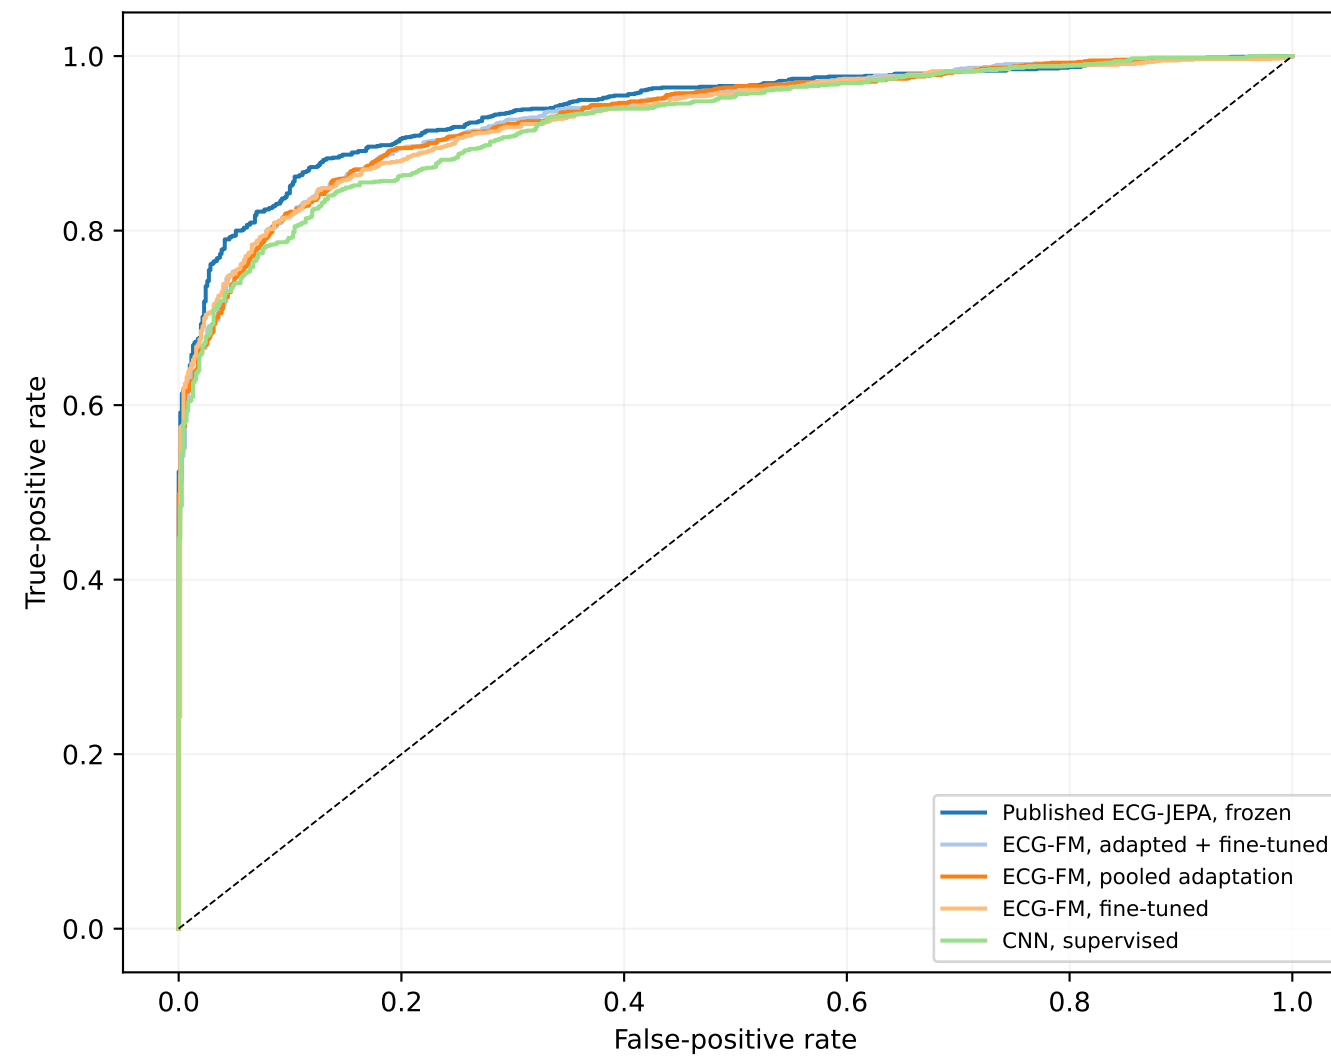

Calibration on the PTB-XL proxy

