

QCDart LJ Chart Report

Data Range	From: 01/09/2026 To: 09/09/2026
Oragnization/Lab name	Noble Diagnostic Centre / Noble Diagnostic Centre DELHI
Lab Address	WZ 409 C HARI NAGAR NEW DELHI,India,Delhi,Delhi,110064
Contact	SHIPRA | M: 9511018366
QC Lot Information	Bio-Rad | Lyphochek Immunoassay Plus Control | 40471 | 31/01/2028 | 40472 | 31/01/2028 | 40473 | 31/01/2028
Instrument Information	Snibe | Maglumi X3 | 01010100340124013 60
Test Information	B-hCG | mIU/mL | CLIA - Chemiluminescence immunoassay

Level 1 - Mean: 8.60 | SD: 0.93 | CV: 10.76 | N: 9

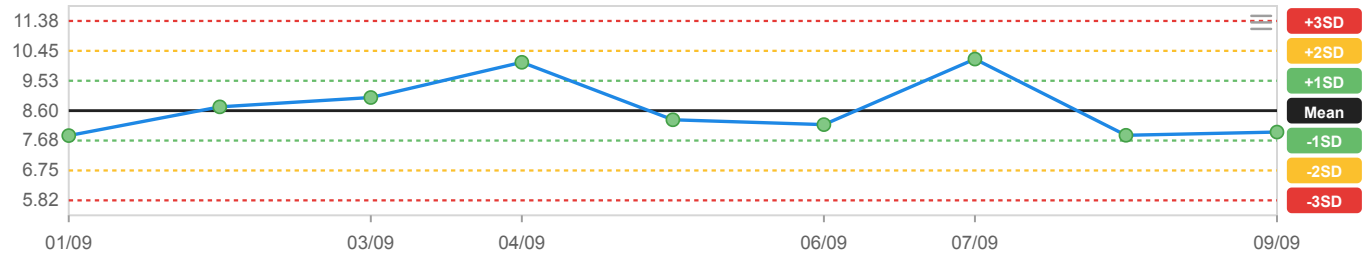

Level 2 - Mean: 22.81 | SD: 2.30 | CV: 10.07 | N: 9

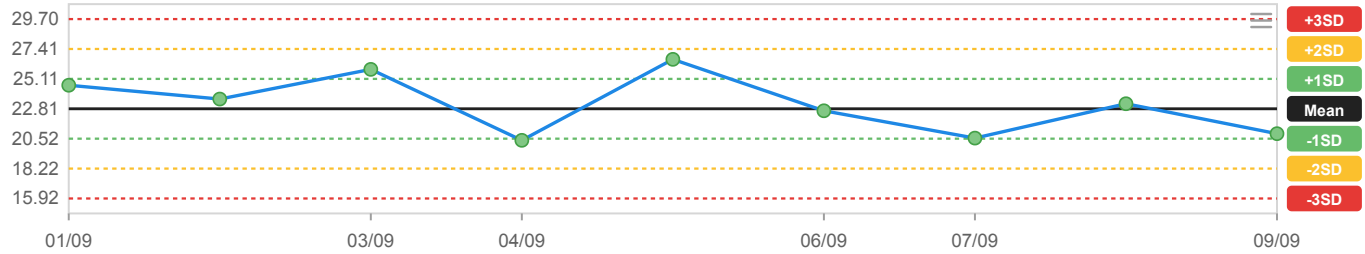


Comments _____ Reviewed by _____ Sign & Date _____

© Copyright 2025 Steller Infomatica. All rights reserved.


QCDart LJ Chart Report

Data Range	From: 01/09/2026 To: 09/09/2026
Oragnization/Lab name	Noble Diagnostic Centre / Noble Diagnostic Centre DELHI
Lab Address	WZ 409 C HARI NAGAR NEW DELHI,India,Delhi,Delhi,110064
Contact	SHIPRA | M: 9511018366
QC Lot Information	Bio-Rad | Lyphochek Immunoassay Plus Control | 40471 | 31/01/2028 | 40472 | 31/01/2028 | 40473 | 31/01/2028
Instrument Information	Snibe | Maglumi X3 | 01010100340124013 60
Test Information	FSH | mIU/mL | CLIA - Chemiluminescence immunoassay

Level 1 - Mean: 7.54 | SD: 0.74 | CV: 9.88 | N: 9

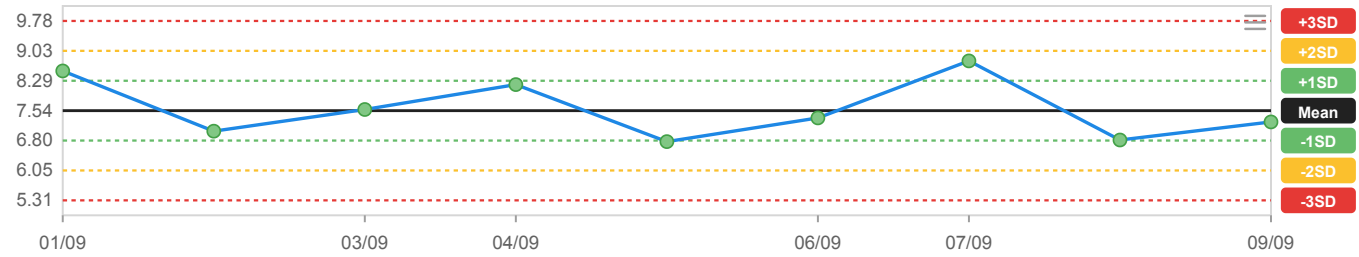

Level 2 - Mean: 25.32 | SD: 2.14 | CV: 8.44 | N: 9

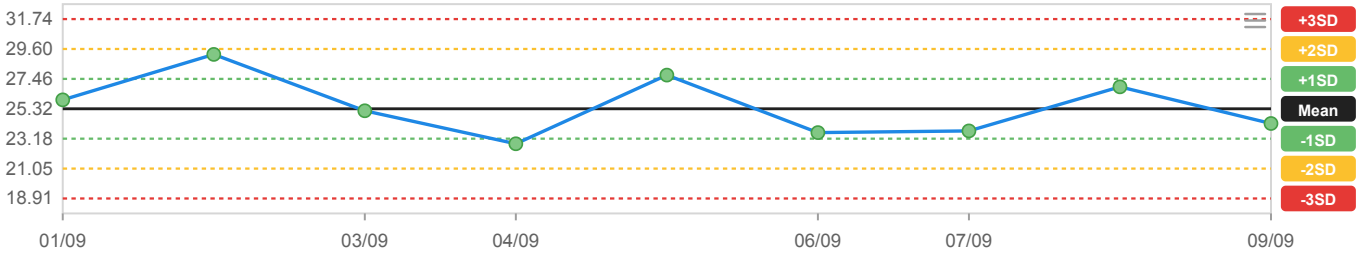


Comments _____ Reviewed by _____ Sign & Date _____

© Copyright 2025 Steller Infomatica. All rights reserved.


QCDart LJ Chart Report

Data Range	From: 01/09/2026 To: 09/09/2026
Oragnization/Lab name	Noble Diagnostic Centre / Noble Diagnostic Centre DELHI
Lab Address	WZ 409 C HARI NAGAR NEW DELHI,India,Delhi,Delhi,110064
Contact	SHIPRA | M: 9511018366
QC Lot Information	Bio-Rad | Lyphochek Immunoassay Plus Control | 40471 | 31/01/2028 | 40472 | 31/01/2028 | 40473 | 31/01/2028
Instrument Information	Snibe | Maglumi X3 | 01010100340124013 60
Test Information	Estradiol, E2 | pg/mL | CLIA - Chemiluminescence immunoassay

Level 1 - Mean: 86.18 | SD: 8.91 | CV: 10.34 | N: 9

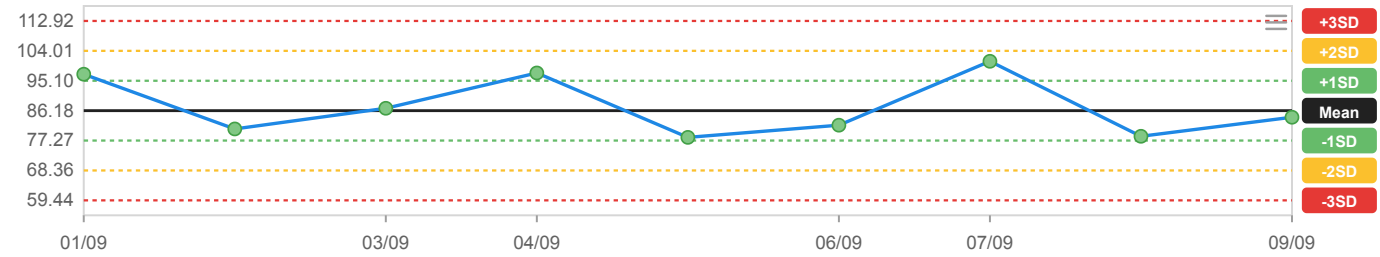

Level 2 - Mean: 319.35 | SD: 28.89 | CV: 9.05 | N: 9

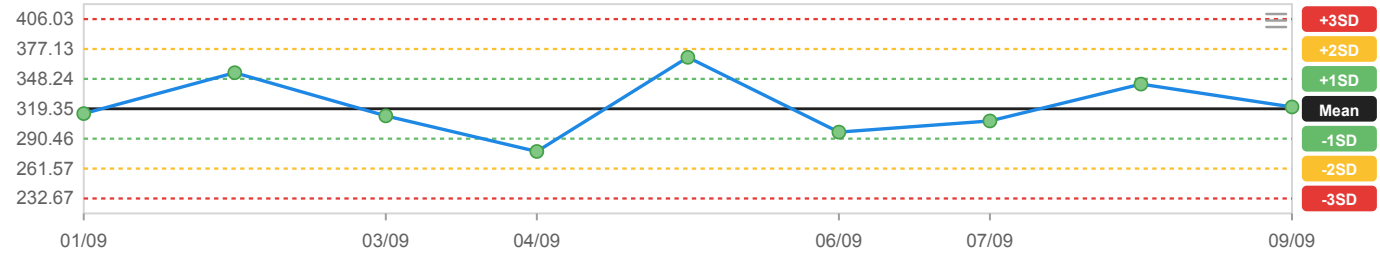


Comments _____ Reviewed by _____ Sign & Date _____

© Copyright 2025 Steller Infomatica. All rights reserved.


QCDart LJ Chart Report

Data Range	From: 01/09/2026 To: 09/09/2026
Oragnization/Lab name	Noble Diagnostic Centre / Noble Diagnostic Centre DELHI
Lab Address	WZ 409 C HARI NAGAR NEW DELHI,India,Delhi,Delhi,110064
Contact	SHIPRA | M: 9511018366
QC Lot Information	Bio-Rad | Lyphochek Immunoassay Plus Control | 40471 | 31/01/2028 | 40472 | 31/01/2028 | 40473 | 31/01/2028
Instrument Information	Snibe | Maglumi X3 | 01010100340124013 60
Test Information	T3 Total | ng/mL | CLIA - Chemiluminescence immunoassay

Level 1 - Mean: 0.700 | SD: 0.073 | CV: 10.49 | N: 9

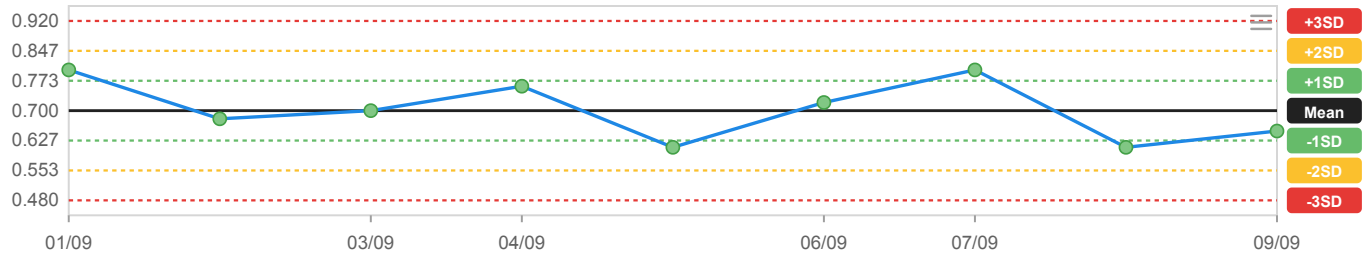

Level 2 - Mean: 1.83 | SD: 0.18 | CV: 9.80 | N: 9

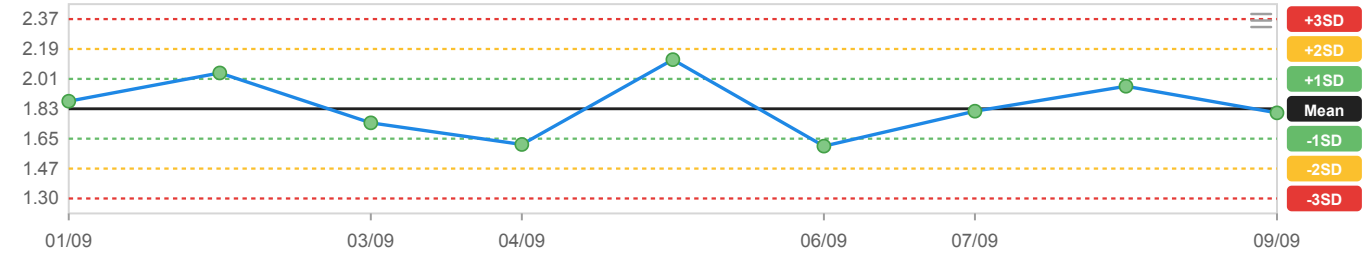


Comments _____ Reviewed by _____ Sign & Date _____

© Copyright 2025 Steller Infomatica. All rights reserved.


QCDart LJ Chart Report

Data Range	From: 01/09/2026 To: 09/09/2026
Oragnization/Lab name	Noble Diagnostic Centre / Noble Diagnostic Centre DELHI
Lab Address	WZ 409 C HARI NAGAR NEW DELHI,India,Delhi,Delhi,110064
Contact	SHIPRA | M: 9511018366
QC Lot Information	Bio-Rad | Lyphochek Immunoassay Plus Control | 40471 | 31/01/2028 | 40472 | 31/01/2028 | 40473 | 31/01/2028
Instrument Information	Snibe | Maglumi X3 | 01010100340124013 60
Test Information	Prolactin | ng/mL | CLIA - Chemiluminescence immunoassay

Level 1 - Mean: 7.07 | SD: 0.66 | CV: 9.29 | N: 9

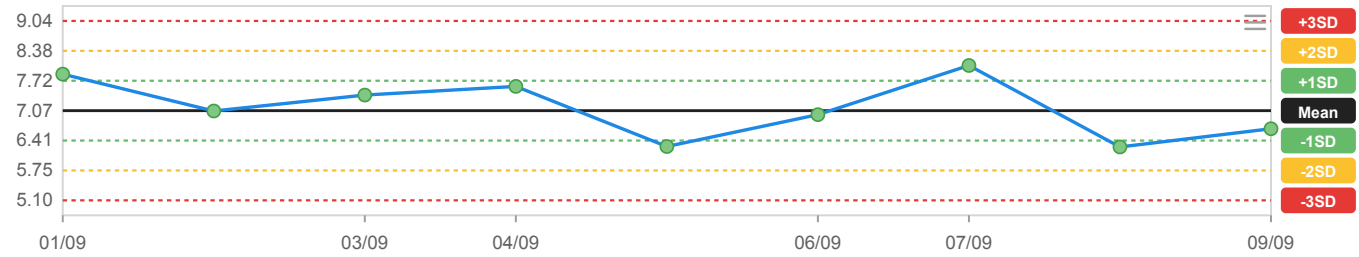

Level 2 - Mean: 21.04 | SD: 2.13 | CV: 10.13 | N: 9

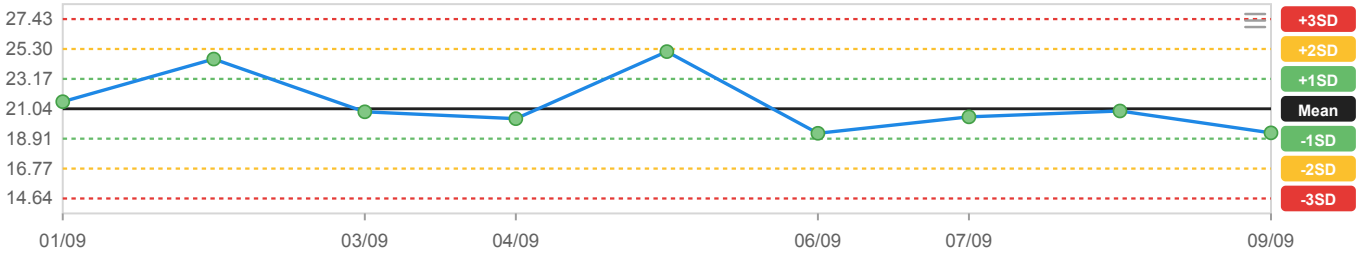


Comments _____ Reviewed by _____ Sign & Date _____

© Copyright 2025 Steller Infomatica. All rights reserved.


QCDart LJ Chart Report

Data Range	From: 01/09/2026 To: 09/09/2026
Oragnization/Lab name	Noble Diagnostic Centre / Noble Diagnostic Centre DELHI
Lab Address	WZ 409 C HARI NAGAR NEW DELHI,India,Delhi,Delhi,110064
Contact	SHIPRA | M: 9511018366
QC Lot Information	Bio-Rad | Lyphochek Immunoassay Plus Control | 40471 | 31/01/2028 | 40472 | 31/01/2028 | 40473 | 31/01/2028
Instrument Information	Snibe | Maglumi X3 | 0101010034012401360
Test Information	Testosterone | ng/dL | CLIA - Chemiluminescence immunoassay

Level 1 - Mean: 124.26 | SD: 11.60 | CV: 9.34 | N: 9

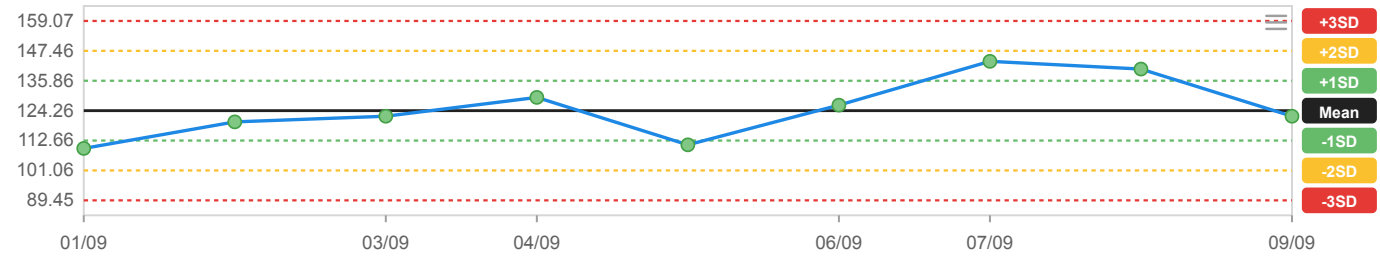

Level 2 - Mean: 300.02 | SD: 31.94 | CV: 10.65 | N: 9

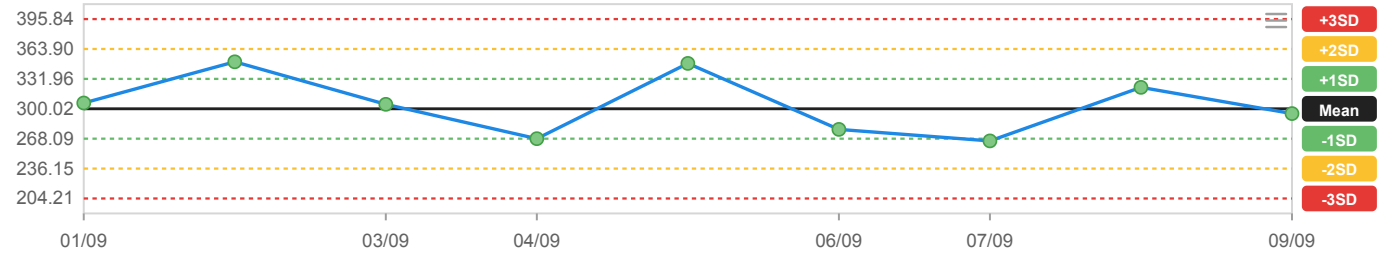


Comments _____ Reviewed by _____ Sign & Date _____

© Copyright 2025 Steller Infomatica. All rights reserved.


QCDart LJ Chart Report

Data Range	From: 01/09/2026 To: 09/09/2026
Oragnization/Lab name	Noble Diagnostic Centre / Noble Diagnostic Centre DELHI
Lab Address	WZ 409 C HARI NAGAR NEW DELHI,India,Delhi,Delhi,110064
Contact	SHIPRA | M: 9511018366
QC Lot Information	Bio-Rad | Lyphochek Immunoassay Plus Control | 40471 | 31/01/2028 | 40472 | 31/01/2028 | 40473 | 31/01/2028
Instrument Information	Snibe | Maglumi X3 | 01010100340124013 60
Test Information	T4 Total | µg/dl | CLIA - Chemiluminescence immunoassay

Level 1 - Mean: 6.15 | SD: 0.53 | CV: 8.67 | N: 9

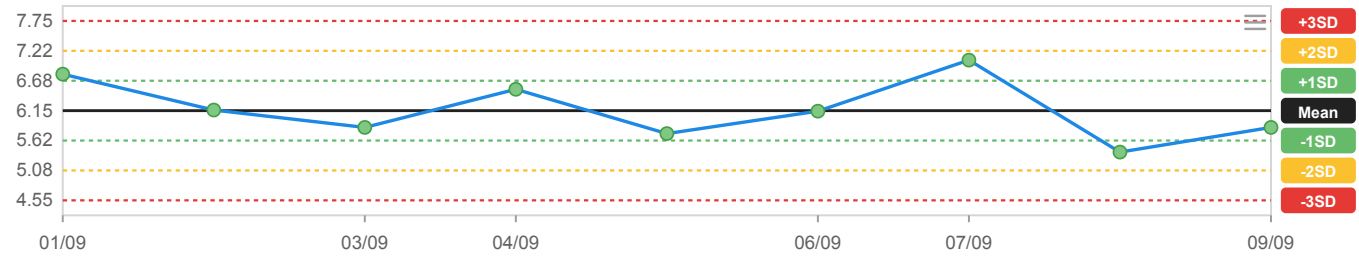

Level 2 - Mean: 10.97 | SD: 1.08 | CV: 9.86 | N: 9

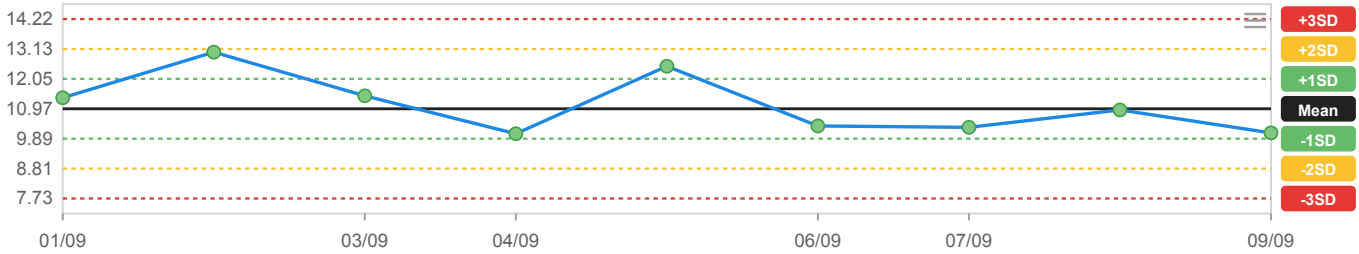


Comments _____ Reviewed by _____ Sign & Date _____

© Copyright 2025 Steller Infomatica. All rights reserved.


QCDart LJ Chart Report

Data Range	From: 01/09/2026 To: 09/09/2026
Oragnization/Lab name	Noble Diagnostic Centre / Noble Diagnostic Centre DELHI
Lab Address	WZ 409 C HARI NAGAR NEW DELHI,India,Delhi,Delhi,110064
Contact	SHIPRA | M: 9511018366
QC Lot Information	Bio-Rad | Lyphochek Immunoassay Plus Control | 40471 | 31/01/2028 | 40472 | 31/01/2028 | 40473 | 31/01/2028
Instrument Information	Snibe | Maglumi X3 | 01010100340124013 60
Test Information	LH | mIU/mL | CLIA - Chemiluminescence immunoassay

Level 1 - Mean: 1.79 | SD: 0.16 | CV: 8.84 | N: 9

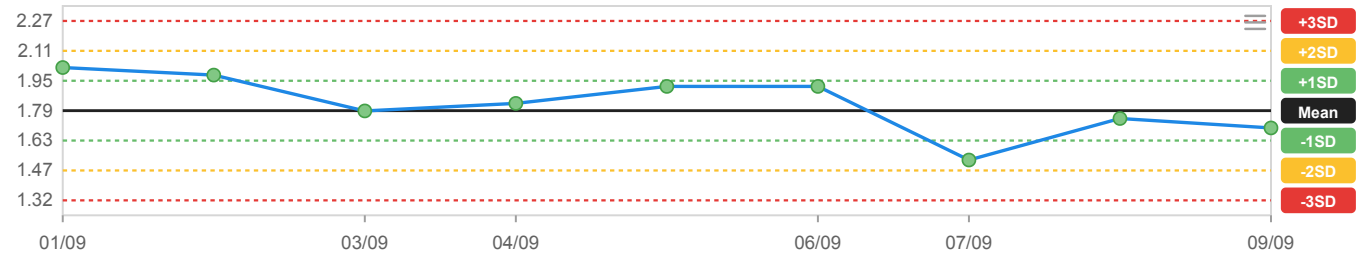

Level 2 - Mean: 24.97 | SD: 2.49 | CV: 9.97 | N: 9

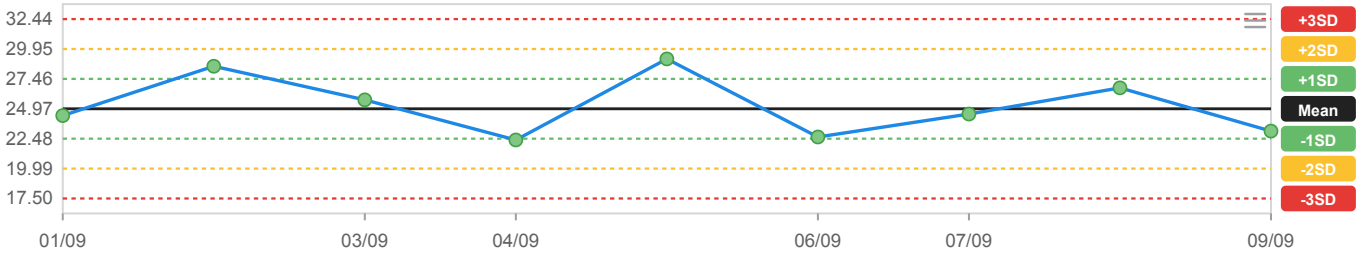


Comments _____ Reviewed by _____ Sign & Date _____

© Copyright 2025 Steller Infomatica. All rights reserved.


QCDart LJ Chart Report

Data Range	From: 01/09/2026 To: 09/09/2026
Oragnization/Lab name	Noble Diagnostic Centre / Noble Diagnostic Centre DELHI
Lab Address	WZ 409 C HARI NAGAR NEW DELHI,India,Delhi,Delhi,110064
Contact	SHIPRA | M: 9511018366
QC Lot Information	Bio-Rad | Lyphochek Immunoassay Plus Control | 40471 | 31/01/2028 | 40472 | 31/01/2028 | 40473 | 31/01/2028
Instrument Information	Snibe | Maglumi X3 | 01010100340124013 60
Test Information	TSH | µIU/mL | CLIA - Chemiluminescence immunoassay

Level 1 - Mean: 0.499 | SD: 0.046 | CV: 9.32 | N: 9

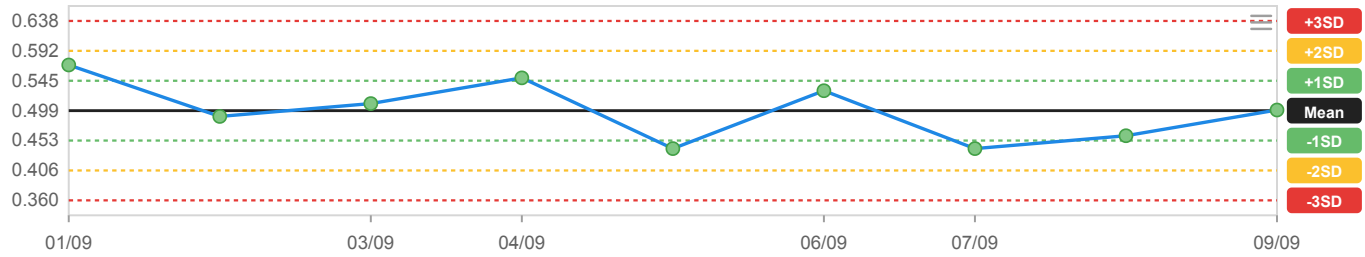

Level 2 - Mean: 5.75 | SD: 0.49 | CV: 8.58 | N: 9

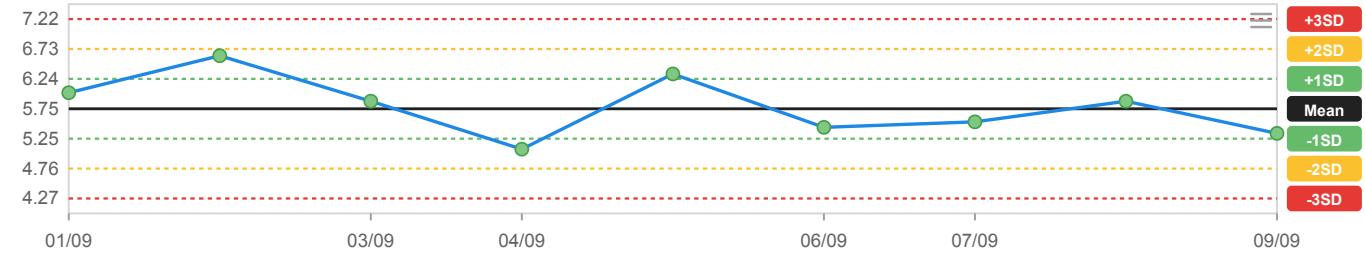

Comments _____ Reviewed by _____ Sign & Date _____

© Copyright 2025 Steller Infomatica. All rights reserved.