

QCDart LJ Chart Report

Data Range	From: 01/10/2025 To: 31/10/2025
Oragnization/Lab name	Noble Diagnostic Centre / Noble Diagnostic Centre DELHI
Lab Address	WZ 409 C HARI NAGAR NEW DELHI,India,Delhi,Delhi,110064
Contact	SHIPRA | M: 9511018366
QC Lot Information	Bio-Rad | Lyphochek Immunoassay Plus Control | 40471 | 31/01/2028 | 40472 | 31/01/2028 | 40473 | 31/01/2028
Instrument Information	Snibe | Maglumi X3 | 01010100340124013 60
Test Information	B-hCG | mIU/mL | CLIA - Chemiluminescence immunoassay

Level 1 - Mean: 8.60 | SD: 0.76 | CV: 8.81 | N: 29

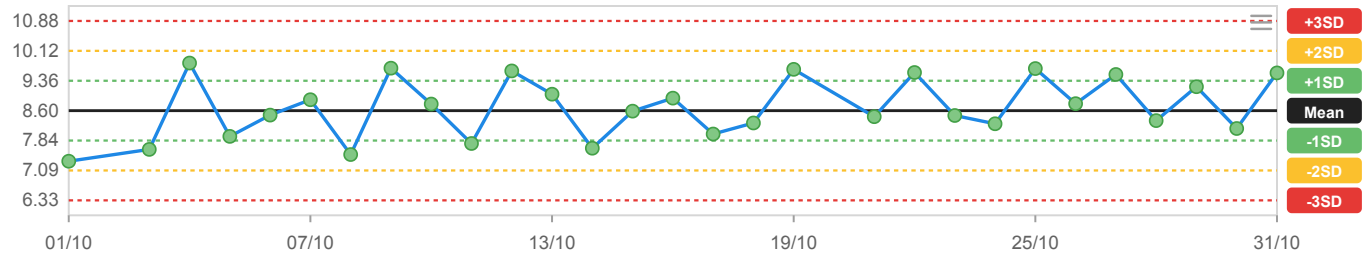

Level 2 - Mean: 22.81 | SD: 2.02 | CV: 8.85 | N: 29

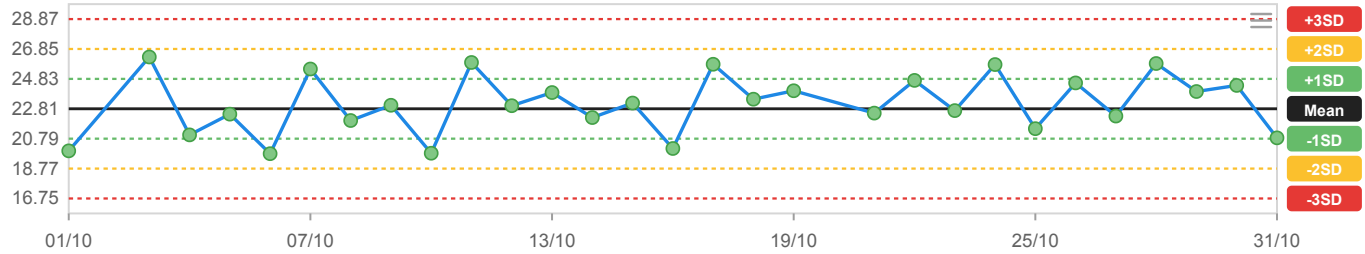


Comments _____ Reviewed by _____ Sign & Date _____

© Copyright 2025 Steller Infomatica. All rights reserved.


QCDart LJ Chart Report

Data Range	From: 01/10/2025 To: 31/10/2025
Oragnization/Lab name	Noble Diagnostic Centre / Noble Diagnostic Centre DELHI
Lab Address	WZ 409 C HARI NAGAR NEW DELHI,India,Delhi,Delhi,110064
Contact	SHIPRA | M: 9511018366
QC Lot Information	Bio-Rad | Lyphochek Immunoassay Plus Control | 40471 | 31/01/2028 | 40472 | 31/01/2028 | 40473 | 31/01/2028
Instrument Information	Snibe | Maglumi X3 | 01010100340124013 60
Test Information	FSH | mIU/mL | CLIA - Chemiluminescence immunoassay

Level 1 - Mean: 7.54 | SD: 0.60 | CV: 7.98 | N: 29

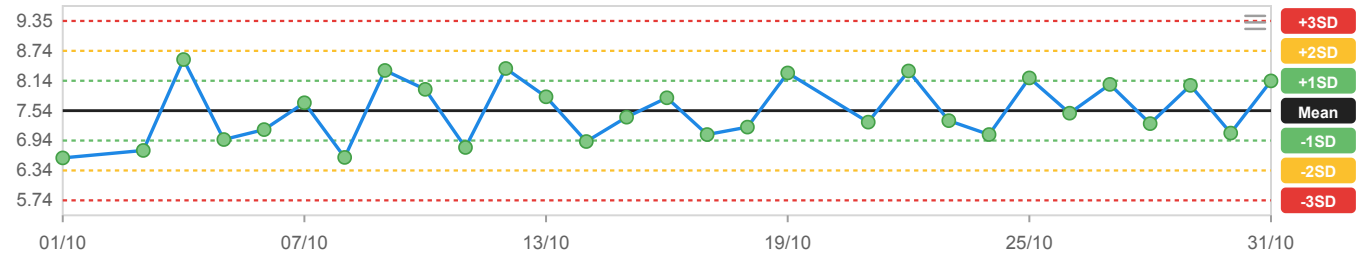

Level 2 - Mean: 25.32 | SD: 2.04 | CV: 8.05 | N: 29

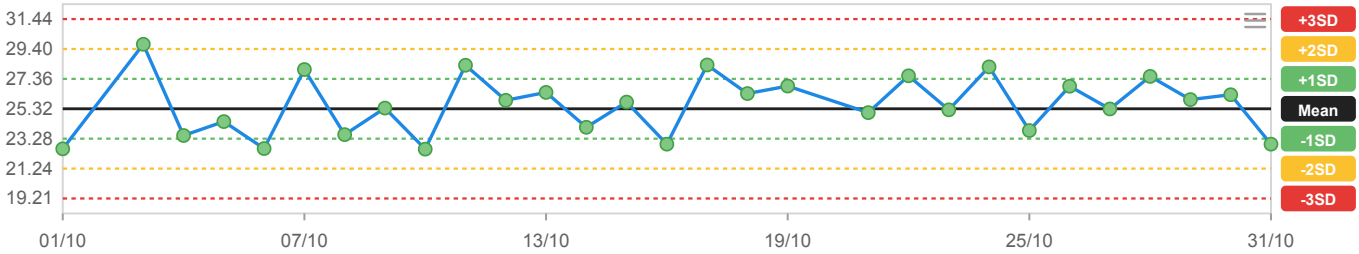


Comments _____ Reviewed by _____ Sign & Date _____

© Copyright 2025 Steller Infomatica. All rights reserved.


QCDart LJ Chart Report

Data Range	From: 01/10/2025 To: 31/10/2025
Oragnization/Lab name	Noble Diagnostic Centre / Noble Diagnostic Centre DELHI
Lab Address	WZ 409 C HARI NAGAR NEW DELHI,India,Delhi,Delhi,110064
Contact	SHIPRA | M: 9511018366
QC Lot Information	Bio-Rad | Lyphochek Immunoassay Plus Control | 40471 | 31/01/2028 | 40472 | 31/01/2028 | 40473 | 31/01/2028
Instrument Information	Snibe | Maglumi X3 | 01010100340124013 60
Test Information	Estradiol, E2 | pg/mL | CLIA - Chemiluminescence immunoassay

Level 1 - Mean: 86.18 | SD: 8.33 | CV: 9.67 | N: 29

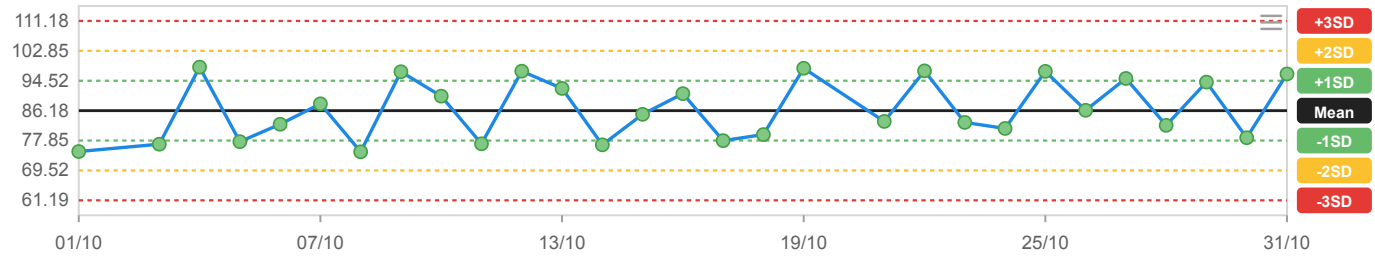

Level 2 - Mean: 319.35 | SD: 28.13 | CV: 8.81 | N: 29

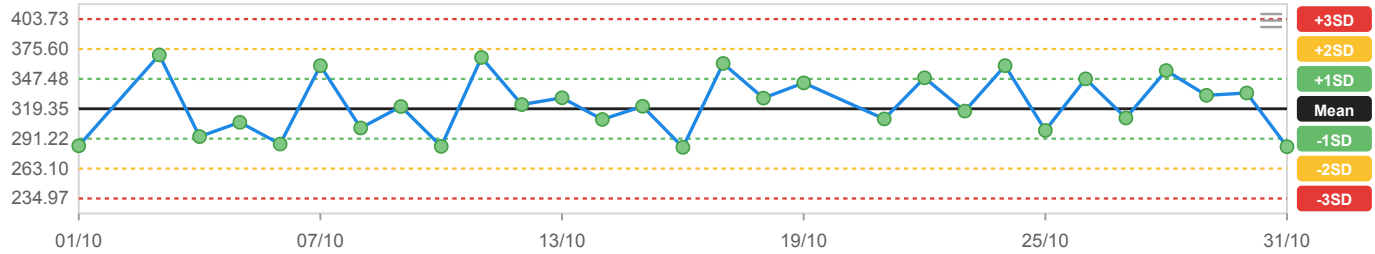


Comments _____ Reviewed by _____ Sign & Date _____

© Copyright 2025 Steller Infomatica. All rights reserved.


QCDart LJ Chart Report

Data Range	From: 01/10/2025 To: 31/10/2025
Oragnization/Lab name	Noble Diagnostic Centre / Noble Diagnostic Centre DELHI
Lab Address	WZ 409 C HARI NAGAR NEW DELHI,India,Delhi,Delhi,110064
Contact	SHIPRA | M: 9511018366
QC Lot Information	Bio-Rad | Lyphochek Immunoassay Plus Control | 40471 | 31/01/2028 | 40472 | 31/01/2028 | 40473 | 31/01/2028
Instrument Information	Snibe | Maglumi X3 | 01010100340124013 60
Test Information	T3 Total | ng/mL | CLIA - Chemiluminescence immunoassay

Level 1 - Mean: 0.700 | SD: 0.064 | CV: 9.14 | N: 29

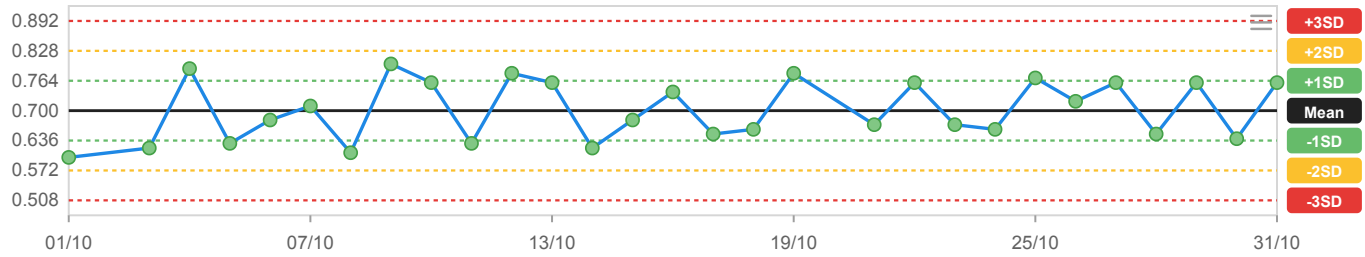

Level 2 - Mean: 1.83 | SD: 0.16 | CV: 8.78 | N: 29

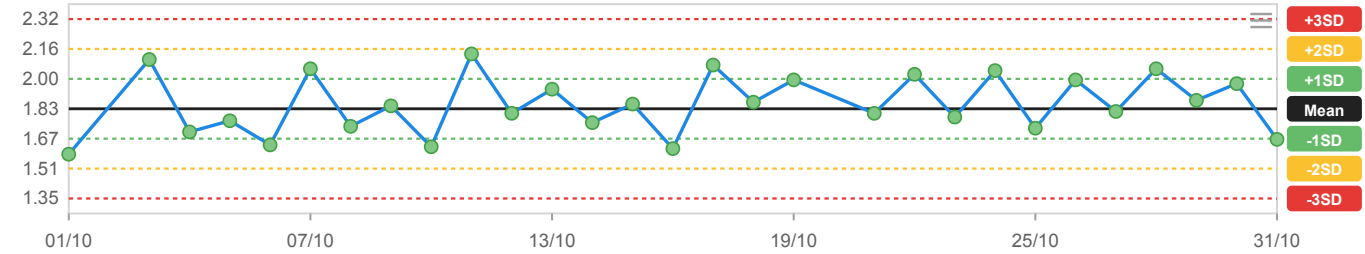


Comments _____ Reviewed by _____ Sign & Date _____

© Copyright 2025 Steller Infomatica. All rights reserved.


QCDart LJ Chart Report

Data Range	From: 01/10/2025 To: 31/10/2025
Oragnization/Lab name	Noble Diagnostic Centre / Noble Diagnostic Centre DELHI
Lab Address	WZ 409 C HARI NAGAR NEW DELHI,India,Delhi,Delhi,110064
Contact	SHIPRA | M: 9511018366
QC Lot Information	Bio-Rad | Lyphochek Immunoassay Plus Control | 40471 | 31/01/2028 | 40472 | 31/01/2028 | 40473 | 31/01/2028
Instrument Information	Snibe | Maglumi X3 | 01010100340124013 60
Test Information	Prolactin | ng/mL | CLIA - Chemiluminescence immunoassay

Level 1 - Mean: 7.07 | SD: 0.52 | CV: 7.39 | N: 29

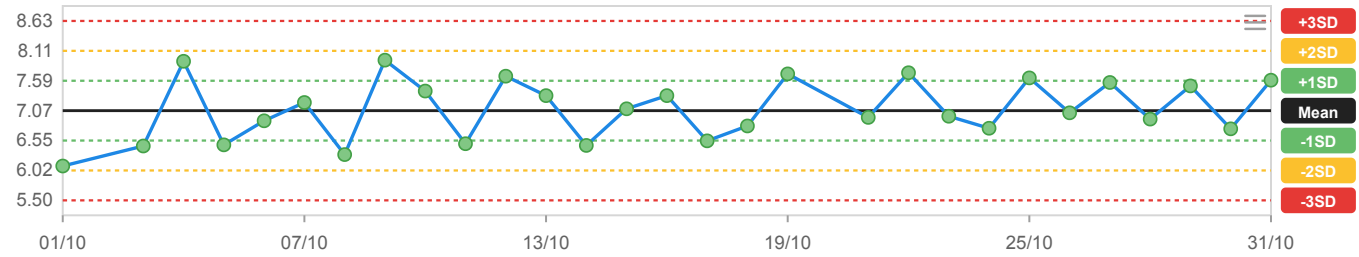

Level 2 - Mean: 21.04 | SD: 1.88 | CV: 8.94 | N: 29

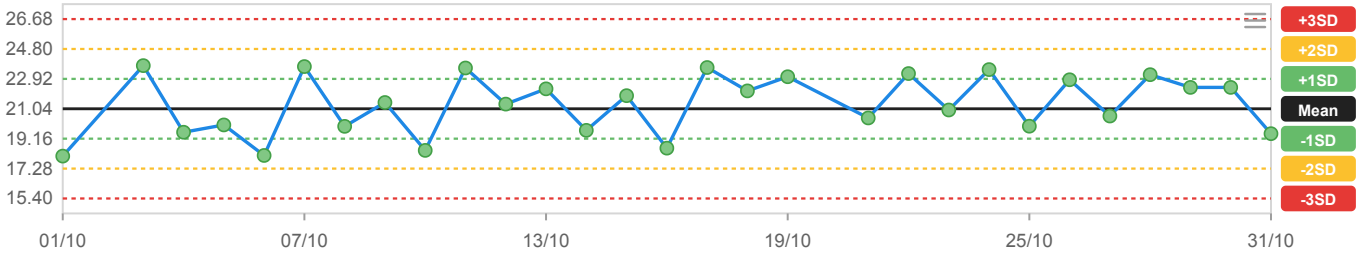


Comments _____ Reviewed by _____ Sign & Date _____

© Copyright 2025 Steller Infomatica. All rights reserved.


QCDart LJ Chart Report

Data Range	From: 01/10/2025 To: 31/10/2025
Oragnization/Lab name	Noble Diagnostic Centre / Noble Diagnostic Centre DELHI
Lab Address	WZ 409 C HARI NAGAR NEW DELHI,India,Delhi,Delhi,110064
Contact	SHIPRA | M: 9511018366
QC Lot Information	Bio-Rad | Lyphochek Immunoassay Plus Control | 40471 | 31/01/2028 | 40472 | 31/01/2028 | 40473 | 31/01/2028
Instrument Information	Snibe | Maglumi X3 | 01010100340124013 60
Test Information	Testosterone | ng/dL | CLIA - Chemiluminescence immunoassay

Level 1 - Mean: 124.26 | SD: 9.62 | CV: 7.74 | N: 29

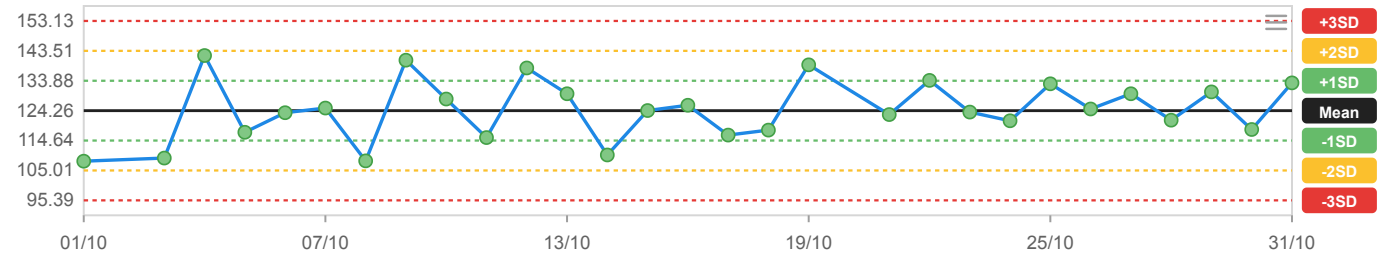

Level 2 - Mean: 300.02 | SD: 29.67 | CV: 9.89 | N: 29

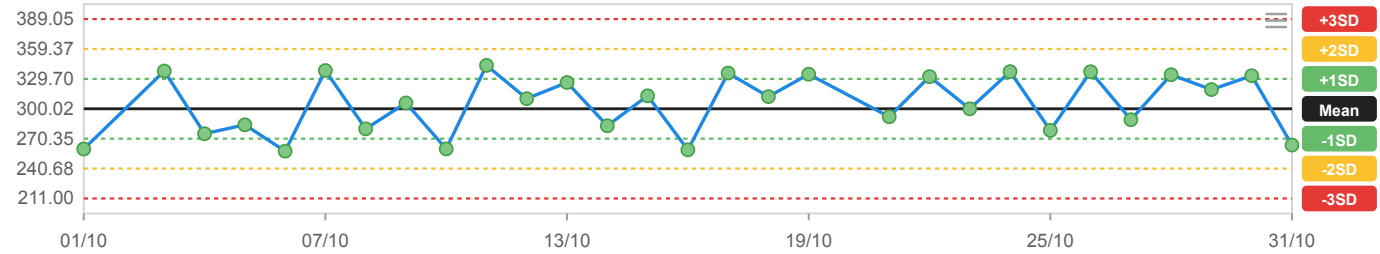


Comments _____ Reviewed by _____ Sign & Date _____

© Copyright 2025 Steller Infomatica. All rights reserved.


QCDart LJ Chart Report

Data Range	From: 01/10/2025 To: 31/10/2025
Oragnization/Lab name	Noble Diagnostic Centre / Noble Diagnostic Centre DELHI
Lab Address	WZ 409 C HARI NAGAR NEW DELHI,India,Delhi,Delhi,110064
Contact	SHIPRA | M: 9511018366
QC Lot Information	Bio-Rad | Lyphochek Immunoassay Plus Control | 40471 | 31/01/2028 | 40472 | 31/01/2028 | 40473 | 31/01/2028
Instrument Information	Snibe | Maglumi X3 | 01010100340124013 60
Test Information	T4 Total | µg/dl | CLIA - Chemiluminescence immunoassay

Level 1 - Mean: 6.15 | SD: 0.52 | CV: 8.53 | N: 29

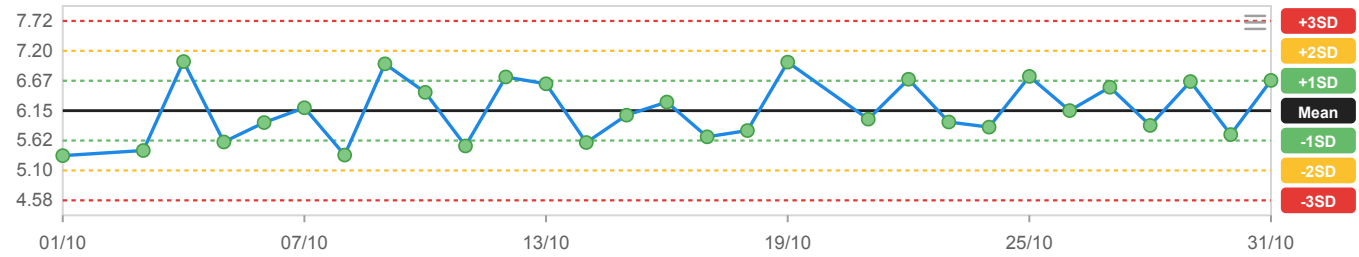

Level 2 - Mean: 10.97 | SD: 1.03 | CV: 9.35 | N: 29

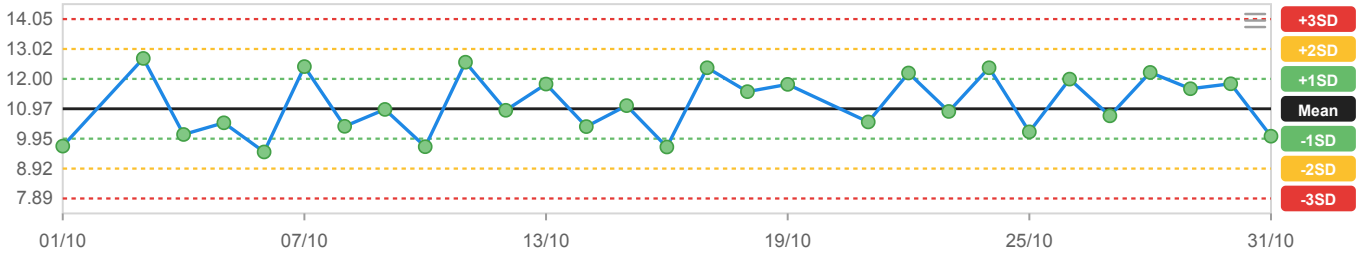


Comments _____ Reviewed by _____ Sign & Date _____

© Copyright 2025 Steller Infomatica. All rights reserved.


QCDart LJ Chart Report

Data Range	From: 01/10/2025 To: 31/10/2025
Oragnization/Lab name	Noble Diagnostic Centre / Noble Diagnostic Centre DELHI
Lab Address	WZ 409 C HARI NAGAR NEW DELHI,India,Delhi,Delhi,110064
Contact	SHIPRA | M: 9511018366
QC Lot Information	Bio-Rad | Lyphochek Immunoassay Plus Control | 40471 | 31/01/2028 | 40472 | 31/01/2028 | 40473 | 31/01/2028
Instrument Information	Snibe | Maglumi X3 | 01010100340124013 60
Test Information	LH | mIU/mL | CLIA - Chemiluminescence immunoassay

Level 1 - Mean: 1.79 | SD: 0.14 | CV: 7.96 | N: 29

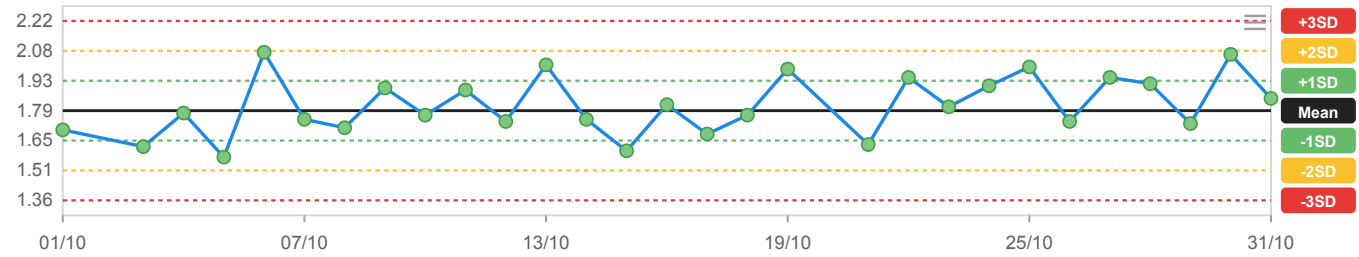

Level 2 - Mean: 24.97 | SD: 2.05 | CV: 8.21 | N: 29

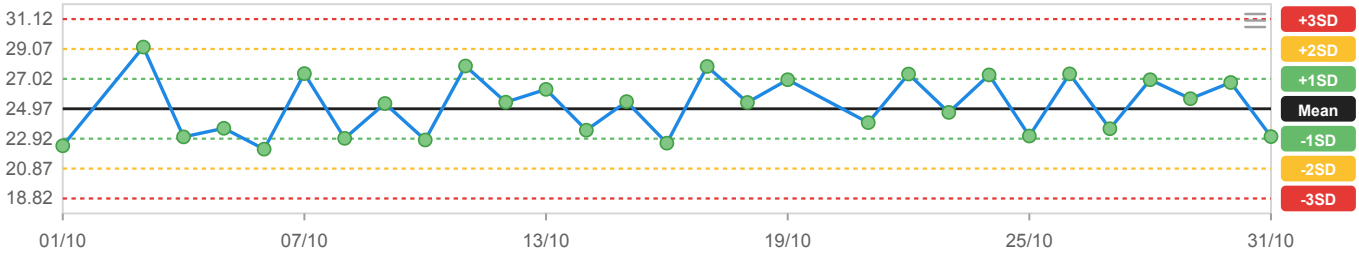


Comments _____ Reviewed by _____ Sign & Date _____

© Copyright 2025 Steller Infomatica. All rights reserved.


QCDart LJ Chart Report

Data Range	From: 01/10/2025 To: 31/10/2025
Oragnization/Lab name	Noble Diagnostic Centre / Noble Diagnostic Centre DELHI
Lab Address	WZ 409 C HARI NAGAR NEW DELHI,India,Delhi,Delhi,110064
Contact	SHIPRA | M: 9511018366
QC Lot Information	Bio-Rad | Lyphochek Immunoassay Plus Control | 40471 | 31/01/2028 | 40472 | 31/01/2028 | 40473 | 31/01/2028
Instrument Information	Snibe | Maglumi X3 | 01010100340124013 60
Test Information	TSH | µIU/mL | CLIA - Chemiluminescence immunoassay

Level 1 - Mean: 0.499 | SD: 0.037 | CV: 7.46 | N: 29

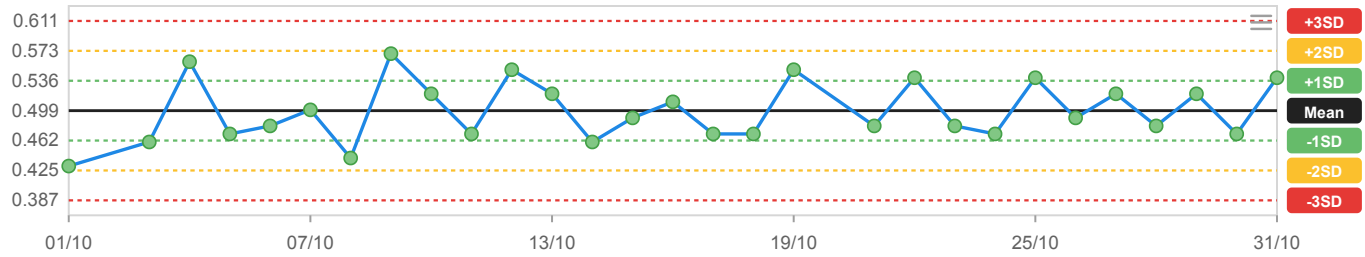

Level 2 - Mean: 5.75 | SD: 0.51 | CV: 8.87 | N: 29

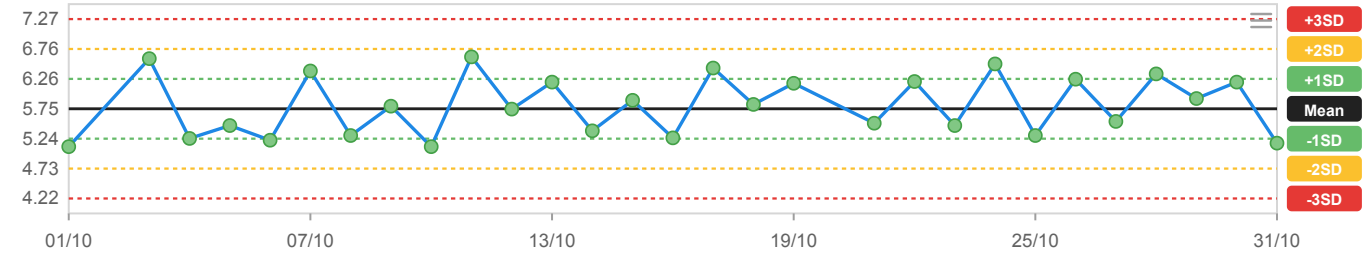

Comments _____ Reviewed by _____ Sign & Date _____

© Copyright 2025 Steller Infomatica. All rights reserved.