


PCP Quality Control Protocol (subject report)

- Subject ID: sub-12.
- Modality: functional.
- Date and time: 2016-05-13, 12:20.
- Sessions and (scans) failed: none.
- Image parameters:


| Session        | Scan ID            | Image size<br>(voxels) | Spacing (mm)             | TR (ms)  | Time steps |
|----------------|--------------------|------------------------|--------------------------|----------|------------|
| single_session | task-flanker_run-1 | 64 × 64 × 40           | 3.000 × 3.000 ×<br>4.000 | 2.000000 | 146        |
| single_session | task-flanker_run-2 | 64 × 64 × 40           | 3.000 × 3.000 ×<br>4.000 | 2.000000 | 146        |

For details on the IQMs (image quality metrics) and further information on the enclosed plots, please read the [user guide](#)


Mean fMRI, subject sub-12 (single\_session\_task-flanker\_run-1)

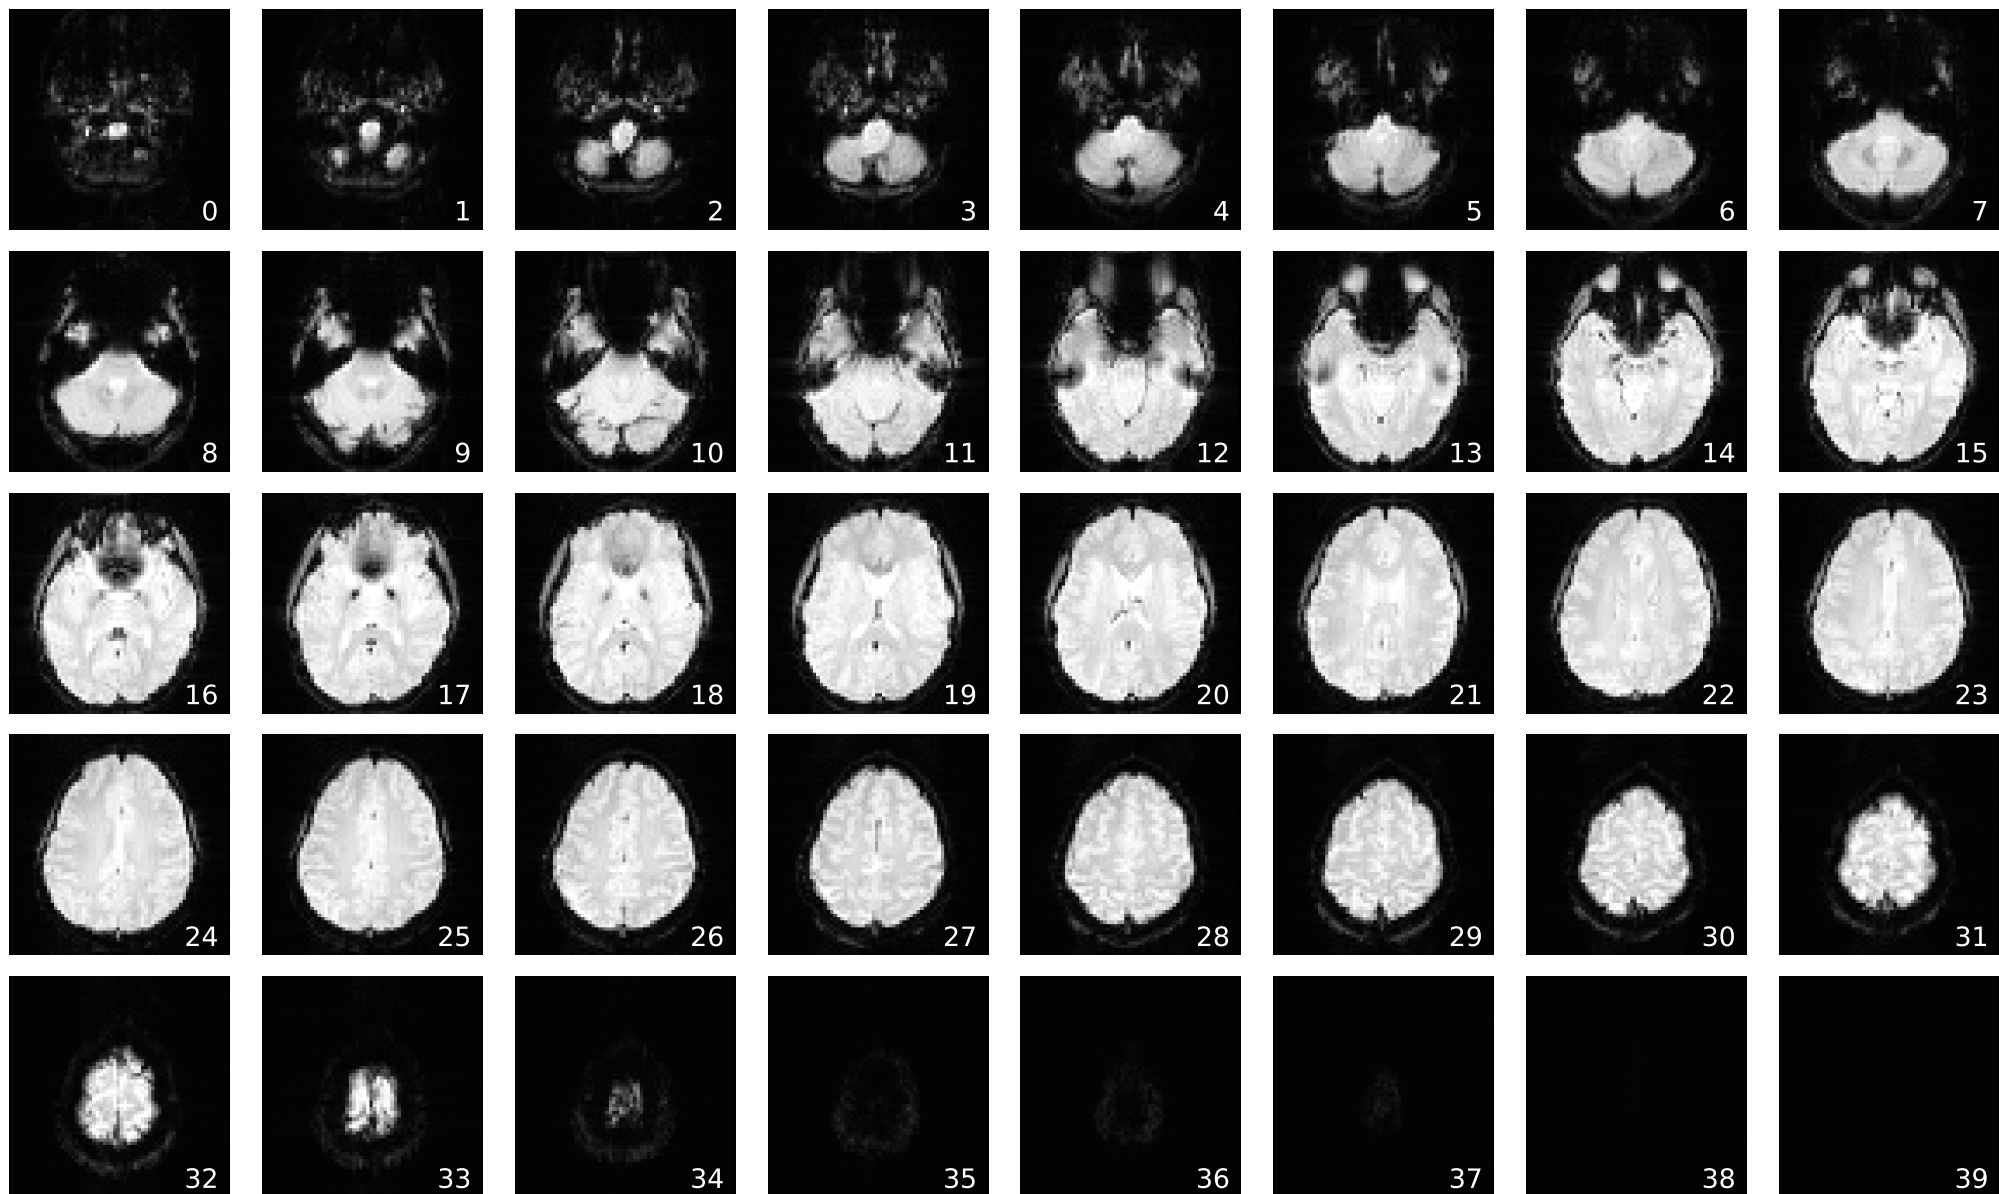


tSNR volume, subject sub-12 (single\_session\_task-flanker\_run-1)

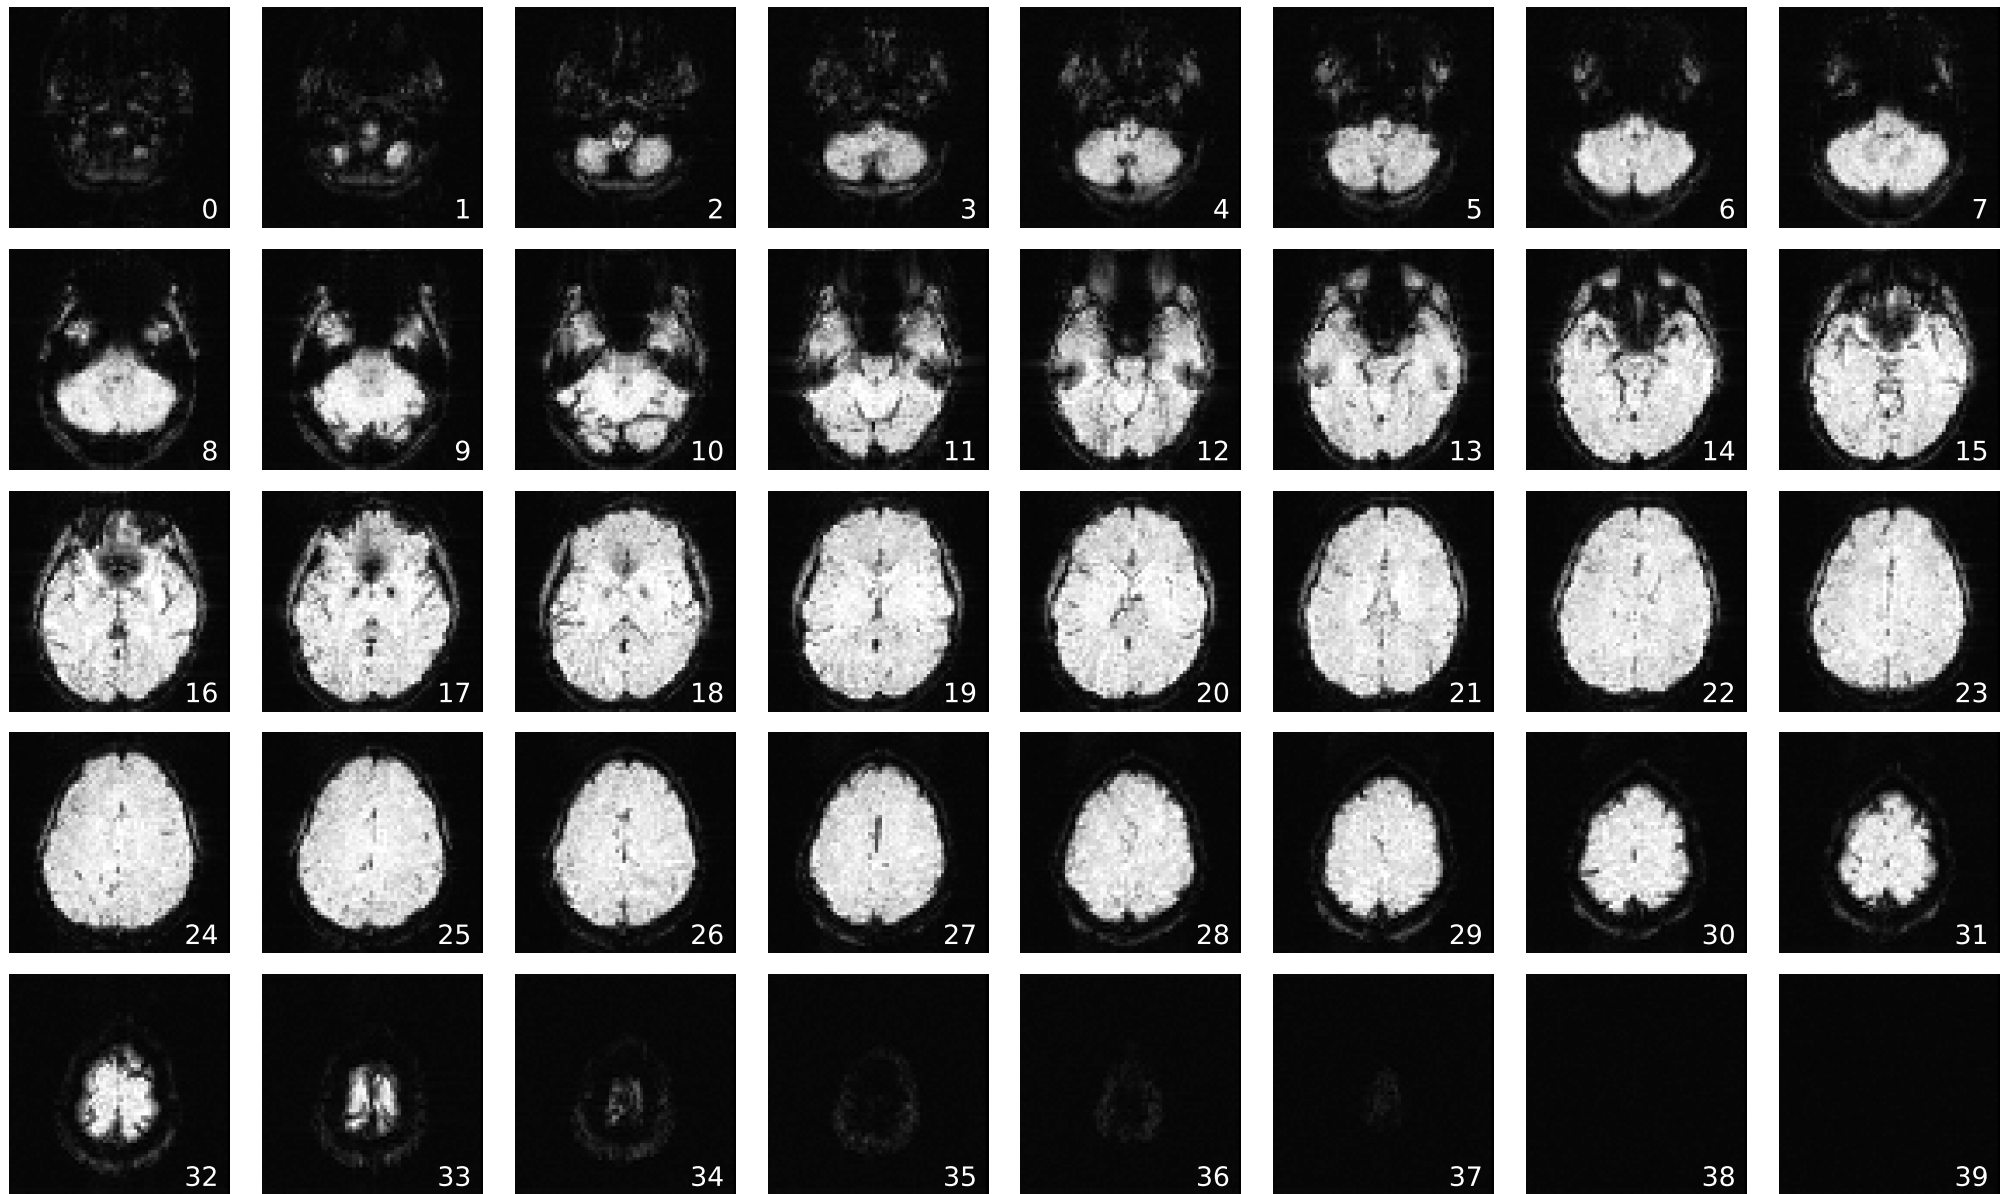


FD, subject sub-12 (single\_session\_task-flanker\_run-1)

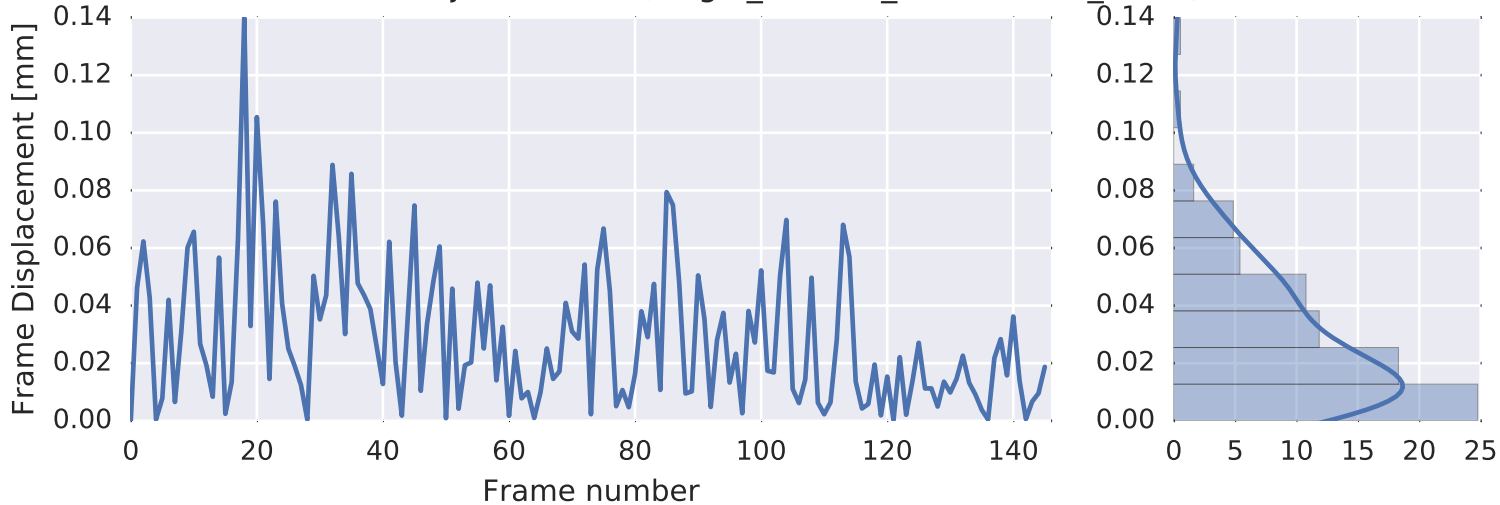


Mean fMRI, subject sub-12 (single\_session\_task-flanker\_run-2)

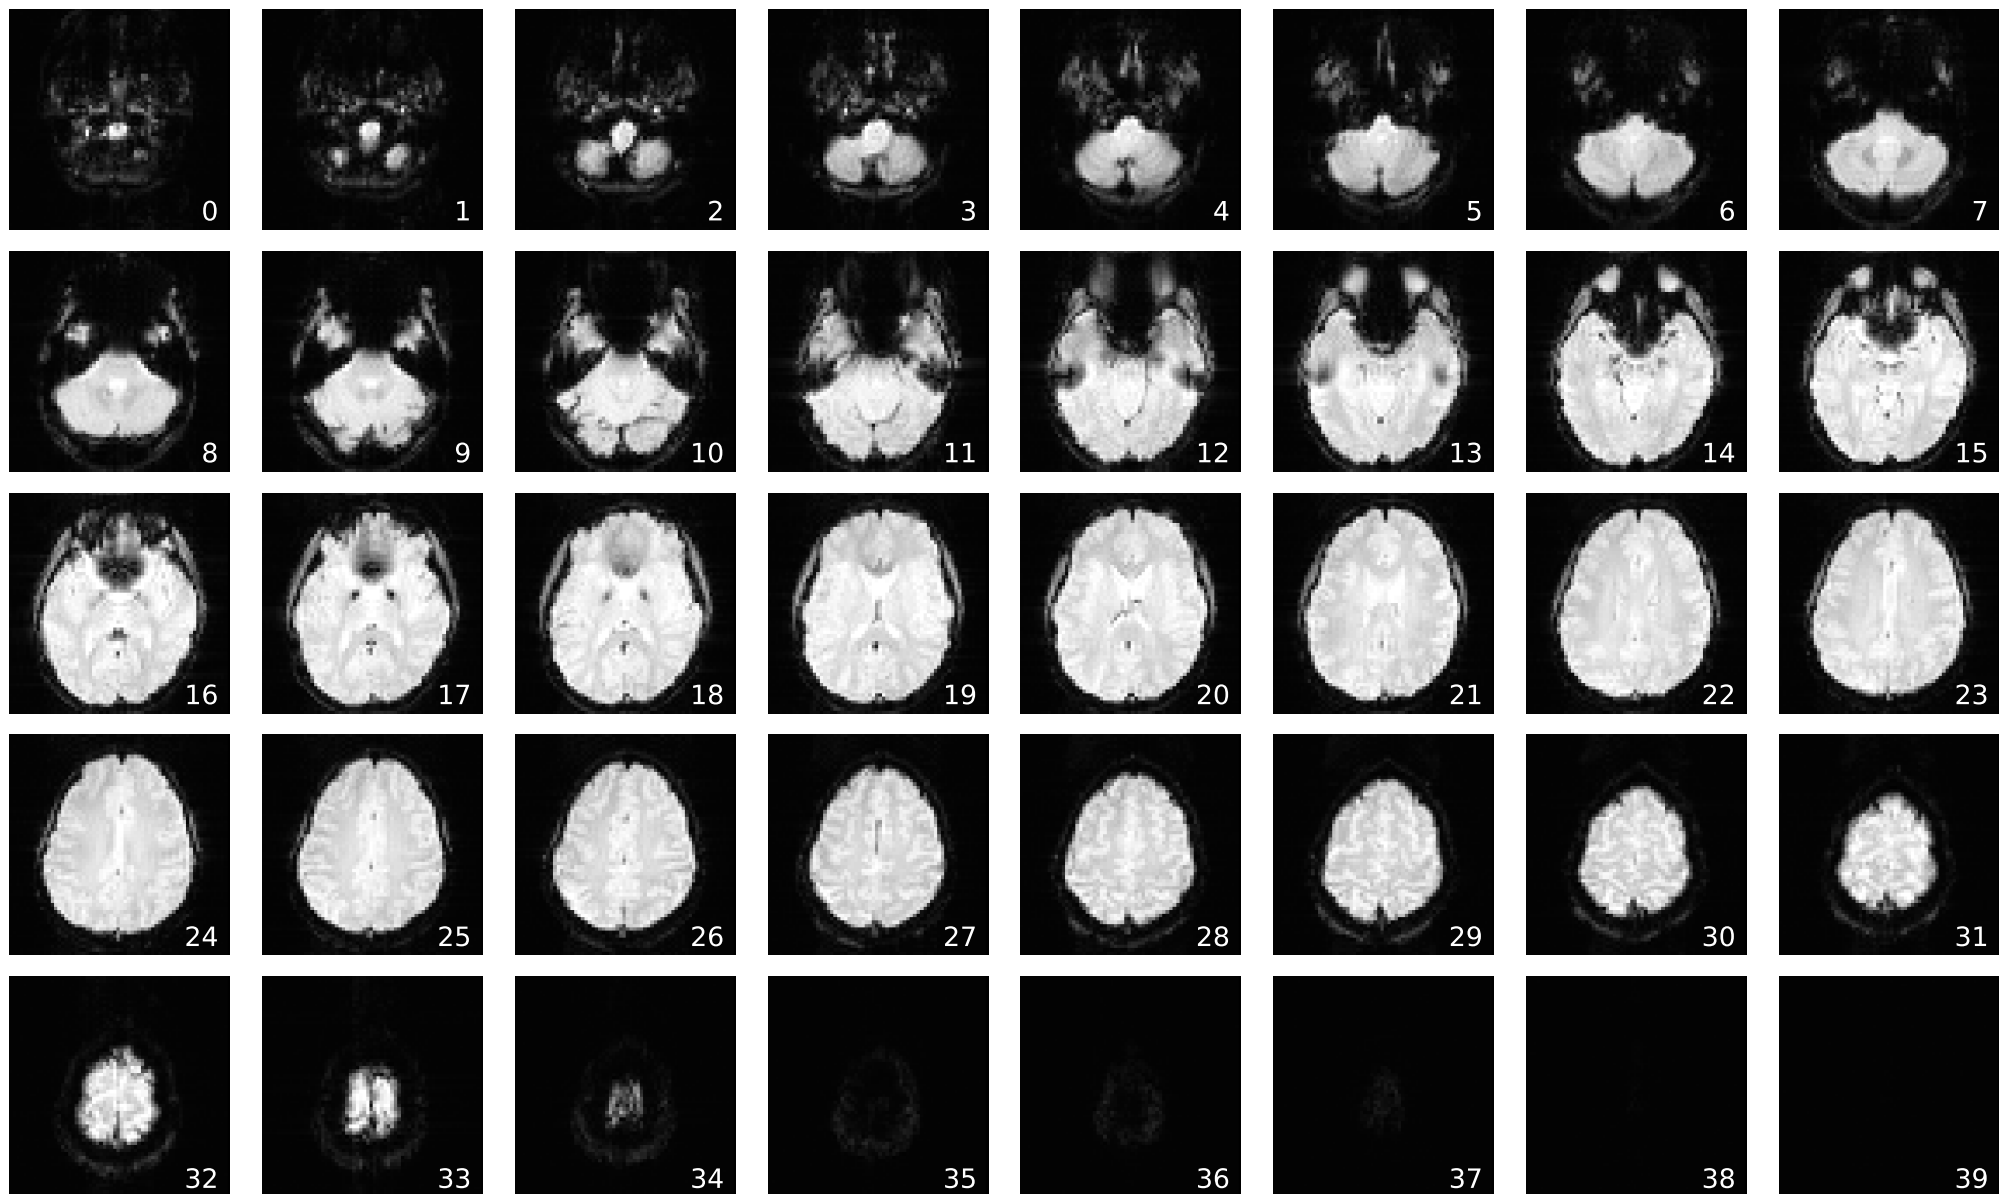


tSNR volume, subject sub-12 (single\_session\_task-flanker\_run-2)

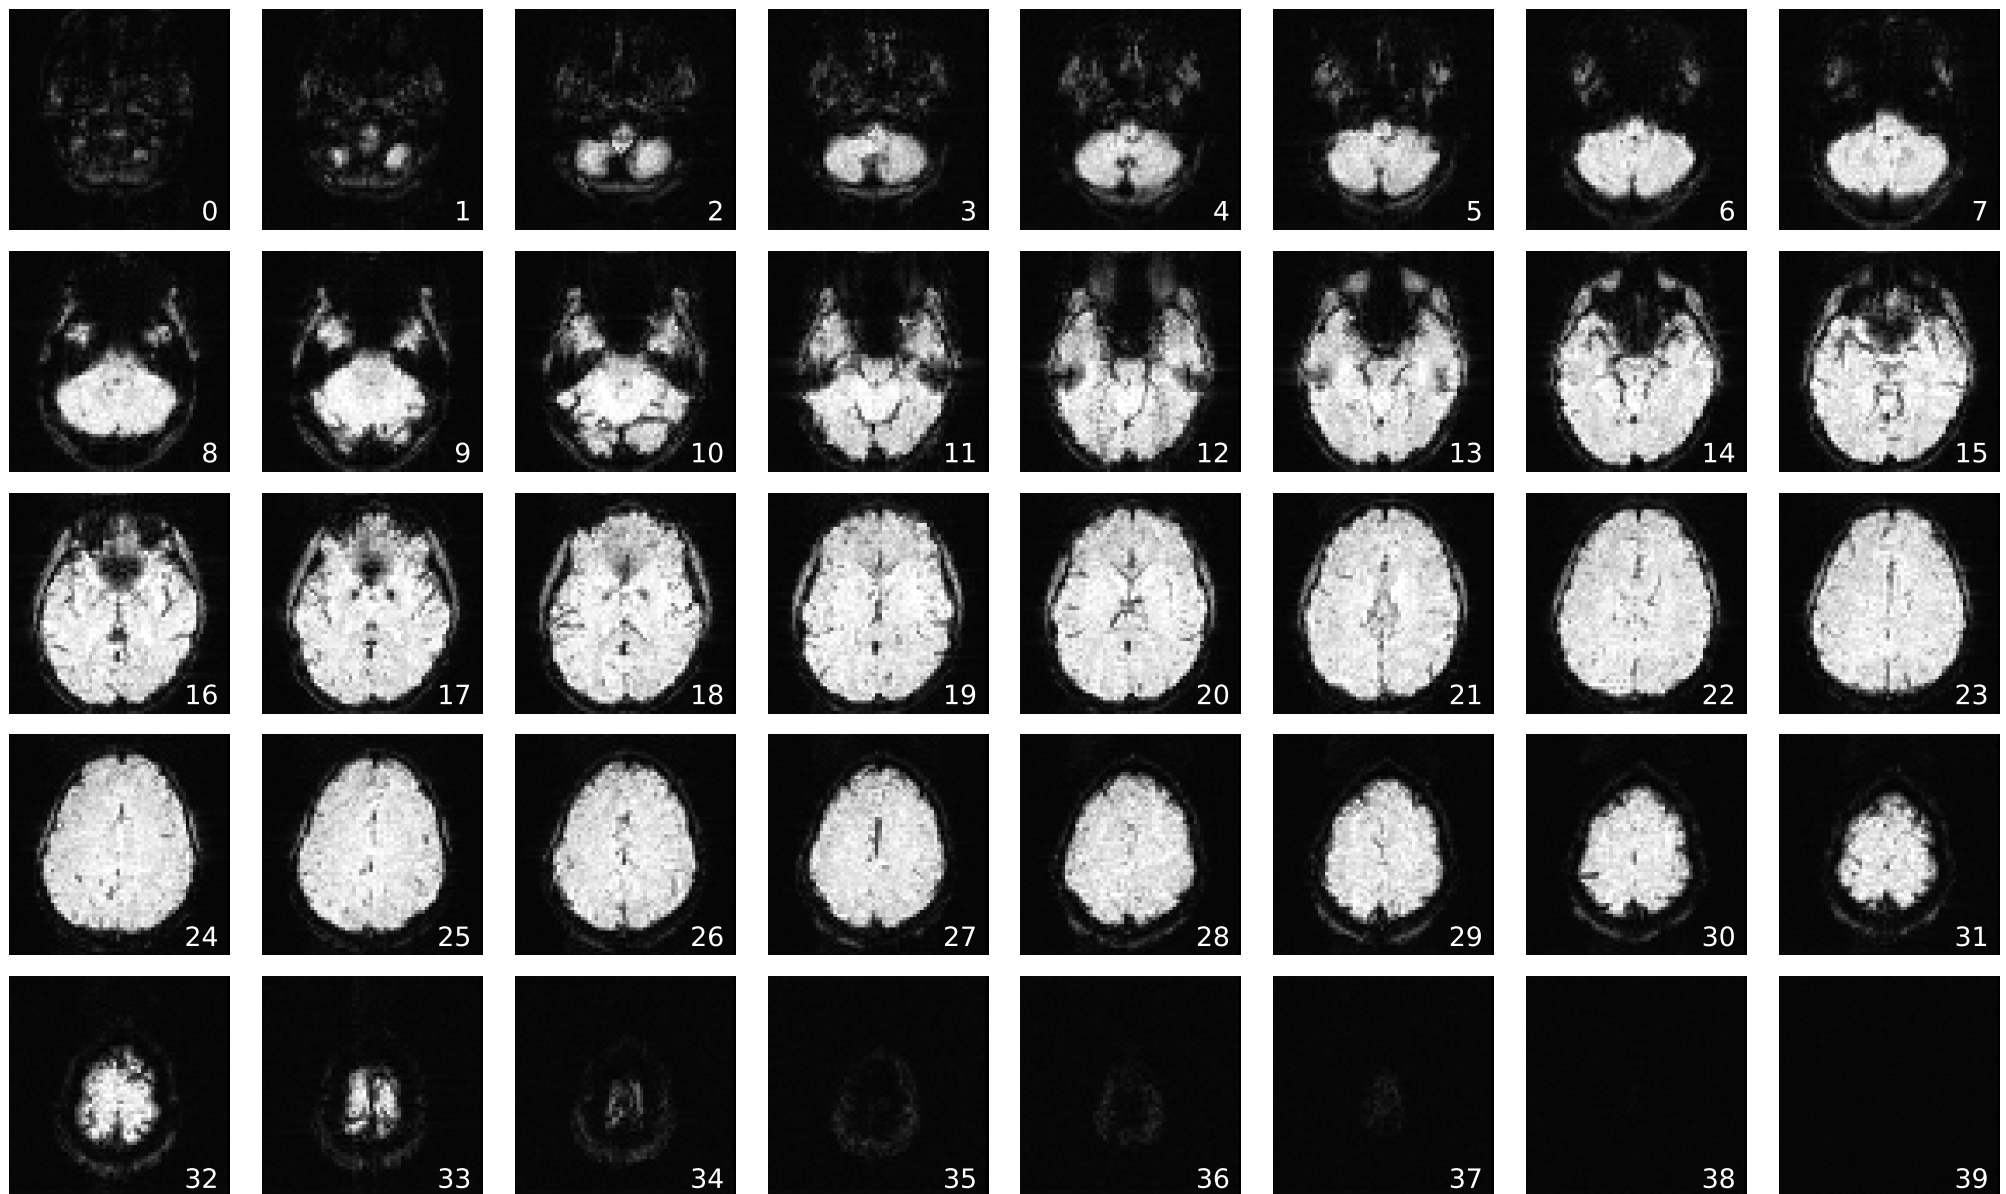

FD, subject sub-12 (single\_session\_task-flanker\_run-2)

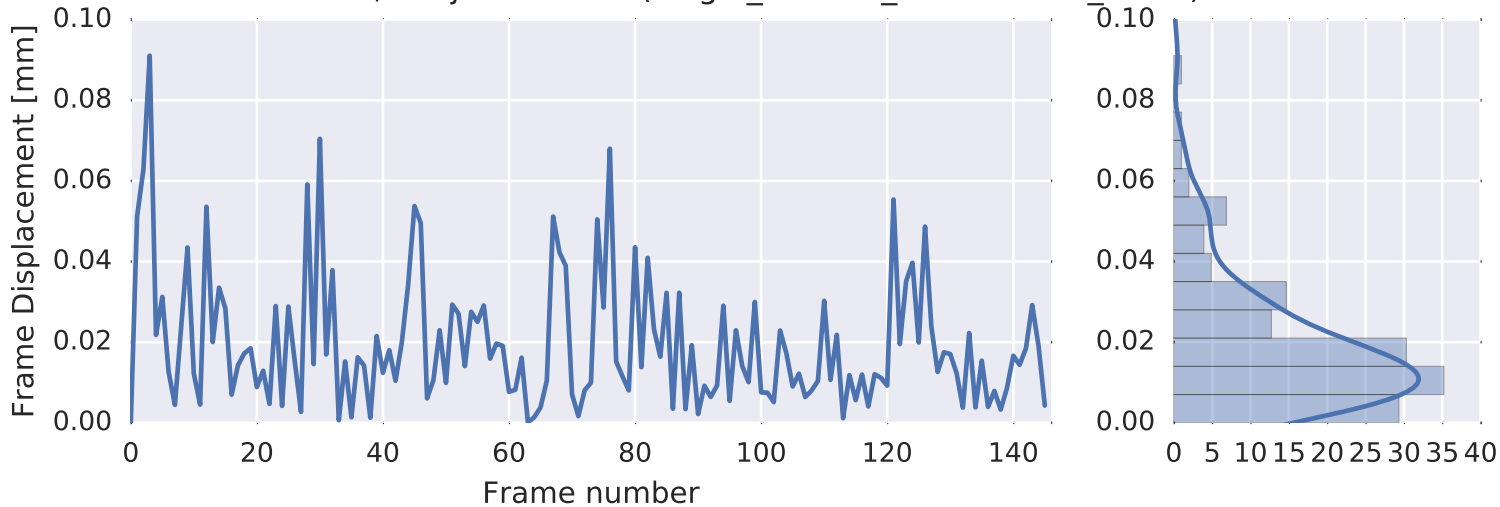

QC measures (subject sub-12\_single\_session)

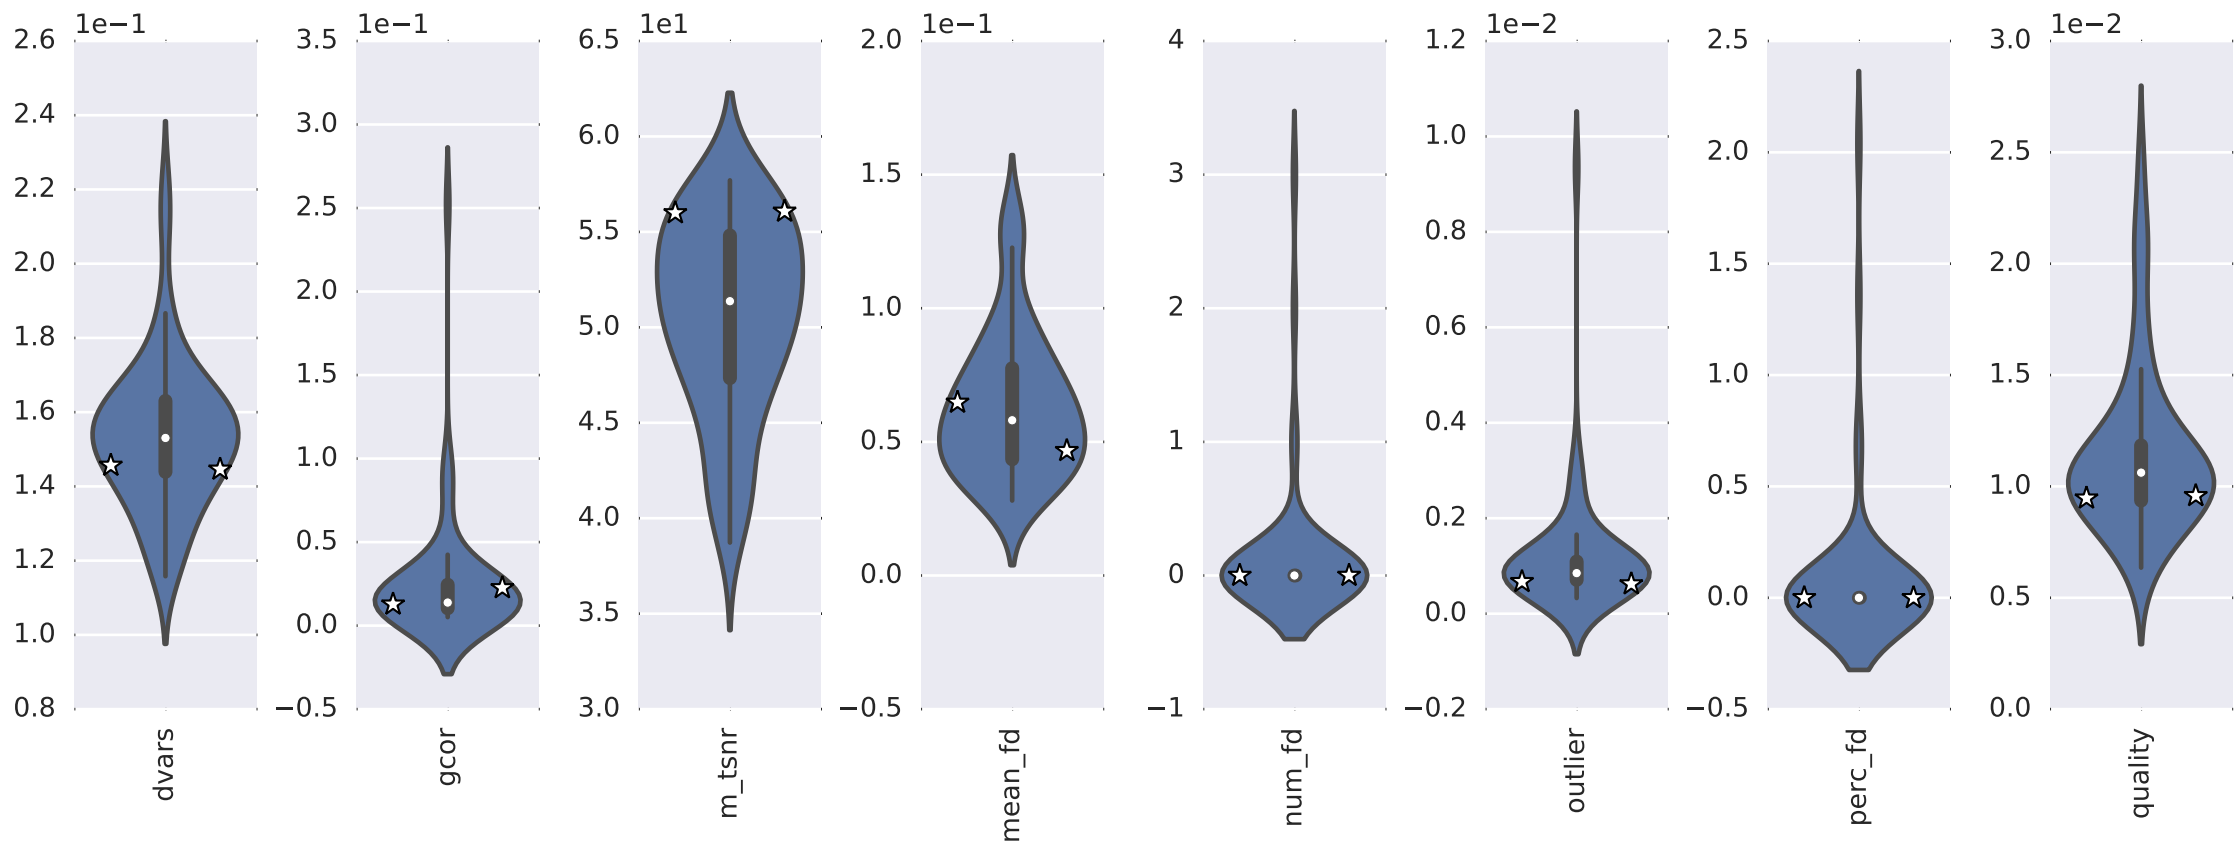



QC measures (subject sub-12\_single\_session)

