


Two different needle in place
holding designs




Push and twist mechanism

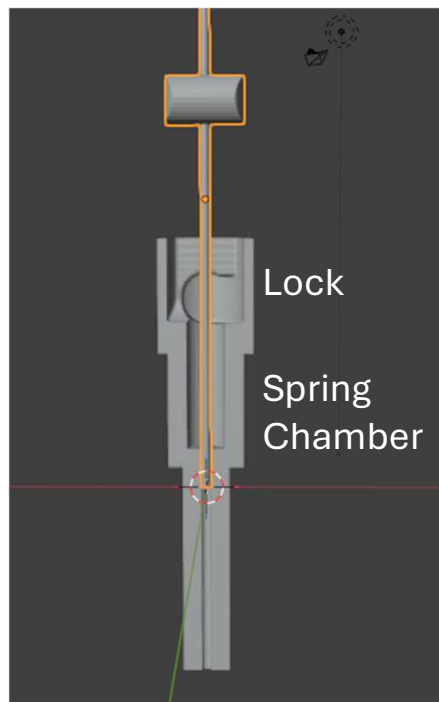


Pro:
Only 3 parts
Case
Needle Holder
Spring

Con:
Requires a 5mm diameter

Push and twist mechanism

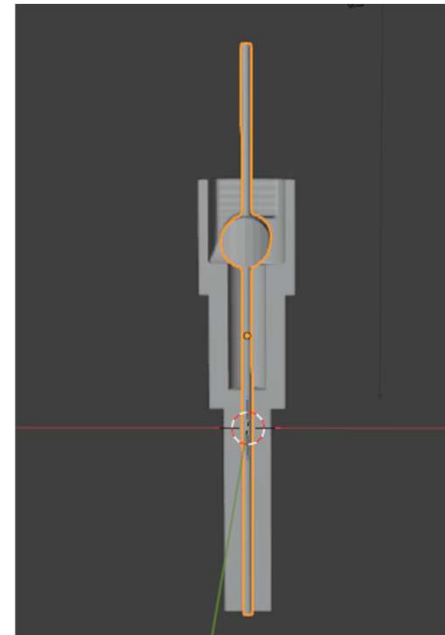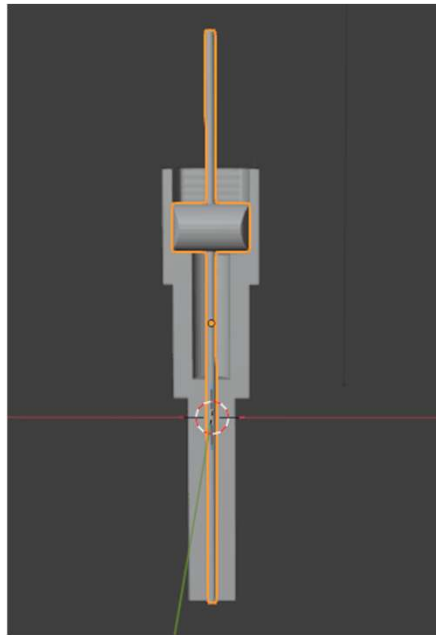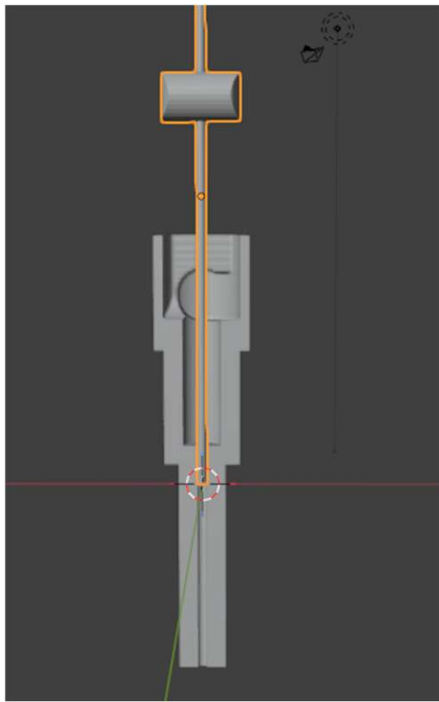

The three part assembly

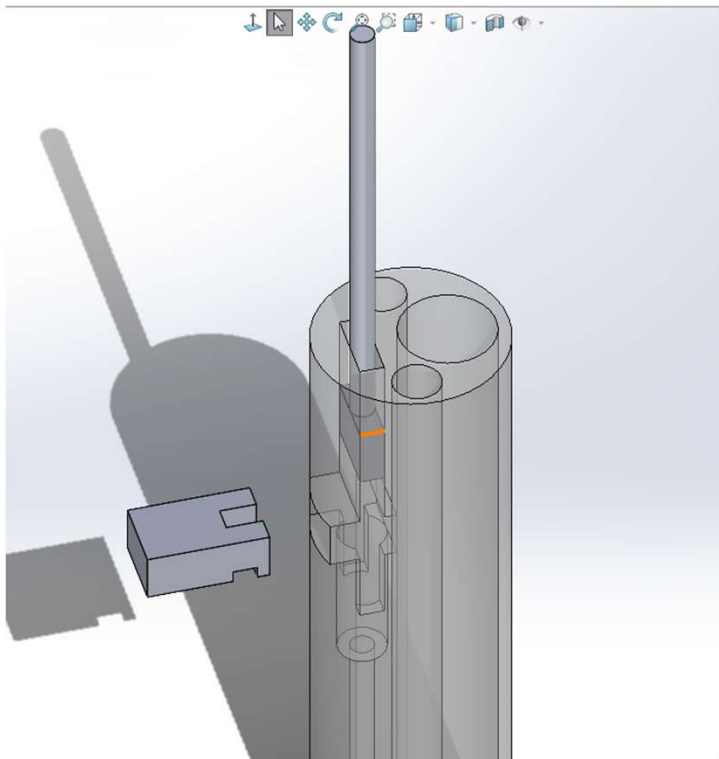

Pro: 4mm Hole for the 2photon allowed through entire assembly

Con: needs 4 parts:

Case

Needle holder

Side holder

Spring

