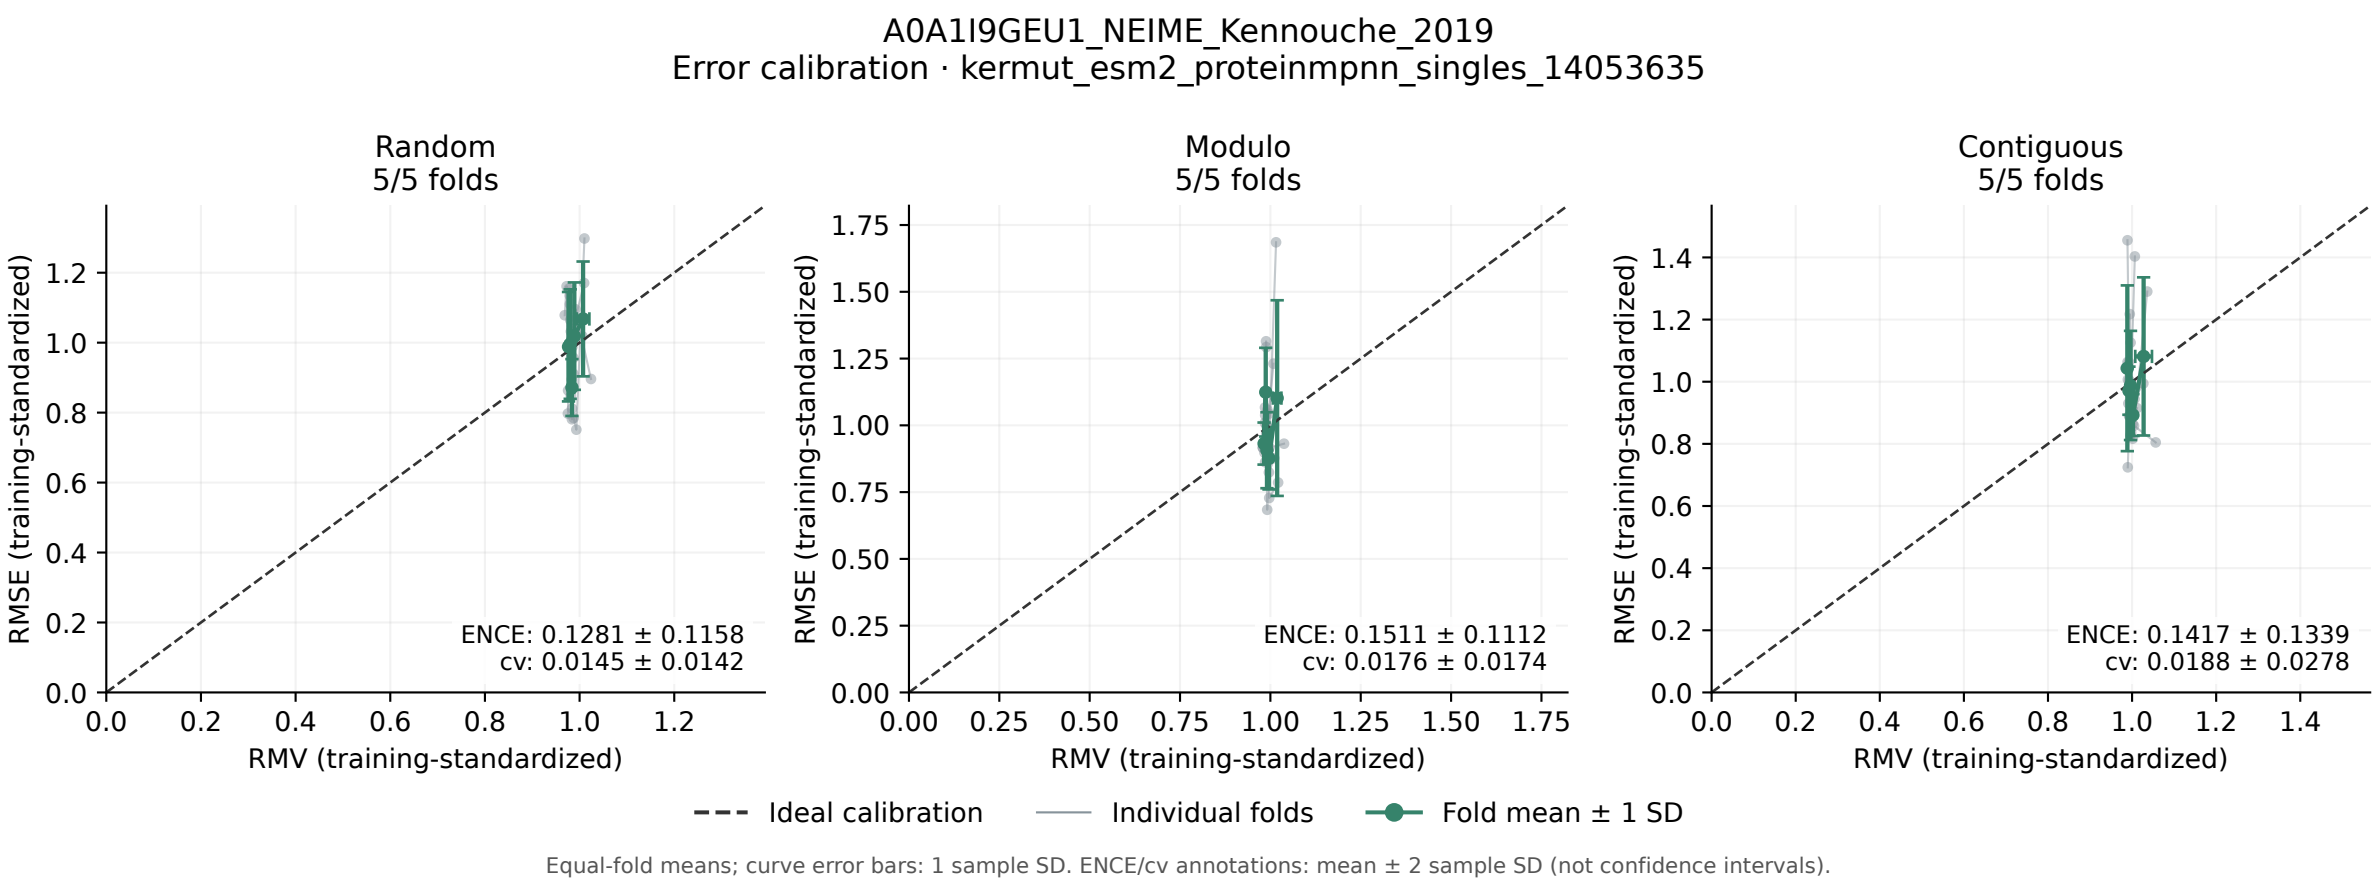
A0A1I9GEU1_NEIME_Kennouche_2019
Error calibration · kermut_esm2_proteinmpnn_singles_14053635
Random
5/5 folds
Modulo
5/5 folds
Contiguous
5/5 folds
RMSE (training-standardized)
RMV (training-standardized)
ENCE: 0.1281 ± 0.1158
cv: 0.0145 ± 0.0142
ENCE: 0.1511 ± 0.1112
cv: 0.0176 ± 0.0174
ENCE: 0.1417 ± 0.1339
cv: 0.0188 ± 0.0278
Ideal calibration
Individual folds
Fold mean ± 1 SD
Equal-fold means; curve error bars: 1 sample SD. ENCE/cv annotations: mean ± 2 sample SD (not confidence intervals).