

Density Changes in Low Pressure Gas Targets for Electron Scattering Experiments

S. N. Santiesteban^e, S. Alsalmi^a, J. Bane^b, J. Castellanos^c, R. Cruz-Torres^d, H. Dai^f, T. Hague^a, F. Hauenstein^g, D. W. Higinbothamⁱ, R. J. Holt^{m,n}, T. Kutz^j, S. Li^e, H. Liu^h, R. E. McClellanⁱ, D. Meekinsⁱ, M. Nycz^a, D. Nguyen^l, B. Pandey^l, Tong Su^a, Z. Ye^m

^aKent State University, Kent, OH 44240

^bThe University of Tennessee, Knoxville, Tennessee 37996, USA

^cFlorida International University, Miami, FL 33199 USA

^dMassachusetts Institute of Technology, Cambridge, Massachusetts 02139, USA

^eUniversity of New Hampshire, Durham, NH 03824 USA

^fVirginia Tech, Blacksburg, Virginia 24061

^gOld Dominion University, Norfolk, Virginia 23529, USA

^hColumbia University, New York, New York 10027, USA

ⁱJefferson Lab, Newport News, VA 23601 USA

^jStony Brook University, Stony Brook, New York 11794, USA

^kDepartment of Physics, University of Virginia, Charlottesville, Virginia 22904, USA

^lHampton University, Hampton, Virginia 23669, USA

^mPhysics Division, Argonne National Laboratory, Argonne, Illinois 60439, USA

ⁿThe Division of Physics Mathematics and Astronomy, California Institute of Technology, Pasadena California 91125 USA

Abstract

A system of modular sealed gas target cells has been developed for use in electron scattering experiments at The Thomas Jefferson National Accelerator Facility (Jefferson Lab). This system was initially developed to complete the *Marathon* experiment which required, among other species, tritium as a target material. The system has been used in several 12 GeV era of experiments in Experimental Hall A using the Jefferson Lab Continuous Electron Beam Accelerator Facility (CEBAF). Thus far, the cells have been loaded with the gas species ^3H , ^3He , ^2H , ^1H and ^{40}Ar and operated in nominal beam currents of up to $22.5\ \mu\text{A}$. Each cell is 25 cm long with a diameter of 1.3 cm. While gas density of the cells at the time of loading is known, the density of the each gas varies uniquely when heated by the electron beam. To extract experimental cross sections using these cells the beam current dependent density of each target fluid must be determined. In this study, data from measurements with several beam currents within the range of 2.5 to $22.5\ \mu\text{A}$ on each target fluid are presented. Additionally, expressions for the beam dependent fluid density of each target are developed.

Keywords: Density, target system, ^3H , ^3He , ^2H , ^1H , ^{40}Ar , CEBAF

1. Introduction

A modular gas cell target system was developed for use in Hall A at Jefferson Lab for the MARATHON experiment (E12-10-103)[1]. The design was specifically developed to safely contain and operate with gaseous tritium. The modular design allows additional gas cells filled with other species of gas to be installed in the system concurrently. The target was also adapted for the additional experiments E12-11-112 ($x_b > 1$) [2], E12-14-011 ($e'p$) [3], E12-17-003 (Hypernuclear) [4] and E12-14-009 (elastic) [5]. MARATHON, together with these experiments, became known as the tritium group experiments which were performed from December 2017 through November 2018. However, prior to tritium operations, a target cell was loaded with argon gas and used by the experiment E12-14-012 (Argon) [6] during Spring of 2017.

While the performance of the target was an important consideration, the primary objective of the target system design and construction was to ensure safe operations with tritium gas under all conditions including reasonable upset conditions. These

conditions included target cell preparations, loading, storage, transportation, installation, removal, and beam operations. This was accomplished with a modular design, rigorous fabrication and testing, proper quality assurance (QA) and quality control (QC) and multiple layers of containment/confinement.

In addition to a brief description of the target, we present the beam current dependent density of the five gases used with the target system, ^3H , ^3He , ^2H , ^1H and ^{40}Ar . The electrons in the beam pass through the target fluid and cell entrance and exit end caps depositing ionization energy. This ionization energy, which is proportional to the beam current, induces heat in the target fluid causing local changes in the density. To determine the magnitude of this effect, data were collected with the Left High Resolution Spectrometer (LHRS) in Jefferson Lab Experimental Hall A during February 2017 for the ^{40}Ar target and December 2017 for the other targets. The beam energy for the study was 2.2 GeV in all cases, The momentum and angle settings were 17.5° and 1.79 GeV for ^{40}Ar , and 17.0° and 1.99 GeV for the other fluids. Analysis of these data shows that a

simple quadratic polynomial function normalized to zero current density provides an excellent model for all target fluids.

2. Target System

The modular design allows multiple cell configurations. It also enables individual cells to be installed in special configurations of the standard Hall A Cryogenic target; this was the case for the ^{40}Ar target (see Figure 1). Another feature is that it allows cells to be filled at off site locations other instead of Jefferson Lab. The tritium cell was filled at Savannah River Site (SRS) by Savannah River Tritium Enterprises (SRTE). The tritium cell was filled with about 0.1 grams of tritium gas to a room temperature pressure of about 200 psia. It was shipped in a special purpose transport container called the Bulk Tritium Shipping Package (BTSP). Including the cell this system provided continuous triple layer confinement though out the shipping and handling process. This design also allowed the tritium cell to be stored in a special storage container in Hall A while normal Hall installation activities were completed. The tritium cell was installed after all other preparatory tasks were completed.



Figure 1: Argon cell installation. A cell filled with ^{40}Ar was installed on the standard Hall A Cryogenic Target in place of the loop 3 cell

The configuration of the tritium target is shown in Figure 2. In this configuration, there are (from top to bottom) four cells loaded with ^3H , ^2H , ^1H , and ^3He as well as a fifth empty cell which was used for background measurements. The cells are contained in a scattering chamber which is under vacuum. The scattering chamber vacuum is isolated from the upstream beam line vacuum by a 0.2 mm thick beryllium window. This window is roughly 30 cm upstream of the target center and is mounted on a reentrant tube that also contains a 15 cm long tungsten collimator with an inner diameter of 12.7 mm. The target vacuum, with a pumping system directed to an exhaust stack, provided a second layer of tritium confinement. An exhaust system, (together with strict access controls) capable of maintaining a slight negative pressure in the experimental Hall ensured that the Hall boundary was a third layer of confinement.

Each cell, excluding the fill valve assembly, is machined from ASTM B209 aluminum 7075-T651 plate. Each target cell has a cigar-tube shaped active fluid space with a length of 25 cm



Figure 2: Ladder Assembly. Five cells were assembled during Fall 2017 to Spring 2018, ^3H , ^2H , ^1H , ^3He and empty cell from top to bottom

and a diameter of 12.7 cm. The total volume of the cell (including the non active region) is $33.38 \pm 0.2 \text{ cm}^3$. The thickness of the nearly flat entrance window and hemispherical exit window is nominally 0.25 mm. The parameters at the time of loading for each cell are summarized in Table 1. Due to machining tolerances, the wall thickness of each cell varies slightly over its length. Thickness measurements were performed for each cell at several locations (schematically represented in Figure ?? and are summarized in Table 4. The ^{40}Ar cell, installed in February 2017 in a special configuration, was later installed as the empty (or dummy) cell for the tritium group of experiments. Table 2 shows the ^{40}Ar and the Empty Cell in a single column. The ^{40}Ar experiment employed two aluminum foils (dummy target), with total thickness matching the radiation length of the argon filled cell, to measure backgrounds.

The entire target assembly, of five cells and assorted solid targets, was cooled with 15K helium from the Jefferson Lab End Station Refrigerator (ESR). The 15K helium was preheated to 40K and used to cool a heat sink to which the cell assemblies were attached. This removed the modest amount of heat generated by the electron beam passing through the target fluid, cell entrance and cell exit, which, in total, was about 15W. To ensure cell integrity, the maximum beam current permitted on any of the cells was $22.5 \mu\text{A}$ [7]. The heat generated by the tritium decay is very small, about 50 mW and was negligible.

3. Experimental Hall A

The data were acquired with the LHRS. For a detailed description of the LHRS see Ref [11]. The basic components of the LHRS are one non superconducting quadrupole(Q1), a super conducting quadrupole (Q2) a superconducting dipole (D)

| Target Fluid | Fill Pressure (kPa) | Fill Temp (K) | Thickness (mg/cm ²) |
|------------------|------------------------|------------------|------------------------------------|
| ⁴⁰ Ar | 3447 | 291 | 1455 ± 9.2 |
| ³ H-1 | 1400 | 296.3 | 85.1 ± 0.83 |
| ³ H-2 | 1393 | 293.8 | 84.79 ± 0.82 |
| ³ He | 1772 | 294.3 | 53.37 ± 0.57 |
| ² H | 3549 | 296.1 | 142.15 ± 0.80 |
| ¹ H | 3549 | 297.4 | 70.80 ± 0.40 |

Table 1: Load data for the gas cells. Temperatures have an uncertainty of 0.1K. Values for the ⁴⁰Ar cell are from Ref[8]; for all others they are from REF[9].

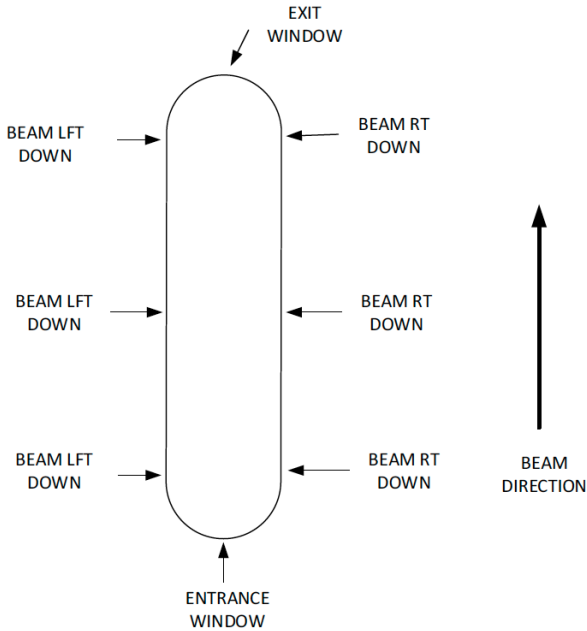


Figure 3: Measurement locations on the cells represented schematically [9].

followed by a super conducting quadrupole (Q3) in a Q-Q-D-Q configuration. The quadrupoles focus scattered charged particles while the dipole directs these particles, within a given momentum range, to the detectors. After passing through the spectrometer magnets, the scattered particles pass through two Vertical Drift Chambers (VDCs), which provide tracking information. Two layers of scintillator hodoscope s0 and s2, sandwich a gas Cherenkov detector filled with CO₂. The hodoscope provides trigger and time of flight (TOF) for the detected particles. The Cherenkov provides identify electrons with 99% efficiency and reject π^- below momentum of 4.8 GeV. The last element in the detector stack is the shower calorimeter. Electrons pass through the calorimeter lead glass blocks induce a cascade of pair production and bremsstrahlung radiation from which their energy can be determined[11].

4. Beam Current Monitor (BCM)

The Beam Current Monitor (BCM) is a system of three independent devices and a current source. This system accounts for most of the systematic uncertainty in the density study. The BCM system consists of a toroidal sensor (Unser), located between two RF cavities, one upstream and one downstream and a data-acquisition system. The current source passes through the Unser and is used to calibrate the Unser prior to each use of the device.

The Unser monitor is composed of two identical toroidal cores driven in opposite ways by an external source. The DC component of the current flowing through the toroid sensor is detected by a magnetic modulator. The beam current in the cores produces a flux imbalance, which generates an output signal proportional to the even harmonics of the frequency of excitation. In the absence of DC current, the sum of the signals is zero [12].

The temperature controlled Unser has sensitivity to beam current of about 4 mV/ μ A and has a noise canceled stability within 0.1% [12]. It also has a large offset drift which prevents the use of the Unser for long term measurements of the beam current. Therefore, the Unser is only used to measure the absolute beam current when calibrating the RF cavities which are then used to continuously monitor the beam current. These calibrations are required periodically though out the course of an experiment. To reduce the effects of the noise from the Unser output, it is first filtered through a voltage to frequency (V/F) converter. This frequency output is then used in the data acquisition system. Figure 5 shows the Unser calibration with a known DC current source, the gain of the Unser is $0.0002497 \pm 9.6 \times 10^{-7} \mu\text{A}/\text{Hz}$. Over time, the Unser gain has shown to be of 4 mV/ μ A.

Two resonant cavities surround the Unser and are tuned to the frequency of the beam 1.497 GHz with a quality coefficient $Q \approx 500$. The cavities are composed of loop antennas located where the magnetic field is maximum. When the beam passes through, the output RF signal is proportional to the current [12]. As consequence, the BCM response is linear with respect to the current. Like the Unser, the signals from the RF cavities are filtered by a V/F converter. Several values of beam current (measured by the calibrated Unser) are used to determine the linear dependence of the BCM as shown in Figure 6. In general, the beam current can be then calculated using

$$I = g_{BCM} \cdot f + O. \quad (1)$$

Where g_{BCM} and O are the fit parameters, which correspond to $0.0003264 \pm 1.4 \times 10^{-6} \mu\text{A}/\text{Hz}$ and $0.1 \pm 0.09 \mu\text{A}$, respectively. Finally, for any given beam induced frequency f , the current I is given by Eq 1. Of unfortunate note, the BCM system becomes much less accurate for beam currents below $\sim 5 \mu\text{A}$.

5. Method Overview

The density of the target is well known when loaded but, experience and simulations have shown that the beam current will

| Location | ^{40}Ar /Empty Cell Thickness (mm) | ^3H Cell Thickness (mm) | ^1H Cell Thickness (mm) | ^2H Cell Thickness (mm) | ^3He Cell Thickness (mm) |
|----------------|------------------------------------------------|-------------------------------------|-------------------------------------|-------------------------------------|--------------------------------------|
| Entrance | 0.254 ± 0.0051 | 0.253 ± 0.004 | 0.311 ± 0.001 | 0.215 ± 0.004 | 0.203 ± 0.007 |
| Exit | 0.279 ± 0.0051 | 0.343 ± 0.047 | 0.330 ± 0.063 | 0.294 ± 0.056 | 0.328 ± 0.041 |
| Exit left | 0.406 ± 0.0051 | 0.379 ± 0.007 | 0.240 ± 0.019 | 0.422 ± 0.003 | 0.438 ± 0.010 |
| Exit right | 0.421 ± 0.0051 | 0.406 ± 0.004 | 0.519 ± 0.009 | 0.361 ± 0.013 | 0.385 ± 0.016 |
| Mid left | 0.457 ± 0.0051 | 0.435 ± 0.001 | 0.374 ± 0.004 | 0.447 ± 0.009 | 0.487 ± 0.060 |
| Mid right | 0.432 ± 0.0051 | 0.447 ± 0.004 | 0.503 ± 0.005 | 0.371 ± 0.012 | 0.478 ± 0.007 |
| Entrance left | 0.508 ± 0.0051 | 0.473 ± 0.003 | 0.456 ± 0.010 | 0.442 ± 0.005 | 0.504 ± 0.003 |
| Entrance right | 0.424 ± 0.0051 | 0.425 ± 0.003 | 0.457 ± 0.006 | 0.332 ± 0.011 | 0.477 ± 0.011 |

Table 2: Cell wall thickness measurements for all gas targets. Values for the ^{40}Ar cell are from Ref[8]; for all others they are from REF[9].

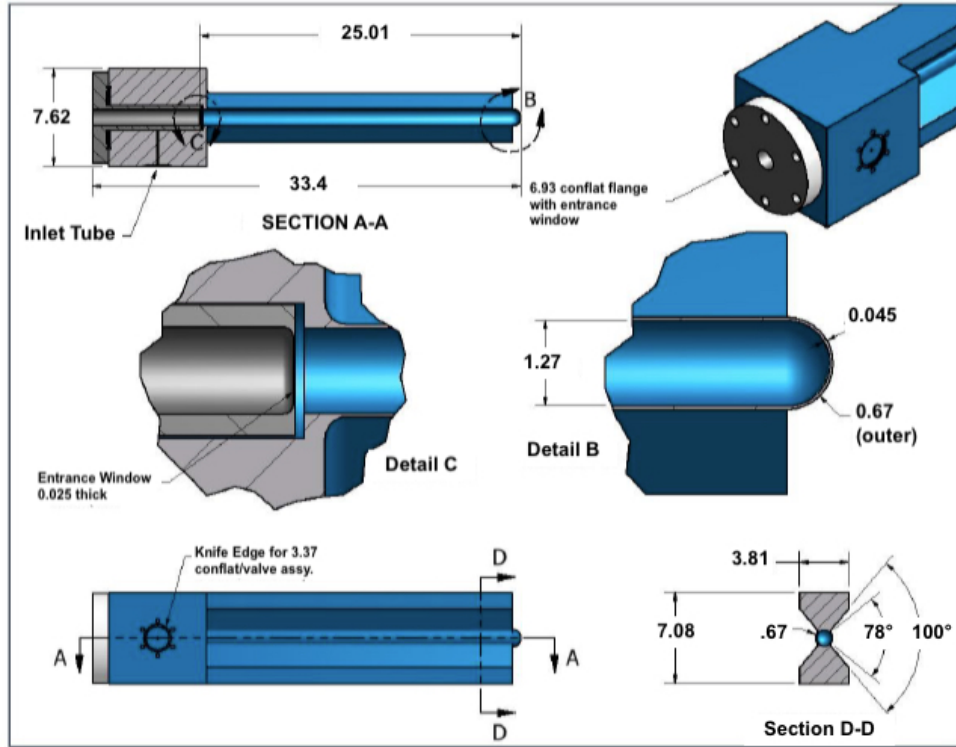


Figure 4: Engineering design of an individual tritium gas target cell [10], units are in *cm*.

decrease the density of the target fluid in the beam path (local density). The magnitude of this effect depends on the beam current and target fluid species and must be quantified to accurately determine cross sections and ratios or other comparisons of data collected with the multiple gas cells [10]. It was shown that the equilibrium density an insignificant amount of time after the electron beam first impinges on the cell and the density was constant with stable beam current. The purpose of these measurements and analysis is to develop a beam current dependent target density function for each gas species used.

In order to extract the density, the raw yield is measured for several beam currents. The normalized yield is determined by applications of corrections to the raw yield. These corrections include: total charge, particle identification, acceptance cuts, detector efficiencies, and live times. The normalized yield Y is

then given by

$$Y_{norm} = \frac{PS \cdot N}{Q \cdot \epsilon \cdot LT} \quad (2)$$

Where N is the number of good electrons, PS is the prescale factor, Q is the total charge, and ϵ is the combined efficiencies of detectors, triggers and events selection cuts and LT is the live-time. Each one of these parameters is explained in detail in the following sections.

5.1. Events Selection

To improve counting efficiency and minimize dead time, a compound trigger was used. This trigger required both scintillator planes and the Cherenkov detector to have a signal above threshold, in order to exclude π^- events. In order to extract

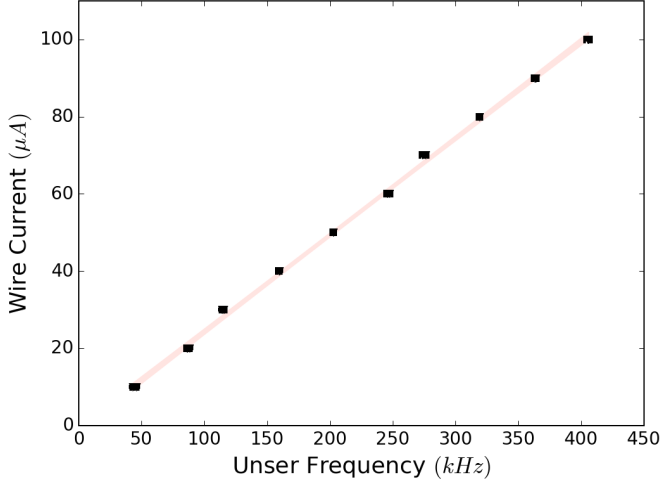


Figure 5: Wire Unser calibration. The band represents the 95% confidence level of the linear fit.

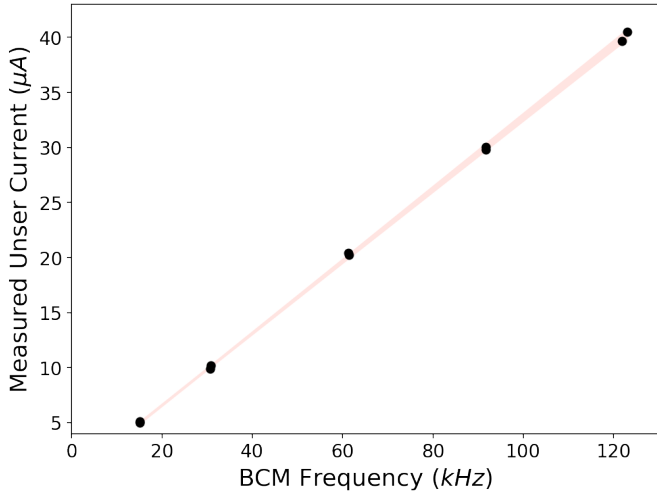


Figure 6: BCM calibration. The band represents the 95% confidence level of the linear fit.

a good electron sample, several cuts were applied to the data. These cuts can be summarized in two groups: Acceptance Cuts, which assure that the events are selected within an acceptable spectrometer phase space, and Tracking/Particle IDentification (PID) Cuts, which focus on the selection of electrons scattered from the target fluid.

- i. Momentum and angular acceptance cuts. Specifically, the ranges used to determine Y_{norm} are $|\delta p/p| < 4.5\%$, $|\theta - \theta_0| < 30\text{ mrad}$ and $|\phi| < 25\text{ mrad}$.
- ii. Target length cut. This cut excluded events reconstructed back to the target windows and reduced background by limiting the effective target length $|y_{tar}| < 8\text{ cm}$.
- iii. Only events with a single track in the VDC were kept.
- iv. A particle ID cut was applied to the Cherenkov ADC sum
- v. A particle ID cut was applied to the shower calorimeter

It was shown through the course of this study that as long as the sample of electrons is chosen consistently, the results will remain invariant within 1 % run to run.

5.2. Efficiencies Estimations

A number of efficiencies were applied to the data to produce Y_{norm} . Only electrons with one track in the VDC were selected. Therefore, the ratio between the total number of particles with one track with respect to the total number of particles (including multi track and non track particles) corresponds to the VDC efficiency. The trigger efficiency was calculated using another trigger type, where only both scintillators were required to record the events. In this sense, the difference between the main trigger and the efficiency trigger is the Cherenkov detector. The ratio between the events recorded with the main and the efficiency trigger corresponds to the trigger efficiency. The Cherenkov efficiency was calculated by selecting a clean sample of electrons detected in the Calorimeter and counting the number of events that also were detected in the Cherenkov detector. The Calorimeter efficiency was measured by selecting a clean sample of electrons in the Cherenkov detector and counting the number of electrons that also fired the Calorimeter.

5.3. Live-Time Calculation

The live-time is related with the limitation of the speed of data acquisition system (DAQ) to record events. It is dependent on the electronics, computers and trigger rate and is calculated using the ratio between the number of events recorded over the total number of events seen by the trigger.

5.4. Total Charge

The beam is not completely stable throughout the run; it may trip off or fluctuate over time. Therefore, only runs where the average current is within a window of $\pm 2\text{ }\mu\text{A}$ of the requested current are used. The charge is calculated using the BCM calibration (See Section 4) result integrated over time.

6. Solid Target Check

The aim of the analysis is to measure the density change when the beam is on the gas targets using the Yield analysis. In order to test the method, the same analysis is applied to a solid target. For the ^{40}Ar experiment, a carbon foil was used, and for the Tritium experiments using an aluminum target. Unlike the fluid targets, the solid target density is not measurably effected by the beam current.

Figure 7 shows Y_{norm} for the solid aluminum target which was calculated using Equation 2 for different beam currents. It was normalized with respect to the lowest current Yield value. The plot shows that the Y_{norm} did not change to within about 0.5% which is well within the uncertainty of the measurement.

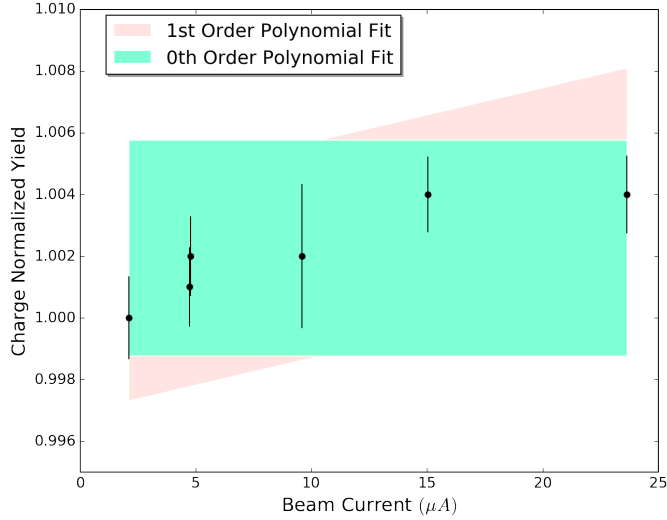


Figure 7: Normalized Yield analysis for the aluminum solid target used during the tritium group experiments

7. Background Contamination

The aluminum windows of the target cell contribute as background to the measured raw yield for each of the gas targets. To measure this background (henceforth referred to as contamination) in the case of the ^{40}Ar experiment, a dummy target with aluminum foils of identical radiation length to that of the cell was used. In the case of the tritium experiments, an empty cell (or dummy cell) was used. The normalized yields from these targets were then subtracted from the applicable Y_{norm} . To check the current dependence of this subtraction, a comparison between the background at low and high current was measured for the dummy/empty targets. The charge yield given by Eq 1 was binned in y_{tar} bites along the target length, and the ratio of the events at high current to low current was determined. The ratio was found to be 1.006, which indicates that the background subtraction is independent of current, as expected.

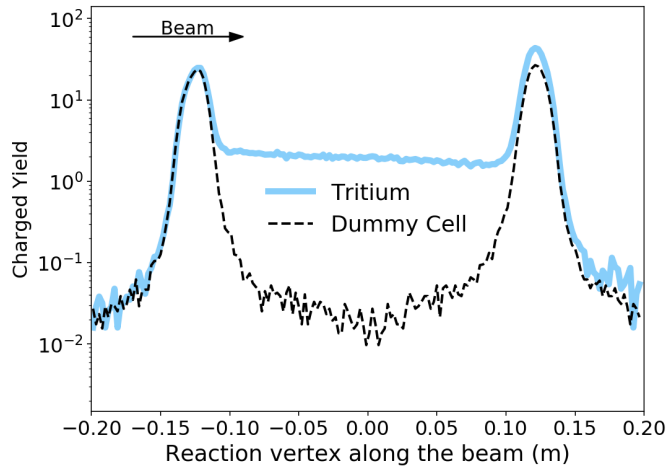


Figure 8: Background contamination spectrum of the dummy target compared with that of tritium at 2.5 μA . Both spectra are normalized.

Figure 8 shows the spectra of the charge normalized yield for the empty (dummy) cell and the tritium gas, for a beam current of 2.5 μA . To optimize the signal to background ratio, events contributing to the Y_{norm} were selected from a symmetric region of $\pm 8\text{ cm}$ about the center of the target. Therefore, the contamination fraction is the ratio of Y_{norm} for the empty cell to Y_{norm} for the gas cell of interest. Table 3 summarizes the percentage of background contamination found in the gas targets for each beam current used in the study. Note that the currents are nominal; the measured current for each run is slightly different, due to the normal operation of the accelerator.

| Current (μA) | ^3H (%) | ^3He (%) | ^2H (%) | ^1H (%) | Current (μA) | Argon (%) |
|------------------------------|---------------------|----------------------|---------------------|---------------------|------------------------------|--------------|
| 2.5 | 1.7 | 1.6 | 0.7 | 1.1 | 2.5 | 0.3 |
| 5 | 1.7 | 1.6 | 0.7 | 1.2 | 4.5 | 0.3 |
| 10 | 1.7 | 1.7 | 0.8 | 1.2 | 8 | 0.3 |
| 15 | 1.8 | 1.8 | 0.8 | 1.3 | 12 | 0.3 |
| 22.5 | 1.8 | 1.8 | 0.8 | 1.3 | 15 | 0.3 |
| | | | | | 18 | 0.3 |

Table 3: Aluminum window contamination in a $\pm 8\text{ cm}$ range with respect to the center of the target at each nominal current. Note that these currents were not the same for both experiments.

8. Gas Target Results

The density correction was determined for each gas species by modeling Y_{norm} as a function of beam current I_{beam} . The function is then normalized to 1 for $I_{beam} = 0$. The density each gas cell for zero beam current is the same as that of the load density. Figures 9, 10a, 10b, 10c and 10d, show the density correction for the different gas targets. It is easily seen that the density decreases with the current and that the behavior of the density correction factor f is modeled well by a quadratic function

$$f = a \cdot I_{beam}^2 + b \cdot I_{beam} + c. \quad (3)$$

Where a , b and c are the fit parameters. Table 4 shows the fit parameters for each target, which can be used to calculate the density change of the gas targets for any current in the range 0 – 22.5 μA . The error bar in the plots represents the statistical uncertainty, and the fit was calculated with respect to those values.

8.1. Density Factor Ratios

The tritium family of experiments measure the $^3\text{H}/^3\text{He}$ cross section ratio, since they are mirror nuclei. Some of the experiments also used the ratio of the $^3\text{H}/^2\text{H}$ and/or $^3\text{He}/^2\text{H}$. Therefore, the ratio of the density factors is used to make the corrections in the cross sections for the analysis. Figure 11 shows the ratio between the factor of density change for those nuclei.

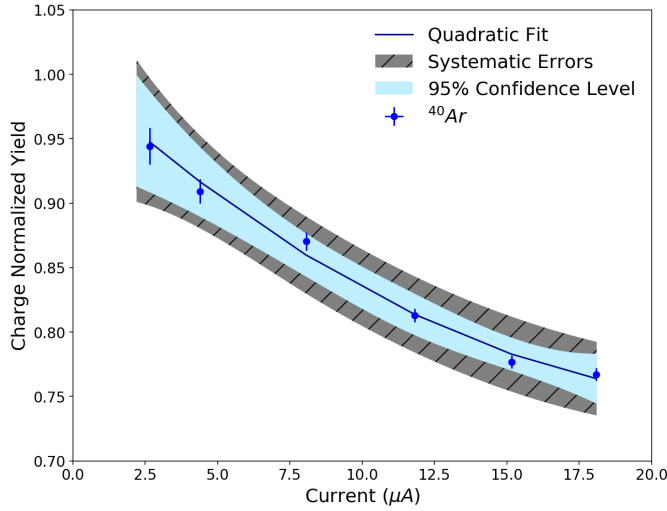


Figure 9: ^{40}Ar density analysis.

| ^3H Fit Parameters | | ^3H Correlation Factors | |
|---------------------------------|-------------------------|--------------------------------------|--------|
| a | $1.06e-04 \pm 3.6e-05$ | C(a, b) | -0.974 |
| b | $-0.0068 \pm 8.9e-04$ | C(b, c) | -0.888 |
| c | $1. \pm 0.003$ | C(a, c) | 0.801 |
| ^3He Fit Parameters | | ^3He Correlation Factors | |
| a | $1.036e-04 \pm 2.5e-05$ | C(a, b) | -0.973 |
| b | $-0.0051 \pm 6.4e-04$ | C(b, c) | -0.879 |
| c | 1 ± 0.003 | C(a, c) | 0.779 |
| ^2H Fit Parameters | | ^2H Correlation Factors | |
| a | $1.16e-04 \pm 2.9e-05$ | C(a, b) | -0.973 |
| b | $-0.0067 \pm 7.1e-04$ | C(b, c) | -0.895 |
| c | $1. \pm 0.003$ | C(a, c) | 0.805 |
| ^1H Fit Parameters | | ^1H Correlation Factors | |
| a | $1.70e-04 \pm 4.7e-05$ | C(a, b) | -0.978 |
| b | -0.009 ± 0.0012 | C(b, c) | -0.881 |
| c | $1. \pm 0.006$ | C(a, c) | 0.788 |
| ^{40}Ar Fit Parameters | | ^{40}Ar Correlation Factors | |
| a | $4.33e-04 \pm 1.5e-04$ | C(a, b) | -0.981 |
| b | -0.021 ± 0.003 | C(b, c) | -0.942 |
| c | $1. \pm 0.02$ | C(a, c) | 0.867 |

Table 4: Fit parameters obtained for the percentage of density change calculation with respect to the beam current.

8.2. Systematic Uncertainties

There are several corrections to take into account in this analysis, and since the current is different for every point, the uncertainties are evaluated at every point. The systematic uncertainties are shown in Figures 9, 10a, 10b, 10c and 10d, they include the uncertainty in the charge, live-time and detectors calculations.

The BCM monitors cover a range of 0 to 100 μA . The Unser has a sensitivity of $4\text{mV}/\mu\text{A}$ [12], but the offset drifts over time. The large background noise implies that the precision of the measurements at low current have a slightly higher uncertainty. In other words, the charge uncertainty is current dependent. Therefore, the uncertainty of the current and charge is estimated

using the BCM calibration showed in Figure 6, using the error covariance matrix, and it represents the highest source of systematic uncertainty in this measurement.

The background contamination coming from the entrance and exit windows also contribute as a source of systematics uncertainty since the calculation implied some assumptions. Specifically, as shown in Figure 8, the exit window thickness is slightly different for every target. Therefore, in order to calculate the background uncertainty in the measurement, the percentage of background was calculated in ranges of 3 cm starting from 8 cm out to 20 cm from the center of the target. The same normalization procedure was followed for each of the different cuts in the reaction vertex region to calculate the percentage of density changed. Finally, the uncertainty in the background contamination is given by the standard deviation of the percentages obtained with the different cuts. The standard deviation was never more than 1 % in each current.

Furthermore, 1% systematic errors were estimated for the live-time, VDC One-Track efficiency, trigger efficiency, detection and cut efficiencies of Gas Cerenkov and Pion Rejetors.


8.3. Conclusions

Hall A at Jefferson Lab successfully ran the tritium set of experiments with an outstanding target system. The maximum density change for each target is $9.7 \pm 0.5\%$, $5.6 \pm 0.5\%$, $6.3 \pm 0.5\%$, $11.6 \pm 0.5\%$ and $26.5 \pm 1\%$ for ^3H , ^3He , ^2H , ^1H and ^3H , respectively at 22.5 μA .


9. Acknowledgments

We would like to thank to the target group for its outstanding work, specially to the Design Authority and Project Manager Dave Meekins. Furthermore, none of this work will be possible without the wonderful group of graduate students and postdocs who were the building blocks of the experiments. Besides, all the hall A staff and experiment spoke people were a big help in every step of the way. And, certainly special thanks to Douglas Higinbotham for all his invaluable support .


- [1] G. Petratos, et al. JLab MARATHON Collaboration, JLab Experiment E12-10-103.
- [2] P. Solvignon, et al., Jlab experiment e12-06-112.
- [3] O. Hen, L. B. Weinstein, S. Gilad, W. B. nd et al., JLab Experiment E12-14-011.
- [4] L. S. Meyers, D. W. Higinbotham, J. Arrington, et al., JLab Experiment E12-14-009.
- [5] L. Tang, F. Garibaldi, P. E. C. Markowitz, S. N. Nakamura, J. Reinhold, G. M. Urciuoli, JLab Experiment E12-14-009.
- [6] O. Benhar, G. M. U. et al., JLab Experiment E12-14-012.
- [7] D. Meekins, Hall a tritium target tgt-rpt-17-003, Jefferson Lab Engineering Report.
- [8] D. Meekins, Hall a target configuration, Jefferson Lab.
- [9] D. Meekins, Hall a tritium target configuration for december 2017, Jefferson Lab TGT-RPT-17-007.
- [10] R. Holt, W. Korsch, D. Meekins, T. O. Connor, G. Petratos, R. Ransome, P. Solvignon, B. Wojtsekhowski, A tritium gas target for jefferson lab, Jefferson Lab.
- [11] J. Alcorn, et al., Basic Instrumentation for Hall A at Jefferson Lab, Nucl. Instrum. Meth. A522 (2004) 294–346. doi:10.1016/j.nima.2003.11.415.
- [12] J. Denard, A. Saha, G. Laveissiere, High accuracy beam current monitor system for cebaf's experimental hall a, in: PACS2001. Proceedings of the 2001 Particle Accelerator Conference (Cat. No.01CH37268), Vol. 3, 2001, pp. 2326–2328 vol.3. doi:10.1109/PAC.2001.987367.

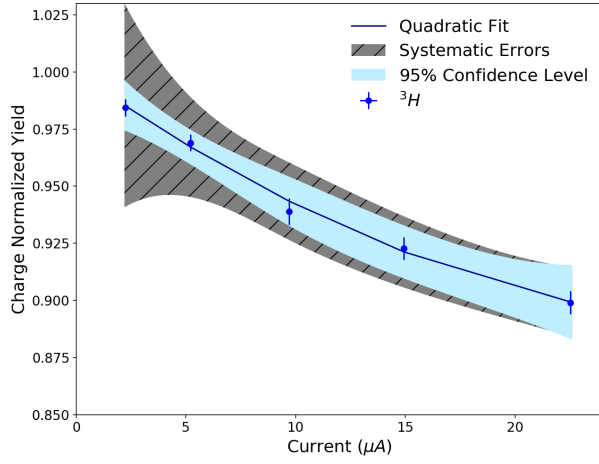


(a) 3H Density Analysis.

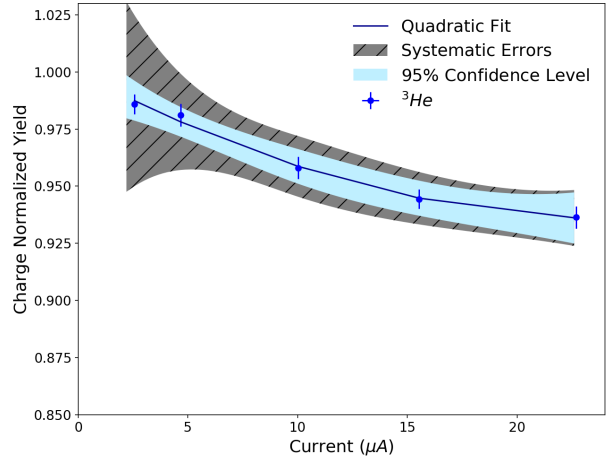

(b) 3He Density Analysis.

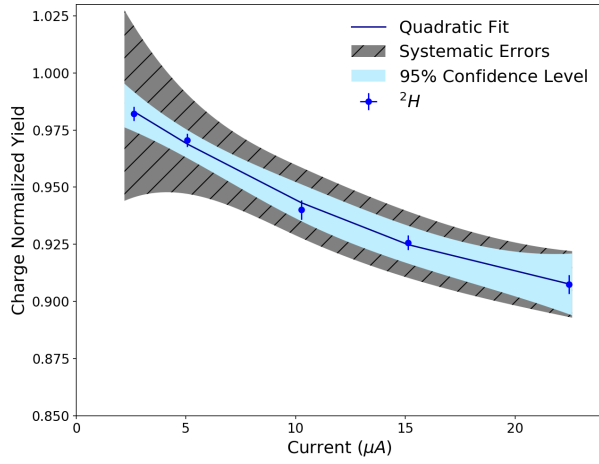

(c) 2H Density Analysis.

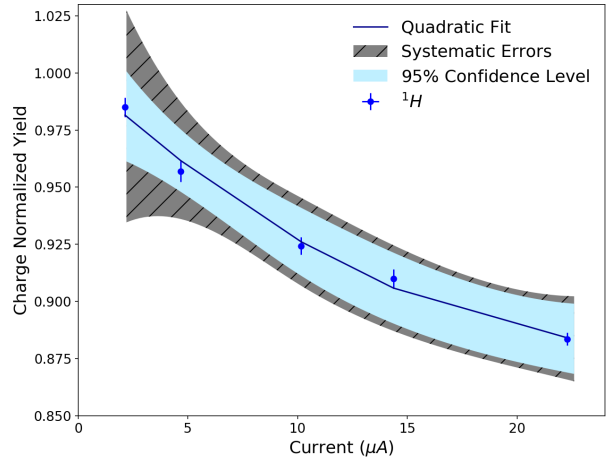

(d) 1H Density Analysis.

Figure 10: Density analysis of 3H , 3He , 2H and 1H .

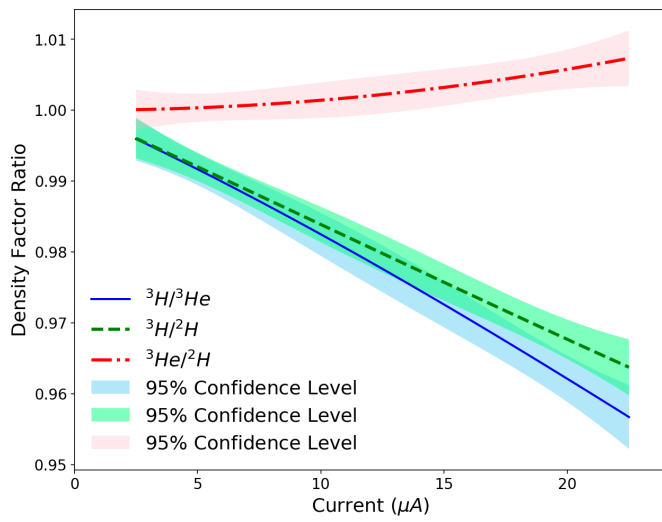


Figure 11: Density Factor Ratios.