

He

Vlv

Trnd

PSU

ILX

Temp

Coil

Q1 Magnet N2 Display


Mon Nov 16 1998
11:30:27

Command Line

psu:standby

Overall State NORMAL
N2 system state N2COLD
He System state HeCOLD
PSU State Enabled

Auto
57.0 % [3]

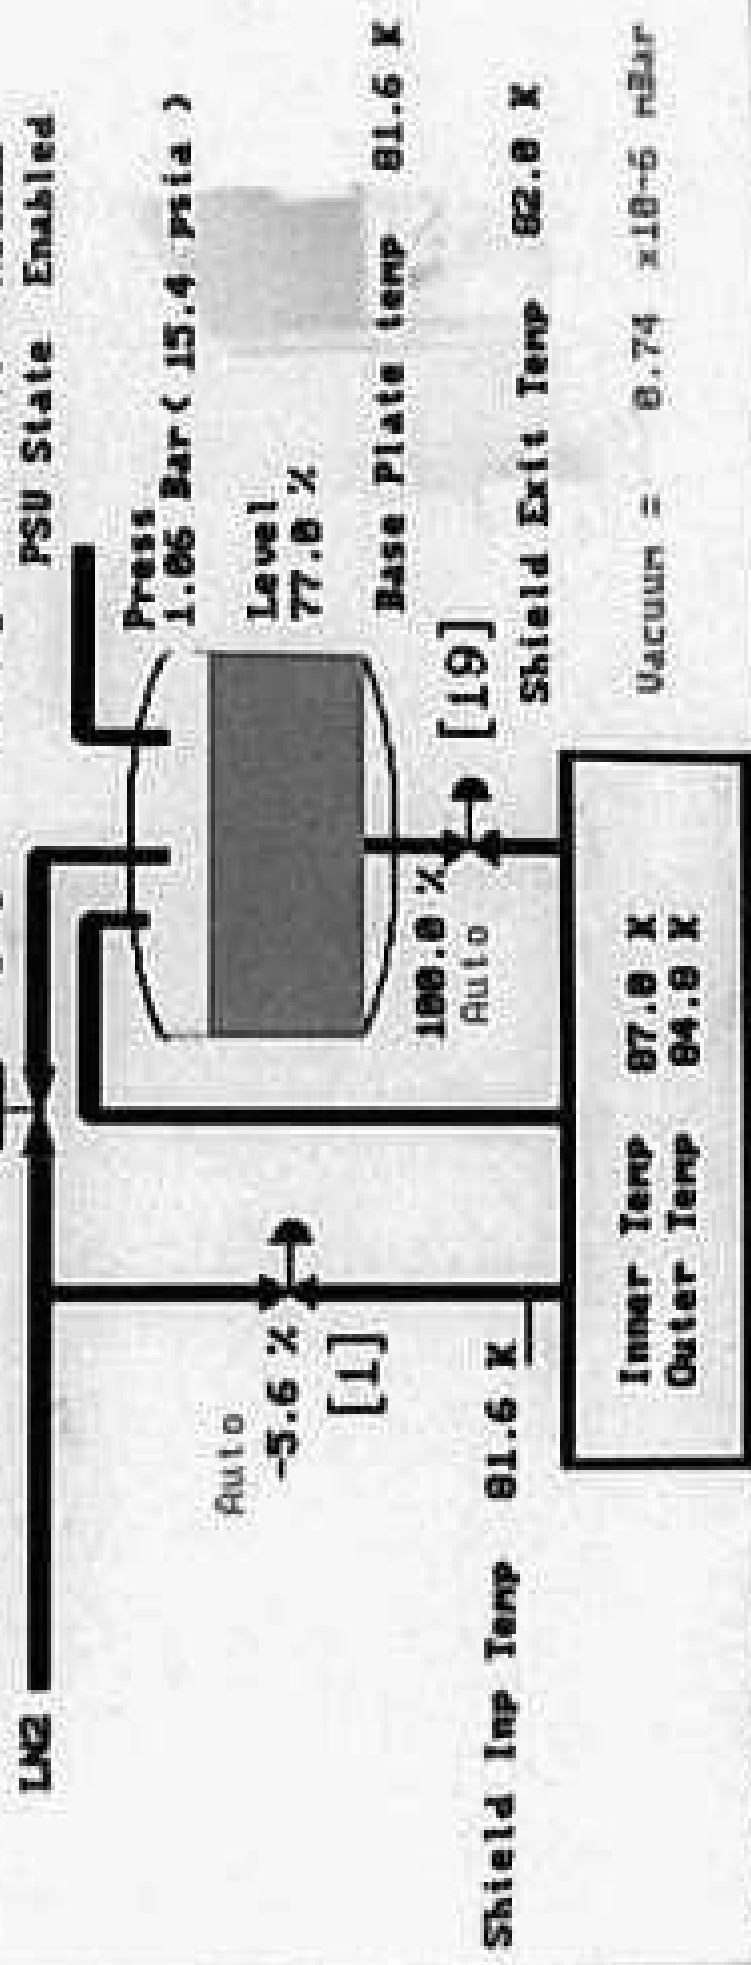

Shield Inp Temp 81.6 K

Inner Temp 87.0 K
Outer Temp 84.0 K

Vacuum = 0.74 x 10^-6 mBar

E6: ALARM POINT

E7: ALARM ACK