


Effect of frozen domain-blind baseline preprocessing by instrument

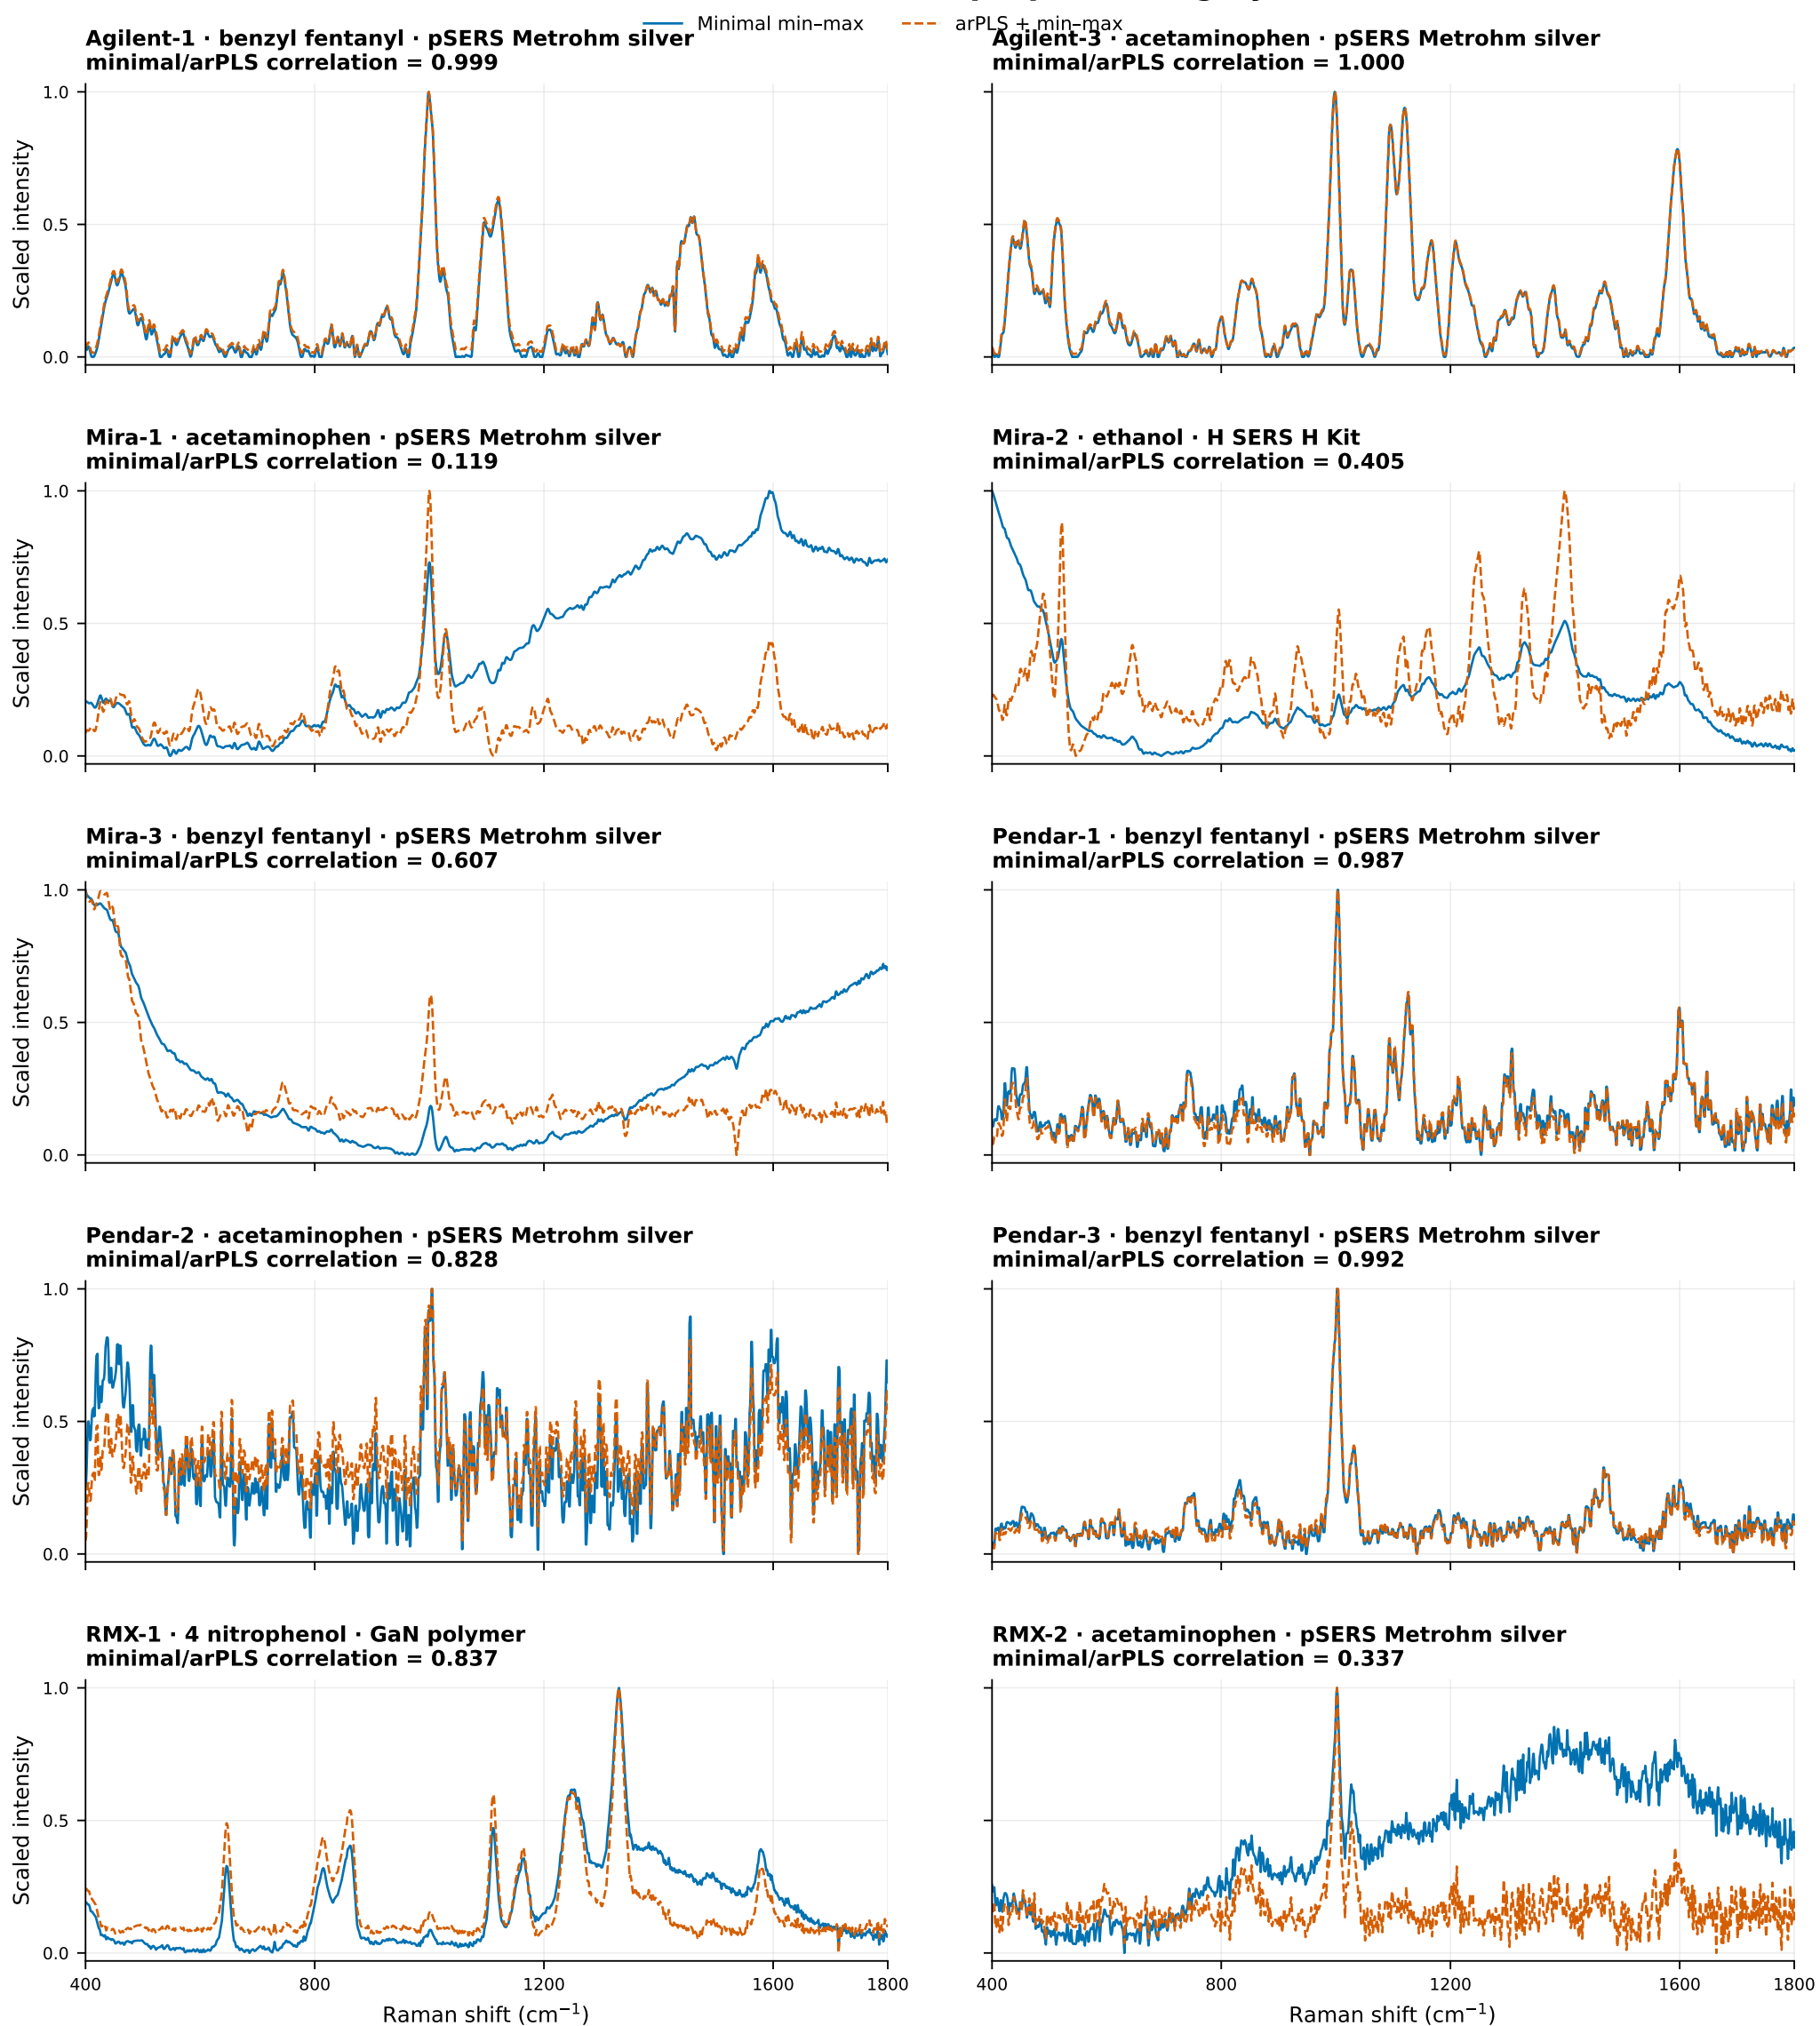

One deterministic quality-pass medoid per instrument. Targets and sensors differ because the field design is not fully crossed; compare transforms within an instrument, not cross-row chemistry.