

Sample Report



Sample Metadata

Sample Name	Scan 04178
Hazard Level	Clear
Sample Type	USP/Pharmaceutical
Last Modified	2024-03-07 10:41:58-05:00
Created	2024-03-07 10:41:58-05:00


Instrument

Serial Number	192600200502138
Firmware Package	8.1.3.55
Last Calibration	2024-03-07 09:58:26-05:00
Last System Suitability Test	Fail, 2024-03-07 09:58:38-05:00


Acquisition Parameters

Operating Procedure Name	Default Procedure
Operating Procedure Version	1
Integration Time	5.45 s
Auto Integration	On
Averages	3
Laser Power	5
Smart Tip Type	Intelligent UA, Bag (Position 2)
Smart Tip Serial Number	6075060600401227

Spectral Data

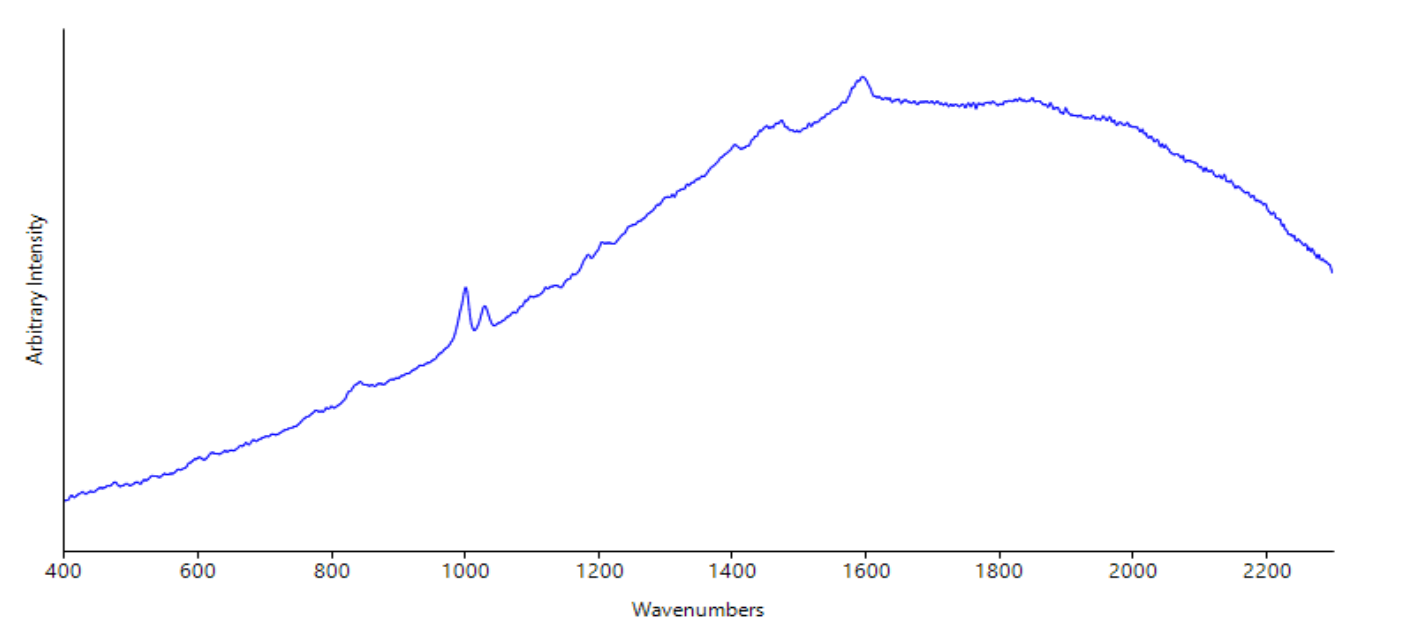

Mixture Identification Results

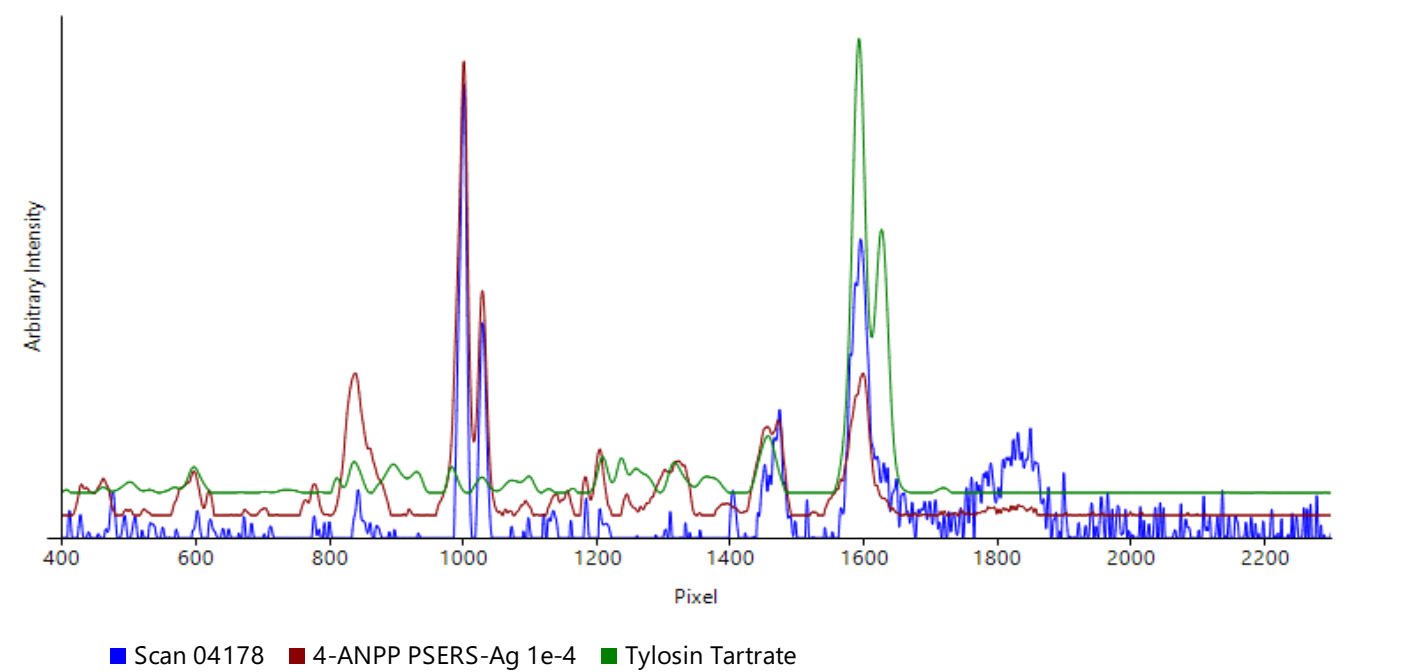

Hazard Level	Match	Sample Type	Source Library	Spectral Weight %
Unknown	4-ANPP PSERS-Ag 1e-4		NATO SERS, Version: 1	53%
Clear	Tylosin Tartrate	USP/Pharmaceutical	Illicit v41, Version: 41	29%