

Sample Report



Sample Metadata

Sample Name	Scan 04182
Hazard Level	Unknown
Last Modified	2024-03-07 10:54:01-05:00
Created	2024-03-07 10:54:01-05:00


Instrument

Serial Number	192600200502138
Firmware Package	8.1.3.55
Last Calibration	2024-03-07 09:58:26-05:00
Last System Suitability Test	Fail, 2024-03-07 09:58:38-05:00


Acquisition Parameters

Operating Procedure Name	Default Procedure
Operating Procedure Version	1
Integration Time	2.87 s
Auto Integration	On
Averages	3
Laser Power	5
Smart Tip Type	Intelligent UA, Surface (Position 1)
Smart Tip Serial Number	6075060600401227

Spectral Data

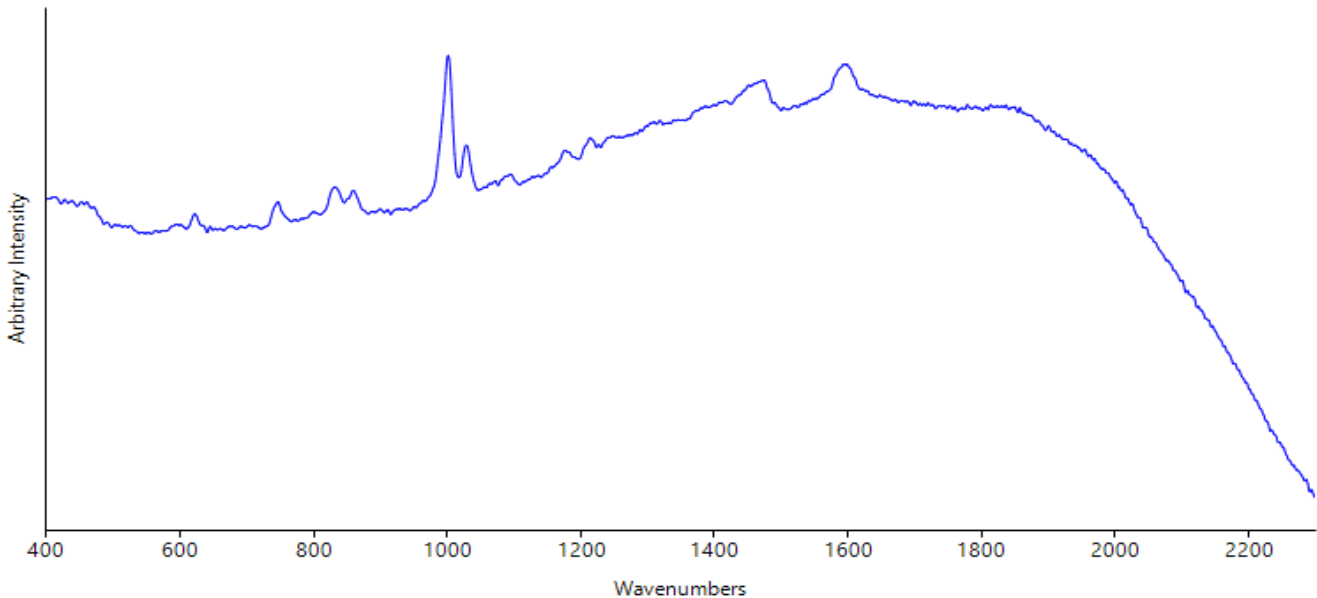


Identification Results

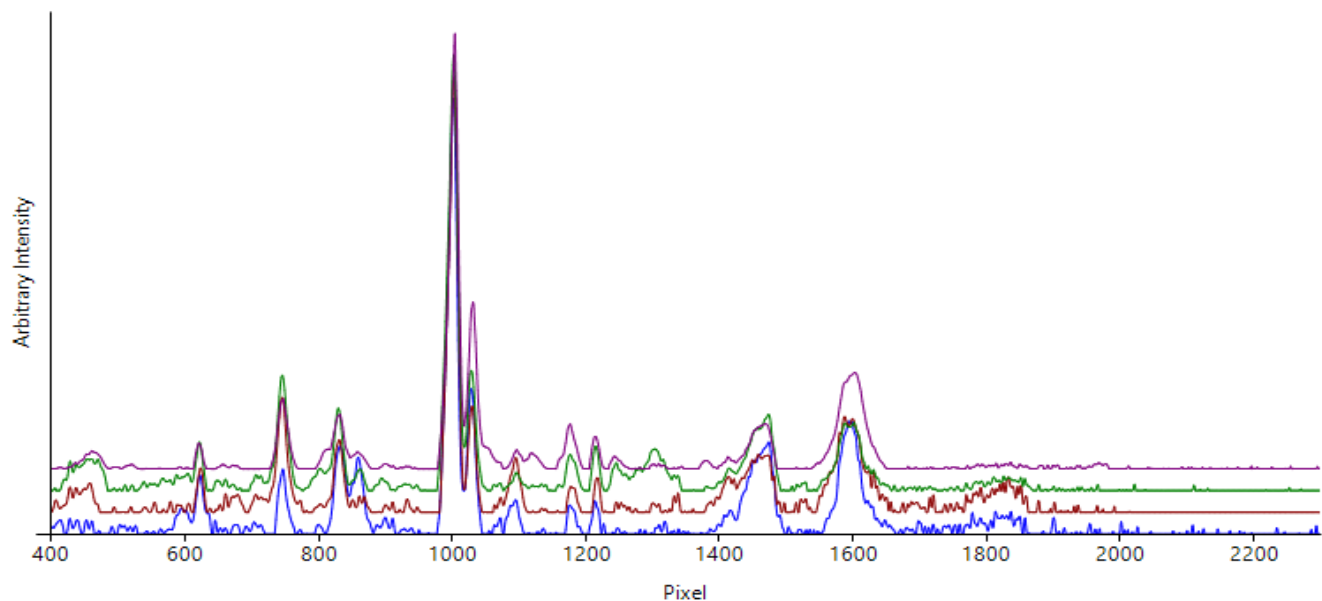

■ Scan 04182 ■ Benzyl Fentanyl PSERS-Ag 1e-4 ■ Benzyl Fentanyl PSERS-Ag 1e-3 ■ BenzylFentanyl

Hazard Level	Match	Sample Type	Match Score	Result Library
Unknown	Benzyl Fentanyl PSERS-Ag 1e-4		0.91	NATO SERS, Version: 1
Unknown	Benzyl Fentanyl PSERS-Ag 1e-3		0.90	NATO SERS, Version: 1
Alarm	BenzylFentanyl		0.89	Fentanyl Analogues_SERS, Version: 7

Mixture Identification Results

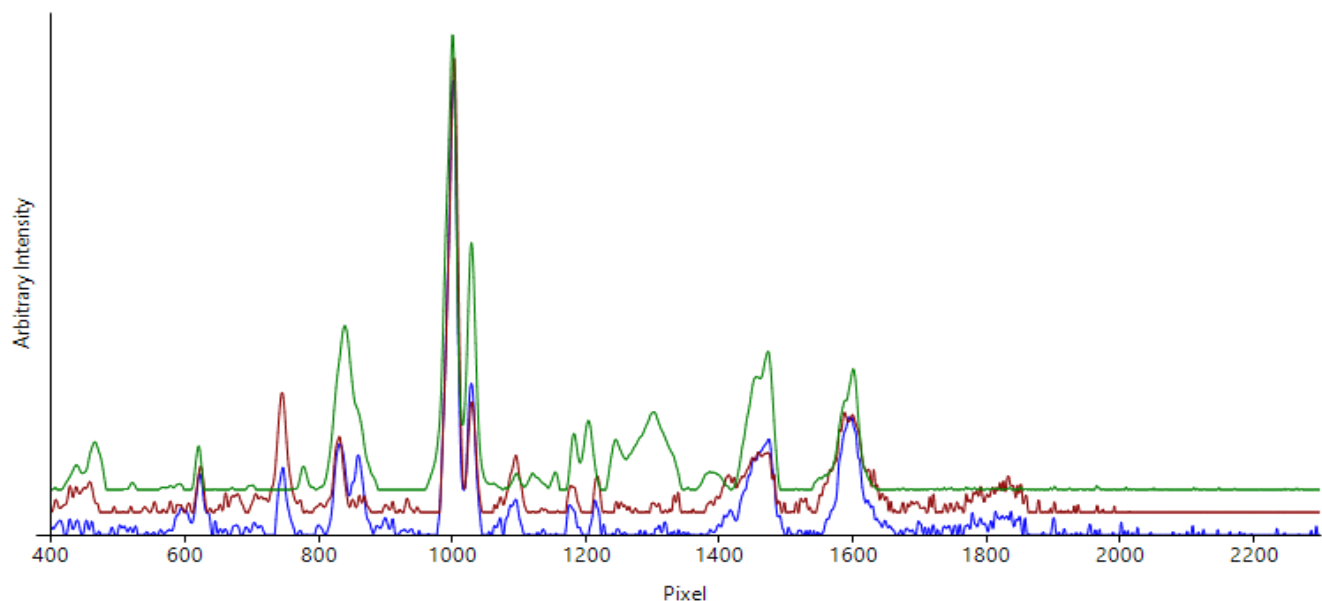

■ Scan 04182 ■ Benzyl Fentanyl PSERS-Ag 1e-4 ■ 4-ANPP PSERS-Ag 1e-3

Hazard Level	Match	Sample Type	Source Library	Spectral Weight %
Unknown	Benzyl Fentanyl PSERS-Ag 1e-4		NATO SERS, Version: 1	64%
Unknown	4-ANPP PSERS-Ag 1e-3		NATO SERS, Version: 1	30%