

Sample Report



Sample Metadata

Sample Name	Scan 04188
Hazard Level	Clear
Sample Type	Chemical, USP/Pharmaceutical
Last Modified	2024-03-07 11:01:54-05:00
Created	2024-03-07 11:01:54-05:00


Instrument

Serial Number	192600200502138
Firmware Package	8.1.3.55
Last Calibration	2024-03-07 09:58:26-05:00
Last System Suitability Test	Fail, 2024-03-07 09:58:38-05:00


Acquisition Parameters

Operating Procedure Name	Default Procedure
Operating Procedure Version	1
Integration Time	0.59 s
Auto Integration	On
Averages	1
Laser Power	5
Smart Tip Type	Intelligent UA, Surface (Position 1)
Smart Tip Serial Number	6075060600401227

Spectral Data

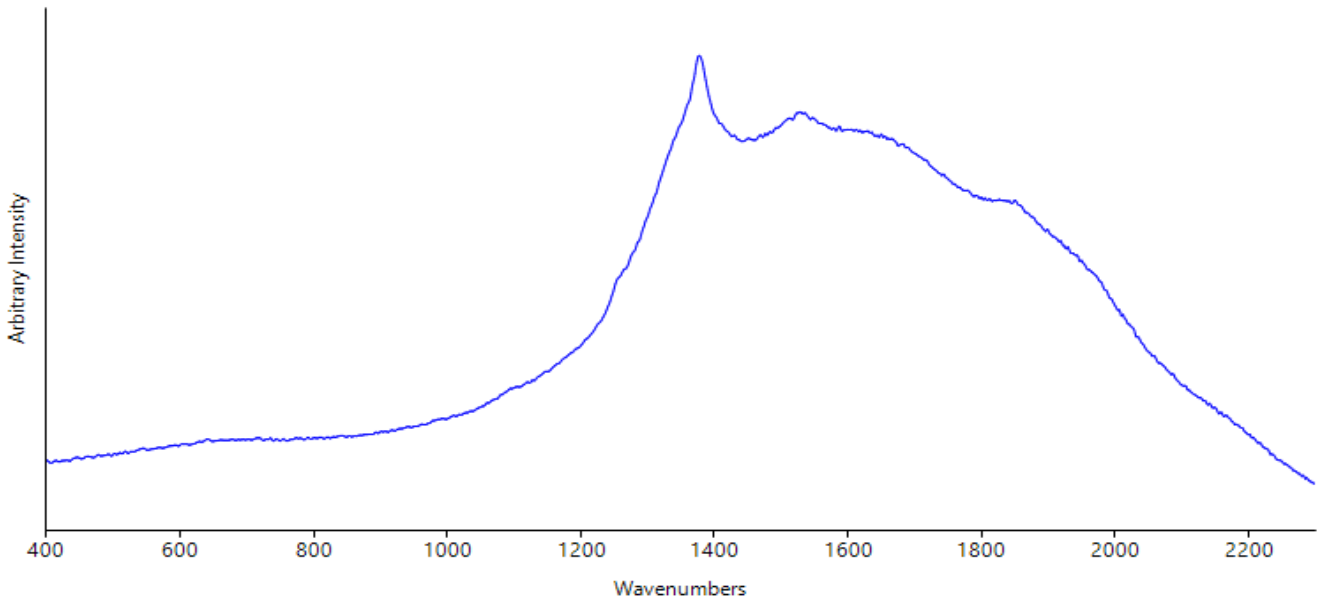


Identification Results

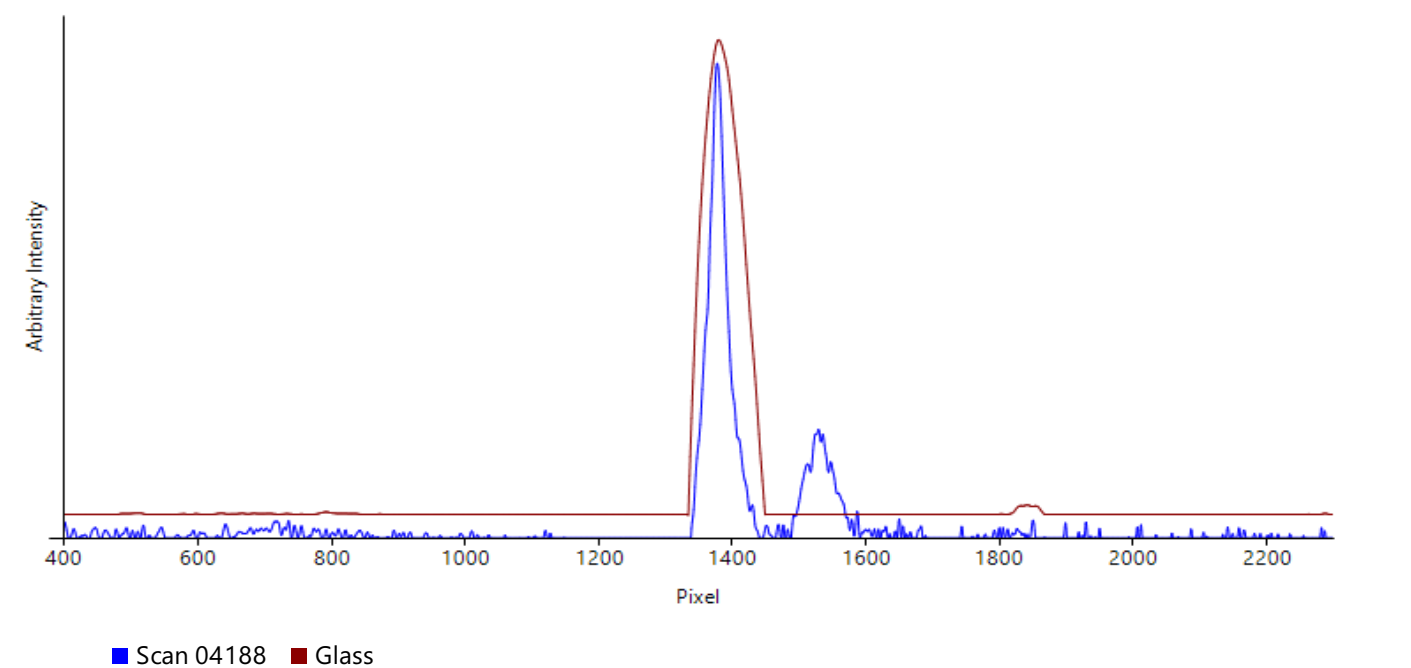

Hazard Level	Match	Sample Type	Match Score	Result Library
Clear	Glass	Chemical	0.76	Illicit v41, Version: 41

Mixture Identification Results

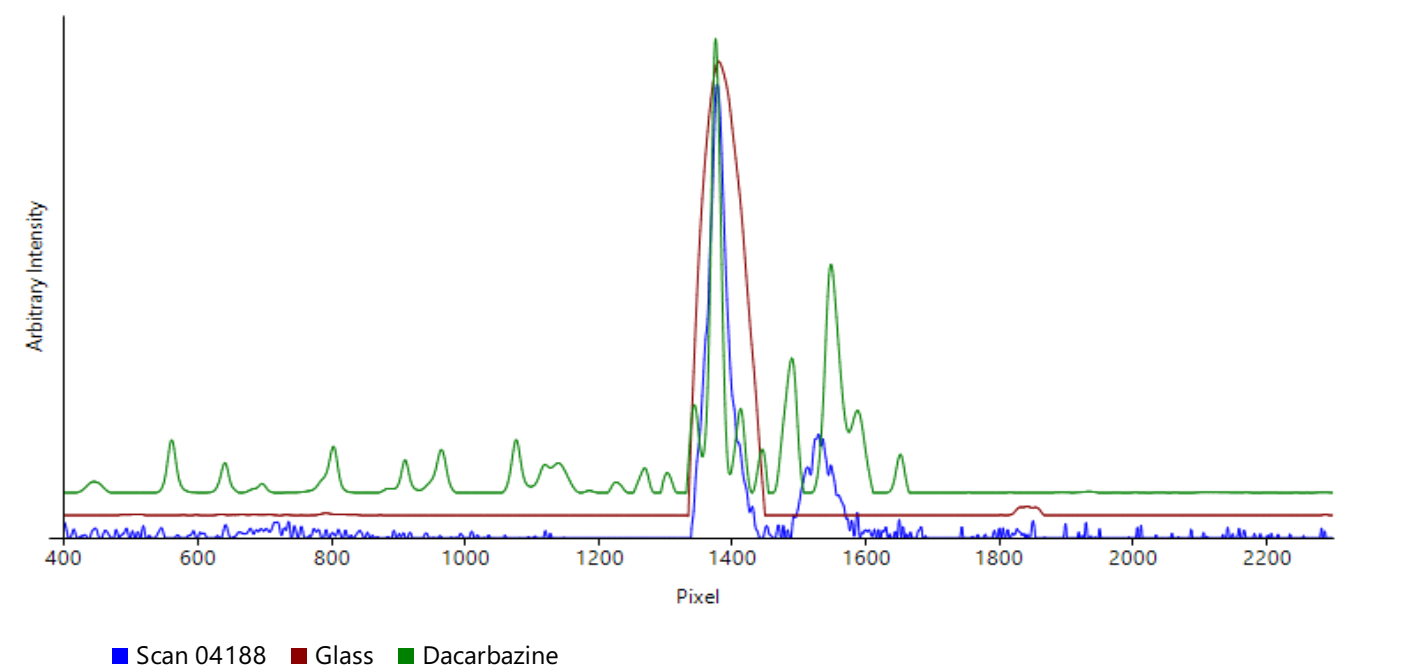

Hazard Level	Match	Sample Type	Source Library	Spectral Weight %
Clear	Glass	Chemical	Illicit v41, Version: 41	43%
Clear	Dacarbazine	USP/Pharmaceutical	Illicit v41, Version: 41	38%