

Sample Report



Sample Metadata

Sample Name	Scan 04194
Hazard Level	Clear
Sample Type	USP/Pharmaceutical, Chemical
Last Modified	2024-03-07 11:05:46-05:00
Created	2024-03-07 11:05:46-05:00


Instrument

Serial Number	192600200502138
Firmware Package	8.1.3.55
Last Calibration	2024-03-07 09:58:26-05:00
Last System Suitability Test	Fail, 2024-03-07 09:58:38-05:00


Acquisition Parameters

Operating Procedure Name	Default Procedure
Operating Procedure Version	1
Integration Time	0.28 s
Auto Integration	On
Averages	1
Laser Power	5
Smart Tip Type	Intelligent UA, Surface (Position 1)
Smart Tip Serial Number	6075060600401227

Spectral Data

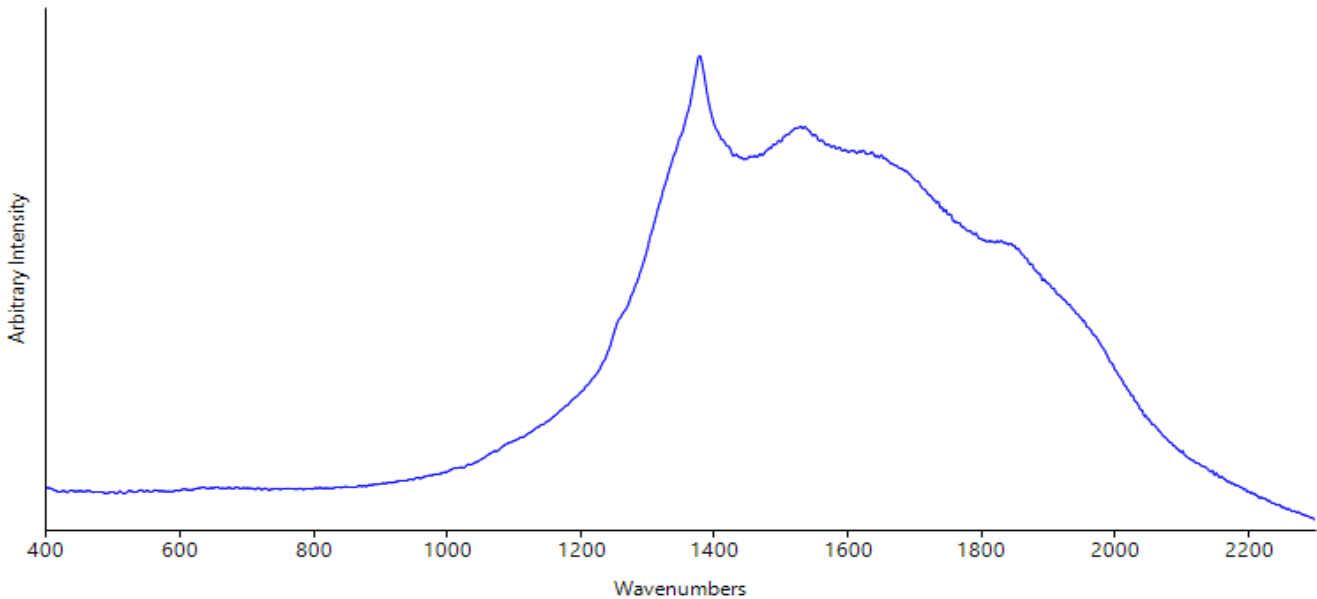


Identification Results

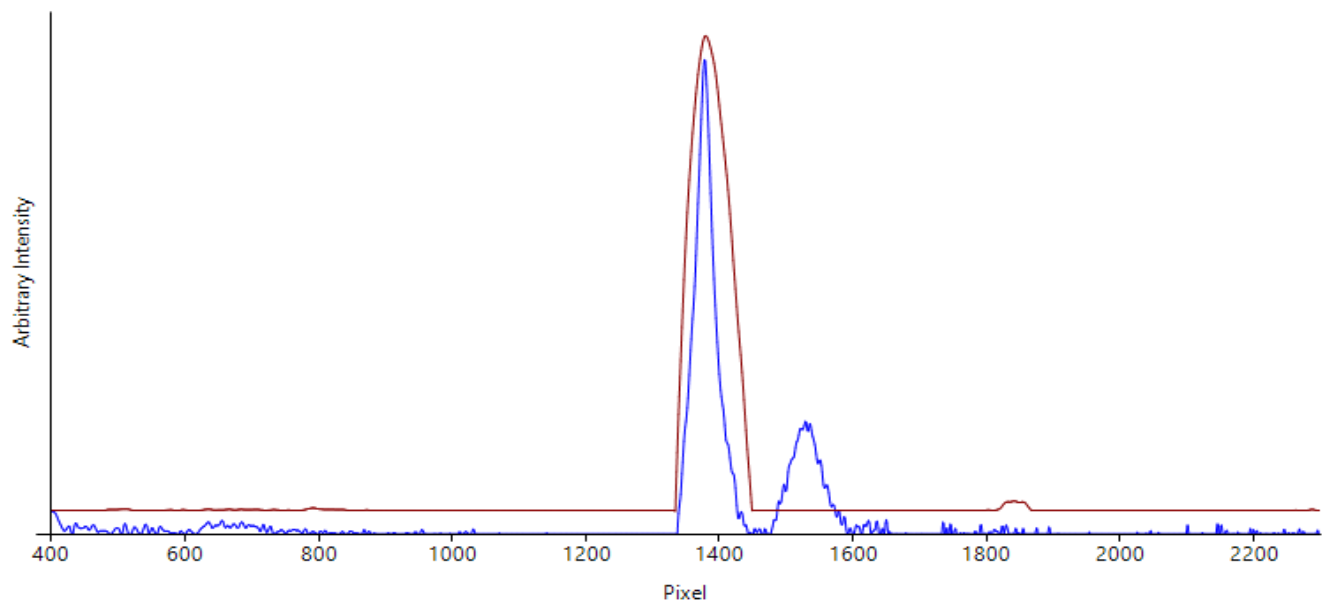

■ Scan 04194 ■ Glass

Hazard Level	Match	Sample Type	Match Score	Result Library
Clear	Glass	Chemical	0.76	Illicit v41, Version: 41

Mixture Identification Results

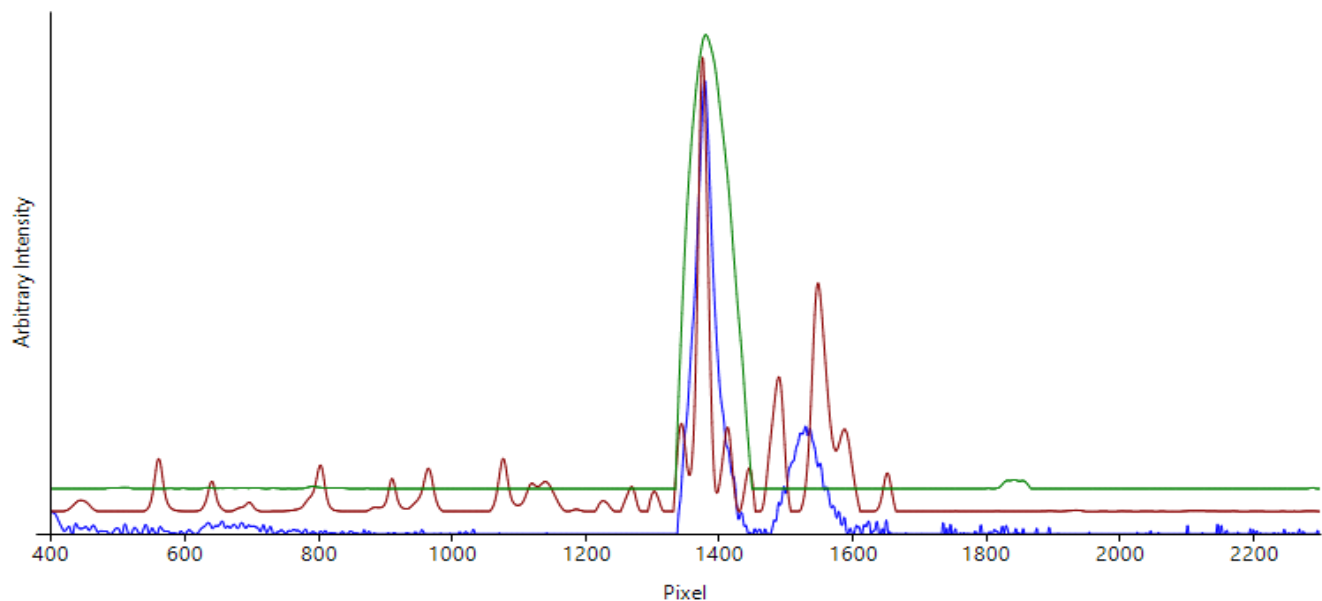

■ Scan 04194 ■ Dacarbazine ■ Glass

Hazard Level	Match	Sample Type	Source Library	Spectral Weight %
Clear	Dacarbazine	USP/Pharmaceutical	Illicit v41, Version: 41	48%
Clear	Glass	Chemical	Illicit v41, Version: 41	46%