

# Sample Report



## Sample Metadata

|               |                           |
|---------------|---------------------------|
| Sample Name   | Scan 04202                |
| Hazard Level  | Unknown                   |
| Last Modified | 2024-03-07 11:20:11-05:00 |
| Created       | 2024-03-07 11:20:11-05:00 |


## Instrument

|                              |                                 |
|------------------------------|---------------------------------|
| Serial Number                | 192600200502138                 |
| Firmware Package             | 8.1.3.55                        |
| Last Calibration             | 2024-03-07 09:58:26-05:00       |
| Last System Suitability Test | Fail, 2024-03-07 09:58:38-05:00 |


## Acquisition Parameters

|                             |                                      |
|-----------------------------|--------------------------------------|
| Operating Procedure Name    | Default Procedure                    |
| Operating Procedure Version | 1                                    |
| Integration Time            | 8.27 s                               |
| Auto Integration            | On                                   |
| Averages                    | 1                                    |
| Laser Power                 | 5                                    |
| Smart Tip Type              | Intelligent UA, Surface (Position 1) |
| Smart Tip Serial Number     | 6075060600401227                     |

## Spectral Data

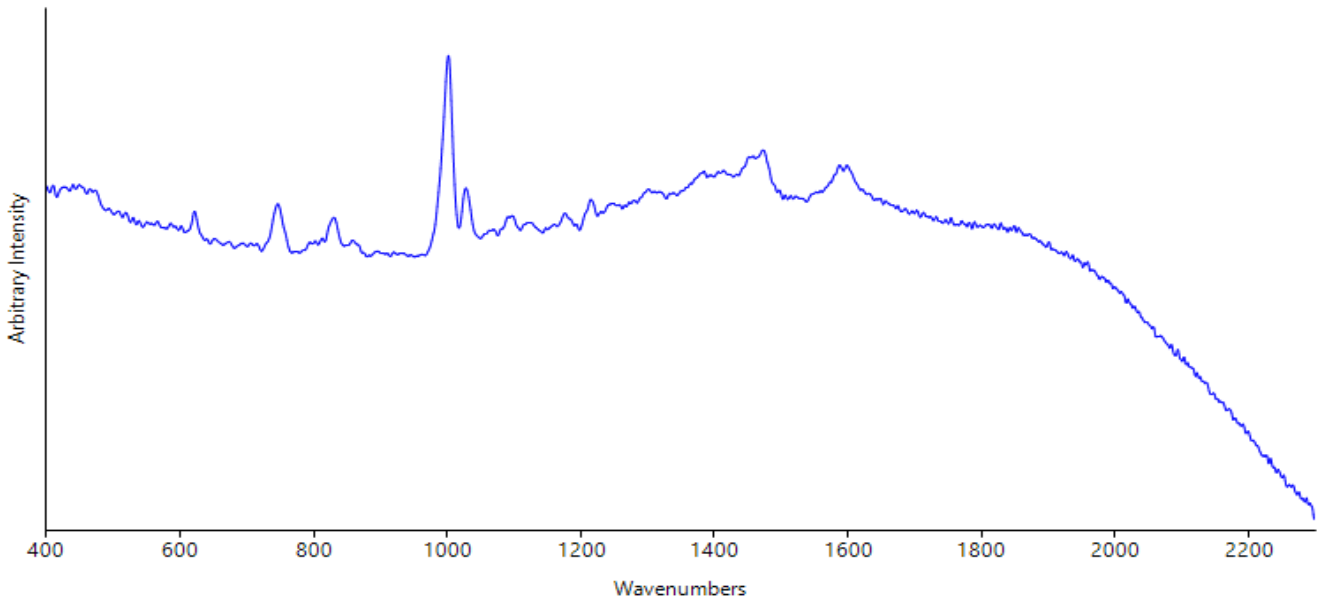


## Identification Results

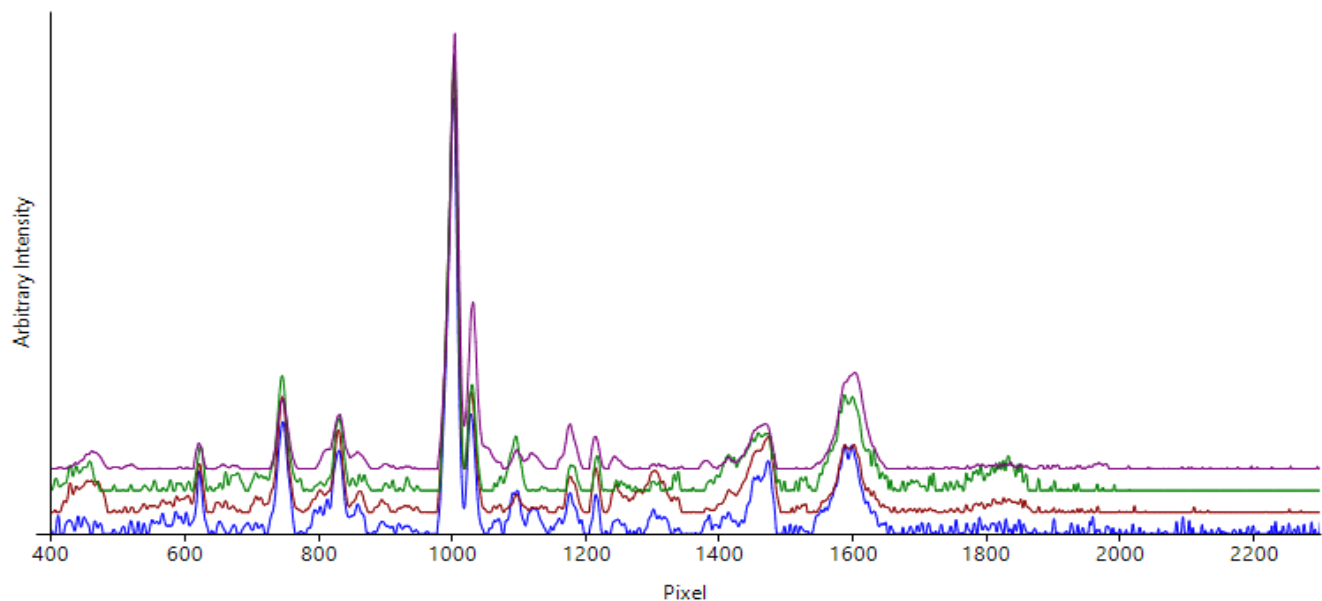

■ Scan 04202 ■ Benzyl Fentanyl PSERS-Ag 1e-3 ■ Benzyl Fentanyl PSERS-Ag 1e-4 ■ BenzylFentanyl

| Hazard Level | Match                         | Sample Type | Match Score | Result Library                      |
|--------------|-------------------------------|-------------|-------------|-------------------------------------|
| Unknown      | Benzyl Fentanyl PSERS-Ag 1e-3 |             | 0.95        | NATO SERS, Version: 1               |
| Unknown      | Benzyl Fentanyl PSERS-Ag 1e-4 |             | 0.94        | NATO SERS, Version: 1               |
| Alarm        | BenzylFentanyl                |             | 0.91        | Fentanyl Analogues_SERS, Version: 7 |

## Mixture Identification Results

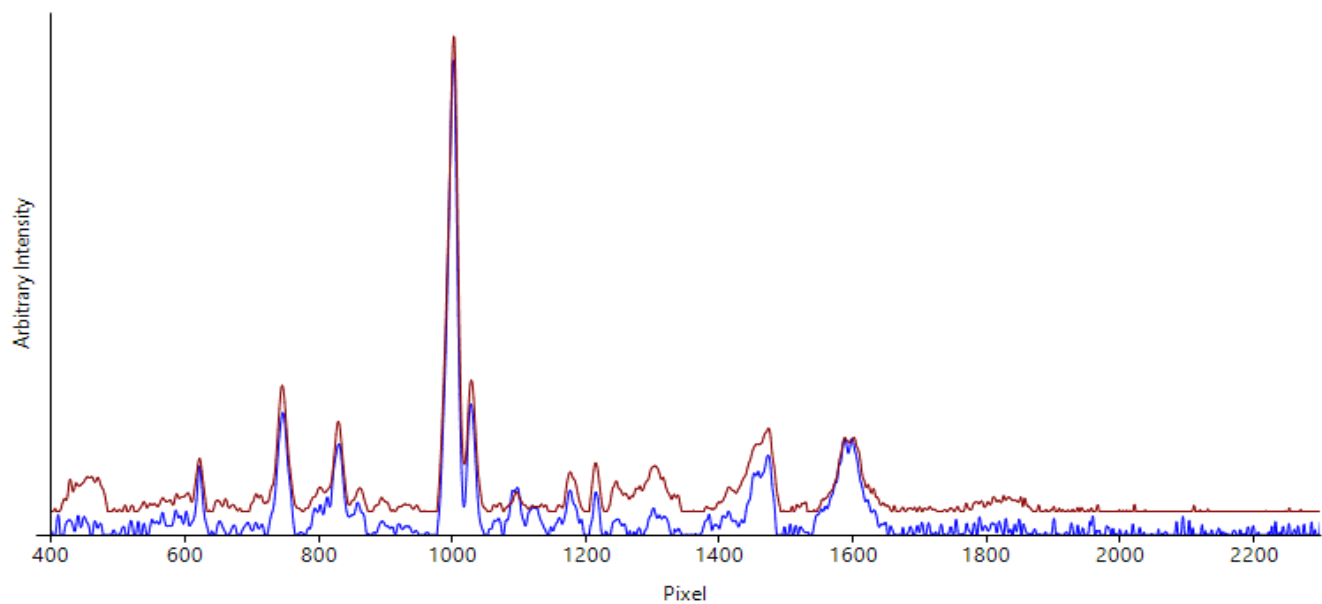

■ Scan 04202 ■ Benzyl Fentanyl PSERS-Ag 1e-3

| Hazard Level | Match                         | Sample Type | Source Library        | Spectral Weight % |
|--------------|-------------------------------|-------------|-----------------------|-------------------|
| Unknown      | Benzyl Fentanyl PSERS-Ag 1e-3 |             | NATO SERS, Version: 1 | 93%               |