

Sample Report



Sample Metadata

Sample Name	Scan 04214
Hazard Level	Clear
Sample Type	USP/Pharmaceutical, Chemical
Last Modified	2024-03-07 11:49:41-05:00
Created	2024-03-07 11:49:41-05:00


Instrument

Serial Number	192600200502138
Firmware Package	8.1.3.55
Last Calibration	2024-03-07 09:58:26-05:00
Last System Suitability Test	Fail, 2024-03-07 09:58:38-05:00


Acquisition Parameters

Operating Procedure Name	Default Procedure
Operating Procedure Version	1
Integration Time	5.78 s
Auto Integration	On
Averages	3
Laser Power	5
Smart Tip Type	Intelligent UA, Surface (Position 1)
Smart Tip Serial Number	6075060600401227

Spectral Data

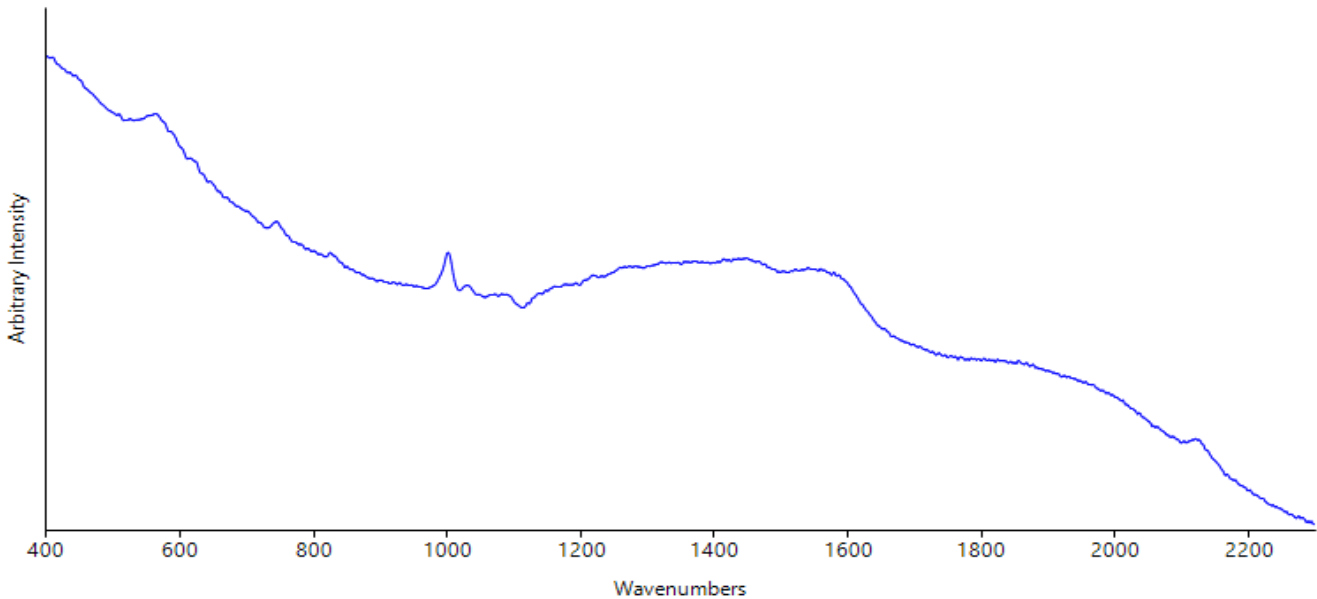

Mixture Identification Results

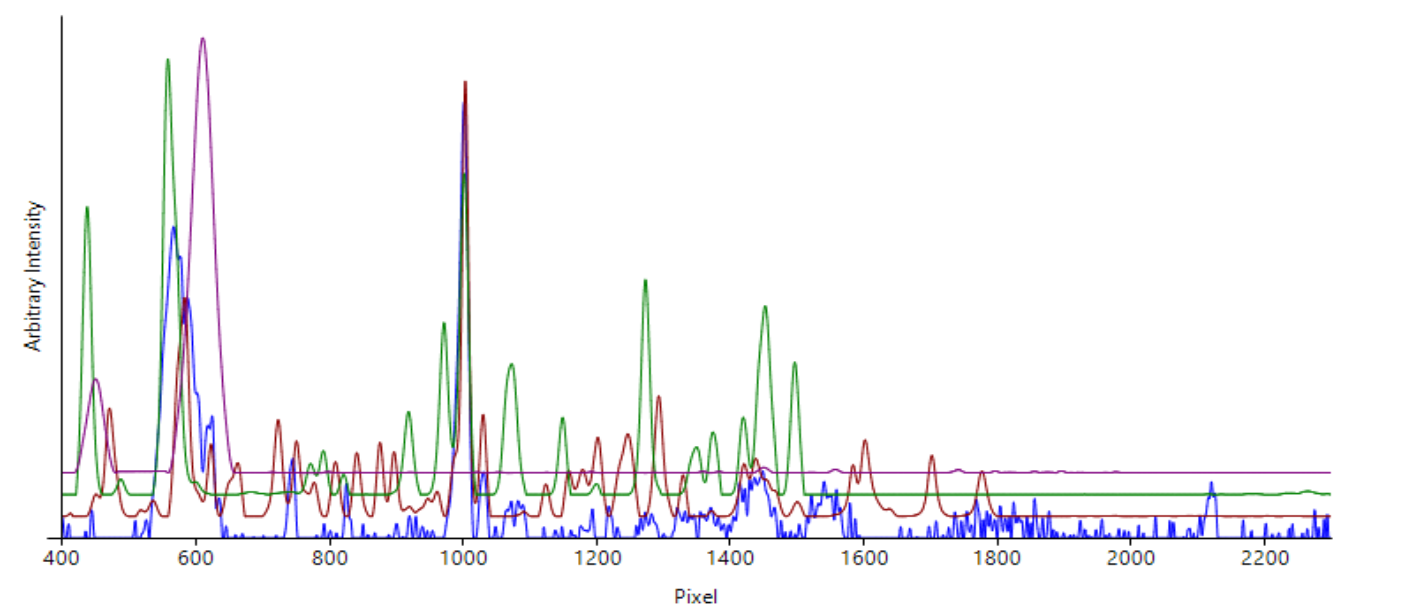

■ Scan 04214 ■ Penicillin G Sodium ■ Disulfiram ■ Titanium Oxide (rutile 2) [XTR processed]				
Hazard Level	Match	Sample Type	Source Library	Spectral Weight %
Clear	Penicillin G Sodium	USP/Pharmaceutical	Illicit v41, Version: 41	34%
Clear	Disulfiram	USP/Pharmaceutical	Illicit v41, Version: 41	32%
Clear	Titanium Oxide (rutile 2) [XTR processed]	Chemical	Illicit v41, Version: 41	17%