

Sample Report



Sample Metadata

Sample Name	Scan 04216
Hazard Level	Alarm
Sample Type	Illicit Drug
Last Modified	2024-03-07 12:04:22-05:00
Created	2024-03-07 12:04:22-05:00


Instrument

Serial Number	192600200502138
Firmware Package	8.1.3.55
Last Calibration	2024-03-07 09:58:26-05:00
Last System Suitability Test	Fail, 2024-03-07 09:58:38-05:00


Acquisition Parameters

Operating Procedure Name	Default Procedure
Operating Procedure Version	1
Integration Time	6.47 s
Auto Integration	On
Averages	1
Laser Power	5
Smart Tip Type	Intelligent UA, Surface (Position 1)
Smart Tip Serial Number	6075060600401227

Spectral Data

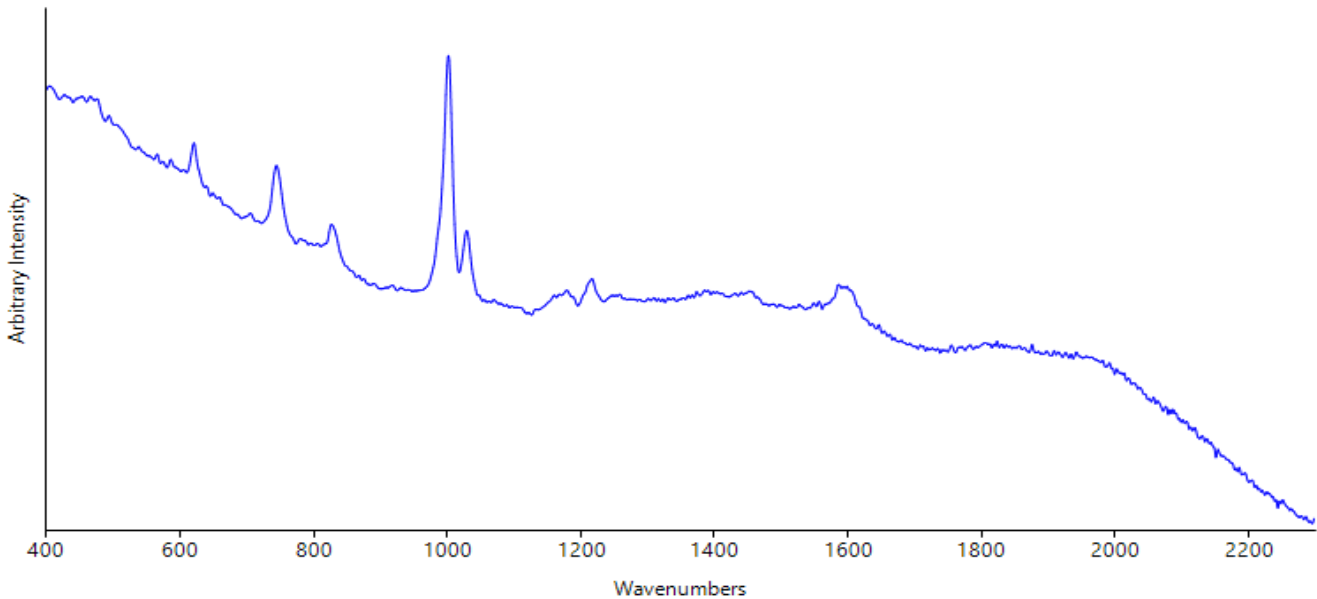


Identification Results

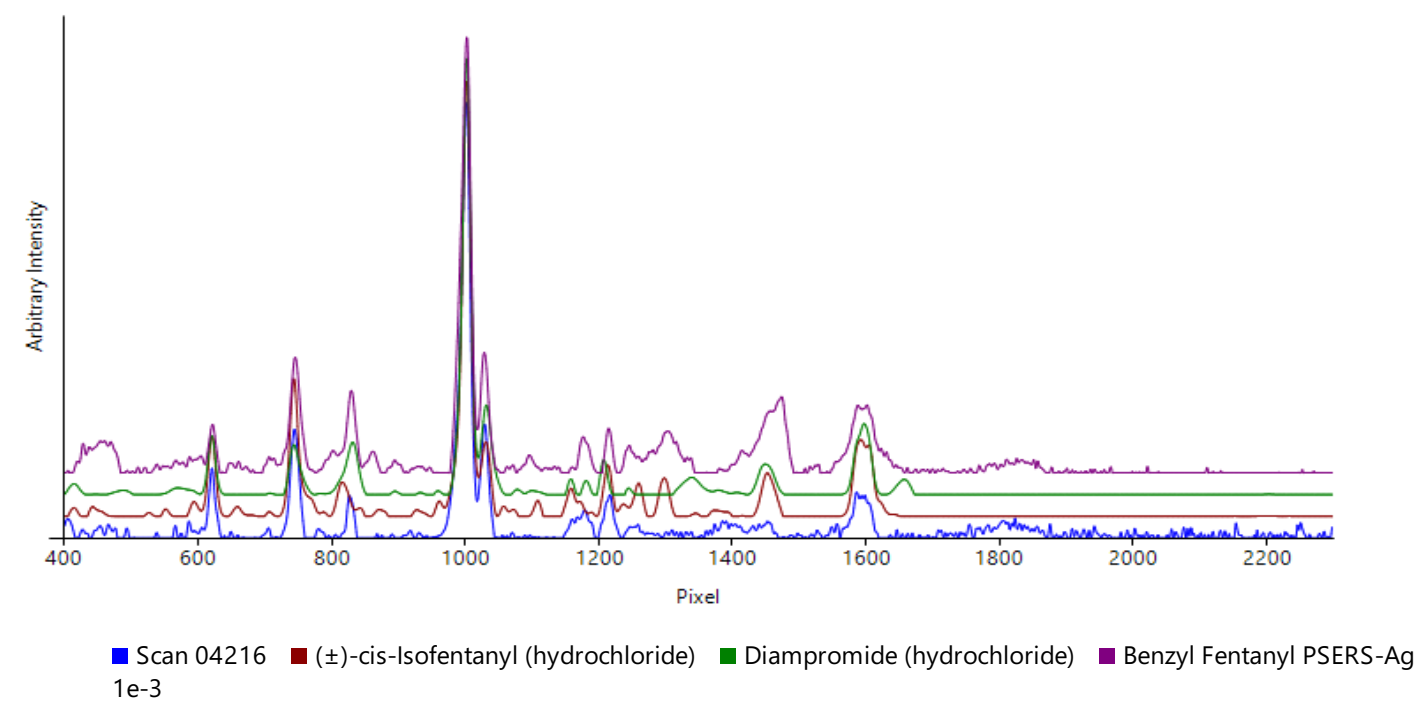

Hazard Level	Match	Sample Type	Match Score	Result Library
Alarm	(±)-cis-Isofentanyl (hydrochloride)	Illicit Drug	0.92	Illicit v41, Version: 41
Alarm	Diampromide (hydrochloride)	Illicit Drug	0.92	Illicit v41, Version: 41
Unknown	Benzyl Fentanyl PSERS-Ag 1e-3		0.89	NATO SERS, Version: 1

Mixture Identification Results

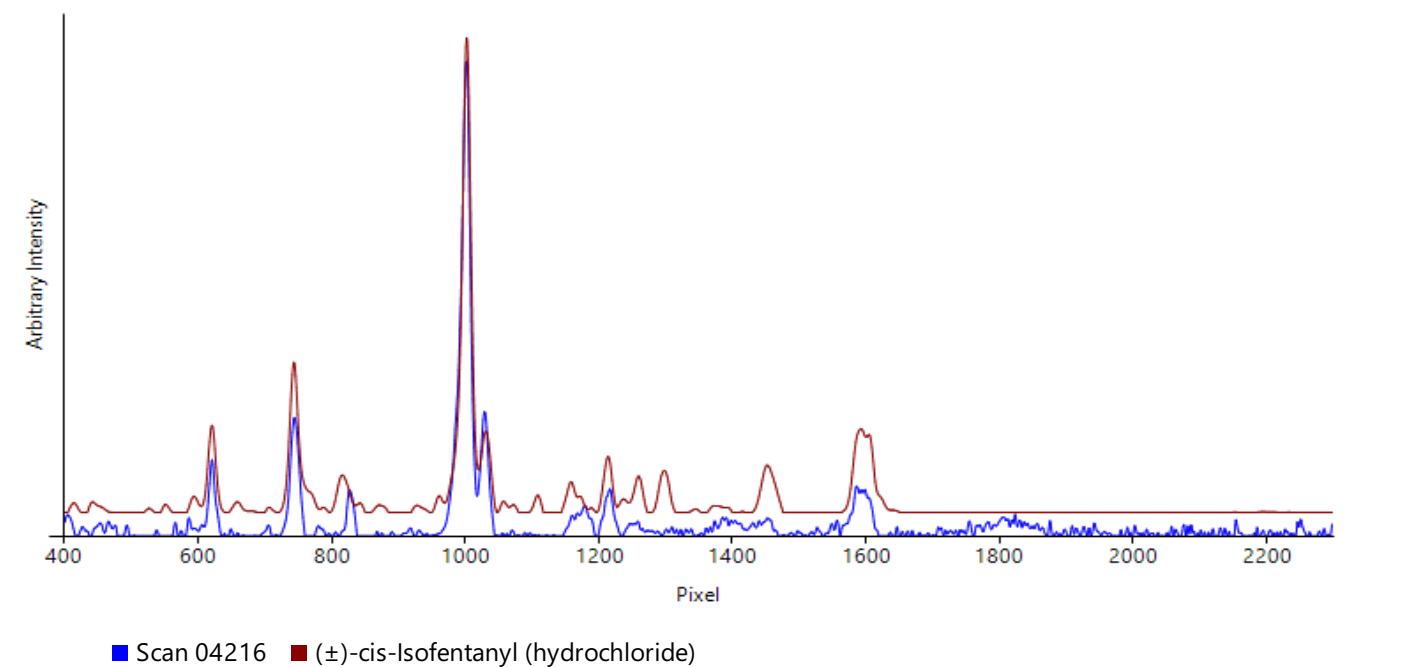

Hazard Level	Match	Sample Type	Source Library	Spectral Weight %
Alarm	(±)-cis-Isofentanyl (hydrochloride)	Illicit Drug	Illicit v41, Version: 41	90%