

# Sample Report



## Sample Metadata

|               |                           |
|---------------|---------------------------|
| Sample Name   | Scan 04220                |
| Hazard Level  | Warning                   |
| Sample Type   | USP/Pharmaceutical        |
| Last Modified | 2024-03-07 14:14:40-05:00 |
| Created       | 2024-03-07 14:14:40-05:00 |


## Instrument

|                              |                                 |
|------------------------------|---------------------------------|
| Serial Number                | 192600200502138                 |
| Firmware Package             | 8.1.3.55                        |
| Last Calibration             | 2024-03-07 09:58:26-05:00       |
| Last System Suitability Test | Fail, 2024-03-07 09:58:38-05:00 |


## Acquisition Parameters

|                             |                                      |
|-----------------------------|--------------------------------------|
| Operating Procedure Name    | Default Procedure                    |
| Operating Procedure Version | 1                                    |
| Integration Time            | 5.81 s                               |
| Auto Integration            | On                                   |
| Averages                    | 1                                    |
| Laser Power                 | 5                                    |
| Smart Tip Type              | Intelligent UA, Surface (Position 1) |
| Smart Tip Serial Number     | 6075060600401227                     |

## Spectral Data

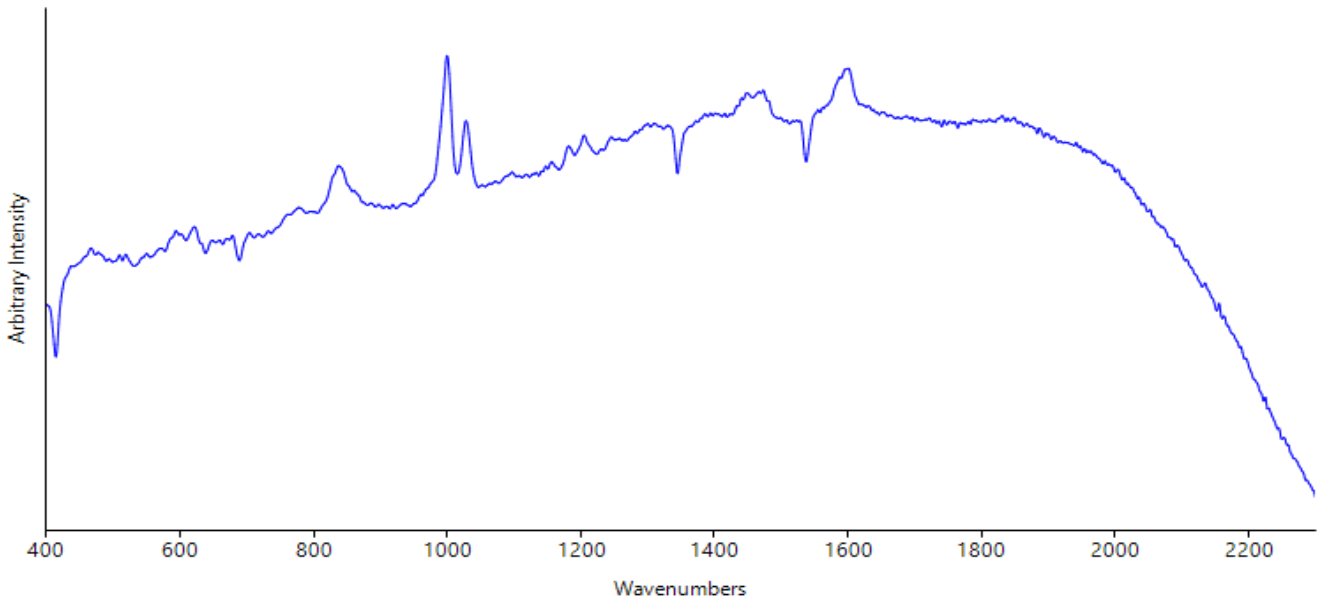


## Identification Results

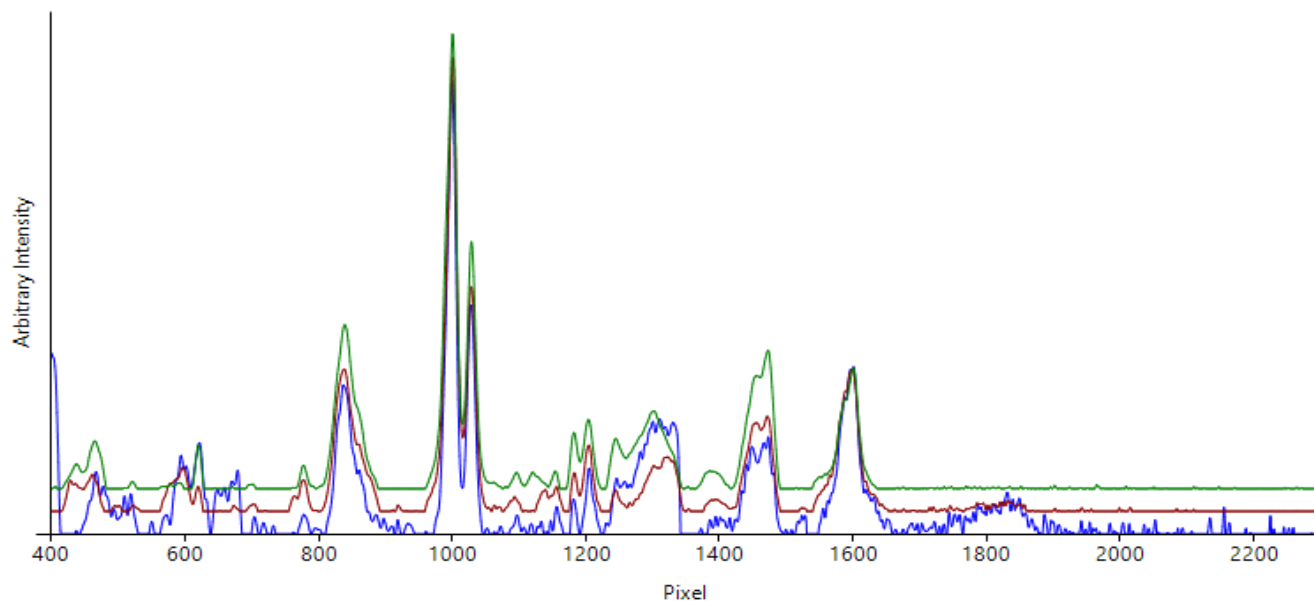

■ Scan 04220 ■ 4-ANPP PSERS-Ag 1e-4 ■ 4-ANPP PSERS-Ag 1e-3

| Hazard Level | Match                | Sample Type | Match Score | Result Library        |
|--------------|----------------------|-------------|-------------|-----------------------|
| Unknown      | 4-ANPP PSERS-Ag 1e-4 |             | 0.82        | NATO SERS, Version: 1 |
| Unknown      | 4-ANPP PSERS-Ag 1e-3 |             | 0.81        | NATO SERS, Version: 1 |

## Mixture Identification Results

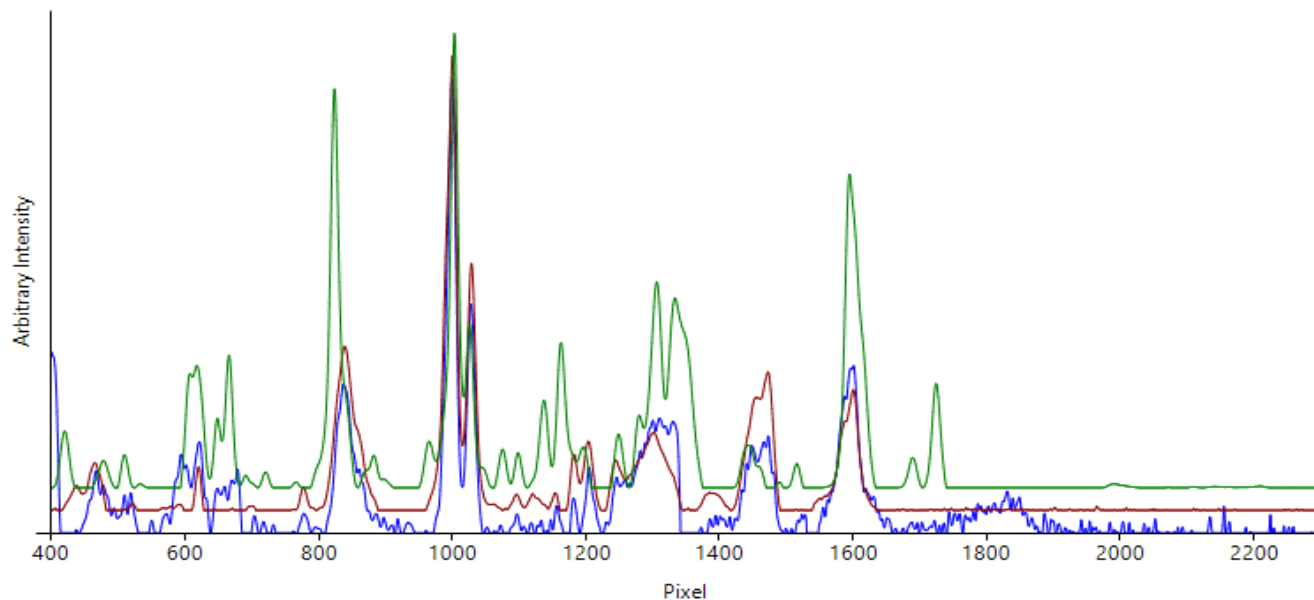

■ Scan 04220 ■ 4-ANPP PSERS-Ag 1e-3 ■ Oxyphenbutazone

| Hazard Level | Match                | Sample Type        | Source Library           | Spectral Weight % |
|--------------|----------------------|--------------------|--------------------------|-------------------|
| Unknown      | 4-ANPP PSERS-Ag 1e-3 |                    | NATO SERS, Version: 1    | 57%               |
| Warning      | Oxyphenbutazone      | USP/Pharmaceutical | Illicit v41, Version: 41 | 12%               |