

Sample Report



Sample Metadata

Sample Name	Scan 00006
Hazard Level	Clear
Sample Type	USP/Pharmaceutical
Last Modified	2024-03-05 13:30:46-05:00
Created	2024-03-05 13:30:46-05:00


Instrument

Serial Number	192601100201104
Firmware Package	8.0.3.56
Last Calibration	2024-03-05 13:17:42-05:00
Last System Suitability Test	Pass, 2024-03-05 13:17:53-05:00


Acquisition Parameters

Operating Procedure Name	Default Procedure
Operating Procedure Version	1
Integration Time	10.00 s
Auto Integration	On
Averages	3
Laser Power	5
Smart Tip Type	Intelligent UA, Surface (Position 1)
Smart Tip Serial Number	6075060600301151

Spectral Data

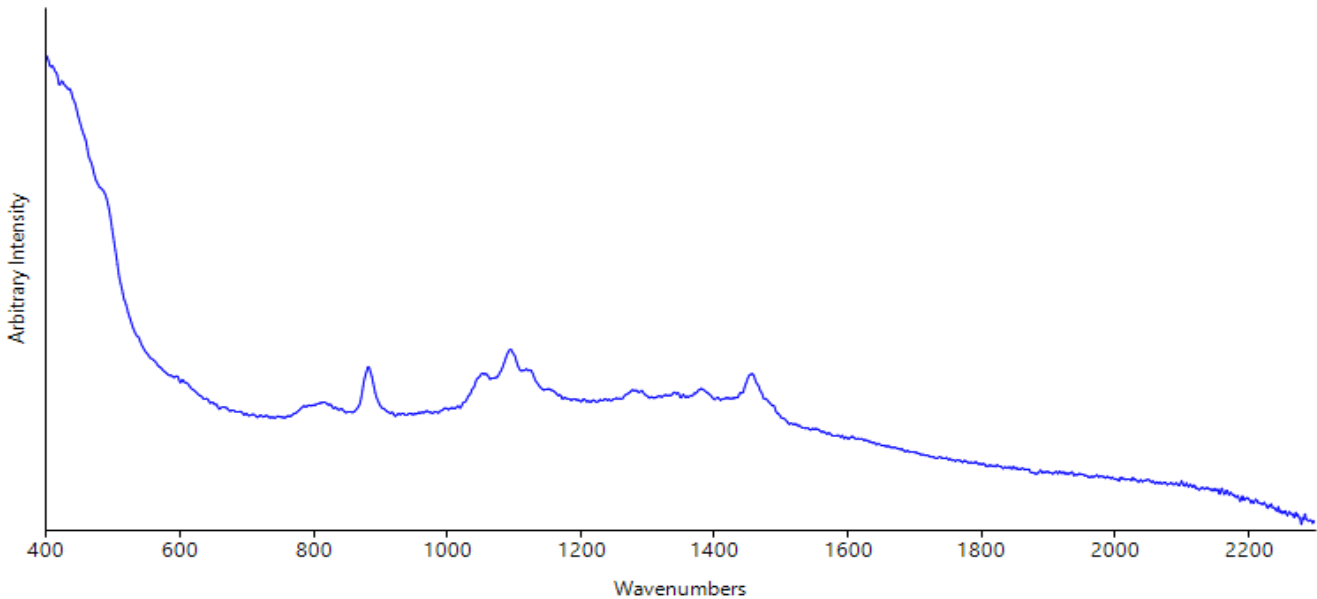


Identification Results

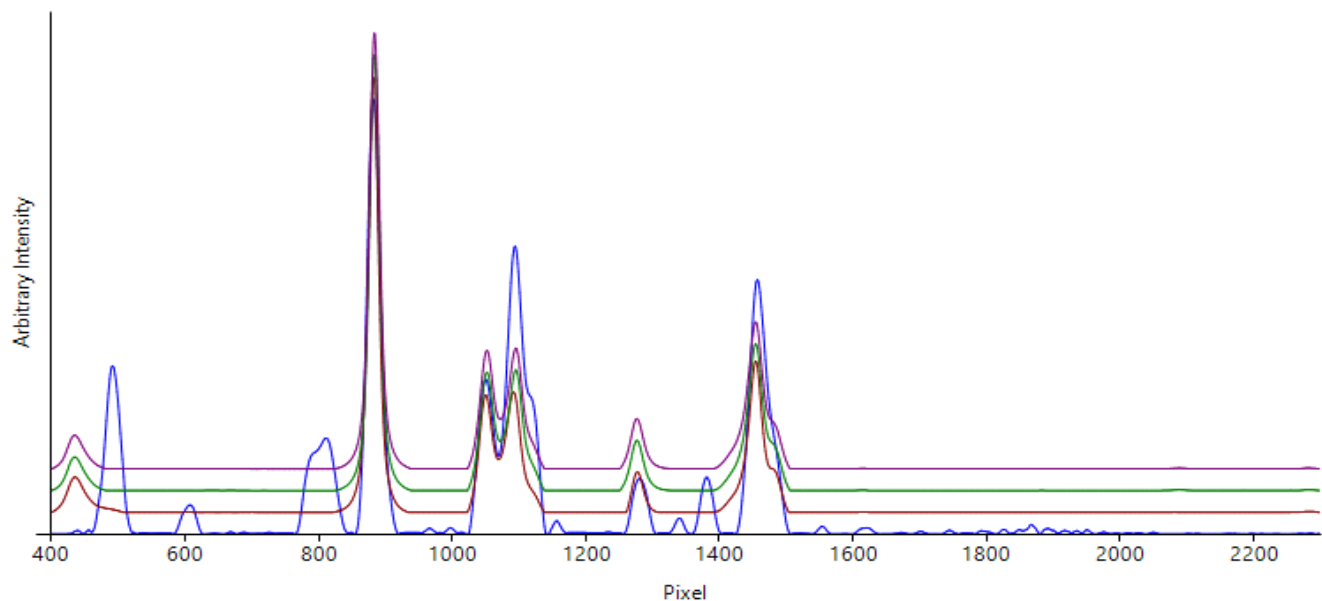

Hazard Level	Match	Sample Type	Match Score	Result Library
Clear	Ethanol (75% solution)	Chemical	0.75	Illicit, Version: 41
Clear	Ethanol	USP/Pharmaceutical	0.75	Illicit, Version: 41
Precursor	Ethanol	Chemical Warfare Agent	0.75	CWA, Version: 3

Mixture Identification Results

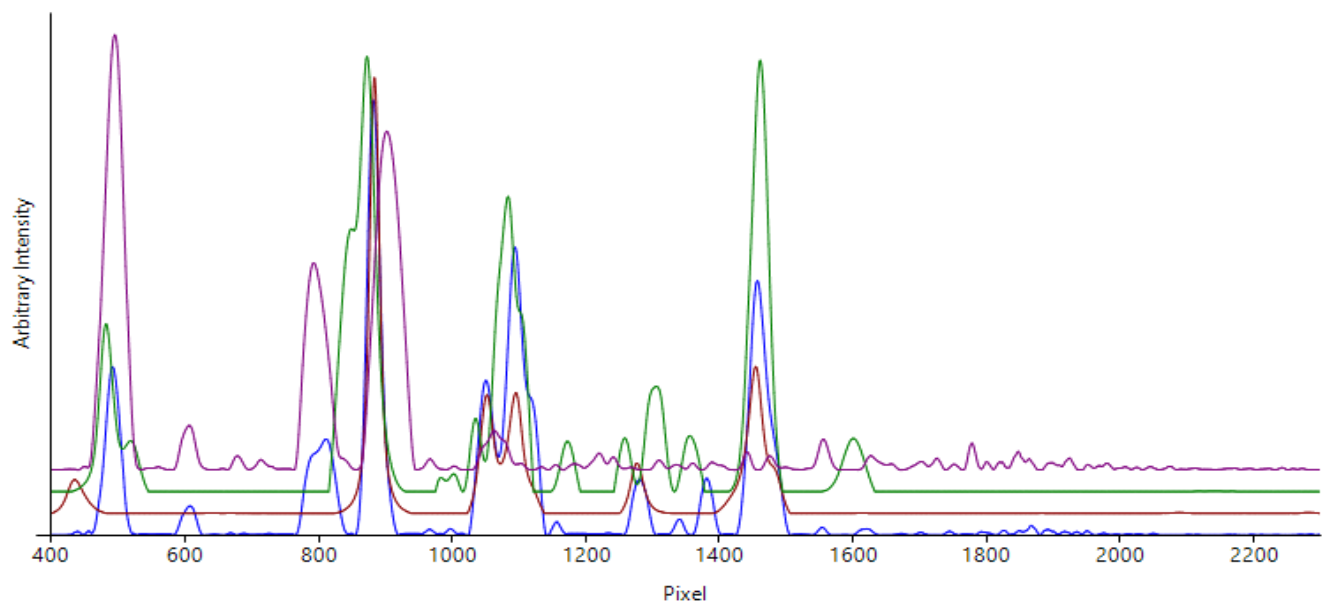

Hazard Level	Match	Sample Type	Source Library	Spectral Weight %
Clear	Ethanol	USP/Pharmaceutical	Illicit, Version: 41	53%
Clear	Monoethanolamine	USP/Pharmaceutical	Illicit, Version: 41	14%
Clear	Right Angle Attachment window		Illicit, Version: 41	11%