

Sample Report



Sample Metadata

Sample Name	Scan 00009
Hazard Level	Clear
Sample Type	USP/Pharmaceutical
Last Modified	2024-03-05 13:36:57-05:00
Created	2024-03-05 13:36:57-05:00


Instrument

Serial Number	192601100201104
Firmware Package	8.0.3.56
Last Calibration	2024-03-05 13:17:42-05:00
Last System Suitability Test	Pass, 2024-03-05 13:17:53-05:00


Acquisition Parameters

Operating Procedure Name	Default Procedure
Operating Procedure Version	1
Integration Time	10.00 s
Auto Integration	On
Averages	1
Laser Power	5
Smart Tip Type	Intelligent UA, Surface (Position 1)
Smart Tip Serial Number	6075060600301151

Spectral Data

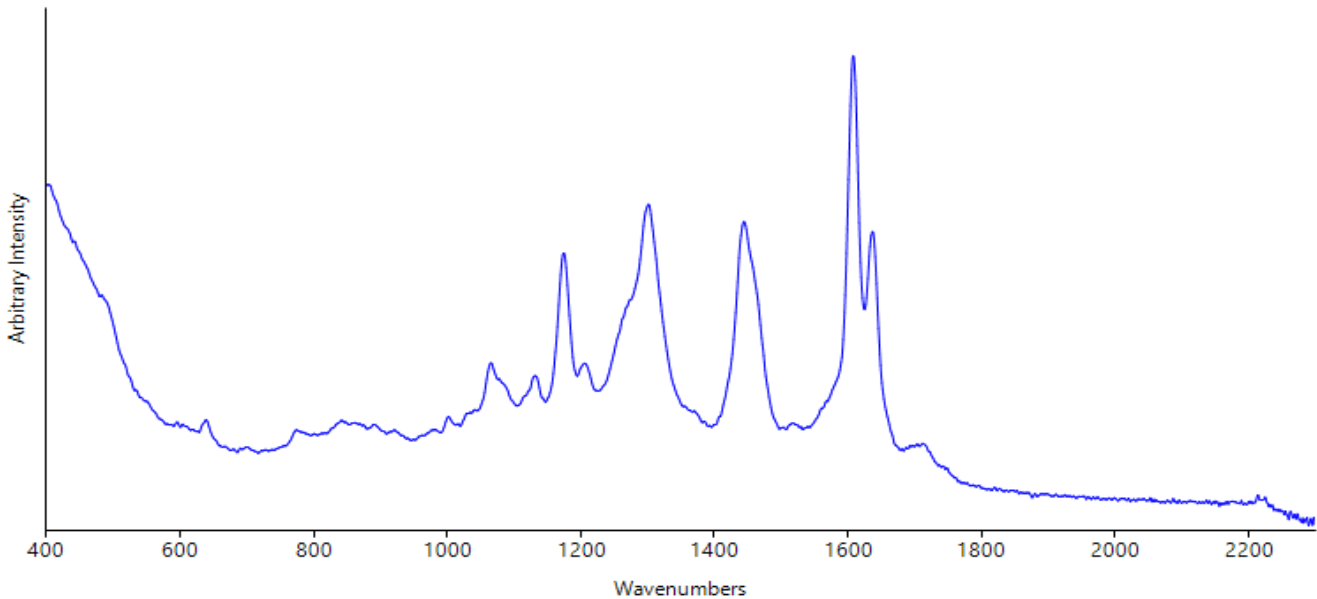


Identification Results

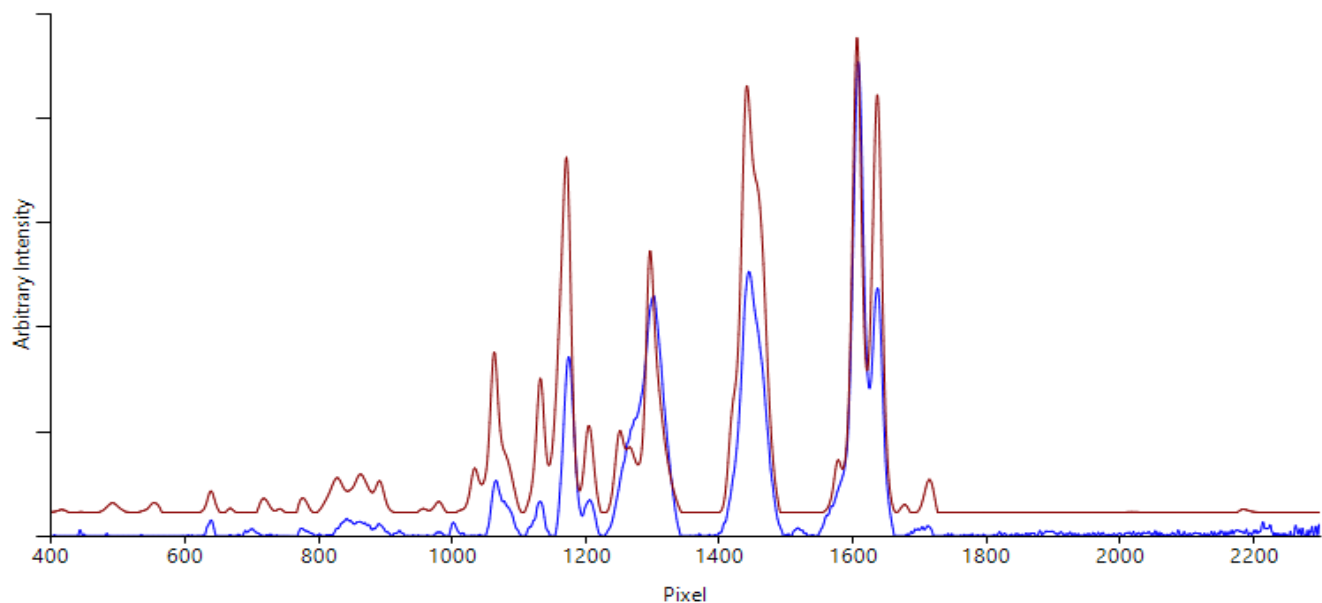

■ Scan 00009 ■ Lip Balm. Blistex

Hazard Level	Match	Sample Type	Match Score	Result Library
Clear	Lip Balm. Blistex	USP/Pharmaceutical	0.83	Illicit, Version: 41

Mixture Identification Results

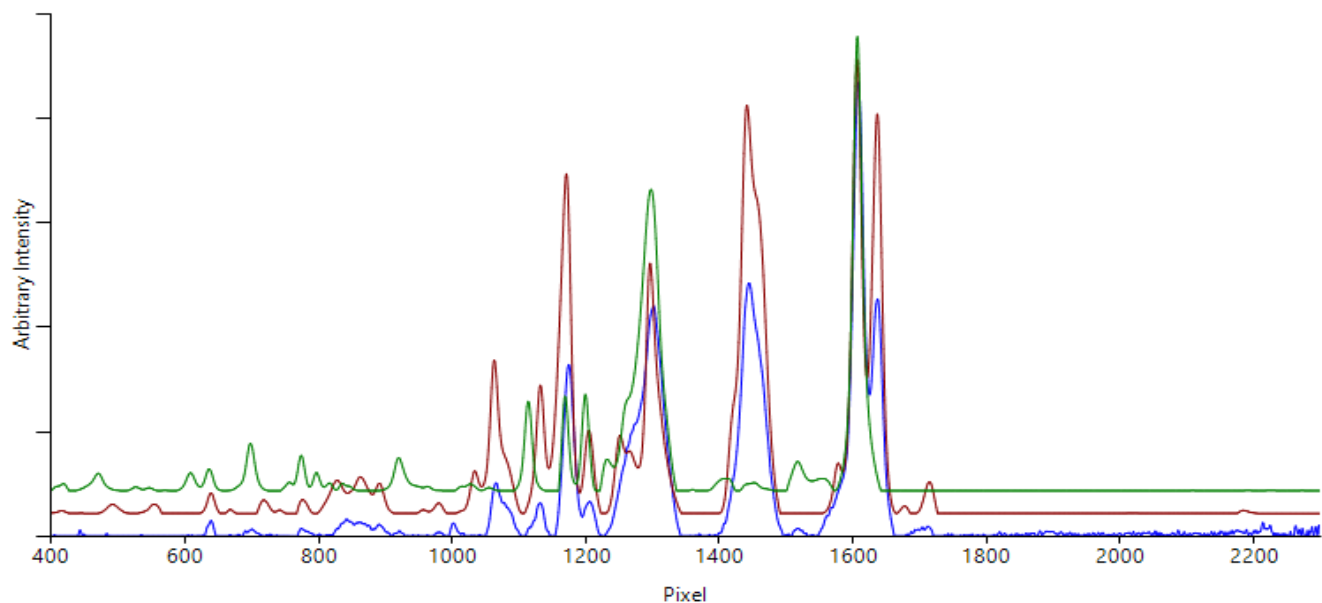

■ Scan 00009 ■ Lip Balm. Blistex ■ Avobenzone

Hazard Level	Match	Sample Type	Source Library	Spectral Weight %
Clear	Lip Balm. Blistex	USP/Pharmaceutical	Illicit, Version: 41	51%
Clear	Avobenzone	USP/Pharmaceutical	Illicit, Version: 41	39%