

Sample Report



Sample Metadata

Sample Name	Scan 00011
Hazard Level	Alarm
Sample Type	Illicit Drug
Last Modified	2024-03-05 13:42:23-05:00
Created	2024-03-05 13:42:23-05:00


Instrument

Serial Number	192601100201104
Firmware Package	8.0.3.56
Last Calibration	2024-03-05 13:17:42-05:00
Last System Suitability Test	Pass, 2024-03-05 13:17:53-05:00


Acquisition Parameters

Operating Procedure Name	Default Procedure
Operating Procedure Version	1
Integration Time	10.00 s
Auto Integration	On
Averages	3
Laser Power	5
Smart Tip Type	Intelligent UA, Bottle (Position 3)
Smart Tip Serial Number	6075060600301151

Spectral Data

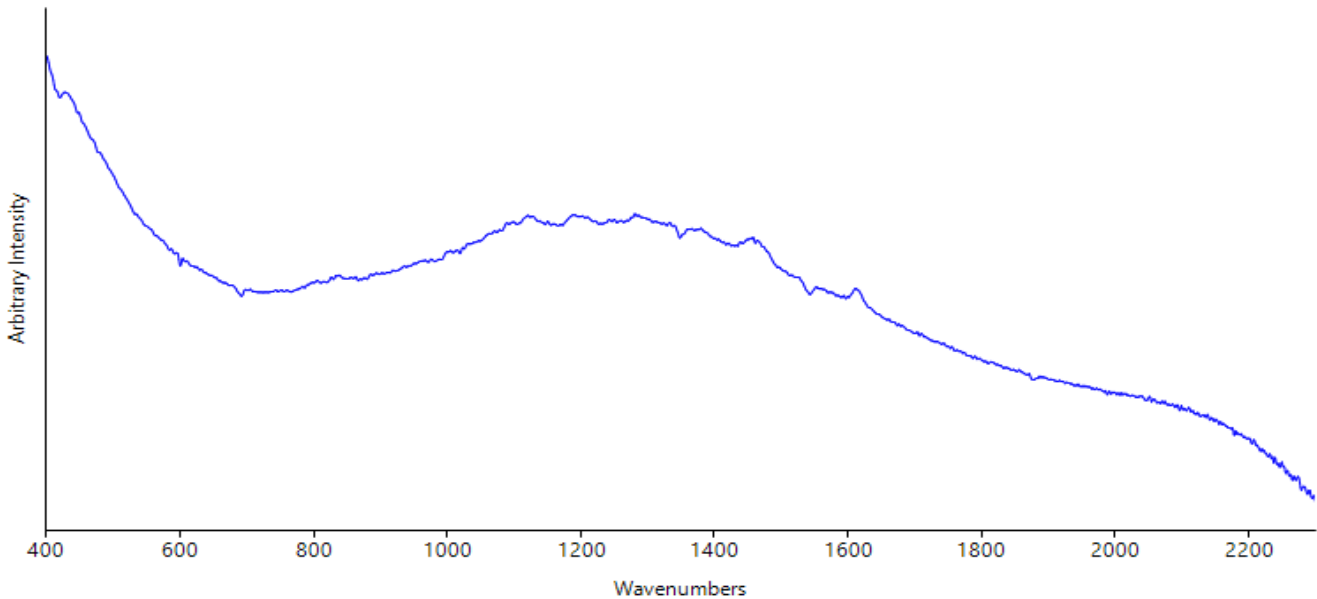

Mixture Identification Results

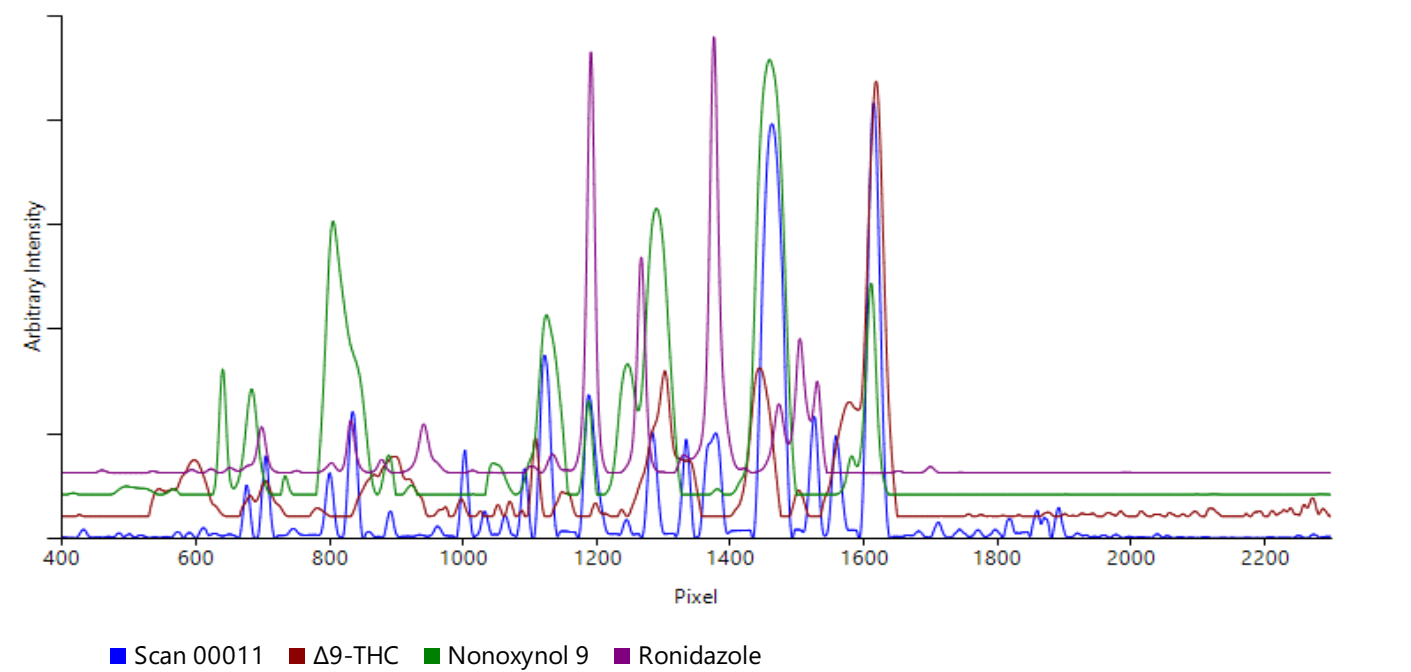

Hazard Level	Match	Sample Type	Source Library	Spectral Weight %
Alarm	Δ9-THC	Illicit Drug	Illicit, Version: 41	33%
Clear	Nonoxynol 9	USP/Pharmaceutical	Illicit, Version: 41	31%
Clear	Ronidazole	USP/Pharmaceutical	Illicit, Version: 41	16%