

Sample Report



Sample Metadata

Sample Name	Scan 00014
Hazard Level	Clear
Sample Type	Chemical
Last Modified	2024-03-05 14:12:30-05:00
Created	2024-03-05 14:12:30-05:00


Instrument

Serial Number	192601100201104
Firmware Package	8.0.3.56
Last Calibration	2024-03-05 13:17:42-05:00
Last System Suitability Test	Pass, 2024-03-05 13:17:53-05:00


Acquisition Parameters

Operating Procedure Name	Default Procedure
Operating Procedure Version	1
Integration Time	1.09 s
Auto Integration	On
Averages	1
Laser Power	5
Smart Tip Type	Intelligent UA, Surface (Position 1)
Smart Tip Serial Number	6075060600301151

Spectral Data

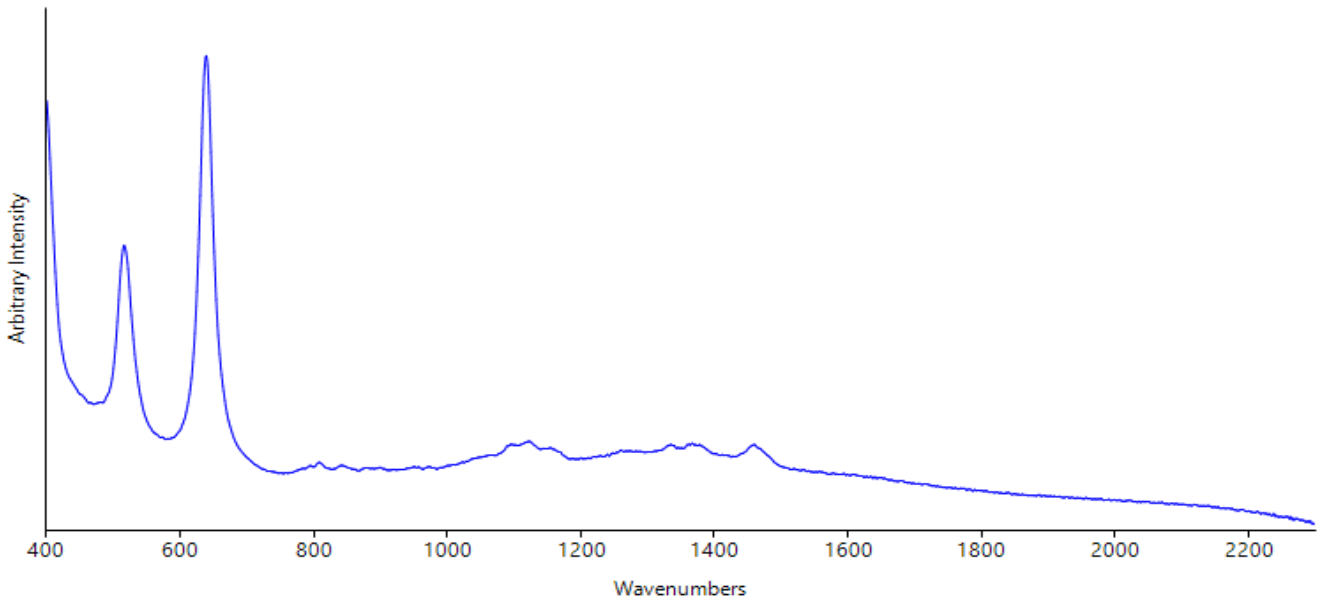


Identification Results

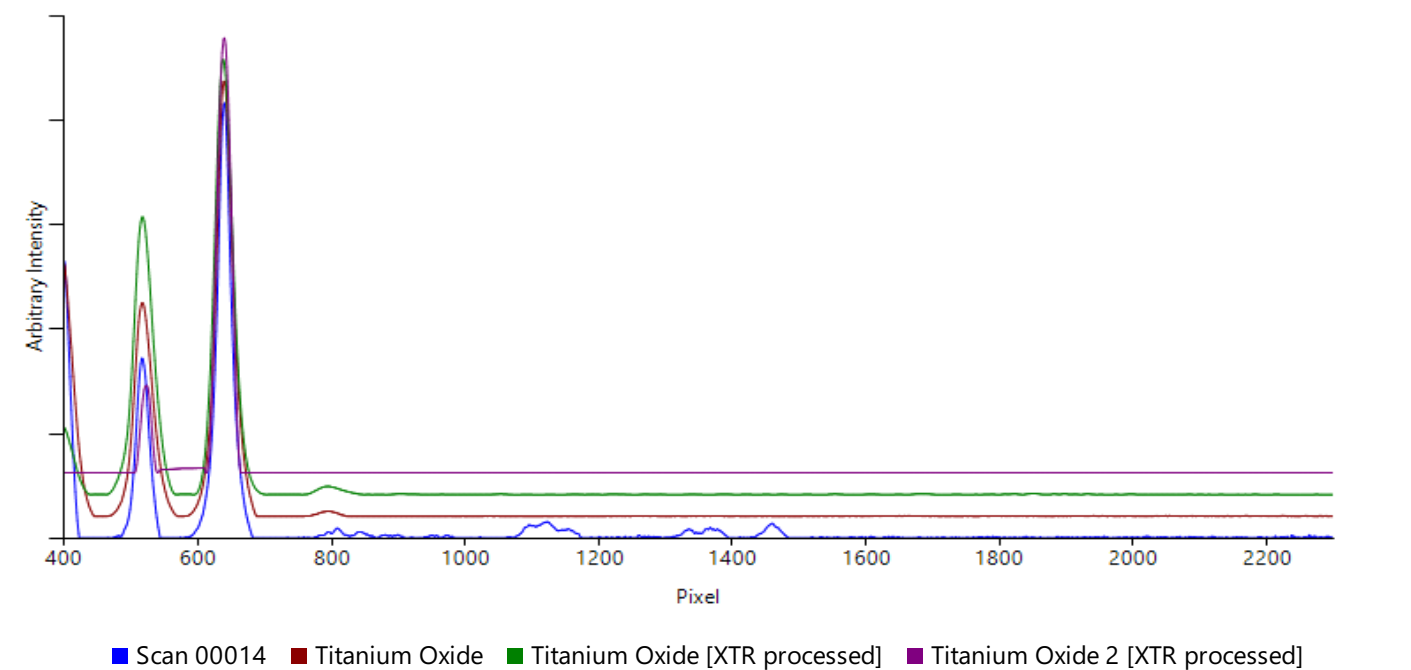

Hazard Level	Match	Sample Type	Match Score	Result Library
Clear	Titanium Oxide	Chemical	0.96	Illicit, Version: 41
Clear	Titanium Oxide [XTR processed]	Chemical	0.85	Illicit, Version: 41
Clear	Titanium Oxide 2 [XTR processed]	Chemical	0.80	Illicit, Version: 41

Mixture Identification Results

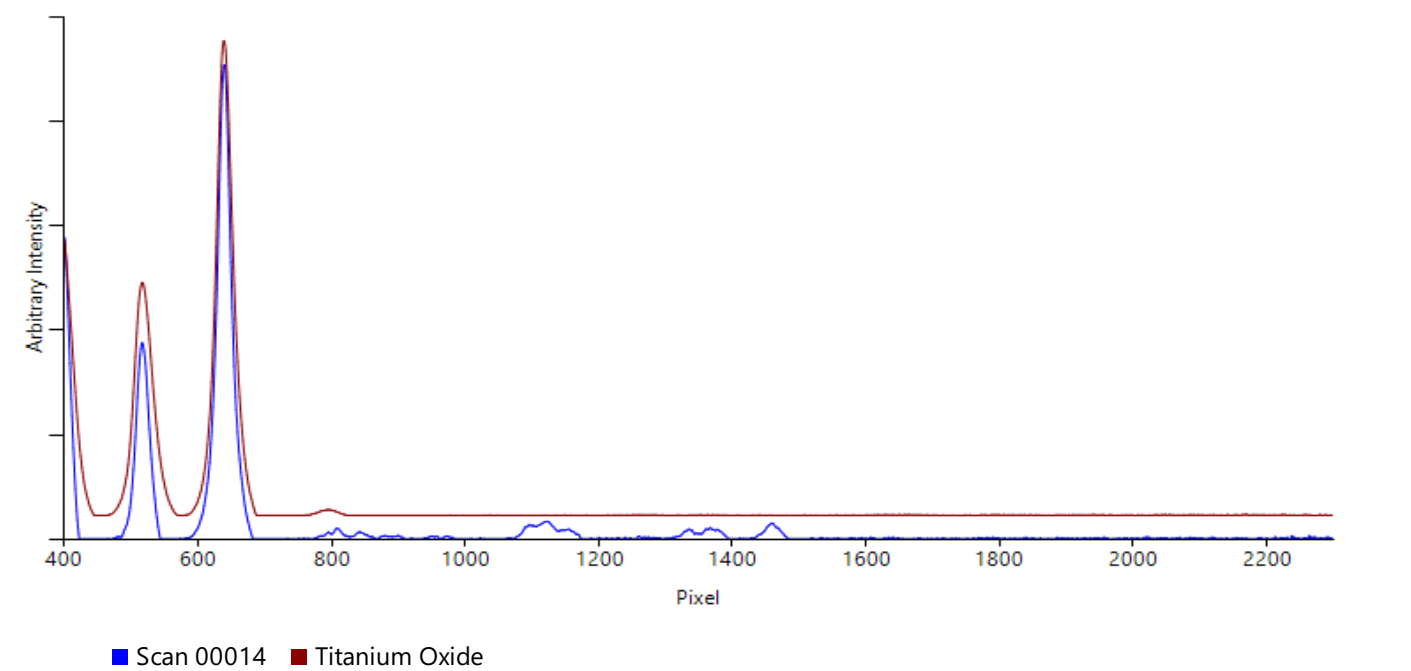

Hazard Level	Match	Sample Type	Source Library	Spectral Weight %
Clear	Titanium Oxide	Chemical	Illicit, Version: 41	92%