

Sample Report



Sample Metadata

Sample Name	Scan 00023
Hazard Level	Alarm
Sample Type	Illicit Drug
Last Modified	2024-03-06 10:31:30-05:00
Created	2024-03-06 10:31:30-05:00


Instrument

Serial Number	192601100201104
Firmware Package	8.0.3.56
Last Calibration	2024-03-06 10:07:19-05:00
Last System Suitability Test	Pass, 2024-03-06 10:07:29-05:00


Acquisition Parameters

Operating Procedure Name	Default Procedure
Operating Procedure Version	1
Integration Time	6.10 s
Auto Integration	On
Averages	3
Laser Power	5
Smart Tip Type	Intelligent UA, Surface (Position 1)
Smart Tip Serial Number	6075060600601336

Spectral Data

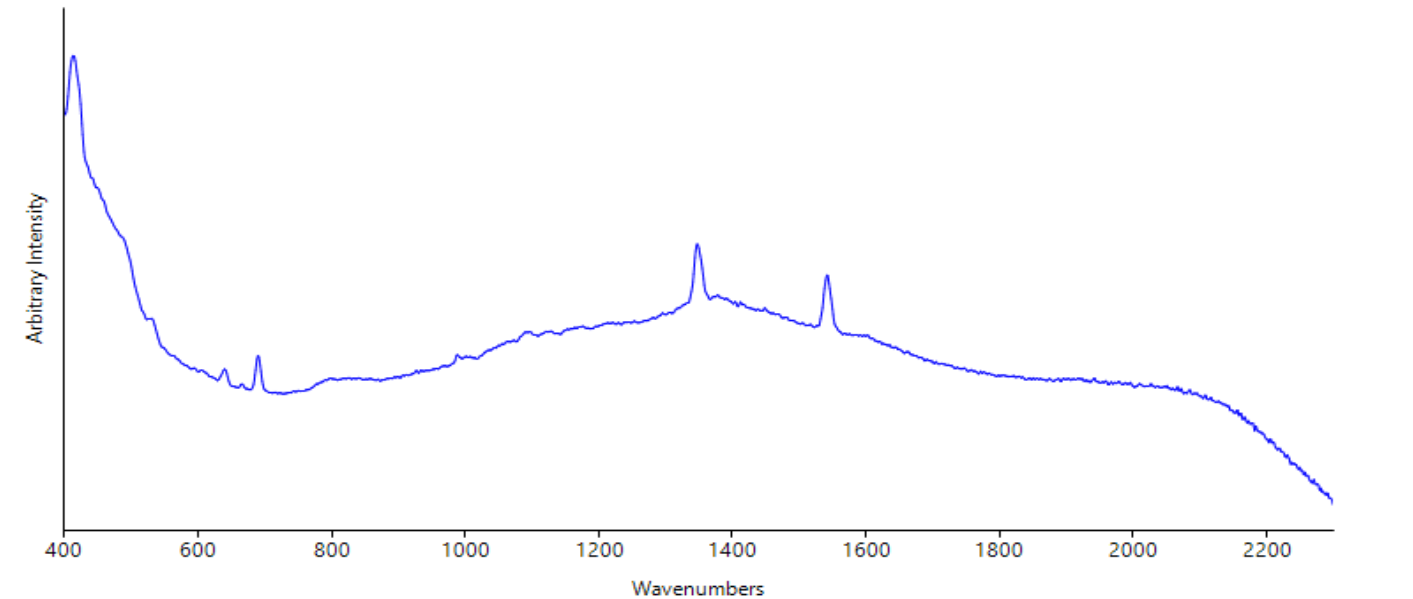

Mixture Identification Results

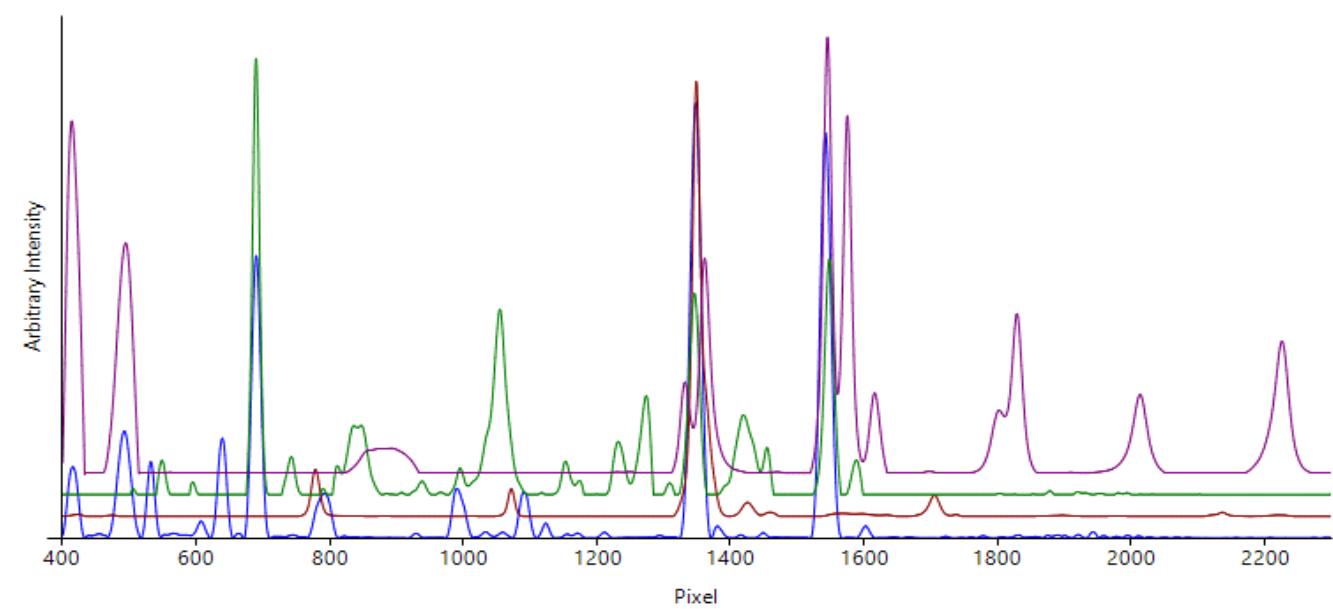

■ Scan 00023 ■ Ammonium formate ■ 4-Hydroxy DMT ■ LUTETIUM(III) OXIDE

Hazard Level	Match	Sample Type	Source Library	Spectral Weight %
Clear	Ammonium formate	Inorganic/Organometallic Chemical	MCRL Inorganic-Organometallics, Version: 1	36%
Alarm	4-Hydroxy DMT	Illicit Drug	Illicit, Version: 41	29%
Clear	LUTETIUM(III) OXIDE	Inorganic/Organometallic Chemical	MCRL Inorganic-Organometallics, Version: 1	12%