

Sample Report



Sample Metadata

Sample Name	Scan 00025
Hazard Level	Clear
Sample Type	USP/Pharmaceutical
Last Modified	2024-03-06 10:59:03-05:00
Created	2024-03-06 10:59:03-05:00


Instrument

Serial Number	192601100201104
Firmware Package	8.0.3.56
Last Calibration	2024-03-06 10:07:19-05:00
Last System Suitability Test	Pass, 2024-03-06 10:07:29-05:00


Acquisition Parameters

Operating Procedure Name	Default Procedure
Operating Procedure Version	1
Integration Time	4.05 s
Auto Integration	On
Averages	3
Laser Power	5
Smart Tip Type	Intelligent UA, Surface (Position 1)
Smart Tip Serial Number	6075060600601336

Spectral Data

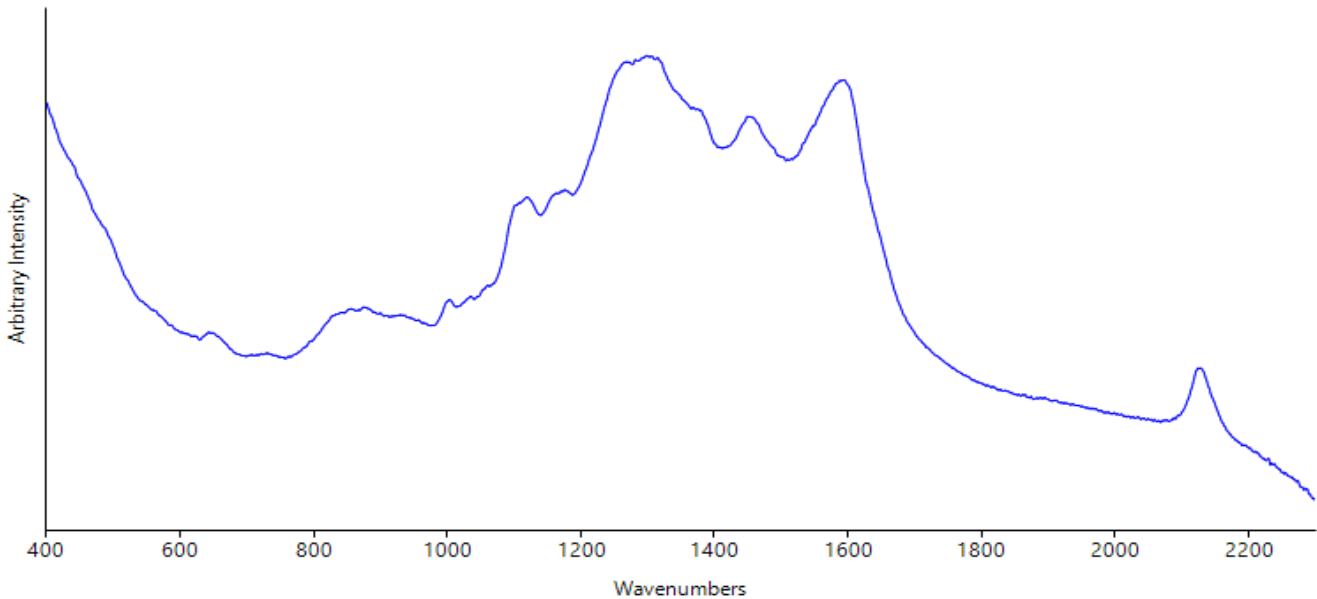

Mixture Identification Results

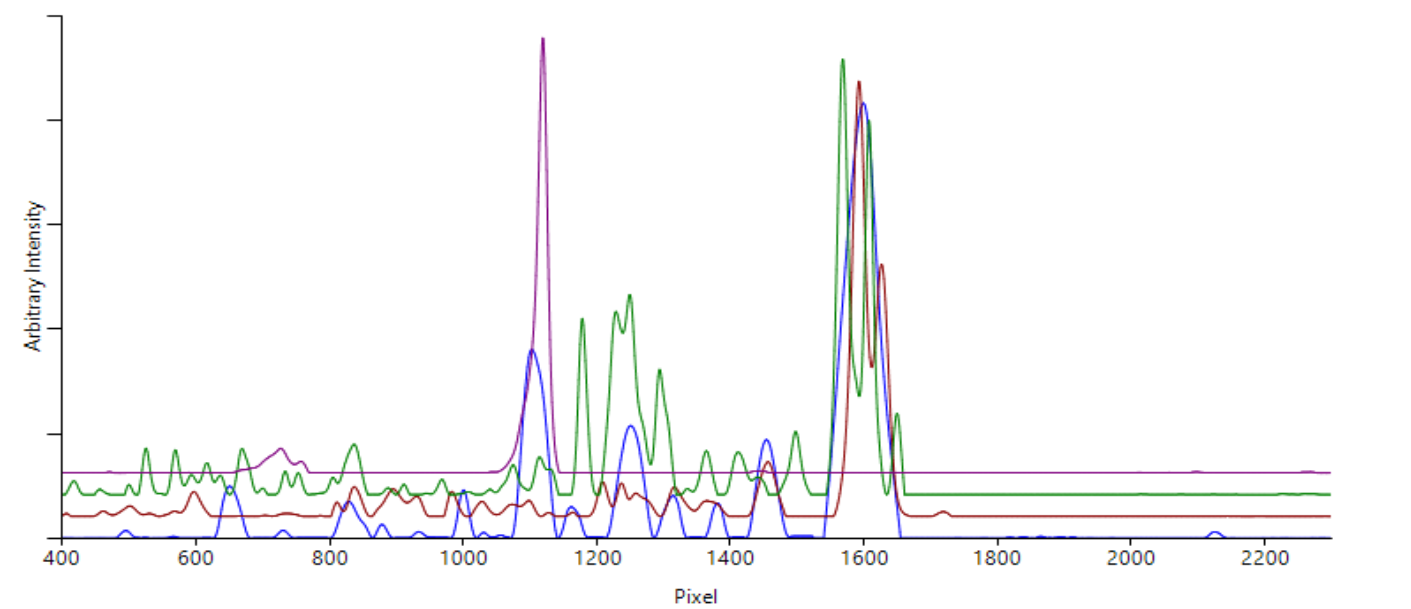

■ Scan 00025 ■ Tylosin Tartrate ■ Apigenin-7-Glucoside ■ Magnesium Carbonate Hydrate				
Hazard Level	Match	Sample Type	Source Library	Spectral Weight %
Clear	Tylosin Tartrate	USP/Pharmaceutical	Illicit, Version: 41	45%
Clear	Apigenin-7-Glucoside	USP/Pharmaceutical	Illicit, Version: 41	21%
Clear	Magnesium Carbonate Hydrate	USP/Pharmaceutical	Illicit, Version: 41	15%