

Sample Report



Sample Metadata

Sample Name	Scan 00041
Hazard Level	Precursor
Sample Type	Explosive
Last Modified	2024-03-06 11:40:42-05:00
Created	2024-03-06 11:40:42-05:00


Instrument

Serial Number	192601100201104
Firmware Package	8.0.3.56
Last Calibration	2024-03-06 10:07:19-05:00
Last System Suitability Test	Pass, 2024-03-06 10:07:29-05:00


Acquisition Parameters

Operating Procedure Name	Default Procedure
Operating Procedure Version	1
Integration Time	0.83 s
Auto Integration	On
Averages	3
Laser Power	5
Smart Tip Type	Intelligent UA, Surface (Position 1)
Smart Tip Serial Number	6075060600601336

Spectral Data

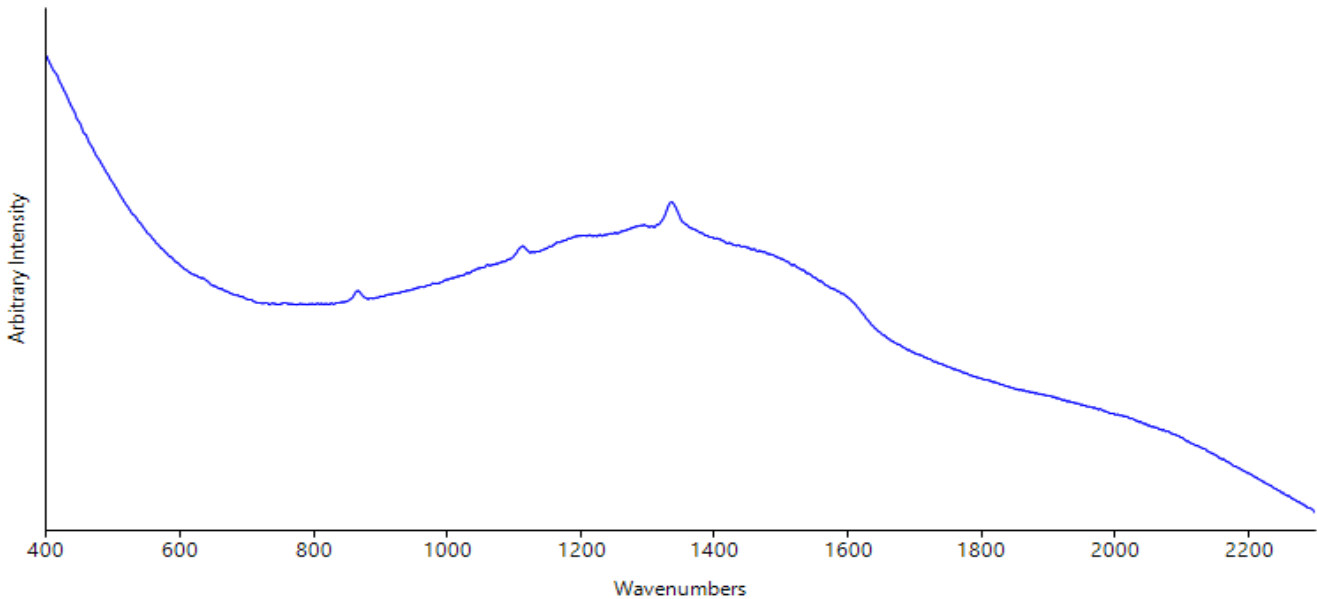


Identification Results

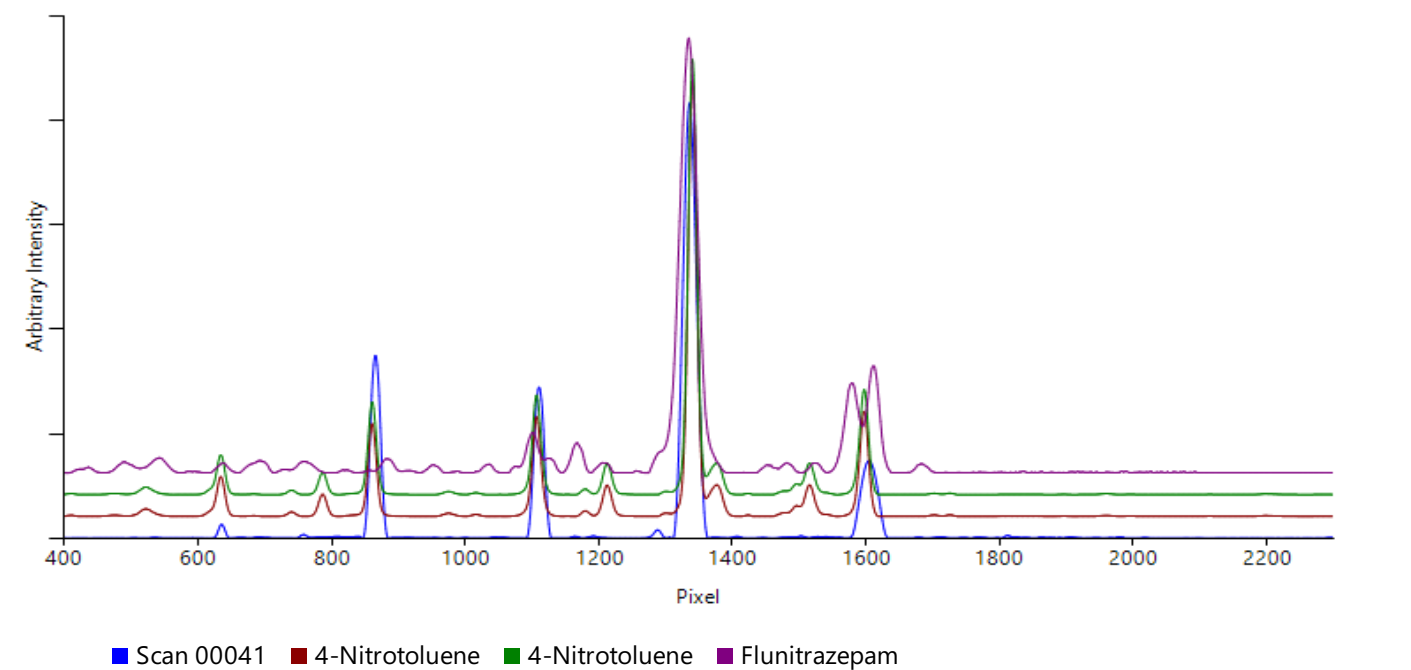

Hazard Level	Match	Sample Type	Match Score	Result Library
Precursor	4-Nitrotoluene	Explosive	0.76	Explosives, Version: 1
Clear	4-Nitrotoluene	Chemical	0.76	Illicit, Version: 41
Alarm	Flunitrazepam	Illicit Drug	0.76	Illicit, Version: 41

Mixture Identification Results

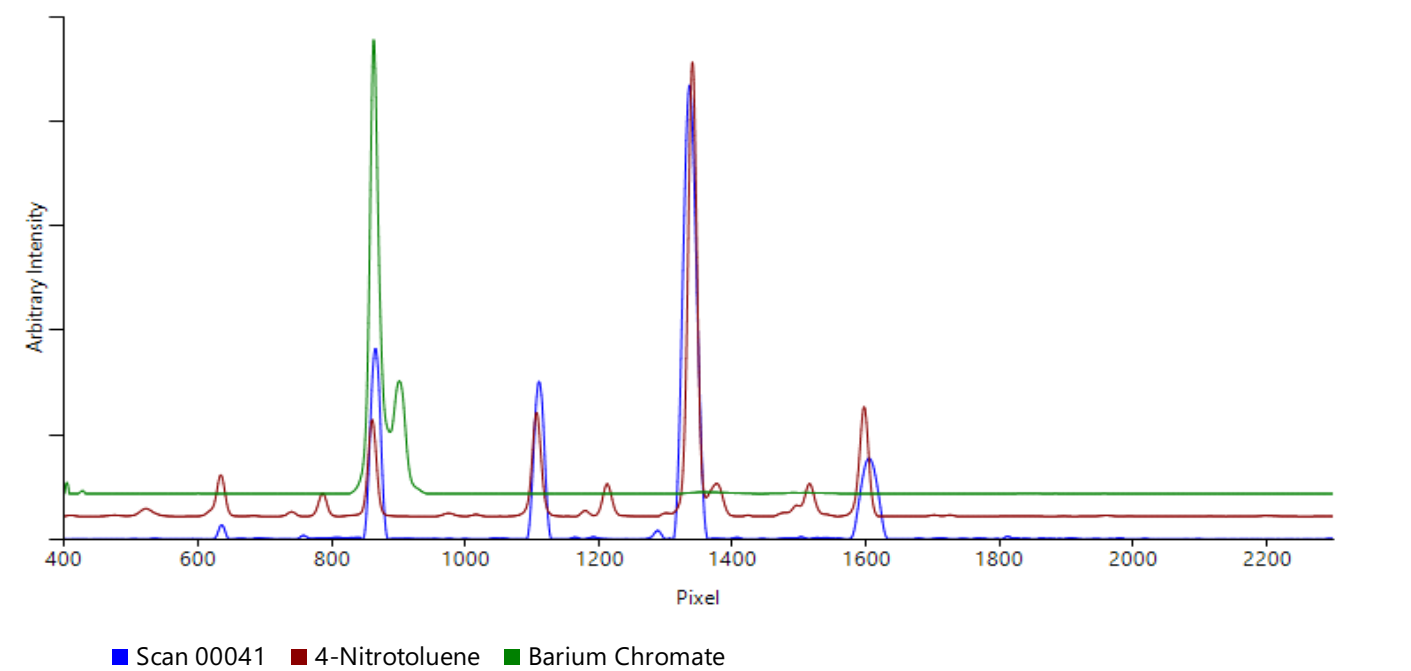

Hazard Level	Match	Sample Type	Source Library	Spectral Weight %
Precursor	4-Nitrotoluene	Explosive	Explosives, Version: 1	73%
Clear	Barium Chromate	Inorganic/Organometallic Chemical	MCRL Inorganic-Organometallics, Version: 1	11%