

Sample Report



Sample Metadata

Sample Name	Scan 00043
Hazard Level	Alarm
Sample Type	Illicit Drug
Last Modified	2024-03-06 11:43:01-05:00
Created	2024-03-06 11:43:01-05:00


Instrument

Serial Number	192601100201104
Firmware Package	8.0.3.56
Last Calibration	2024-03-06 10:07:19-05:00
Last System Suitability Test	Pass, 2024-03-06 10:07:29-05:00


Acquisition Parameters

Operating Procedure Name	Default Procedure
Operating Procedure Version	1
Integration Time	1.12 s
Auto Integration	On
Averages	3
Laser Power	5
Smart Tip Type	Intelligent UA, Surface (Position 1)
Smart Tip Serial Number	6075060600601336

Spectral Data

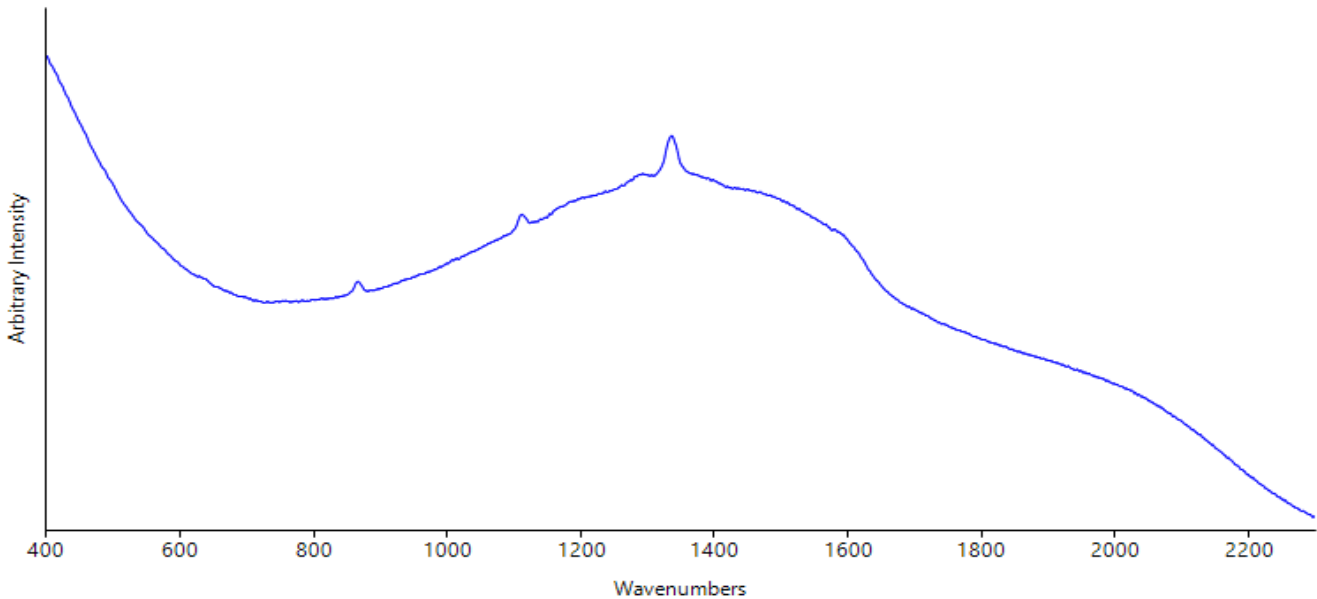


Identification Results

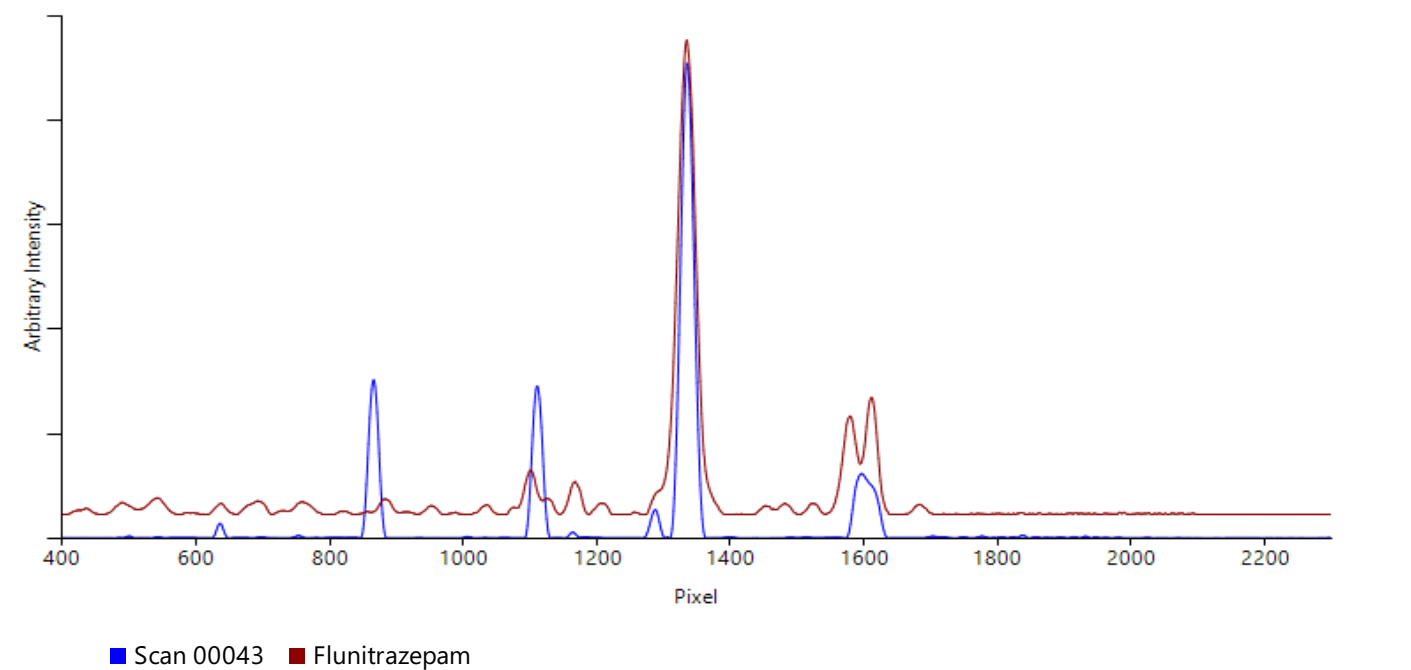

Hazard Level	Match	Sample Type	Match Score	Result Library
Alarm	Flunitrazepam	Illicit Drug	0.80	Illicit, Version: 41

Mixture Identification Results

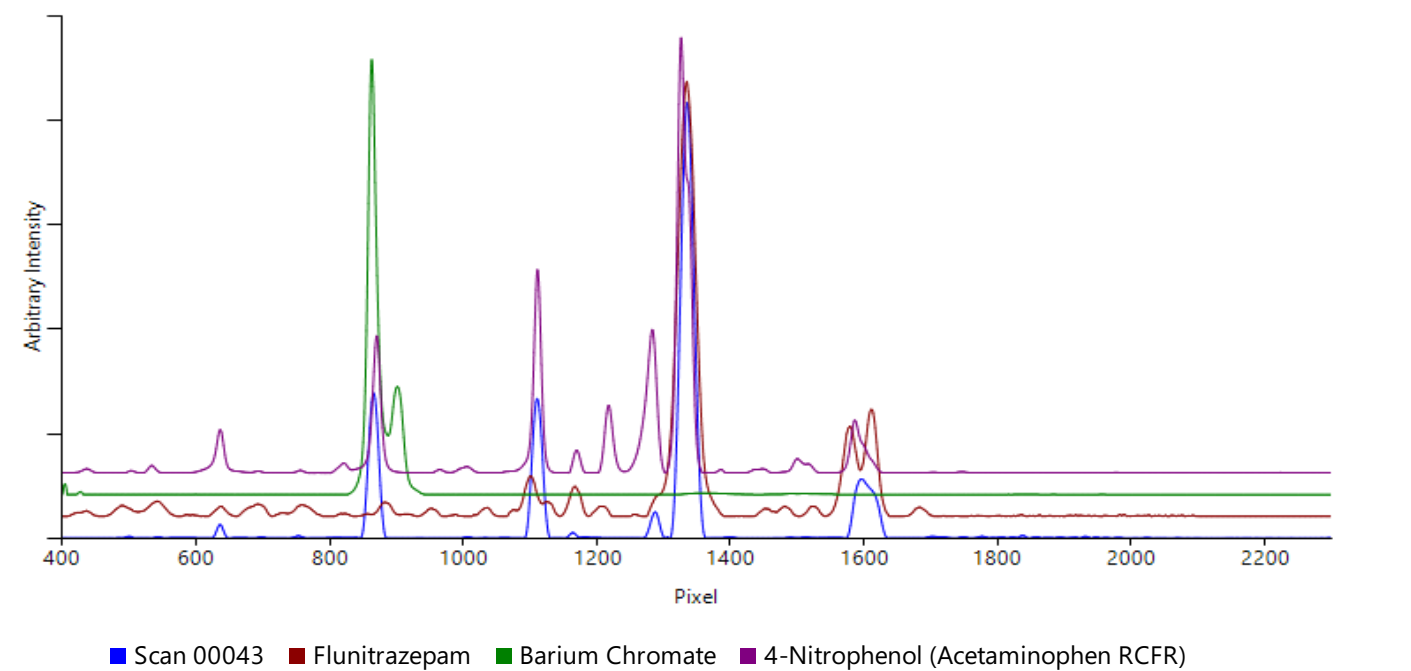

Hazard Level	Match	Sample Type	Source Library	Spectral Weight %
Alarm	Flunitrazepam	Illicit Drug	Illicit, Version: 41	50%
Clear	Barium Chromate	Inorganic/Organometallic Chemical	MCRL Inorganic-Organometallics, Version: 1	20%
Clear	4-Nitrophenol (Acetaminophen RCFR)	USP/Pharmaceutical	Illicit, Version: 41	13%