

Sample Report



Sample Metadata

Sample Name	Scan 00048
Hazard Level	Alarm
Sample Type	Explosive
Last Modified	2024-03-06 12:02:30-05:00
Created	2024-03-06 12:02:30-05:00


Instrument

Serial Number	192601100201104
Firmware Package	8.0.3.56
Last Calibration	2024-03-06 10:07:19-05:00
Last System Suitability Test	Pass, 2024-03-06 10:07:29-05:00


Acquisition Parameters

Operating Procedure Name	Default Procedure
Operating Procedure Version	1
Integration Time	2.30 s
Auto Integration	On
Averages	1
Laser Power	5
Smart Tip Type	Intelligent UA, Surface (Position 1)
Smart Tip Serial Number	6075060600601336

Spectral Data

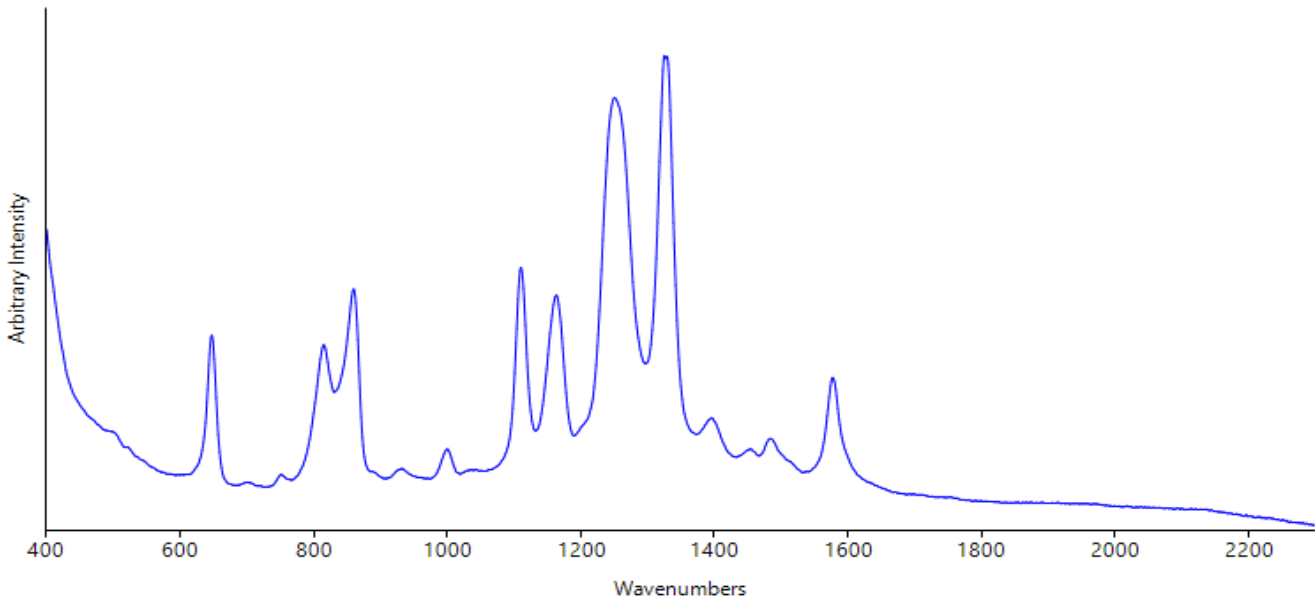


Identification Results

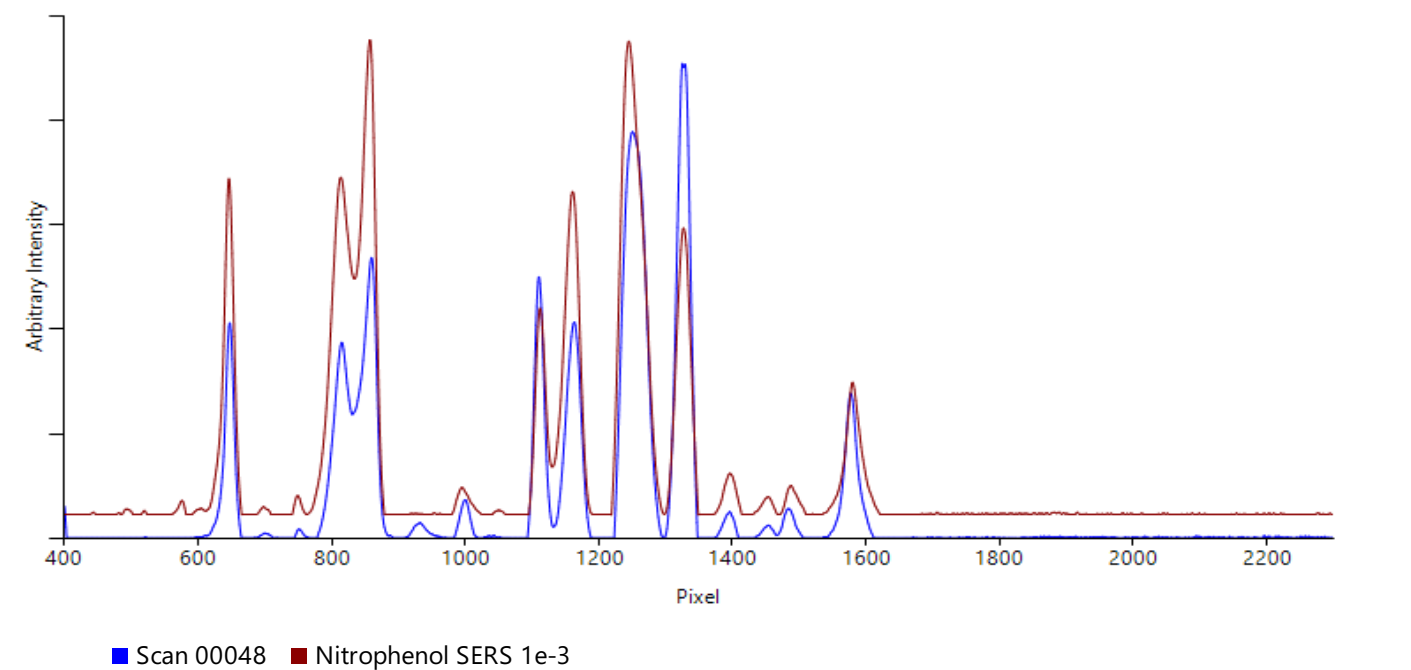

Hazard Level	Match	Sample Type	Match Score	Result Library
Unknown	Nitrophenol SERS 1e-3		0.83	NATO SERS, Version: 1

Mixture Identification Results

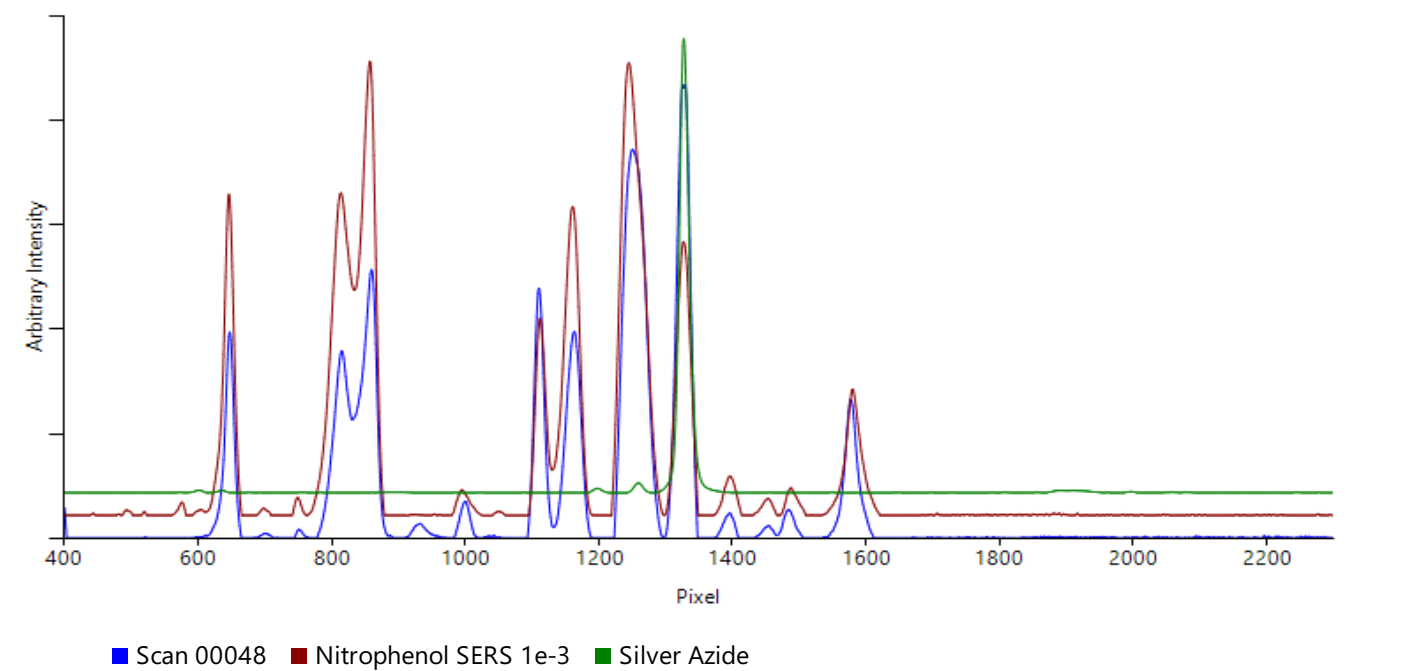

Hazard Level	Match	Sample Type	Source Library	Spectral Weight %
Unknown	Nitrophenol SERS 1e-3		NATO SERS, Version: 1	40%
Alarm	Silver Azide	Explosive	Explosives, Version: 1	38%